

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
 Data File : VX037536.D
 Acq On : 06 Sep 2023 06:47
 Operator : JC/MD
 Sample : 04232-07DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SBG-7DL

Quant Time: Sep 06 07:46:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 18 09:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	135210	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	226393	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	206374	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	93687	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	81214	41.663	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	83.320%		
35) Dibromofluoromethane	5.385	113	68993	46.015	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	92.040%		
50) Toluene-d8	8.647	98	266983	49.089	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	98.180%		
62) 4-Bromofluorobenzene	11.079	95	98218	45.954	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	91.900%		
Target Compounds						Qvalue
11) Tert butyl alcohol	2.947	59	15175	33.187	ug/l #	80
13) Acrolein	2.239	56	145	0.417	ug/l #	60
15) Acrylonitrile	2.947	53	217	0.266	ug/l #	17
16) Acetone	2.380	43	8475	11.114	ug/l #	77
17) Carbon Disulfide	2.502	76	988	0.279	ug/l	96
18) Methyl Acetate	2.715	43	773	0.269	ug/l	100
20) Methylene Chloride	2.788	84	2664	1.562	ug/l #	80
25) 2-Butanone	4.580	43	3978	3.464	ug/l #	85
36) 1,1-Dichloropropene	5.550	75	9945	4.669	ug/l #	52
37) Ethyl Acetate	4.739	43	701	0.322	ug/l #	76
38) Carbon Tetrachloride	5.556	117	14063	6.077	ug/l #	15
40) Benzene	6.037	78	148210	24.260	ug/l	98
43) Isopropyl Acetate	6.342	43	18142	5.252	ug/l #	89
44) Trichloroethene	7.123	130	486	0.281	ug/l	37
48) Methyl methacrylate	7.610	41	601	0.357	ug/l #	16
51) 4-Methyl-2-Pentanone	8.549	43	20807	9.919	ug/l #	37
52) Toluene	8.720	92	80075	19.837	ug/l	99
54) cis-1,3-Dichloropropene	8.549	75	7328	2.802	ug/l #	51
55) 1,1,2-Trichloroethane	9.013	97	553	0.336	ug/l #	17
57) 1,3-Dichloropropane	9.482	76	830	0.300	ug/l #	42
59) 2-Hexanone	9.482	43	9870	6.171	ug/l #	60
67) Ethyl Benzene	10.195	91	9366	1.220	ug/l	99
68) m/p-Xylenes	10.299	106	17791	6.003	ug/l	98
69) o-Xylene	10.640	106	11063	3.783	ug/l	99
70) Styrene	10.659	104	3314	0.688	ug/l #	59
76) 1,2,3-Trichloropropane	11.079	75	47777	23.946	ug/l #	38
80) 1,3,5-Trimethylbenzene	11.451	105	2945	0.518	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	47777	66.881	ug/l #	5
84) 1,2,4-Trimethylbenzene	11.756	105	8354	1.455	ug/l	90
90) Hexachloroethane	12.414	117	1490	1.639	ug/l #	17
95) Naphthalene	13.774	128	69912	8.946	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 06 07:46:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 18 09:30:38 2023
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion:168 Resp: 135210
Ion Ratio Lower Upper
168 100
99 62.6 56.6 85.0

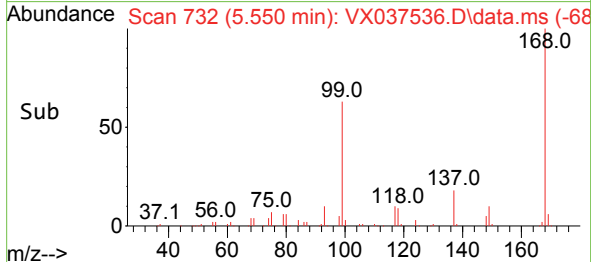

#11
Tert butyl alcohol
Concen: 33.187 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.030 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion: 59 Resp: 15175
Ion Ratio Lower Upper
59 100
57 0.7 6.0 9.0#


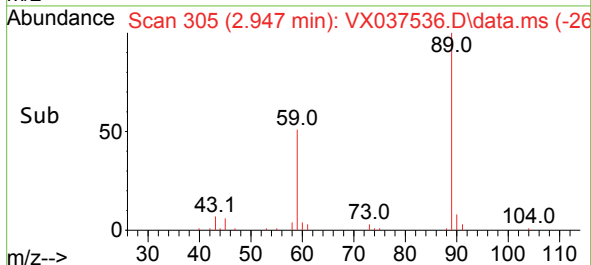
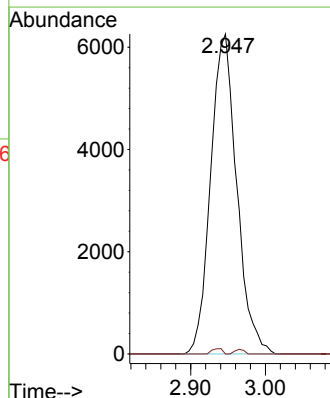
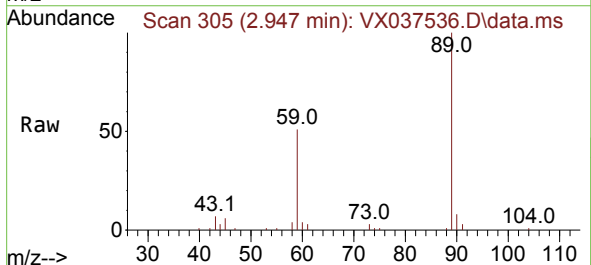




#13
Acrolein
Concen: 0.417 ug/l
RT: 2.239 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion: 56 Resp: 145
Ion Ratio Lower Upper
56 100
55 104.8 57.1 85.7#

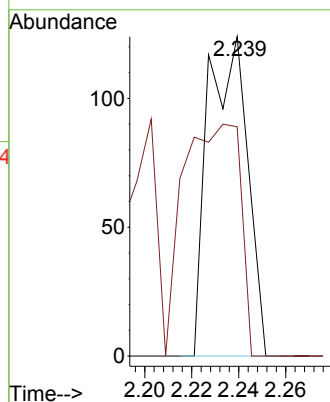

#15
Acrylonitrile
Concen: 0.266 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.116 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion: 53 Resp: 217
Ion Ratio Lower Upper
53 100
52 0.0 66.0 99.0#
51 0.0 29.8 44.6#


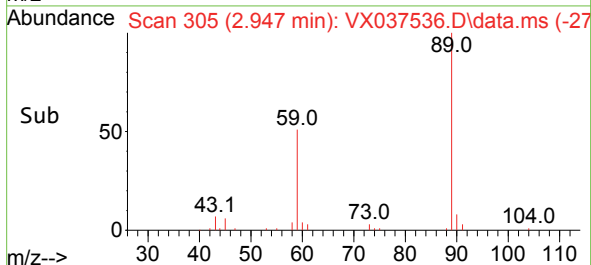

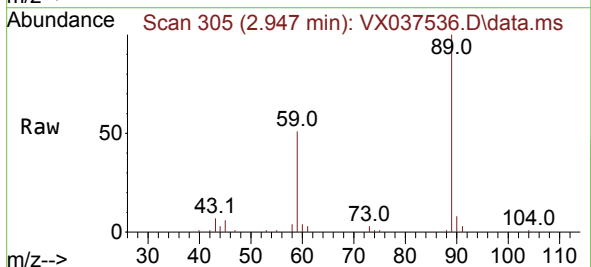


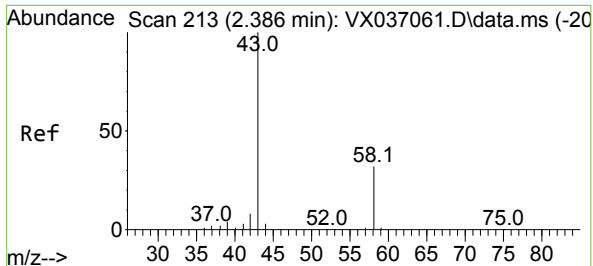

#16
Acetone
Concen: 11.114 ug/l
RT: 2.380 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion: 43 Resp: 8475
Ion Ratio Lower Upper
43 100
58 39.6 21.9 32.9#

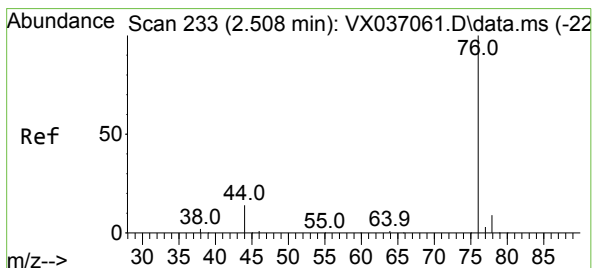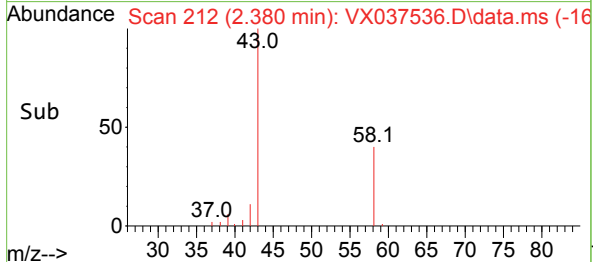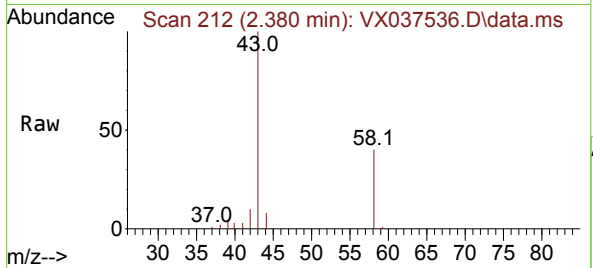

#17
Carbon Disulfide
Concen: 0.279 ug/l
RT: 2.502 min Scan# 232
Delta R.T. -0.006 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion: 76 Resp: 988
Ion Ratio Lower Upper
76 100
78 10.2 7.0 10.6


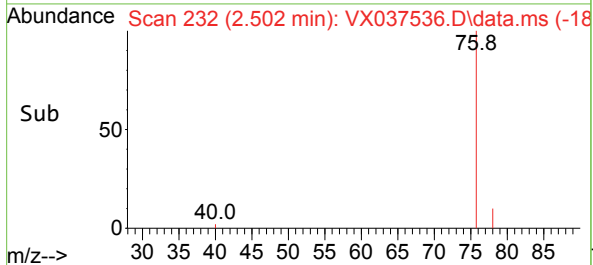

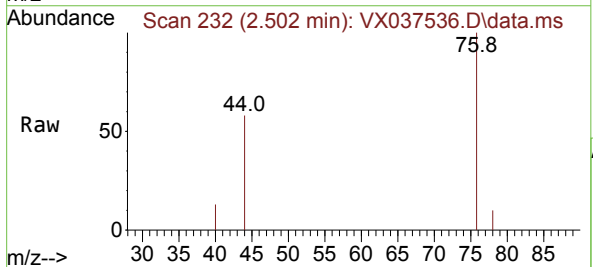




#18
Methyl Acetate
Concen: 0.269 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.012 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion: 43 Resp: 773
Ion Ratio Lower Upper
43 100
74 22.1 17.8 26.8



#20
Methylene Chloride
Concen: 1.562 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion: 84 Resp: 2664
Ion Ratio Lower Upper
84 100
49 102.1 103.6 155.4#
51 26.4 33.8 50.6#
86 67.4 49.4 74.0

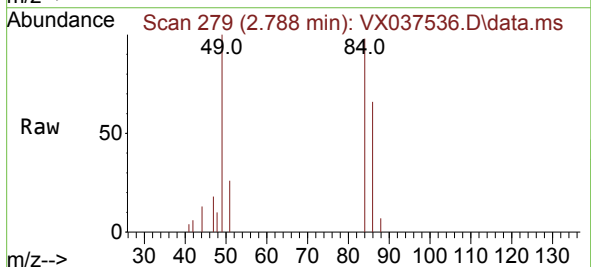



#25

2-Butanone

Concen: 3.464 ug/l

RT: 4.580 min Scan# 51

Delta R.T. 0.024 min

Lab File: VX037536.D

Acq: 06 Sep 2023 06:47

Instrument :

MSVOA_X

ClientSampleId :





SBG-7DL

Tgt Ion: 43 Resp: 3978

Ion Ratio Lower Upper

43 100

72 31.5 19.4 29.2#

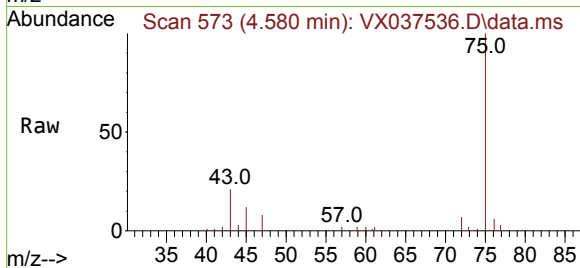

#33

1,2-Dichloroethane-d4

Concen: 41.663 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX037536.D




Acq: 06 Sep 2023 06:47


Tgt Ion: 65 Resp: 81214

Ion Ratio Lower Upper

65 100

67 52.9 0.0 100.2


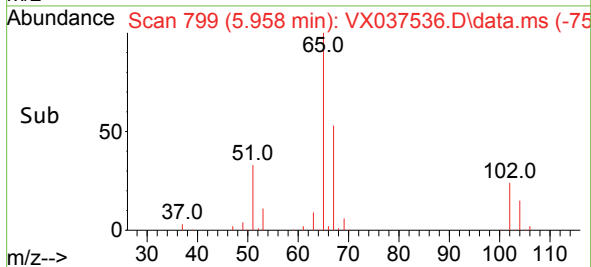

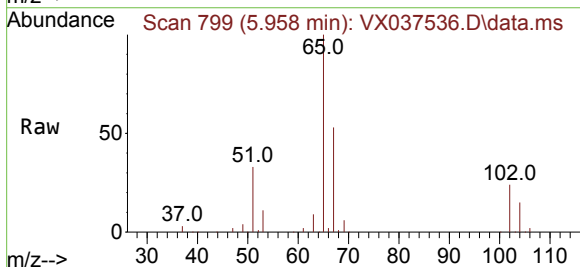




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion:114 Resp: 226393
Ion Ratio Lower Upper
114 100
63 18.4 0.0 45.0
88 16.5 0.0 36.6

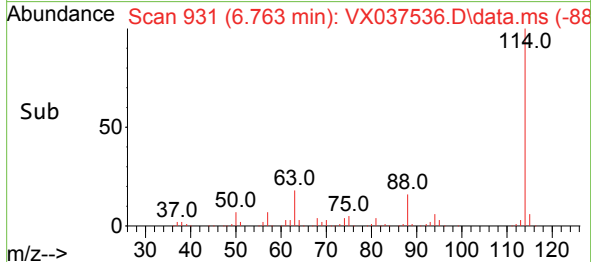

#35
Dibromofluoromethane
Concen: 46.015 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion:113 Resp: 68993
Ion Ratio Lower Upper
113 100
111 102.8 82.9 124.3
192 18.7 13.3 19.9


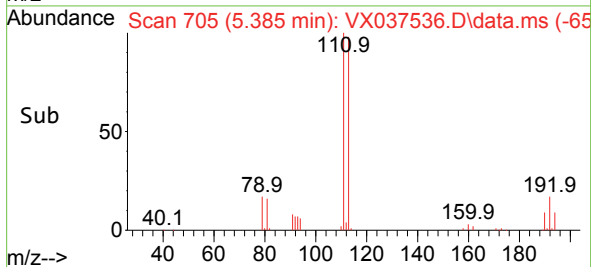

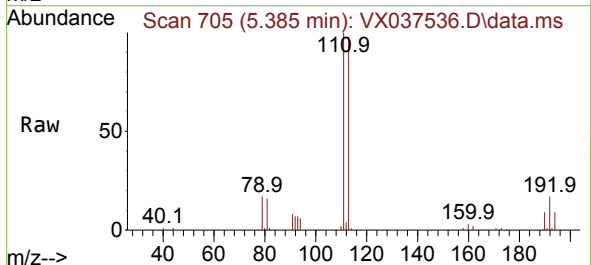




#36
1,1-Dichloropropene
Concen: 4.669 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion: 75 Resp: 9945
Ion Ratio Lower Upper
75 100
110 10.7 17.0 50.9#
77 0.0 24.7 37.1#

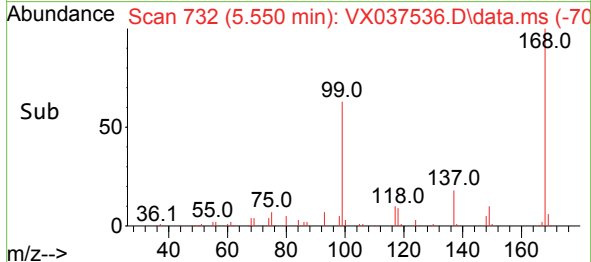

#37
Ethyl Acetate
Concen: 0.322 ug/l
RT: 4.739 min Scan# 599
Delta R.T. 0.024 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion: 43 Resp: 701
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 6.0 8.3 12.5#

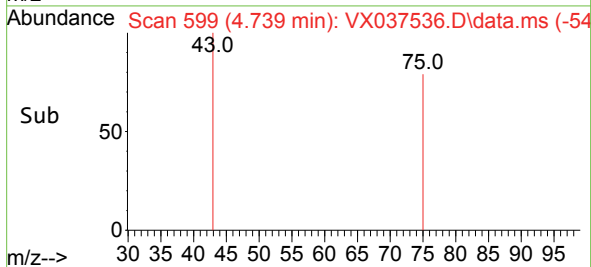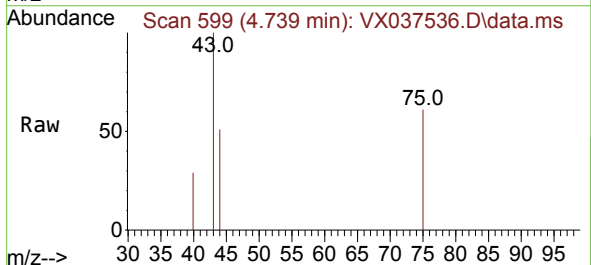

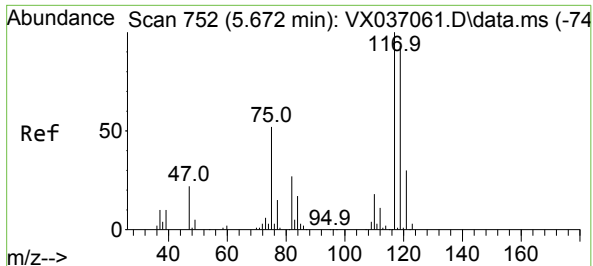

#38

Carbon Tetrachloride

Concen: 6.077 ug/l

RT: 5.556 min Scan# 71

Delta R.T. -0.116 min

Lab File: VX037536.D

Acq: 06 Sep 2023 06:47

Instrument :

MSVOA_X

ClientSampleId :

SBG-7DL





Tgt Ion:117 Resp: 14063

Ion Ratio Lower Upper

117 100

119 4.6 78.2 117.2#

121 0.0 24.4 36.6#

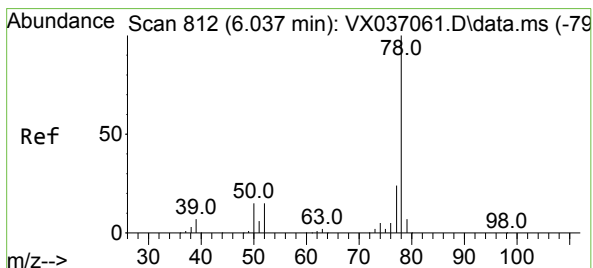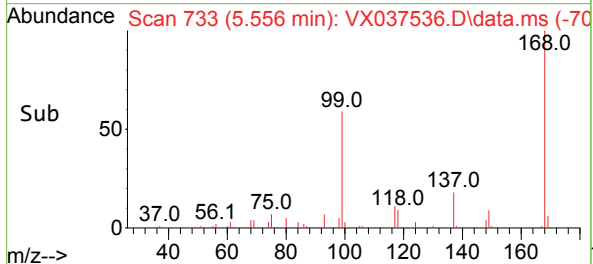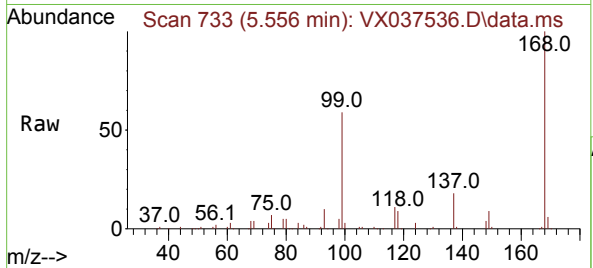

#40

Benzene

Concen: 24.260 ug/l

RT: 6.037 min Scan# 812

Delta R.T. 0.000 min

Lab File: VX037536.D




Acq: 06 Sep 2023 06:47


Tgt Ion: 78 Resp: 148210

Ion Ratio Lower Upper

78 100

77 23.3 19.3 28.9


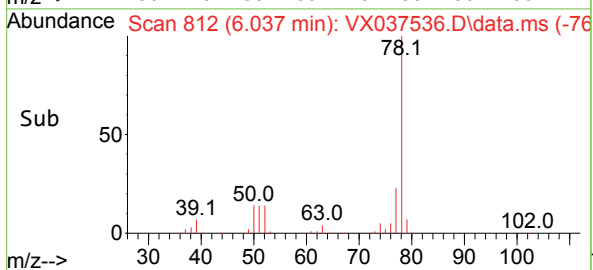

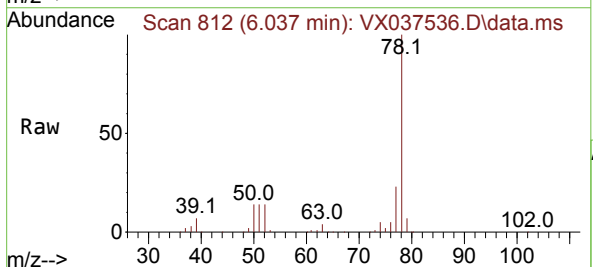




#43
Isopropyl Acetate
Concen: 5.252 ug/l
RT: 6.342 min Scan# 862
Delta R.T. 0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion: 43 Resp: 18142
Ion Ratio Lower Upper
43 100
61 23.5 15.2 22.8#
87 16.8 9.8 14.6#



#44
Trichloroethene
Concen: 0.281 ug/l
RT: 7.123 min Scan# 990
Delta R.T. 0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion:130 Resp: 486
Ion Ratio Lower Upper
130 100
95 166.4 0.0 204.4


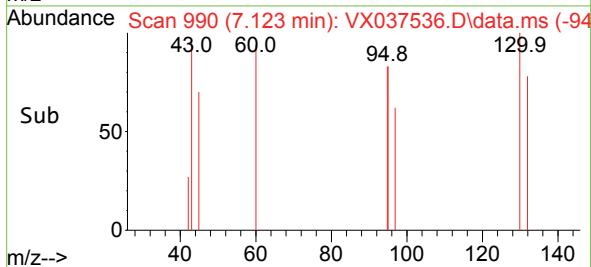

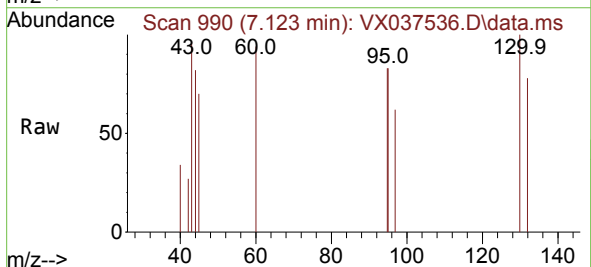




#48
Methyl methacrylate
Concen: 0.357 ug/l
RT: 7.610 min Scan# 1070
Delta R.T. -0.085 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion: 41 Resp: 601
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 0.0 47.7 71.5#



#50
Toluene-d8
Concen: 49.089 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion: 98 Resp: 266983
Ion Ratio Lower Upper
98 100
100 65.8 53.1 79.7




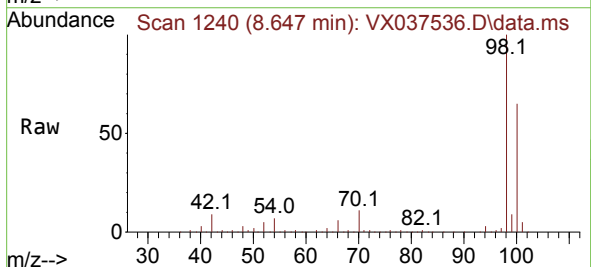




#51
4-Methyl-2-Pentanone
Concen: 9.919 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion: 43 Resp: 20807
Ion Ratio Lower Upper
43 100
58 0.0 30.4 45.6#

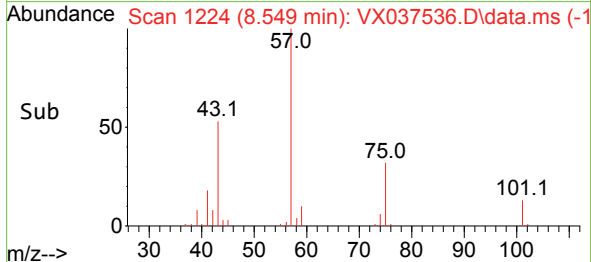

#52
Toluene
Concen: 19.837 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion: 92 Resp: 80075
Ion Ratio Lower Upper
92 100
91 168.5 134.2 201.2


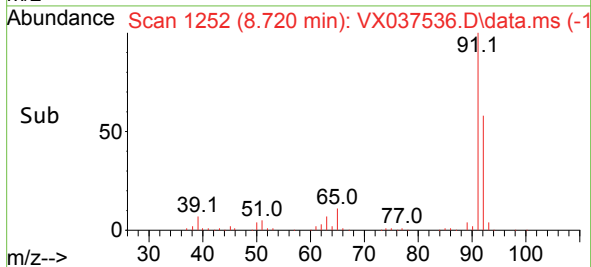

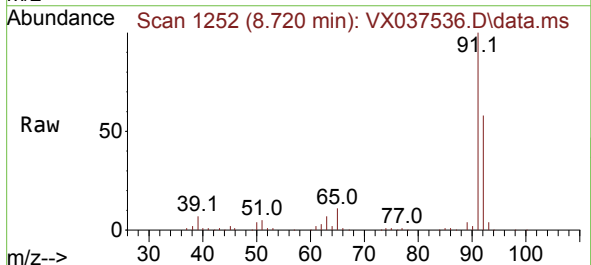




#54
 cis-1,3-Dichloropropene
 Concen: 2.802 ug/l
 RT: 8.549 min Scan# 11
 Delta R.T. 0.183 min
 Lab File: VX037536.D
 Acq: 06 Sep 2023 06:47




Instrument :
 MSVOA_X
 ClientSampleId :
 SBG-7DL


Tgt Ion: 75 Resp: 7328
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.3 37.9#
 39 24.6 46.7 70.1#



#55
 1,1,2-Trichloroethane
 Concen: 0.336 ug/l
 RT: 9.013 min Scan# 1300
 Delta R.T. -0.140 min
 Lab File: VX037536.D
 Acq: 06 Sep 2023 06:47

Tgt Ion: 97 Resp: 553
 Ion Ratio Lower Upper
 97 100
 83 0.0 65.8 98.8#
 85 0.0 41.6 62.4#
 99 0.0 47.8 71.8#





#57

1,3-Dichloropropane

Concen: 0.300 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.177 min

Lab File: VX037536.D

Acq: 06 Sep 2023 06:47

Instrument :

MSVOA_X

ClientSampleId :





SBG-7DL

Tgt Ion: 76 Resp: 830

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#



#59

2-Hexanone

Concen: 6.171 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.049 min

Lab File: VX037536.D




Acq: 06 Sep 2023 06:47


Tgt Ion: 43 Resp: 9870

Ion Ratio Lower Upper

43 100

58 24.1 26.2 78.5#









#62
4-Bromofluorobenzene
Concen: 45.954 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion: 95 Resp: 98218
Ion Ratio Lower Upper
95 100
174 74.3 0.0 135.6
176 73.4 0.0 131.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion: 117 Resp: 206374
Ion Ratio Lower Upper
117 100
82 53.7 46.2 69.4
119 32.3 25.5 38.3









#67
Ethyl Benzene
Concen: 1.220 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47




Instrument :
MSVOA_X
ClientSampleId :
SBG-7DL


Tgt Ion: 91 Resp: 9366
Ion Ratio Lower Upper
91 100
106 31.6 24.9 37.3

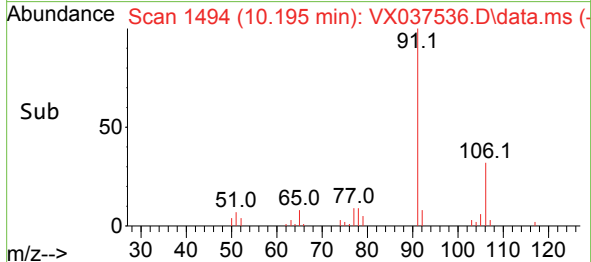

#68
m/p-Xylenes
Concen: 6.003 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX037536.D
Acq: 06 Sep 2023 06:47

Tgt Ion: 106 Resp: 17791
Ion Ratio Lower Upper
106 100
91 204.0 165.5 248.3

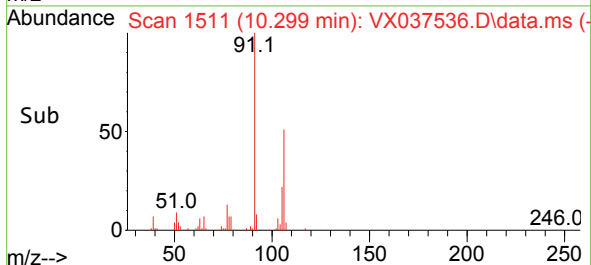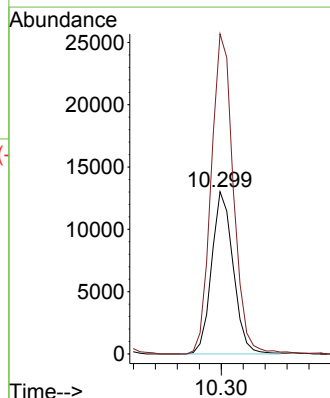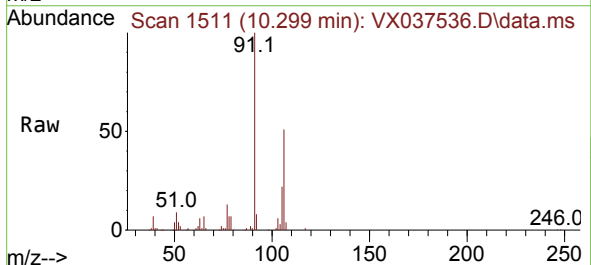



#69

o-Xylene

Concen: 3.783 ug/l

RT: 10.640 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX037536.D

Acq: 06 Sep 2023 06:47

Instrument :

MSVOA_X

ClientSampleId :





SBG-7DL

Tgt Ion:106 Resp: 11063

Ion Ratio Lower Upper

106 100

91 216.3 108.9 326.8



#70

Styrene

Concen: 0.688 ug/l

RT: 10.659 min Scan# 1570

Delta R.T. 0.007 min

Lab File: VX037536.D

Acq: 06 Sep 2023 06:47




Tgt Ion:104 Resp: 3314


Ion Ratio Lower Upper

104 100

78 85.4 43.6 65.4#

103 82.5 43.6 65.4#









#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX037536.D
 Acq: 06 Sep 2023 06:47




Instrument :
 MSVOA_X
 ClientSampleId :
 SBG-7DL


Tgt Ion:152 Resp: 93687
 Ion Ratio Lower Upper
 152 100
 115 61.5 43.3 129.9
 150 156.3 0.0 345.0

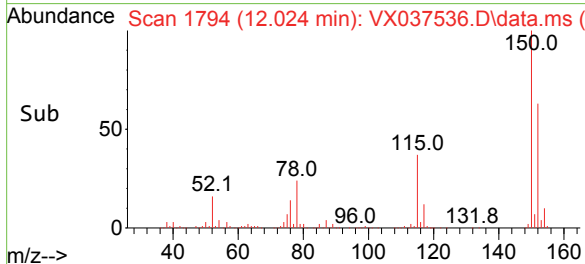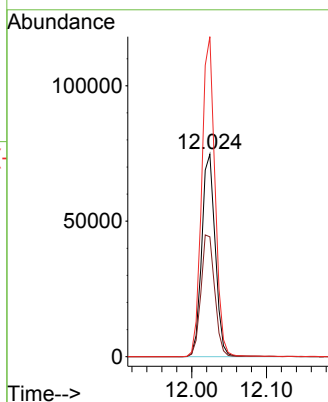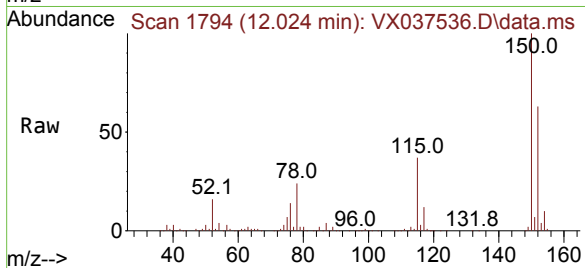

#76
 1,2,3-Trichloropropane
 Concen: 23.946 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.159 min
 Lab File: VX037536.D
 Acq: 06 Sep 2023 06:47

Tgt Ion: 75 Resp: 47777
 Ion Ratio Lower Upper
 75 100
 77 1.0 19.1 57.5#

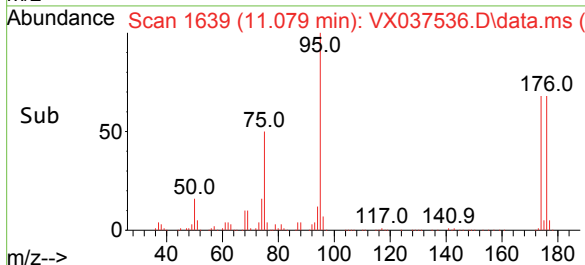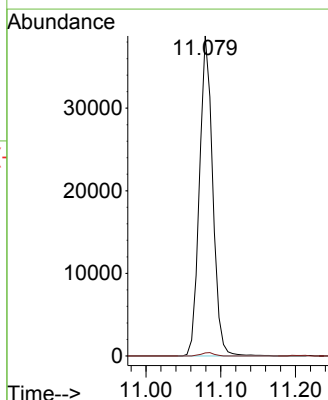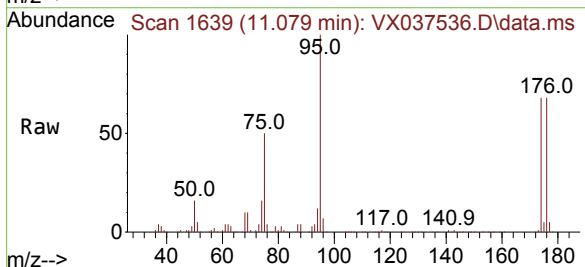



#80

1,3,5-Trimethylbenzene

Concen: 0.518 ug/l

RT: 11.451 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX037536.D

Acq: 06 Sep 2023 06:47

Instrument :

MSVOA_X

ClientSampleId :





SBG-7DL

Tgt Ion:105 Resp: 2945

Ion Ratio Lower Upper

105 100

120 45.8 24.1 72.3

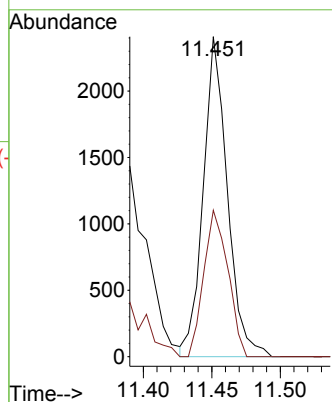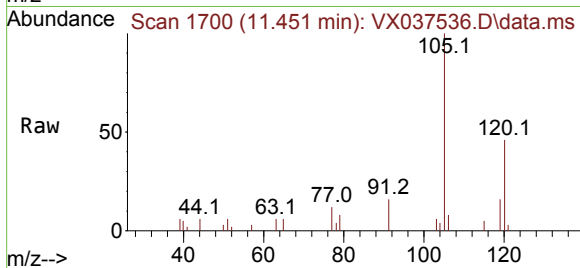

#81

trans-1,4-Dichloro-2-butene

Concen: 66.881 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX037536.D

Acq: 06 Sep 2023 06:47




Tgt Ion: 75 Resp: 47777


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.0 36.9 55.3#

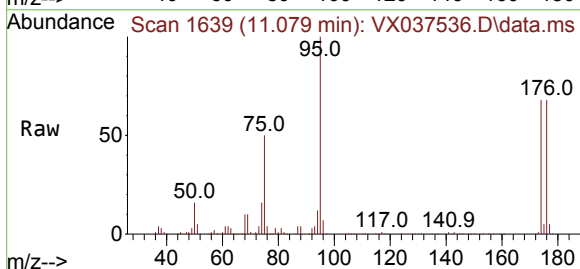



#84

1,2,4-Trimethylbenzene

Concen: 1.455 ug/l

RT: 11.756 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX037536.D

Acq: 06 Sep 2023 06:47

Instrument :

MSVOA_X

ClientSampleId :





SBG-7DL

Tgt Ion:105 Resp: 8354

Ion Ratio Lower Upper

105 100

120 36.2 21.2 63.6

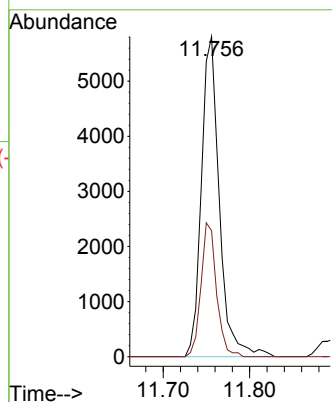

#90

Hexachloroethane

Concen: 1.639 ug/l

RT: 12.414 min Scan# 1858

Delta R.T. -0.122 min

Lab File: VX037536.D




Acq: 06 Sep 2023 06:47


Tgt Ion:117 Resp: 1490

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#





#95

Naphthalene

Concen: 8.946 ug/l

RT: 13.774 min Scan# 20

Delta R.T. 0.000 min

Lab File: VX037536.D


Acq: 06 Sep 2023 06:47

Instrument :

MSVOA_X

ClientSampleId :

SBG-7DL

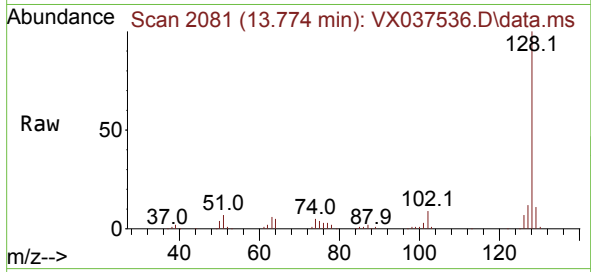

Tgt Ion:128 Resp: 69912

Ion Ratio Lower Upper

128 100

127 12.3 10.3 15.5

129 11.0 8.8 13.2

