

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090523\  
 Data File : VX037523.D  
 Acq On : 05 Sep 2023 19:39  
 Operator : JC/MD  
 Sample : IBLK  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK

Quant Time: Sep 06 02:59:33 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Aug 18 09:30:38 2023  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 5.550  | 168  | 127052   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 6.763  | 114  | 210624   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 10.055 | 117  | 188282   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 12.024 | 152  | 79549    | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |         |
|-----------------------------|--------|-------|----------|----------|------|---------|
| System Monitoring Compounds |        |       |          |          |      |         |
| 33) 1,2-Dichloroethane-d4   | 5.958  | 65    | 74331    | 40.581   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 78 - 117 | Recovery | =    | 81.160% |
| 35) Dibromofluoromethane    | 5.391  | 113   | 63525    | 45.540   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 75 - 124 | Recovery | =    | 91.080% |
| 50) Toluene-d8              | 8.647  | 98    | 248403   | 49.093   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 92 - 112 | Recovery | =    | 98.180% |
| 62) 4-Bromofluorobenzene    | 11.079 | 95    | 86300    | 43.400   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 83 - 123 | Recovery | =    | 86.800% |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090523\  
Data File : VX037523.D  
Acq On : 05 Sep 2023 19:39  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Quant Time: Sep 06 02:59:33 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
Quant Title : SW846 8260  
QLast Update : Fri Aug 18 09:30:38 2023  
Response via : Initial Calibration

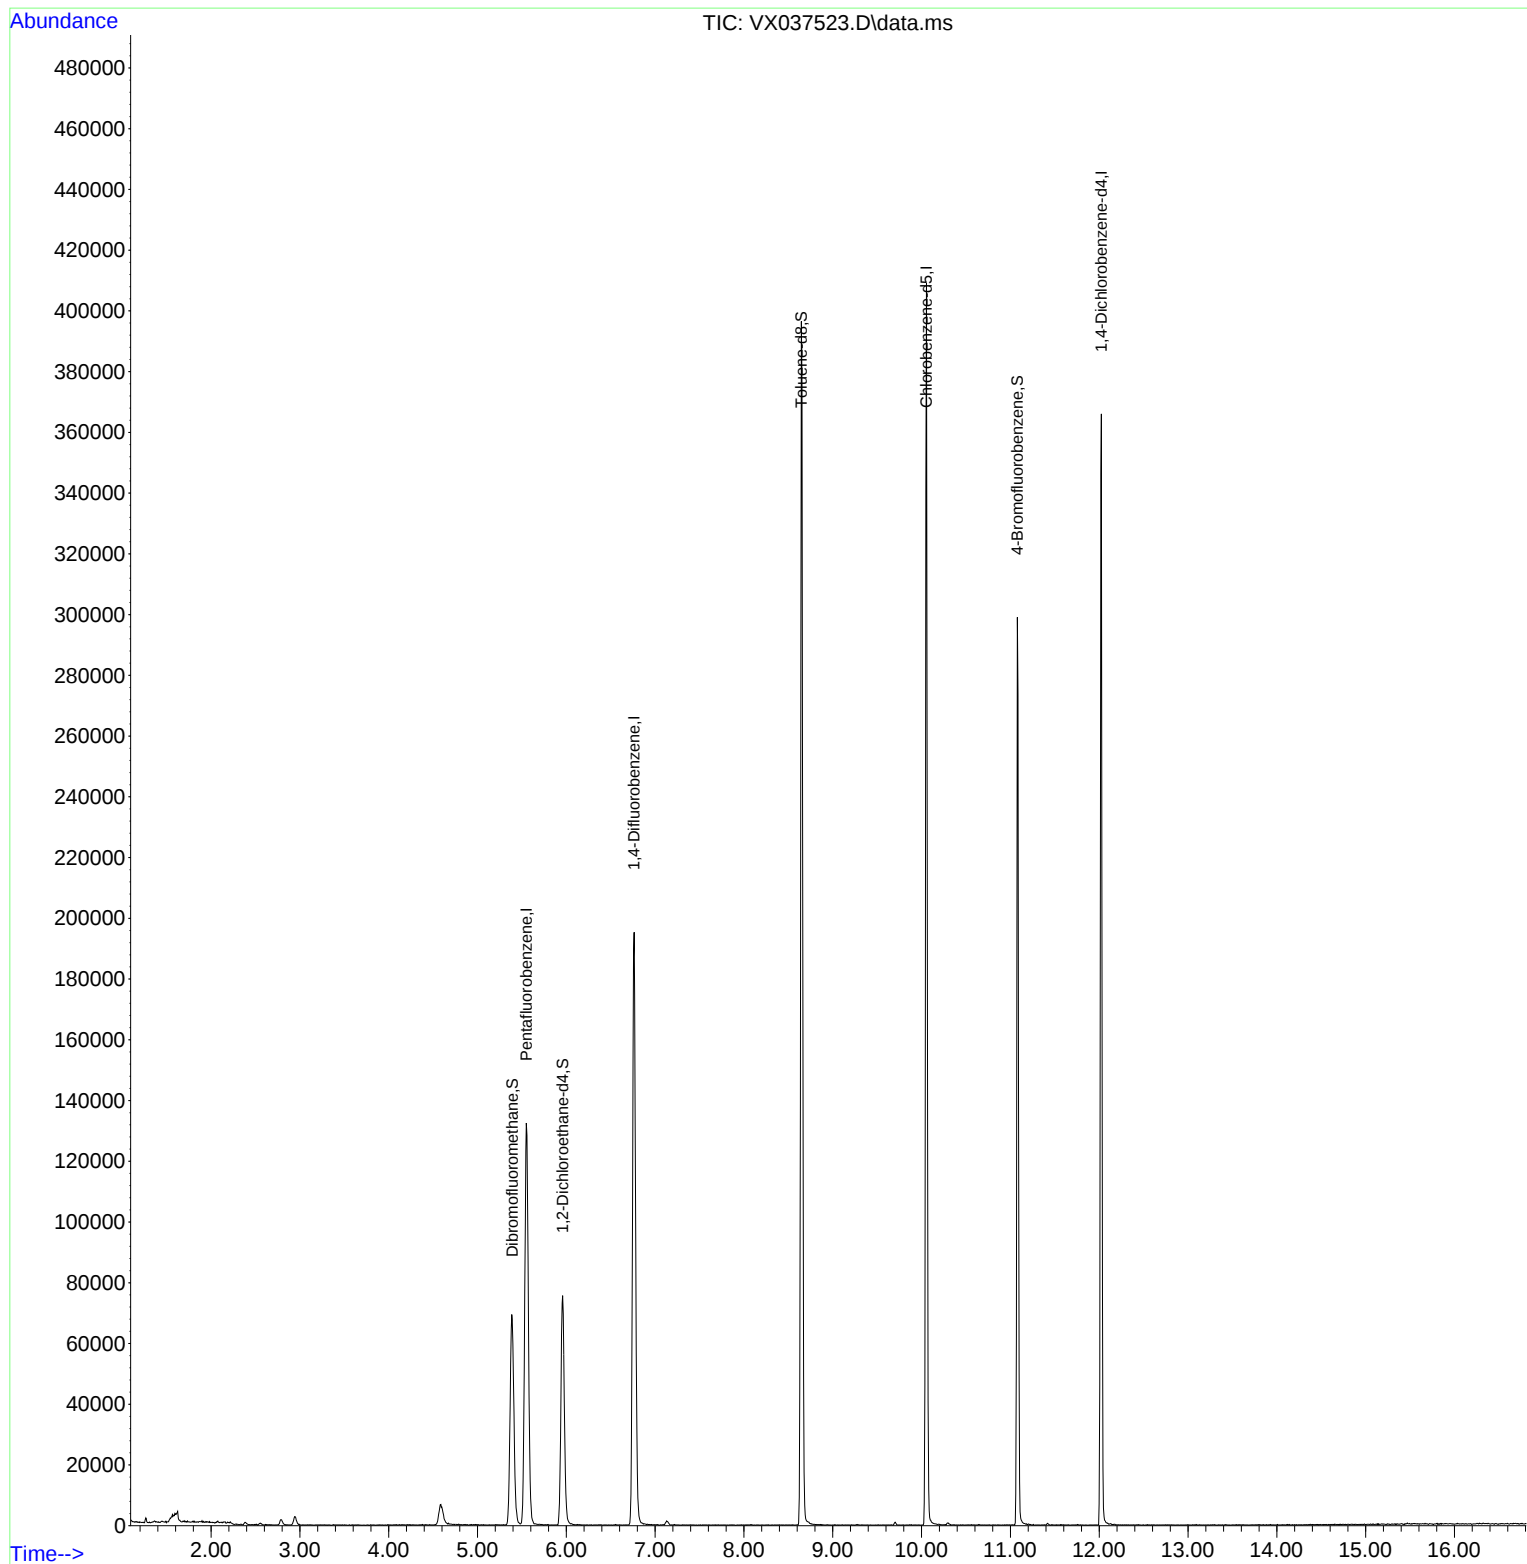



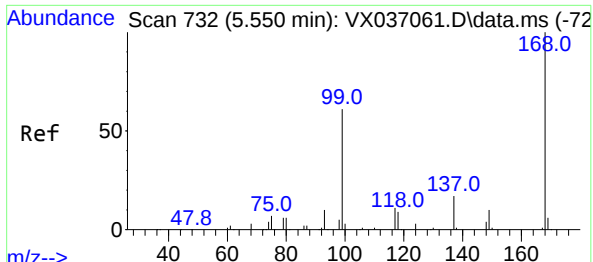


#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 712  
Delta R.T. -0.000 min  
Lab File: VX037523.D  
Acq: 05 Sep 2023 19:39

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK



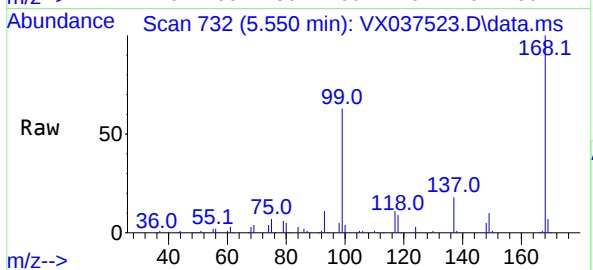



Tgt Ion:168 Resp: 127052  
Ion Ratio Lower Upper  
168 100  
99 63.3 56.6 85.0

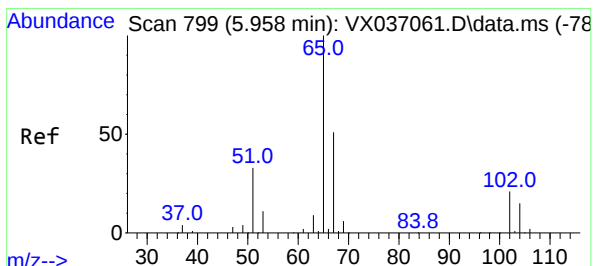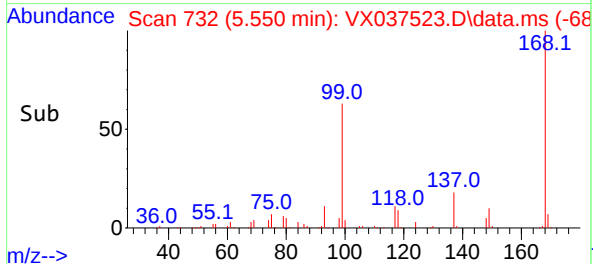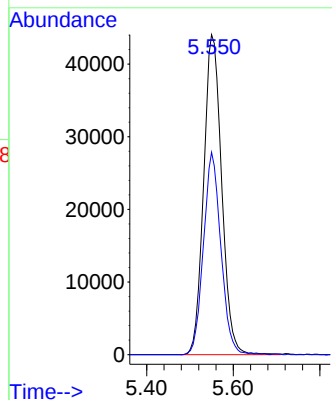

#33  
1,2-Dichloroethane-d4  
Concen: 40.581 ug/l  
RT: 5.958 min Scan# 799  
Delta R.T. 0.000 min  
Lab File: VX037523.D  
Acq: 05 Sep 2023 19:39

Tgt Ion: 65 Resp: 74331  
Ion Ratio Lower Upper  
65 100  
67 52.6 0.0 100.2


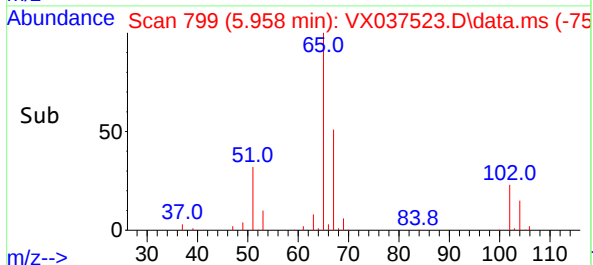
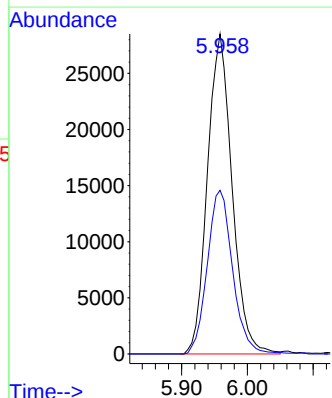
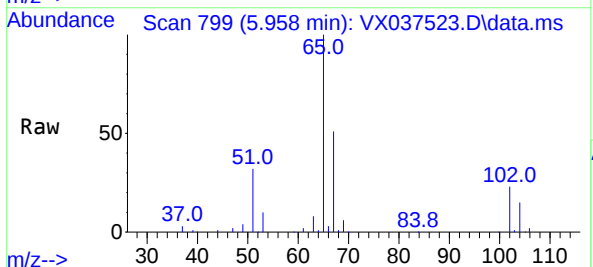


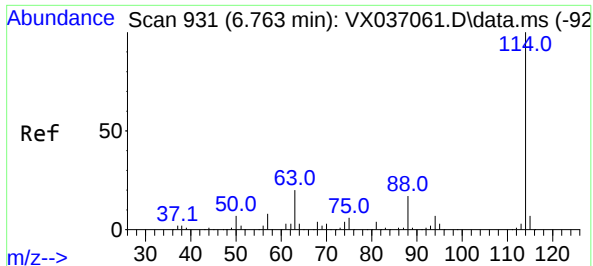

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.763 min Scan# 911  
Delta R.T. 0.000 min  
Lab File: VX037523.D  
Acq: 05 Sep 2023 19:39




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion:114 Resp: 210624  
Ion Ratio Lower Upper  
114 100  
63 18.3 0.0 45.0  
88 16.7 0.0 36.6

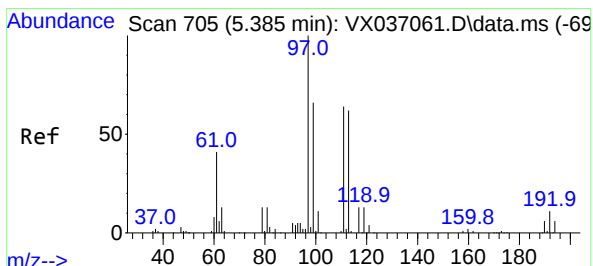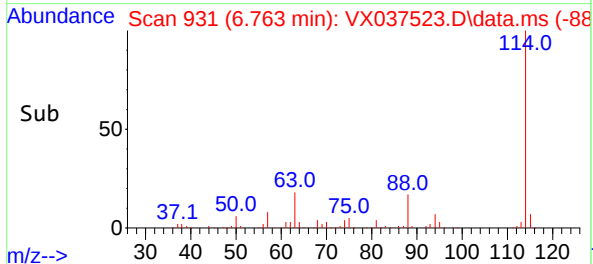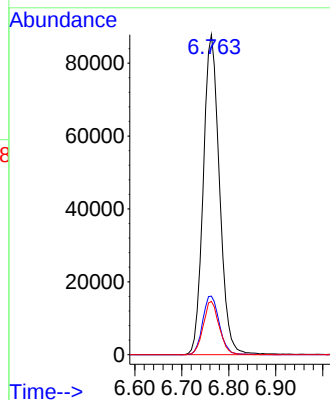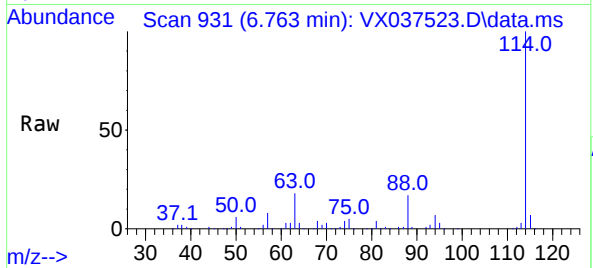

#35  
Dibromofluoromethane  
Concen: 45.540 ug/l  
RT: 5.391 min Scan# 706  
Delta R.T. 0.006 min  
Lab File: VX037523.D  
Acq: 05 Sep 2023 19:39

Tgt Ion:113 Resp: 63525  
Ion Ratio Lower Upper  
113 100  
111 102.7 82.9 124.3  
192 19.1 13.3 19.9


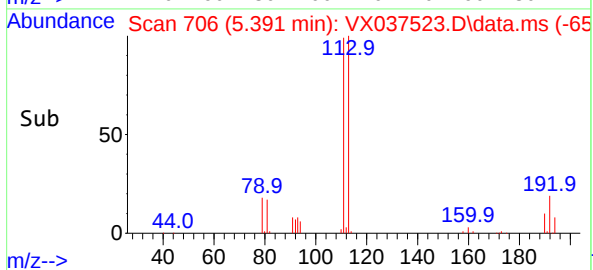
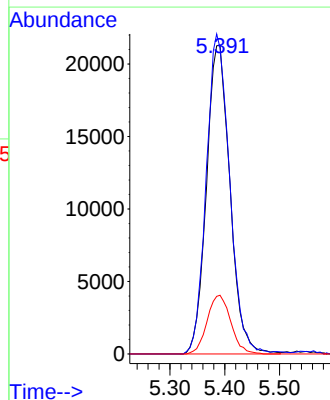
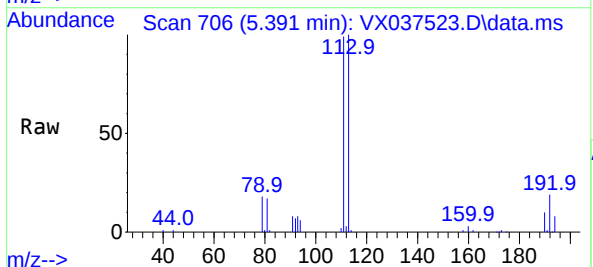


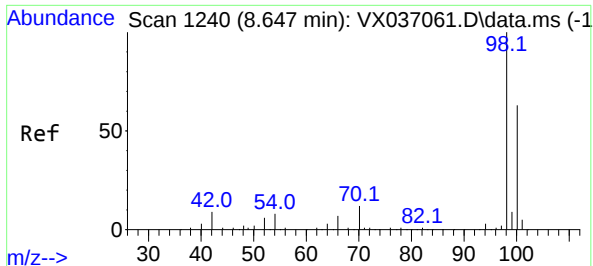

#50  
Toluene-d8  
Concen: 49.093 ug/l  
RT: 8.647 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX037523.D  
Acq: 05 Sep 2023 19:39




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 98 Resp: 248403  
Ion Ratio Lower Upper  
98 100  
100 66.5 53.1 79.7

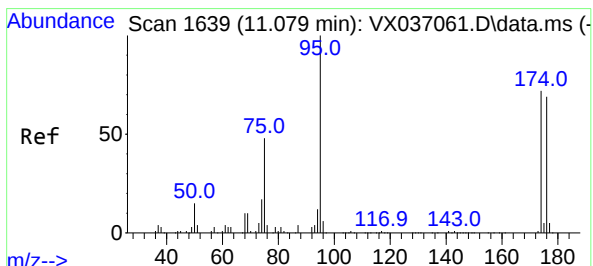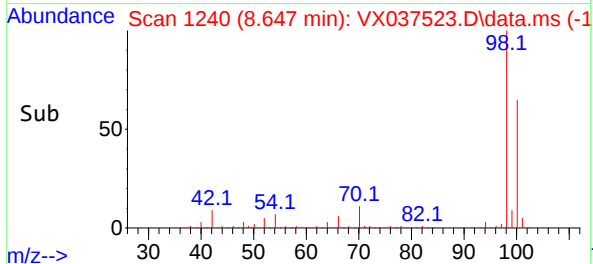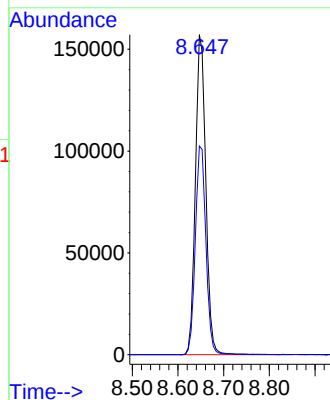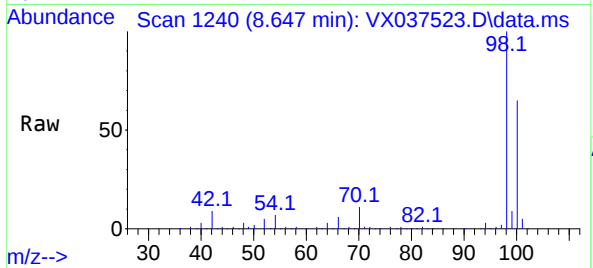

#62  
4-Bromofluorobenzene  
Concen: 43.400 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.000 min  
Lab File: VX037523.D  
Acq: 05 Sep 2023 19:39

Tgt Ion: 95 Resp: 86300  
Ion Ratio Lower Upper  
95 100  
174 74.7 0.0 135.6  
176 72.3 0.0 131.0


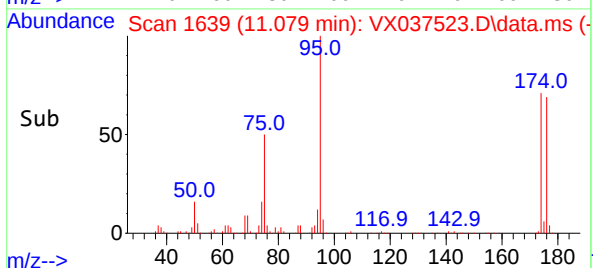
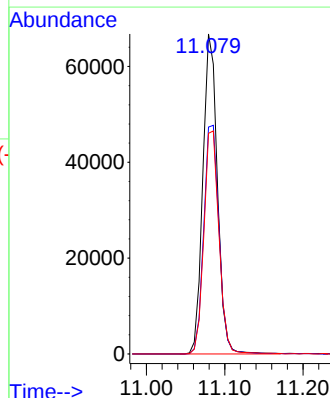
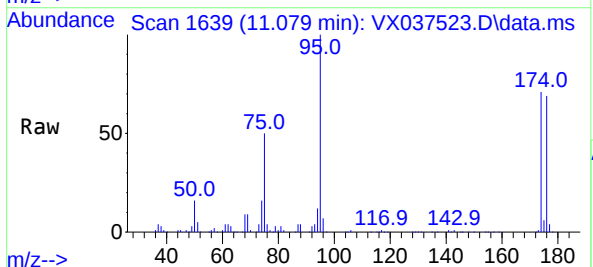


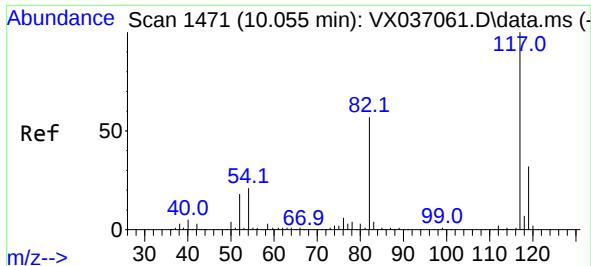

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.000 min  
Lab File: VX037523.D  
Acq: 05 Sep 2023 19:39

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Tgt Ion:117 Resp: 188282  
Ion Ratio Lower Upper  
117 100  
82 54.4 46.2 69.4  
119 32.2 25.5 38.3

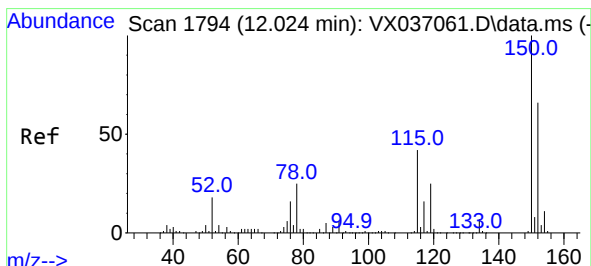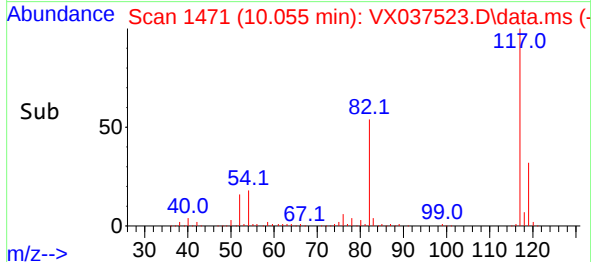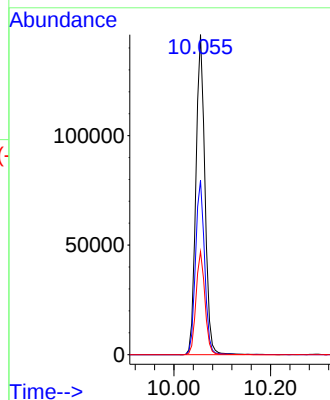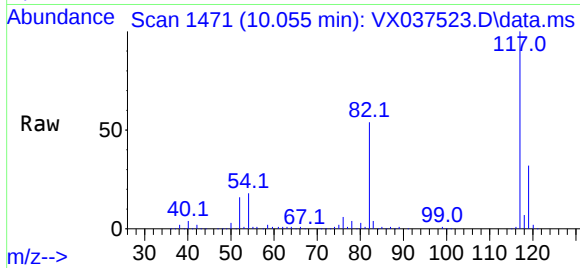

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 1794  
Delta R.T. 0.000 min  
Lab File: VX037523.D  
Acq: 05 Sep 2023 19:39

Tgt Ion:152 Resp: 79549  
Ion Ratio Lower Upper  
152 100  
115 63.4 43.3 129.9  
150 155.5 0.0 345.0

