

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090523\  
Data File : VX037520.D  
Acq On : 05 Sep 2023 18:25  
Operator : JC/MD  
Sample : 04254-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TT161S1-20230829

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M

Title : SW846 8260

Signal : TIC: VX037520.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.611       | 406           | 414         | 423          | rVB2     | 4848           | 11262         | 1.86%           | 0.355%        |
| 2         | 5.385       | 695           | 705         | 720          | rBV      | 68411          | 201162        | 33.20%          | 6.334%        |
| 3         | 5.550       | 720           | 732         | 747          | rVB      | 127168         | 363747        | 60.04%          | 11.453%       |
| 4         | 5.958       | 789           | 799         | 818          | rBV      | 74047          | 198630        | 32.78%          | 6.254%        |
| 5         | 6.763       | 921           | 931         | 945          | rBV      | 192361         | 453039        | 74.77%          | 14.265%       |
| 6         | 7.129       | 985           | 991         | 999          | rBV3     | 4177           | 8773          | 1.45%           | 0.276%        |
| 7         | 8.647       | 1234          | 1240        | 1257         | rBV      | 373277         | 605889        | 100.00%         | 19.077%       |
| 8         | 10.055      | 1465          | 1471        | 1485         | rBV      | 387388         | 516184        | 85.19%          | 16.253%       |
| 9         | 11.079      | 1634          | 1639        | 1657         | rBV      | 290080         | 376439        | 62.13%          | 11.853%       |
| 10        | 12.024      | 1789          | 1794        | 1808         | rBV      | 353941         | 440837        | 72.76%          | 13.880%       |


Sum of corrected areas: 3175962

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090523\  
Data File : VX037520.D  
Acq On : 05 Sep 2023 18:25  
Operator : JC/MD  
Sample : 04254-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TT161S1-20230829

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

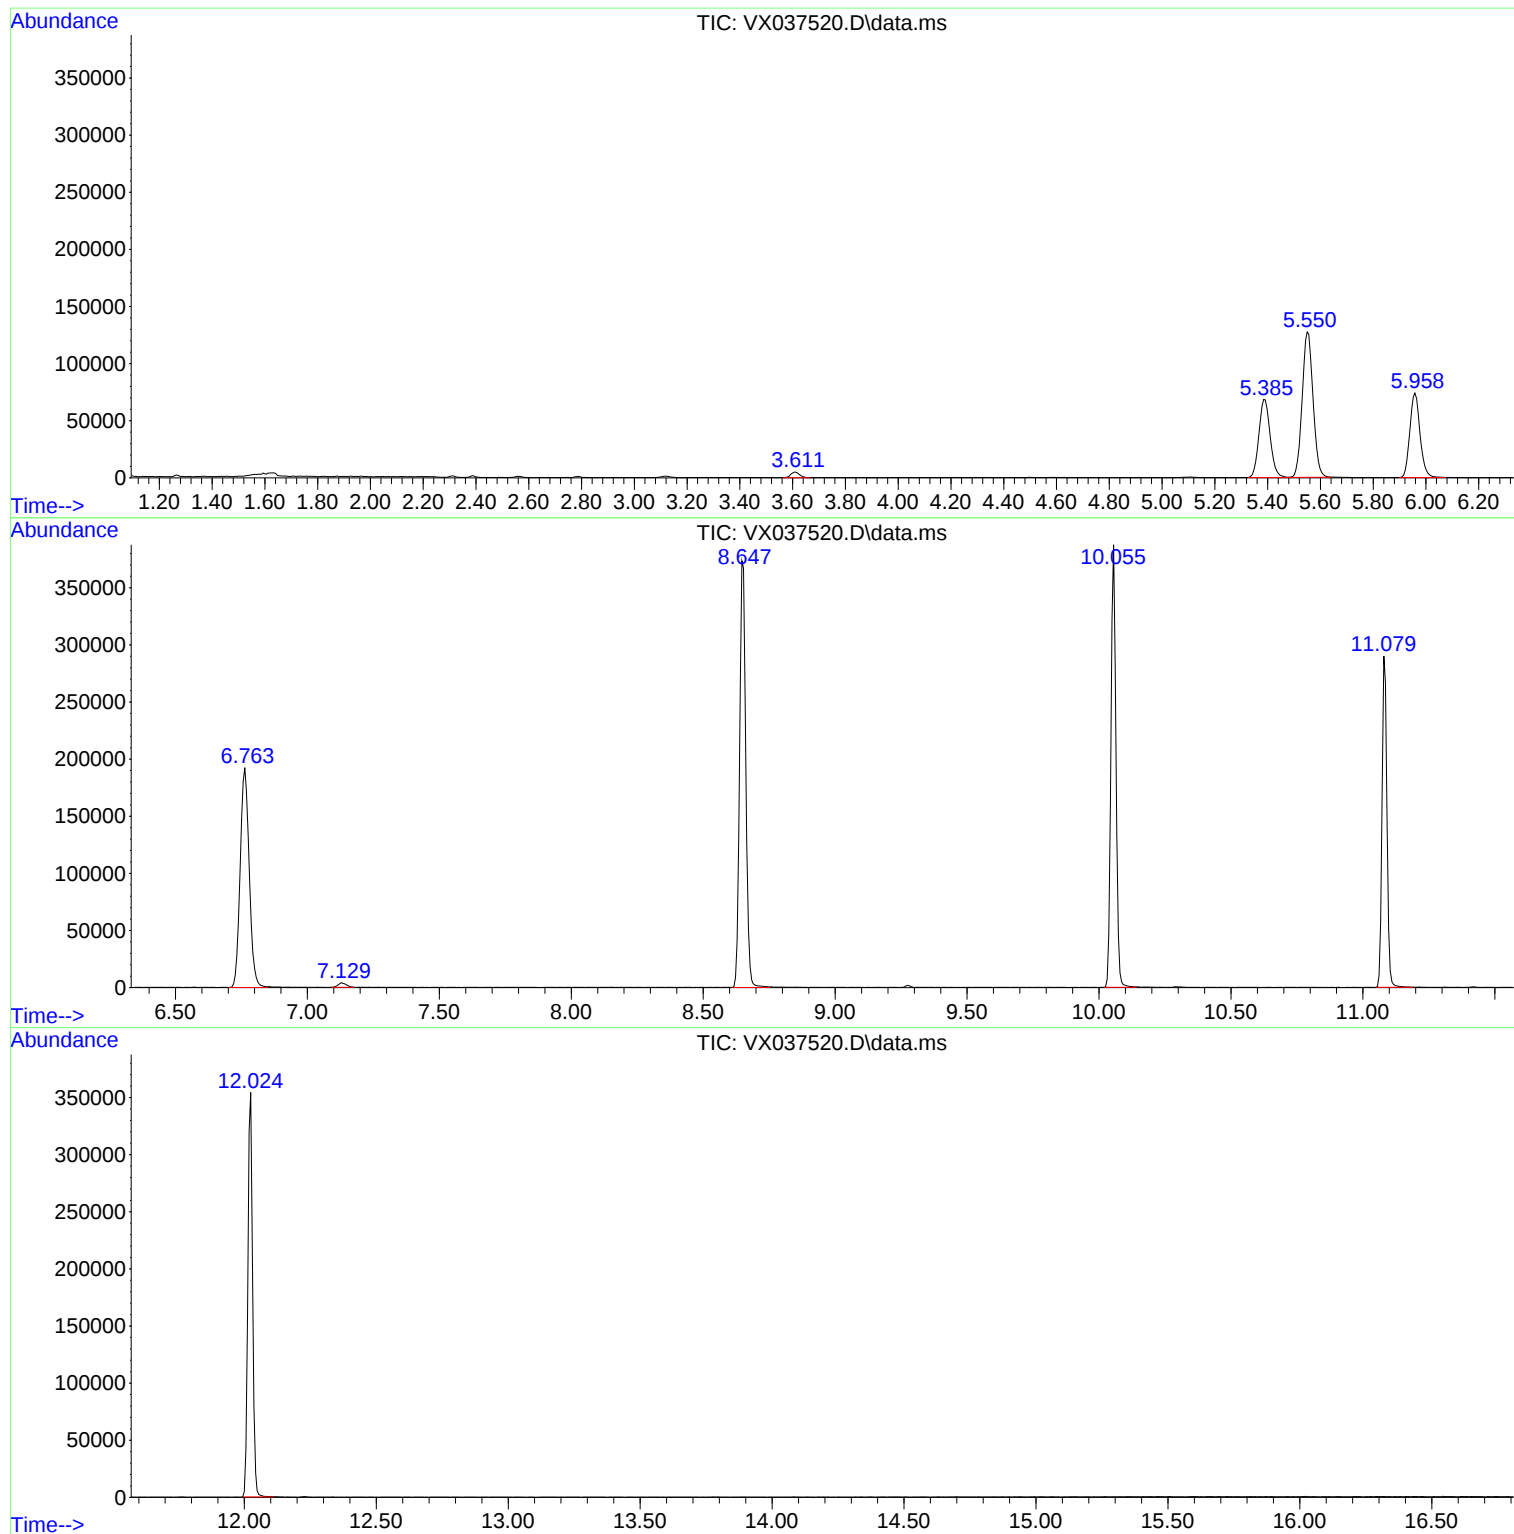

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090523\  
Data File : VX037520.D  
Acq On : 05 Sep 2023 18:25  
Operator : JC/MD  
Sample : 04254-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TT161S1-20230829

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090523\  
Data File : VX037520.D  
Acq On : 05 Sep 2023 18:25  
Operator : JC/MD  
Sample : 04254-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TT161S1-20230829

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|