

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
Data File : VX037521.D
Acq On : 05 Sep 2023 18:50
Operator : JC/MD
Sample : 04254-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP11-20230830

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M

Title : SW846 8260

Signal : TIC: VX037521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.556	235	241	252	rBV	10092	18030	2.91%	0.547%
2	2.940	295	304	314	rBV	4225	9811	1.58%	0.298%
3	4.586	564	574	591	rBV	8892	31384	5.06%	0.953%
4	5.385	695	705	720	rBV	70524	205690	33.15%	6.243%
5	5.550	720	732	752	rVB2	131082	371562	59.89%	11.277%
6	5.958	787	799	819	rBV	75751	203177	32.75%	6.166%
7	6.763	921	931	946	rBV	194117	457551	73.75%	13.887%
8	8.647	1234	1240	1250	rBV	383929	620421	100.00%	18.830%
9	10.055	1465	1471	1487	rBV	395330	529633	85.37%	16.075%
10	11.085	1634	1640	1652	rBV	294858	388932	62.69%	11.804%
11	12.024	1789	1794	1807	rBV	367220	458666	73.93%	13.921%




Sum of corrected areas: 3294857

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
Data File : VX037521.D
Acq On : 05 Sep 2023 18:50
Operator : JC/MD
Sample : 04254-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP11-20230830

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

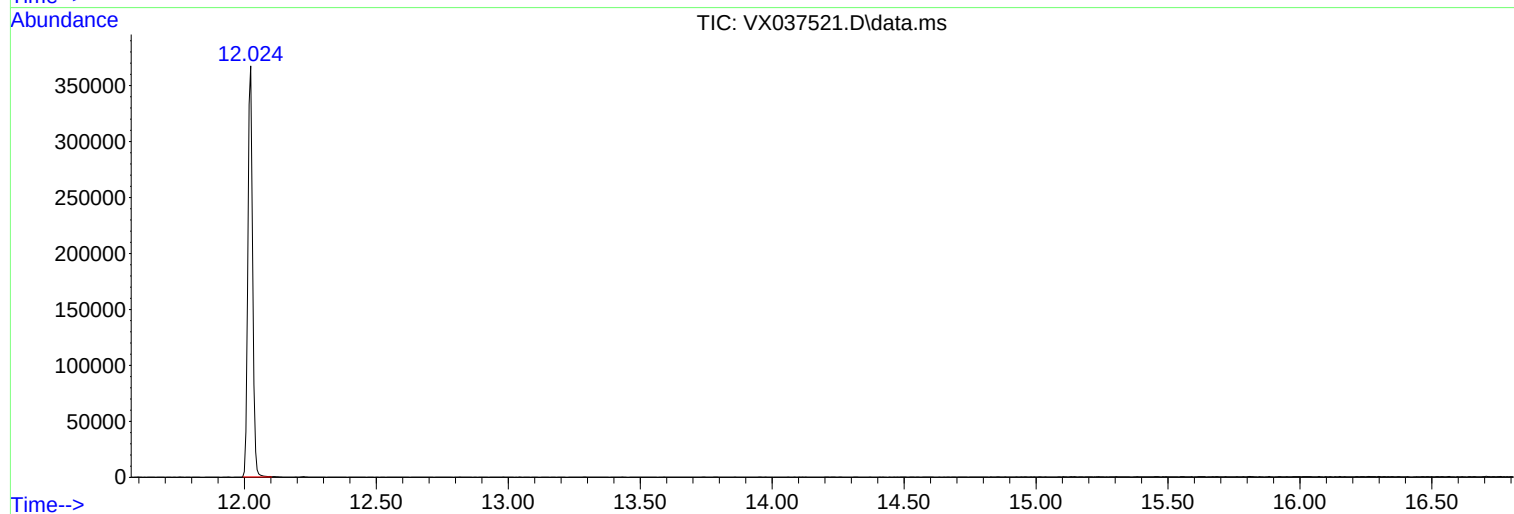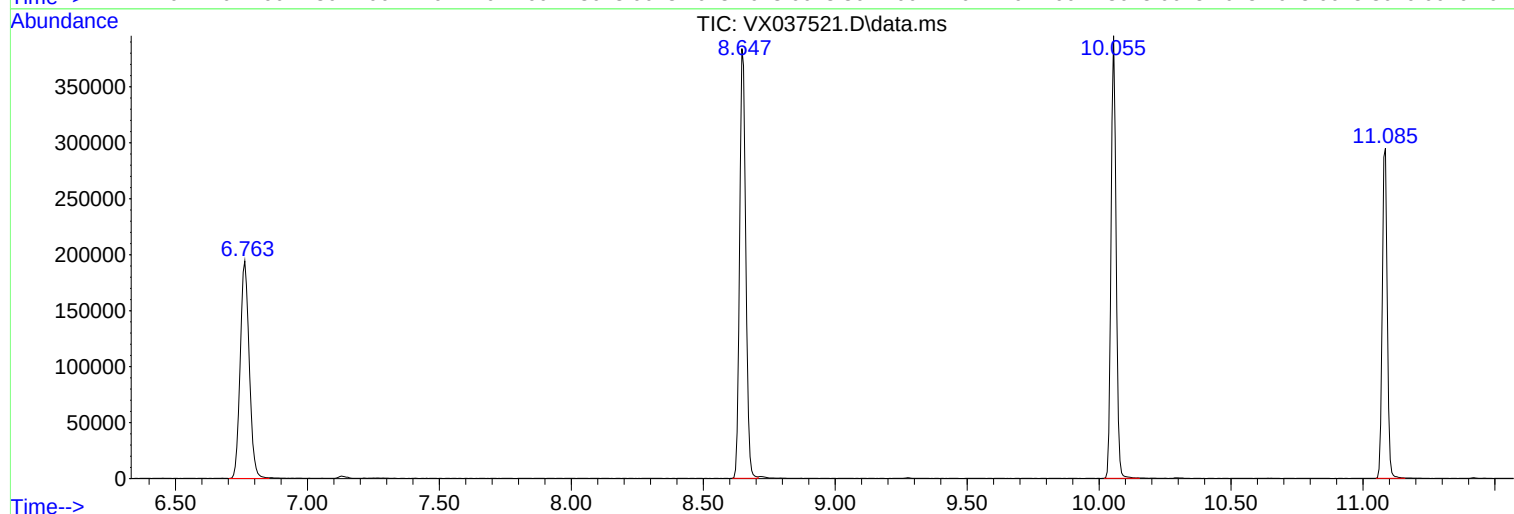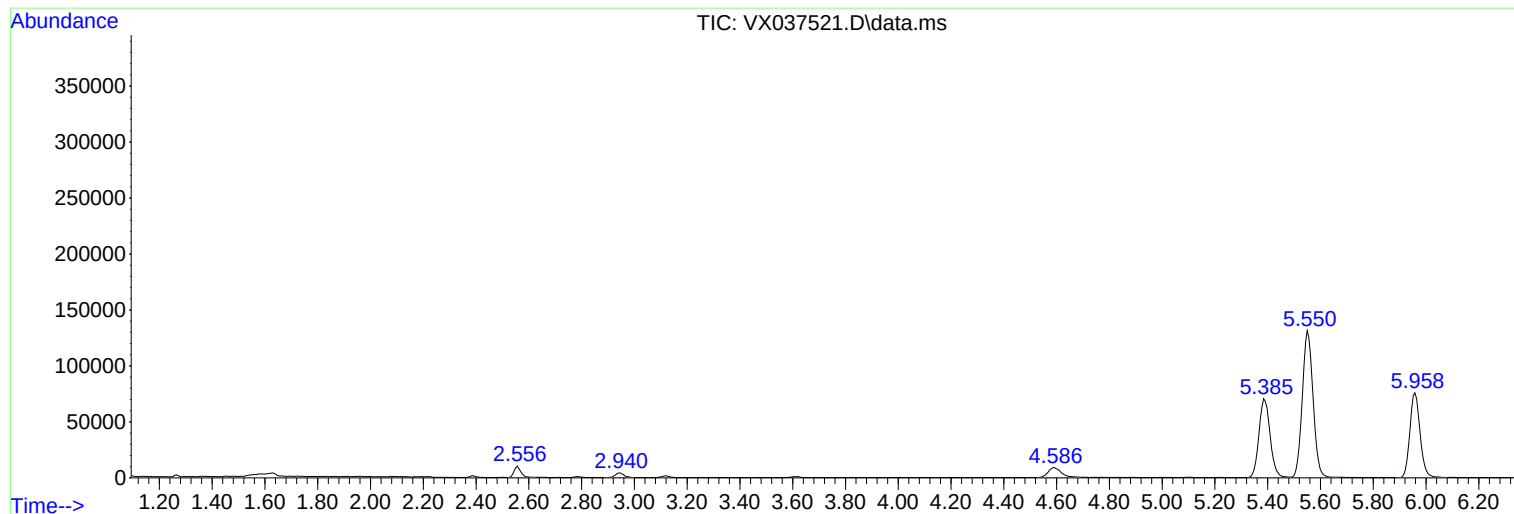

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
Data File : VX037521.D
Acq On : 05 Sep 2023 18:50
Operator : JC/MD
Sample : 04254-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP11-20230830

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
Data File : VX037521.D
Acq On : 05 Sep 2023 18:50
Operator : JC/MD
Sample : 04254-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP11-20230830

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------