

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
 Data File : VX037539.D
 Acq On : 06 Sep 2023 07:59
 Operator : JC/MD
 Sample : 04285-02 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 831

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Title : SW846 8260

Signal : TIC: VX037539.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	72	rBV	166932	207328	1.70%	0.261%
2	2.063	153	160	167	rBV	101016	173020	1.42%	0.218%
3	2.130	167	171	183	rVB	283133	418402	3.44%	0.527%
4	2.380	206	212	230	rBV	191498	336691	2.77%	0.424%
5	2.538	230	238	253	rBV	159025	295035	2.42%	0.372%
6	2.965	298	308	325	rBV	479395	1000753	8.22%	1.260%
7	3.325	359	367	387	rVB	58668	137452	1.13%	0.173%
8	3.696	415	428	449	rBV	4265859	11754935	96.58%	14.804%
9	4.239	501	517	531	rBV	2998165	8389031	68.93%	10.565%
10	4.556	561	569	585	rVB	65370	189340	1.56%	0.238%
11	5.385	696	705	719	rVV	77993	230910	1.90%	0.291%
12	5.550	721	732	746	rVV	142630	401981	3.30%	0.506%
13	5.958	789	799	806	rBV	80426	215215	1.77%	0.271%
14	6.123	806	826	839	rVV	931379	2827304	23.23%	3.561%
15	6.336	853	861	875	rVB5	44955	132138	1.09%	0.166%
16	6.763	921	931	949	rVB	211195	505926	4.16%	0.637%
17	7.257	984	1012	1036	rBV	3916659	12171164	100.00%	15.328%
18	7.580	1059	1065	1072	rBV	265799	487665	4.01%	0.614%
19	7.952	1121	1126	1138	rVB	213627	353347	2.90%	0.445%
20	8.336	1182	1189	1197	rBV	98814	166077	1.36%	0.209%
21	8.647	1234	1240	1246	rVV	430459	673147	5.53%	0.848%
22	8.720	1246	1252	1256	rVV	645971	989913	8.13%	1.247%
23	8.769	1256	1260	1270	rVV	699039	1053305	8.65%	1.326%
24	8.860	1270	1275	1288	rVB2	88288	154291	1.27%	0.194%
25	9.238	1331	1337	1346	rBV	1511557	2033946	16.71%	2.561%
26	9.488	1372	1378	1389	rVB	1177369	1703080	13.99%	2.145%
27	10.073	1464	1474	1483	rVB3	694708	1564030	12.85%	1.970%
28	10.153	1483	1487	1490	rBV	155952	205881	1.69%	0.259%
29	10.195	1490	1494	1499	rVB	403465	521480	4.28%	0.657%
30	10.299	1504	1511	1519	rVB	2479661	3288114	27.02%	4.141%
31	10.506	1540	1545	1551	rVB	372263	459568	3.78%	0.579%
32	10.640	1562	1567	1572	rBV	1444647	1870996	15.37%	2.356%
33	10.756	1578	1586	1595	rBV	333827	587939	4.83%	0.740%
34	10.951	1613	1618	1624	rBV3	135501	224233	1.84%	0.282%
35	11.079	1633	1639	1643	rBV2	564699	831302	6.83%	1.047%
36	11.134	1643	1648	1653	rVB	1043456	1288296	10.58%	1.622%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
Data File : VX037539.D
Acq On : 06 Sep 2023 07:59
Operator : JC/MD
Sample : 04285-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
831

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Title : SW846 8260

37	11.238	1660	1665	1668	rBV	148079	177372	1.46%	0.223%
38	11.280	1668	1672	1681	rVB2	570637	777363	6.39%	0.979%
39	11.378	1681	1688	1692	rBV	386500	637251	5.24%	0.803%
40	11.421	1692	1695	1698	rVV	829552	1037833	8.53%	1.307%
41	11.451	1698	1700	1712	rVB2	407973	522571	4.29%	0.658%
42	11.573	1712	1720	1723	rBV	112560	165684	1.36%	0.209%
43	11.610	1723	1726	1731	rVV2	280043	363418	2.99%	0.458%
44	11.683	1734	1738	1745	rVV	6942913	8358765	68.68%	10.527%
45	11.750	1745	1749	1753	rVV	881361	1069175	8.78%	1.346%
46	11.793	1753	1756	1761	rVV	265408	303524	2.49%	0.382%
47	11.902	1771	1774	1779	rVV2	117409	158795	1.30%	0.200%
48	11.988	1779	1788	1792	rVV	2271131	2834456	23.29%	3.570%
49	12.024	1792	1794	1798	rVV	511487	556454	4.57%	0.701%
50	12.085	1801	1804	1809	rVB	261926	313731	2.58%	0.395%
51	12.219	1821	1826	1836	rBV	1619699	2136968	17.56%	2.691%
52	12.305	1836	1840	1852	rVB4	314482	525789	4.32%	0.662%
53	12.408	1852	1857	1862	rBV	119920	154099	1.27%	0.194%
54	12.597	1884	1888	1894	rVB2	121906	213168	1.75%	0.268%
55	12.786	1914	1919	1925	rBV3	132349	209664	1.72%	0.264%
56	12.847	1925	1929	1932	rVV	124843	155065	1.27%	0.195%
57	12.908	1935	1939	1945	rVV2	92621	196089	1.61%	0.247%
58	12.994	1950	1953	1957	rVB	113420	137856	1.13%	0.174%
59	13.286	1997	2001	2007	rVB2	89522	128720	1.06%	0.162%
60	13.609	2045	2054	2062	rBV2	184007	293006	2.41%	0.369%
61	13.774	2073	2081	2087	rBV2	67300	135017	1.11%	0.170%




Sum of corrected areas: 79405068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
Data File : VX037539.D
Acq On : 06 Sep 2023 07:59
Operator : JC/MD
Sample : 04285-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
831

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

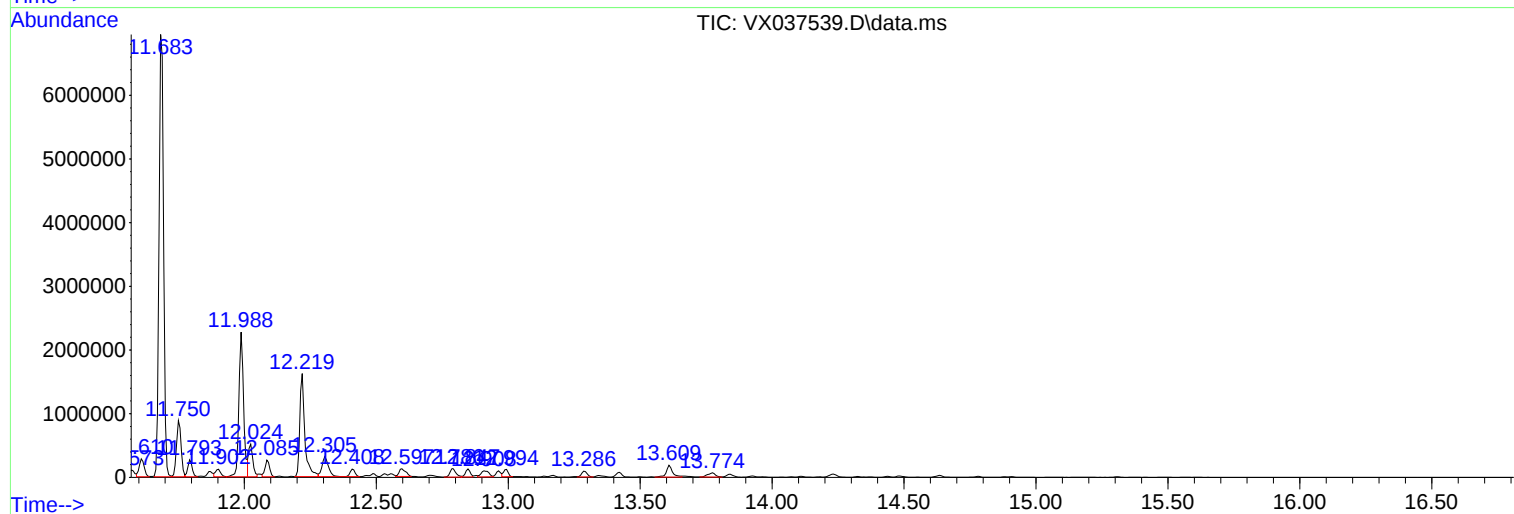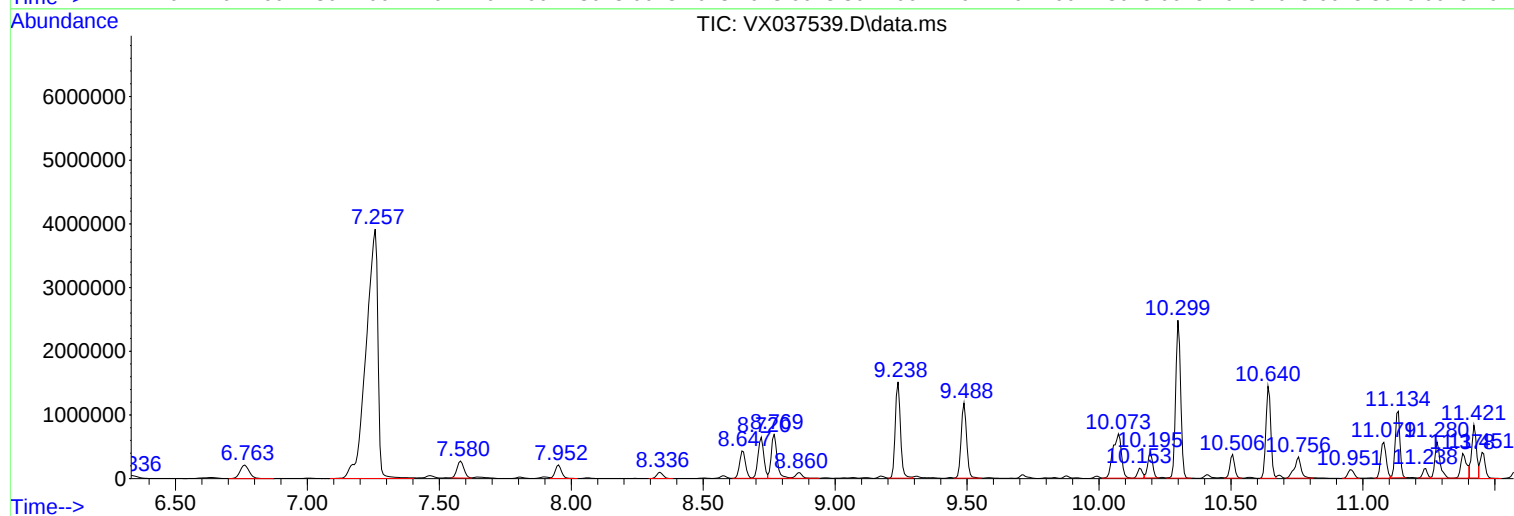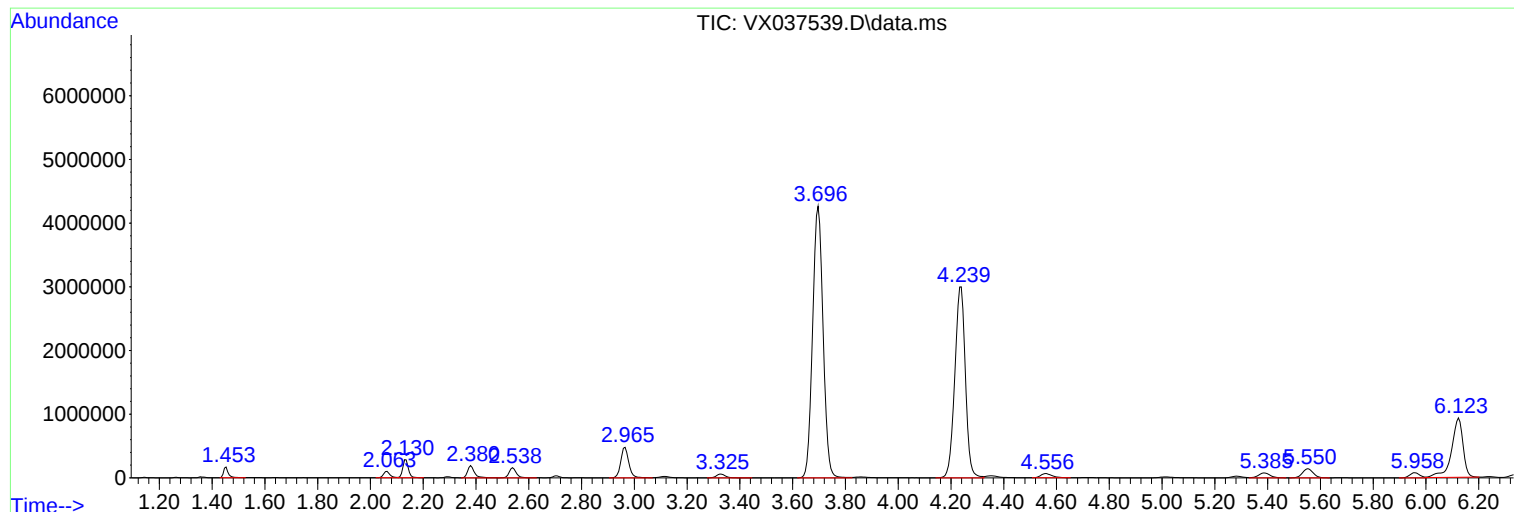

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
Data File : VX037539.D
Acq On : 06 Sep 2023 07:59
Operator : JC/MD
Sample : 04285-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
831

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
Data File : VX037539.D
Acq On : 06 Sep 2023 07:59
Operator : JC/MD
Sample : 04285-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
831

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------