


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090523\
Data File : VX037527.D
Acq On : 06 Sep 2023 02:12
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Title : SW846 8260
Last Update : Fri Aug 18 09:30:38 2023

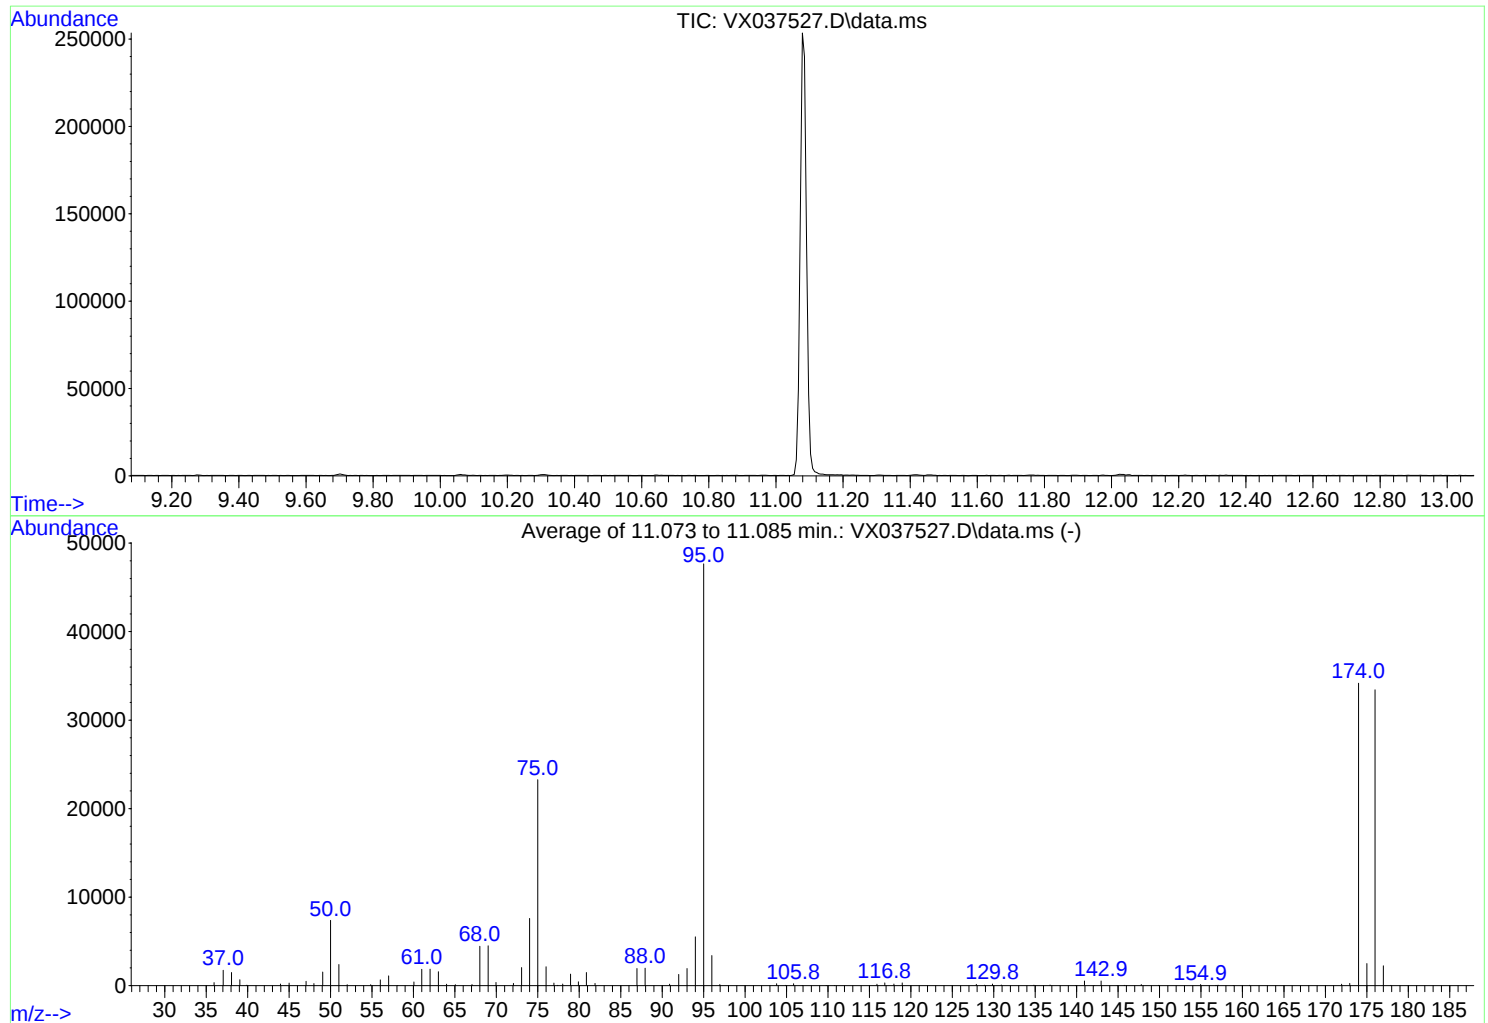

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.5	7368	PASS
75	95	30	60	48.8	23264	PASS
95	95	100	100	100.0	47659	PASS
96	95	5	9	7.1	3401	PASS
173	174	0.00	2	0.8	262	PASS
174	95	50	100	71.7	34173	PASS
175	174	5	9	7.3	2491	PASS
176	174	95	101	97.8	33437	PASS
177	176	5	9	6.7	2235	PASS