


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090618\
Data File : VX004378.D
Acq On : 06 Sep 2018 10:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Title : SW846 8260
Last Update : Thu Aug 23 05:39:44 2018

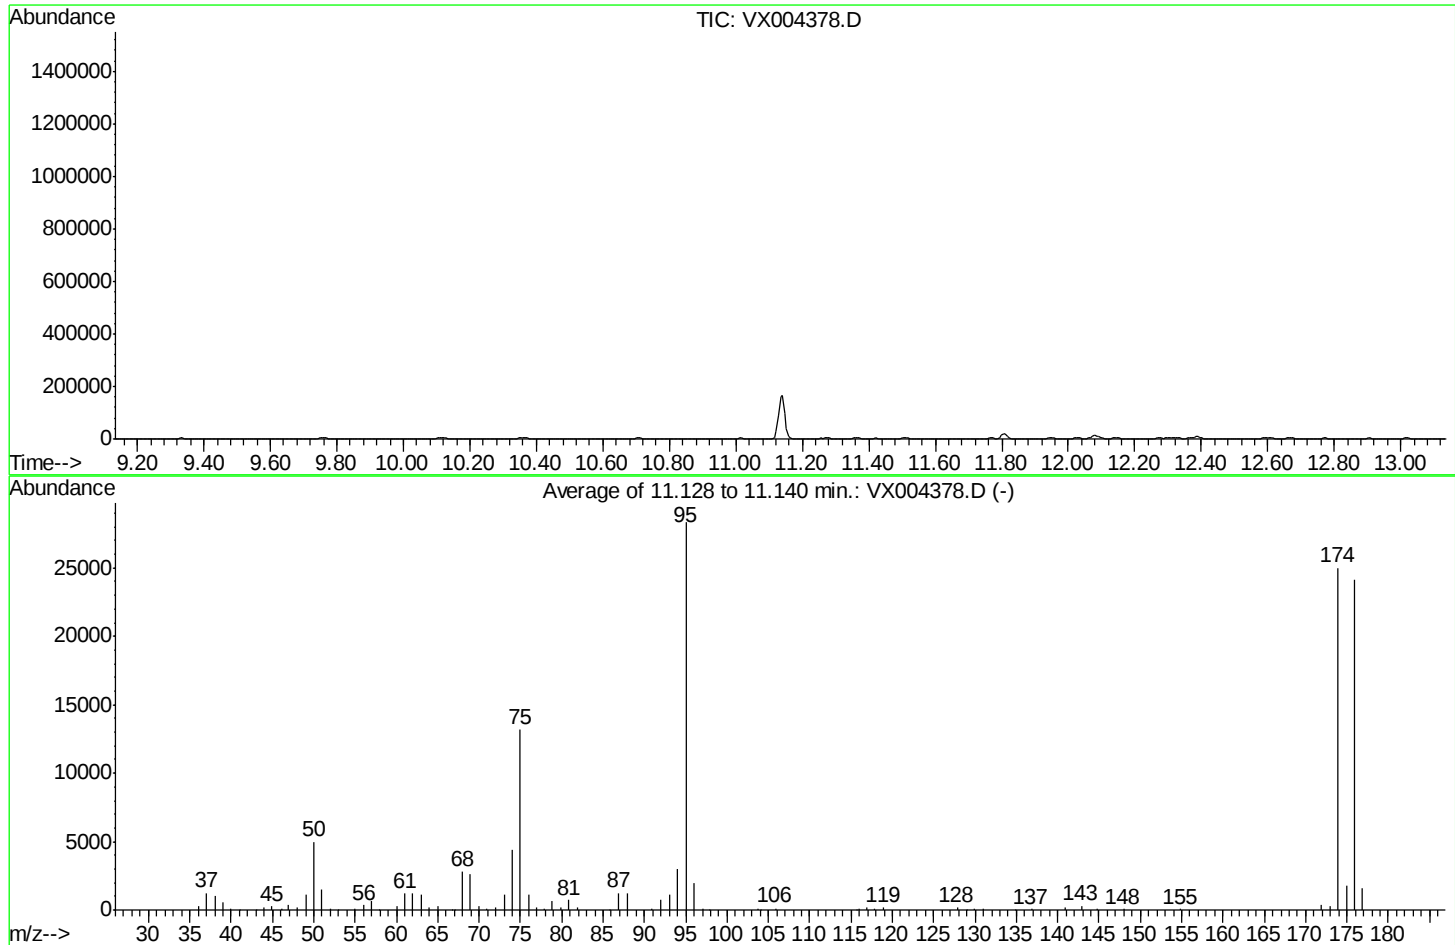

AutoFind: Scans 1729, 1730, 1731; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	4961	PASS
75	95	30	60	46.5	13166	PASS
95	95	100	100	100.0	28333	PASS
96	95	5	9	6.9	1961	PASS
173	174	0.00	2	1.1	282	PASS
174	95	50	100	88.2	24993	PASS
175	174	5	9	7.0	1753	PASS
176	174	95	101	96.4	24097	PASS
177	176	5	9	6.6	1591	PASS