


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090619\  
 Data File : VX012142.D  
 Acq On : 06 Sep 2019 12:18  
 Operator : SY/SP  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA X/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X090319S.M  
 Title : SW846 8260  
 Last Update : Tue Sep 03 15:26:48 2019

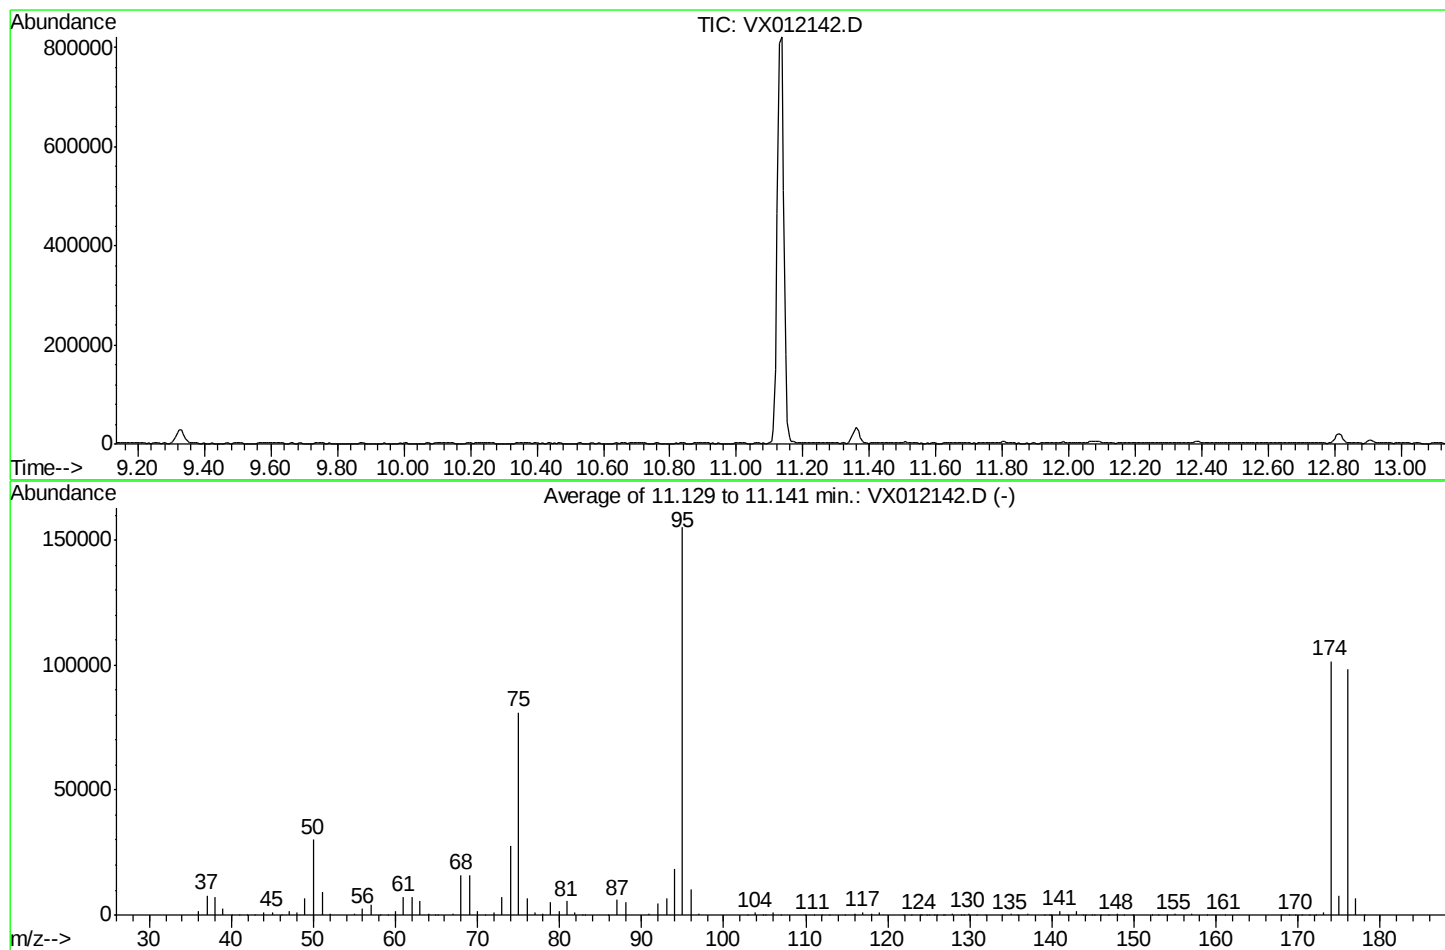

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1672

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.4      | 30109   | PASS             |
| 75          | 95           | 30           | 60           | 52.3      | 81133   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 155165  | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 10224   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.9       | 964     | PASS             |
| 174         | 95           | 50           | 100          | 65.4      | 101549  | PASS             |
| 175         | 174          | 5            | 9            | 7.7       | 7827    | PASS             |
| 176         | 174          | 95           | 101          | 96.9      | 98400   | PASS             |
| 177         | 176          | 5            | 9            | 6.7       | 6545    | PASS             |