

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090622\
 Data File : VX031144.D
 Acq On : 06 Sep 2022 21:30
 Operator : JC/MD
 Sample : N4479-07RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-14

Quant Time: Sep 07 01:15:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 02 02:49:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	225134	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	337322	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	298927	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	140419	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	129586	44.734	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	89.460%		
35) Dibromofluoromethane	5.391	113	121027	49.165	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	98.320%		
50) Toluene-d8	8.653	98	433289	47.825	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	95.660%		
62) 4-Bromofluorobenzene	11.079	95	155964	48.740	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.480%		
Target Compounds						Qvalue
3) Chloromethane	1.288	50	272	0.822	ug/l #	42
6) Chloroethane	1.685	64	129	1.810	ug/l #	41
10) Methyl Iodide	2.465	142	152	2.963	ug/l #	45
11) Tert butyl alcohol	2.947	59	6993	Below Cal	#	79
13) Acrolein	2.252	56	542	1.022	ug/l	88
16) Acetone	2.386	43	26680	23.858	ug/l	92
18) Methyl Acetate	2.709	43	2128	0.662	ug/l	99
20) Methylene Chloride	2.788	84	14312	3.209	ug/l #	80
25) 2-Butanone	4.574	43	8859	5.131	ug/l #	87
29) Tetrahydrofuran	5.032	42	1279	1.149	ug/l #	75
31) Cyclohexane	5.550	56	3433	0.868	ug/l #	1
36) 1,1-Dichloropropene	5.562	75	14097	4.088	ug/l #	45
37) Ethyl Acetate	4.715	43	24253	8.095	ug/l #	91
38) Carbon Tetrachloride	5.544	117	21152	5.910	ug/l #	18
40) Benzene	6.037	78	5981	0.604	ug/l	99
41) Methacrylonitrile	5.032	41	656	0.411	ug/l #	45
43) Isopropyl Acetate	6.342	43	107746	23.012	ug/l #	92
48) Methyl methacrylate	7.592	41	2837	1.200	ug/l #	13
49) 1,4-Dioxane	7.690	88	23	0.320	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	77904	25.882	ug/l #	50
52) Toluene	8.720	92	6595	1.027	ug/l	97
54) cis-1,3-Dichloropropene	8.549	75	45069	11.473	ug/l #	58
57) 1,3-Dichloropropane	9.482	76	5617	1.302	ug/l #	42
59) 2-Hexanone	9.378	43	85969	37.769	ug/l #	24
68) m/p-Xylenes	10.299	106	3261	0.680	ug/l	89
69) o-Xylene	10.640	106	2035	0.433	ug/l	96
70) Styrene	10.659	104	3430	0.451	ug/l	95
74) N-amyl acetate	10.768	43	1282	0.375	ug/l #	51
76) 1,2,3-Trichloropropane	11.079	75	69654	20.984	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	69654	65.947	ug/l #	13
84) 1,2,4-Trimethylbenzene	11.756	105	7793	0.823	ug/l #	49
85) sec-Butylbenzene	11.756	105	7793	0.628	ug/l #	56
95) Naphthalene	13.774	128	71746	5.637	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
SB-14

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090622\
Data File : VX031144.D
Acq On : 06 Sep 2022 21:30
Operator : JC/MD
Sample : N4479-07RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-14

Quant Time: Sep 07 01:15:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 02 02:49:21 2022
Response via : Initial Calibration




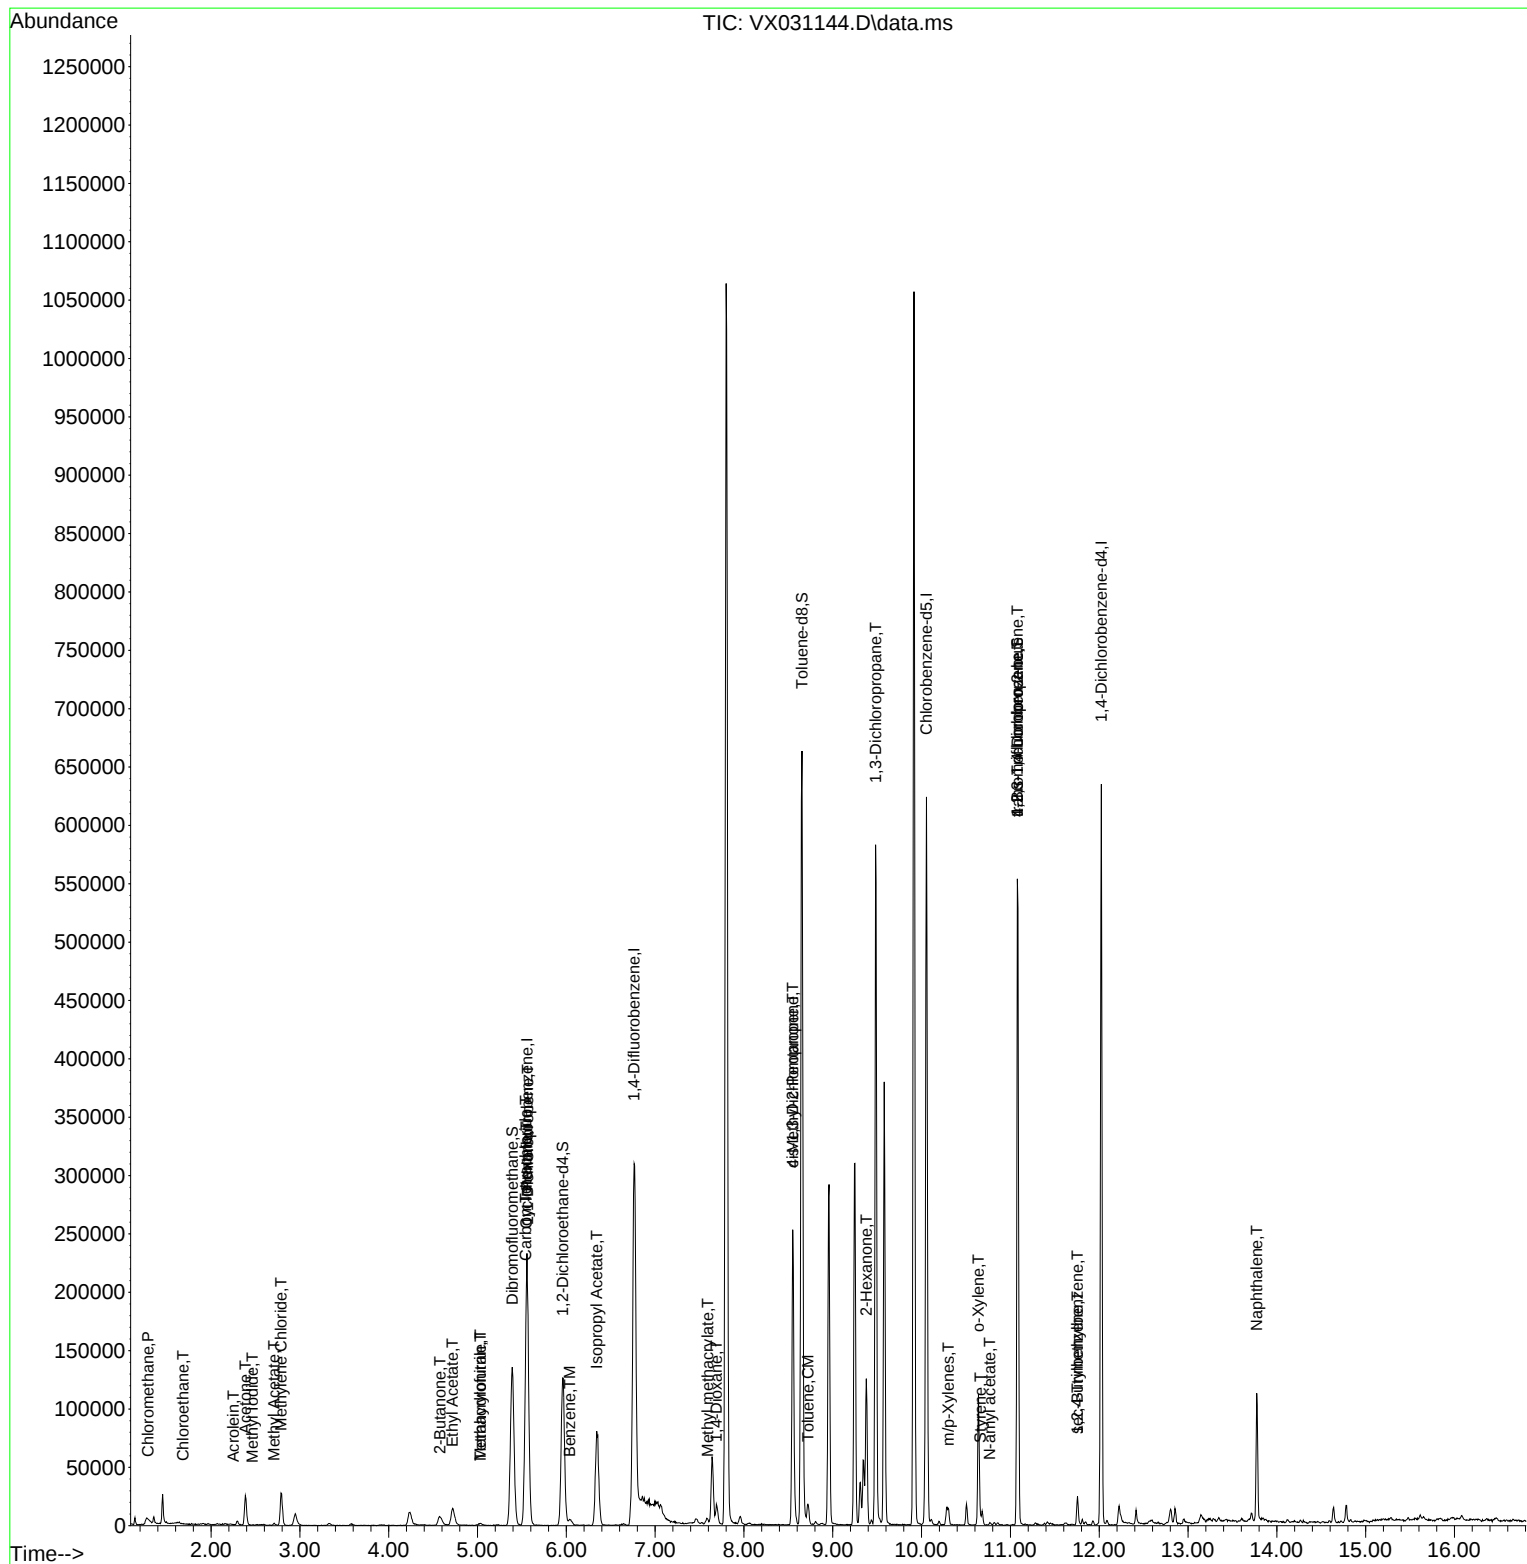




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion:168 Resp: 225134
Ion Ratio Lower Upper
168 100
99 45.0 44.0 66.0

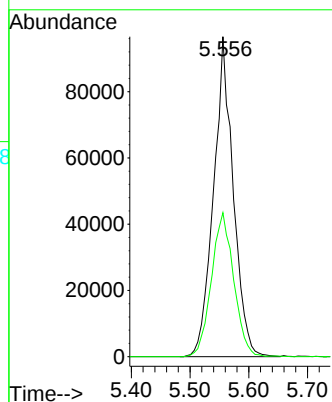

#3
Chloromethane
Concen: 0.822 ug/l
RT: 1.288 min Scan# 33
Delta R.T. 0.000 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion: 50 Resp: 272
Ion Ratio Lower Upper
50 100
52 0.0 26.3 39.5#


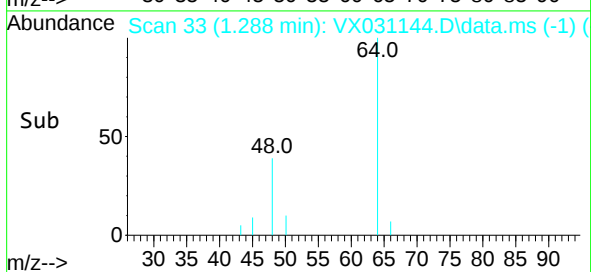
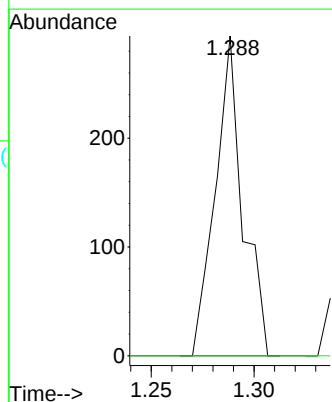



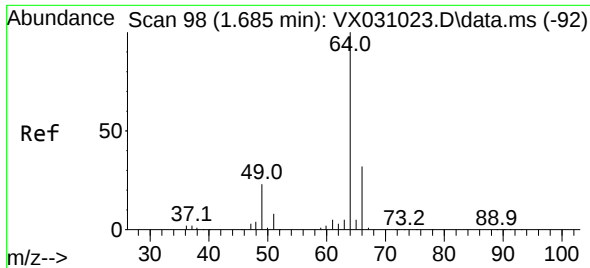

#6
Chloroethane
Concen: 1.810 ug/l
RT: 1.685 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion: 64 Resp: 129
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#

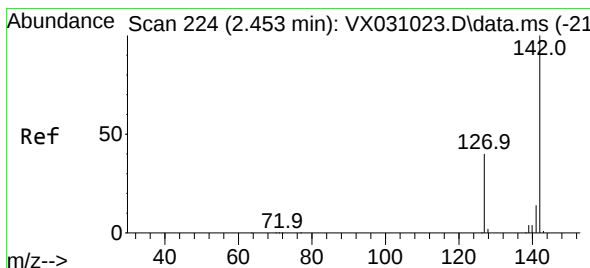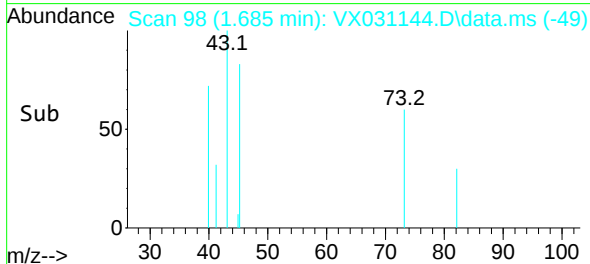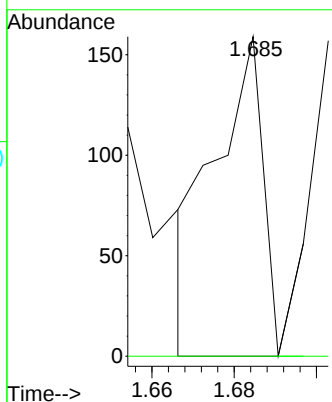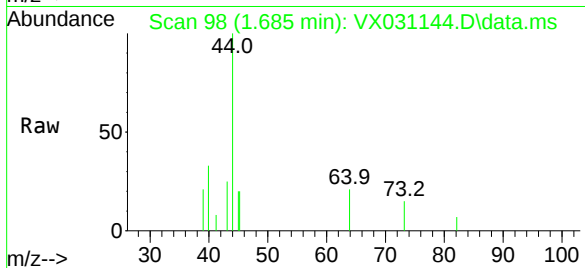

#10
Methyl Iodide
Concen: 2.963 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion: 142 Resp: 152
Ion Ratio Lower Upper
142 100
127 0.0 30.2 45.2#
141 0.0 11.3 16.9#


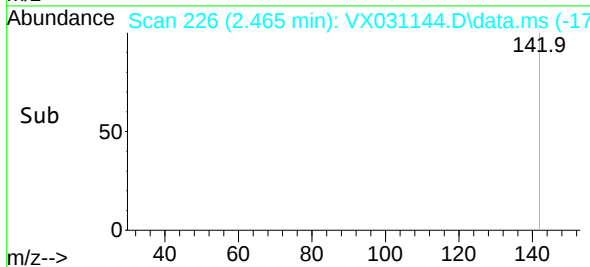

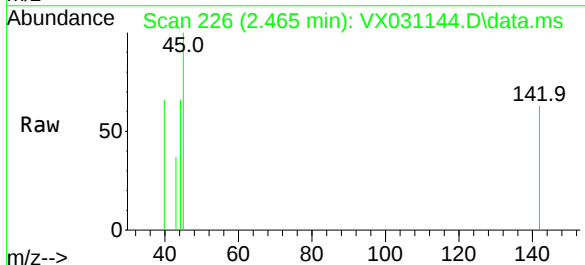




#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.947 min Scan# 30
Delta R.T. -0.042 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion: 59 Resp: 6993
Ion Ratio Lower Upper
59 100
57 1.7 7.4 11.2#

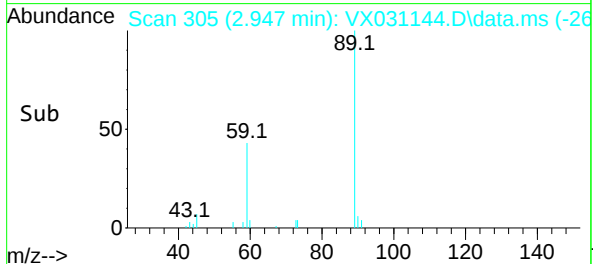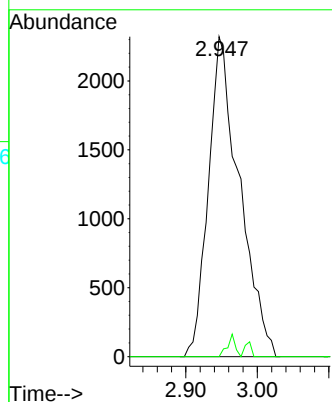

#13
Acrolein
Concen: 1.022 ug/l
RT: 2.252 min Scan# 191
Delta R.T. 0.013 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion: 56 Resp: 542
Ion Ratio Lower Upper
56 100
55 80.4 56.6 84.8




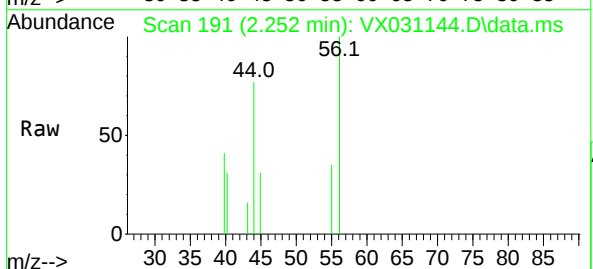




#16
Acetone
Concen: 23.858 ug/l
RT: 2.386 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion: 43 Resp: 26680
Ion Ratio Lower Upper
43 100
58 29.7 27.7 41.5

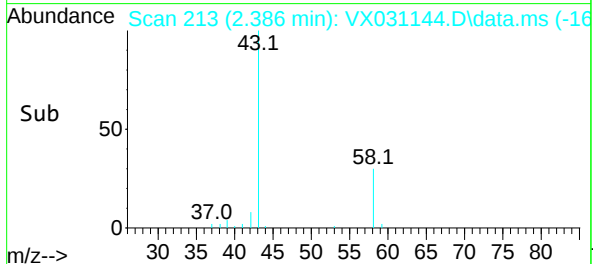

#18
Methyl Acetate
Concen: 0.662 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion: 43 Resp: 2128
Ion Ratio Lower Upper
43 100
74 23.7 19.4 29.2

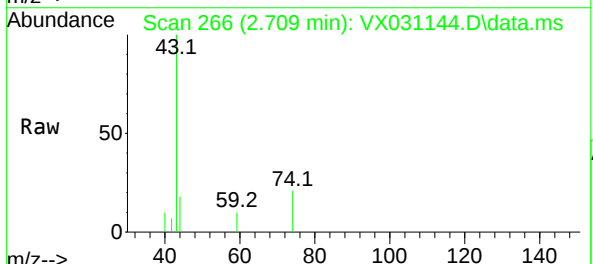



#20

Methylene Chloride

Concen: 3.209 ug/l

RT: 2.788 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30

Instrument :

MSVOA_X

ClientSampleId :

SB-14

Tgt Ion: 84 Resp: 14312





Ion Ratio Lower Upper

84 100

49 83.6 93.8 140.6#

51 26.2 29.4 44.0#

86 65.8 51.0 76.4

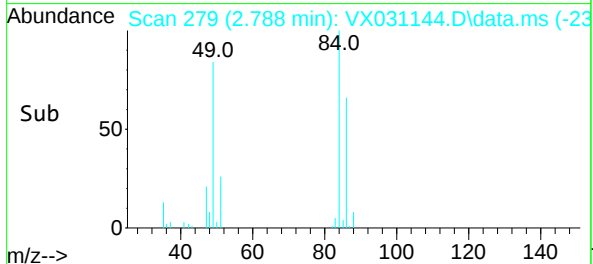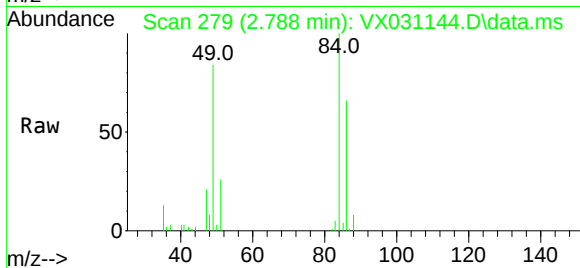

#25

2-Butanone

Concen: 5.131 ug/l

RT: 4.574 min Scan# 572

Delta R.T. 0.006 min

Lab File: VX031144.D




Acq: 06 Sep 2022 21:30


Tgt Ion: 43 Resp: 8859

Ion Ratio Lower Upper

43 100

72 33.6 21.7 32.5#

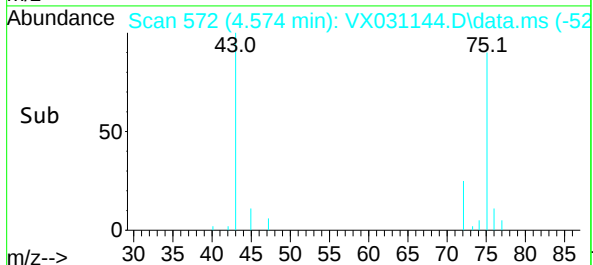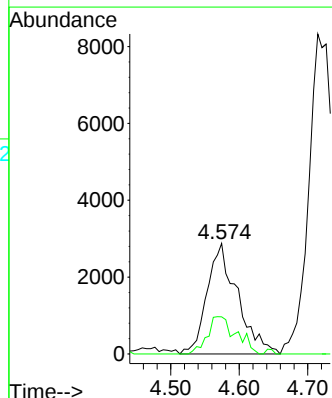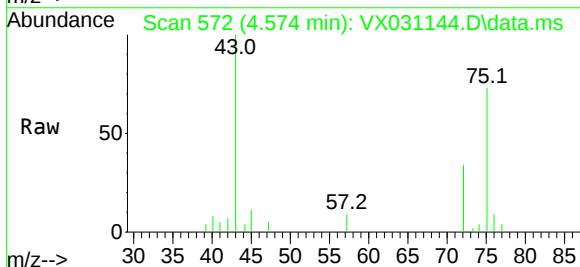



#29

Tetrahydrofuran

Concen: 1.149 ug/l

RT: 5.032 min Scan# 644

Delta R.T. 0.019 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30

Instrument :

MSVOA_X

ClientSampleId :

SB-14





Tgt Ion: 42 Resp: 1279

Ion Ratio Lower Upper

42 100

72 25.6 36.5 54.7#

71 54.7 33.9 50.9#



#31

Cyclohexane

Concen: 0.868 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.073 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30




Tgt Ion: 56 Resp: 3433


Ion Ratio Lower Upper

56 100

69 156.1 25.4 38.0#

84 178.2 68.9 103.3#

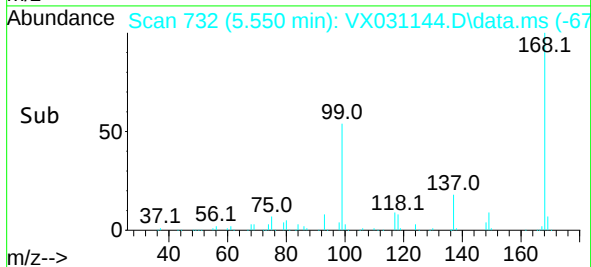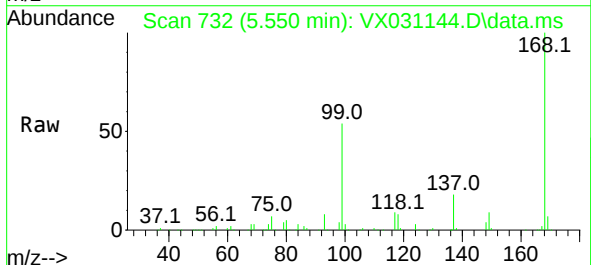



#33

1,2-Dichloroethane-d4

Concen: 44.734 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30

Instrument :

MSVOA_X

ClientSampleId :





SB-14

Tgt Ion: 65 Resp: 129586

Ion Ratio Lower Upper

65 100

67 51.7 0.0 109.6

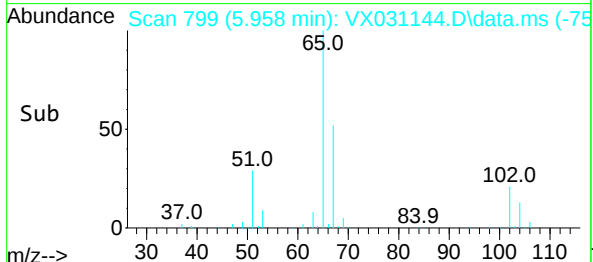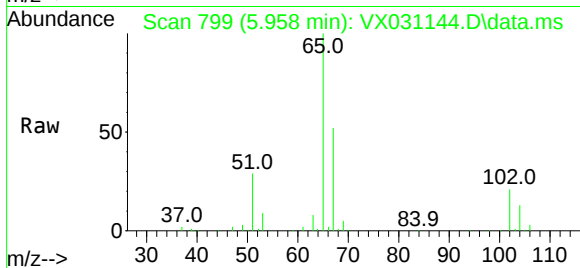

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30




Tgt Ion: 114 Resp: 337322


Ion Ratio Lower Upper

114 100

63 16.6 0.0 38.4

88 15.2 0.0 31.8


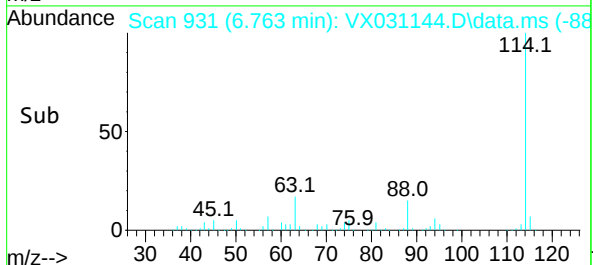

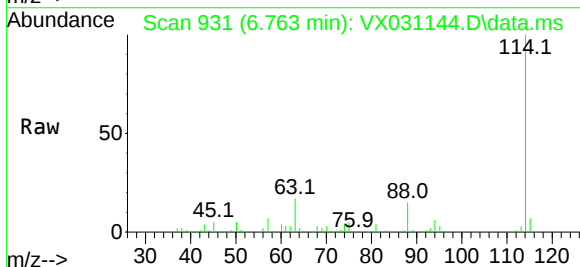




#35
Dibromofluoromethane
Concen: 49.165 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion:113 Resp: 121027
Ion Ratio Lower Upper
113 100
111 103.1 83.2 124.8
192 20.0 14.8 22.2

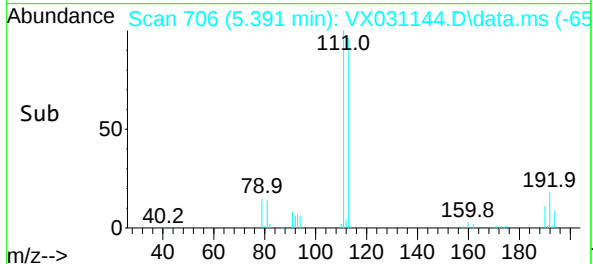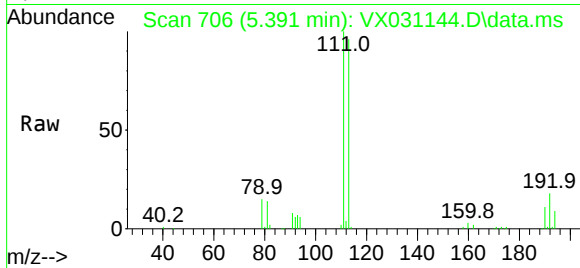

#36
1,1-Dichloropropene
Concen: 4.088 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.134 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion: 75 Resp: 14097
Ion Ratio Lower Upper
75 100
110 5.6 19.3 57.9#
77 0.0 24.4 36.6#

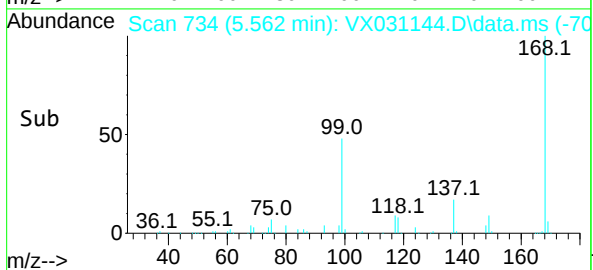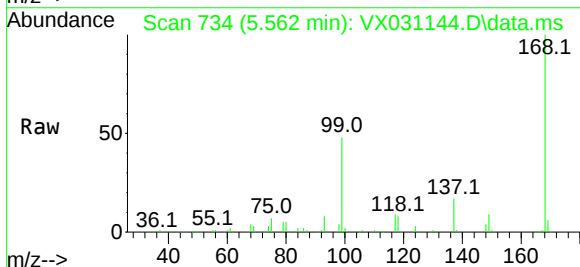



#37

Ethyl Acetate

Concen: 8.095 ug/l

RT: 4.715 min Scan# 51

Delta R.T. -0.006 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30

Instrument :

MSVOA_X

ClientSampleId :

SB-14





Tgt Ion: 43 Resp: 24253

Ion Ratio Lower Upper

43 100

61 18.3 11.7 17.5#

70 15.1 9.3 13.9#

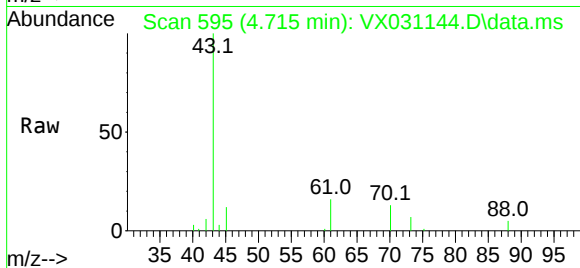

#38

Carbon Tetrachloride

Concen: 5.910 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.140 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30




Tgt Ion: 117 Resp: 21152


Ion Ratio Lower Upper

117 100

119 6.3 74.1 111.1#

121 0.0 25.8 38.8#


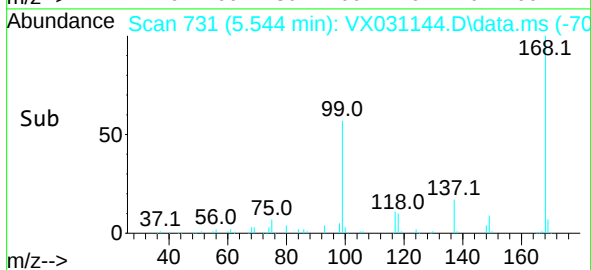

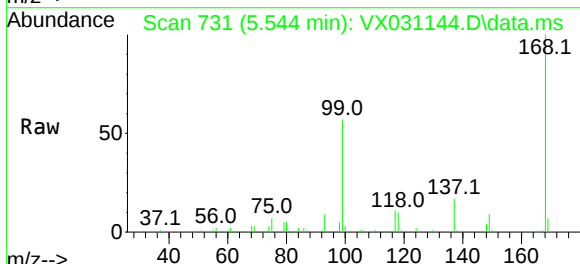




#40
Benzene
Concen: 0.604 ug/l
RT: 6.037 min Scan# 813
Delta R.T. -0.007 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion: 78 Resp: 5981
Ion Ratio Lower Upper
78 100
77 21.9 18.0 27.0

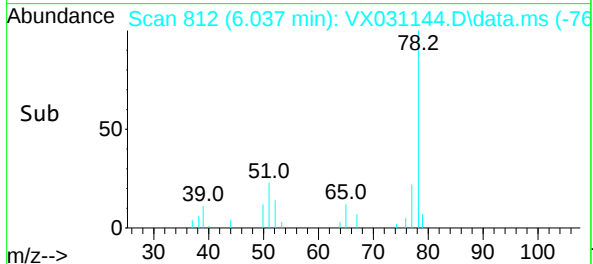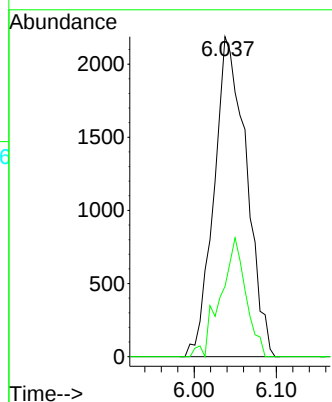

#41
Methacrylonitrile
Concen: 0.411 ug/l
RT: 5.032 min Scan# 647
Delta R.T. 0.104 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion: 41 Resp: 656
Ion Ratio Lower Upper
41 100
39 61.0 42.9 64.3
67 0.0 60.1 90.1#
52 0.0 22.6 34.0#


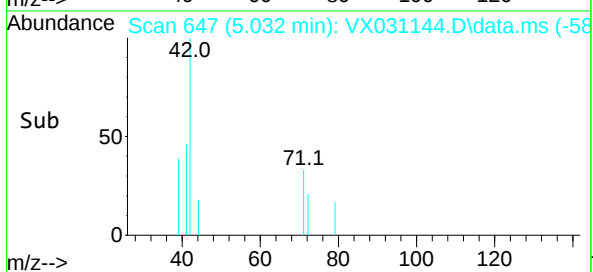






#43
Isopropyl Acetate
Concen: 23.012 ug/l
RT: 6.342 min Scan# 862
Delta R.T. -0.006 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion: 43 Resp: 107746
Ion Ratio Lower Upper
43 100
61 23.4 16.5 24.7
87 18.6 11.1 16.7#

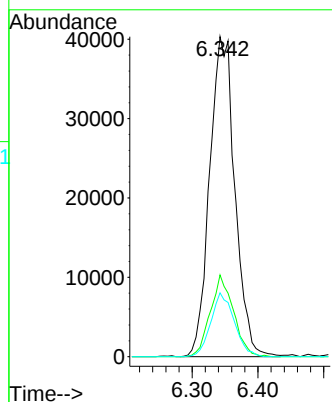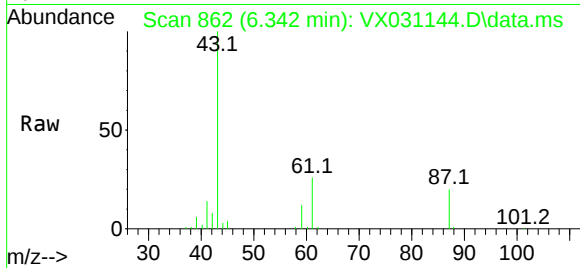

#48
Methyl methacrylate
Concen: 1.200 ug/l
RT: 7.592 min Scan# 1067
Delta R.T. -0.104 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion: 41 Resp: 2837
Ion Ratio Lower Upper
41 100
69 0.0 68.8 103.2#
39 0.0 44.6 66.8#

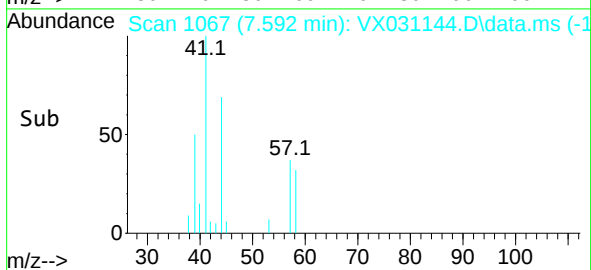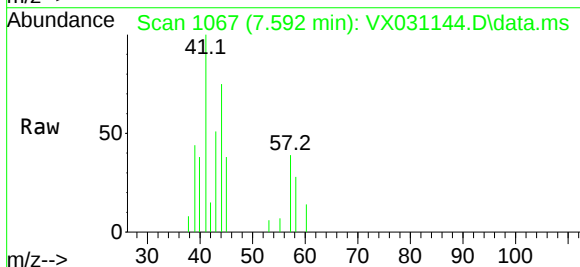



#49

1,4-Dioxane

Concen: 0.320 ug/l

RT: 7.690 min Scan# 1083

Delta R.T. 0.013 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30

Instrument :





MSVOA_X

ClientSampleId :

SB-14

Tgt Ion: 88 Resp: 23

Ion	Ratio	Lower	Upper
88	100		
43	0.0	23.8	35.8#
58	2326.1	53.8	80.6#

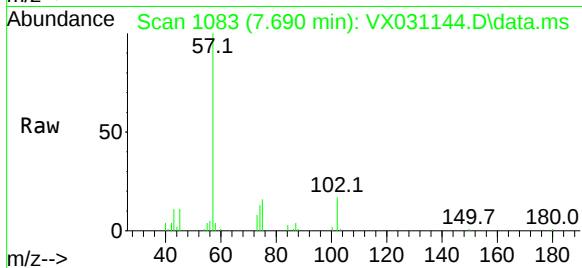

#50

Toluene-d8

Concen: 47.825 ug/l

RT: 8.653 min Scan# 1241




Delta R.T. -0.000 min


Lab File: VX031144.D

Acq: 06 Sep 2022 21:30

Tgt Ion: 98 Resp: 433289

Ion	Ratio	Lower	Upper
98	100		
100	64.1	52.3	78.5

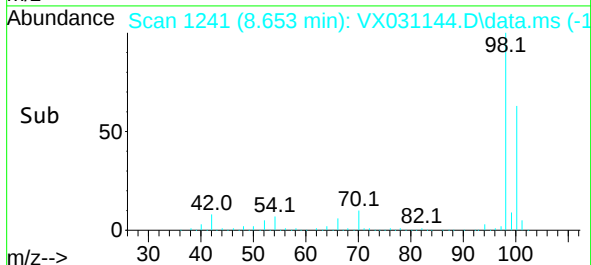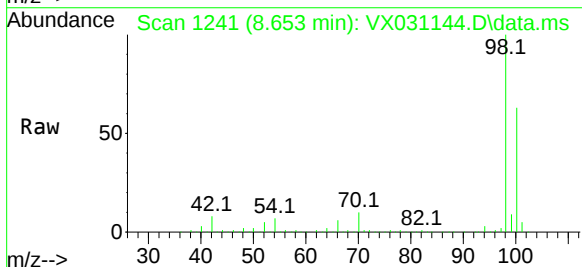



#51

4-Methyl-2-Pentanone

Concen: 25.882 ug/l

RT: 8.549 min Scan# 11

Delta R.T. -0.031 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30

Instrument :

MSVOA_X

ClientSampleId :





SB-14

Tgt Ion: 43 Resp: 77904

Ion Ratio Lower Upper

43 100

58 8.8 31.4 47.2#

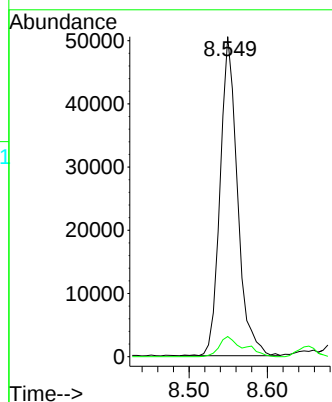

#52

Toluene

Concen: 1.027 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX031144.D




Acq: 06 Sep 2022 21:30


Tgt Ion: 92 Resp: 6595

Ion Ratio Lower Upper

92 100

91 178.5 139.2 208.8


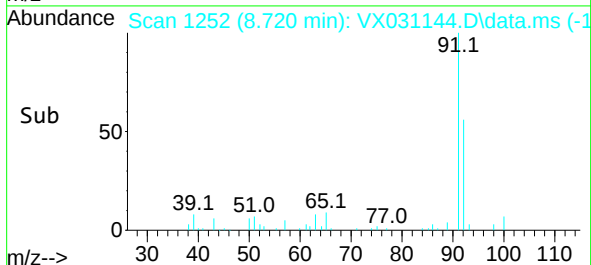

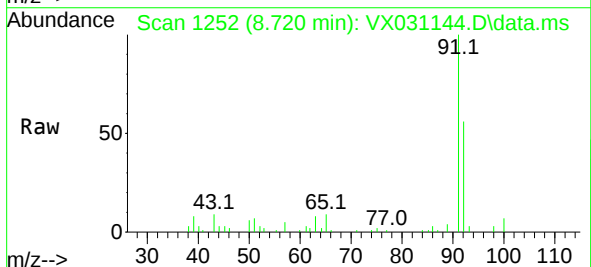




#54
 cis-1,3-Dichloropropene
 Concen: 11.473 ug/l
 RT: 8.549 min Scan# 1195
 Delta R.T. 0.177 min
 Lab File: VX031144.D
 Acq: 06 Sep 2022 21:30




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-14


Tgt Ion: 75 Resp: 45069
 Ion Ratio Lower Upper
 75 100
 77 0.5 25.0 37.4#
 39 24.6 37.5 56.3#

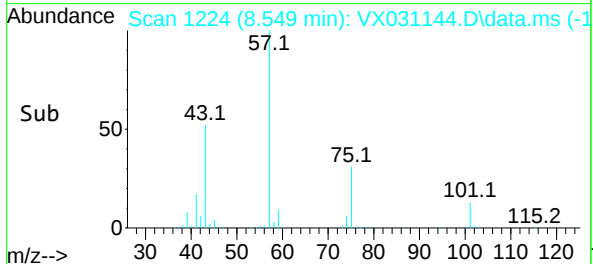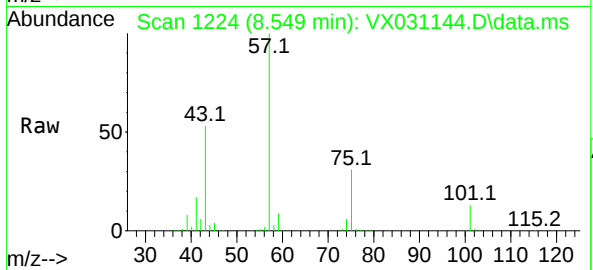

#57
 1,3-Dichloropropane
 Concen: 1.302 ug/l
 RT: 9.482 min Scan# 1377
 Delta R.T. 0.171 min
 Lab File: VX031144.D
 Acq: 06 Sep 2022 21:30

Tgt Ion: 76 Resp: 5617
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.9 38.9#




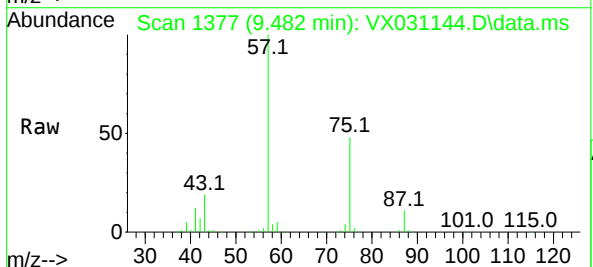




#59
2-Hexanone
Concen: 37.769 ug/l
RT: 9.378 min Scan# 11
Delta R.T. -0.055 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion: 43 Resp: 85969
Ion Ratio Lower Upper
43 100
58 0.0 27.6 82.8#

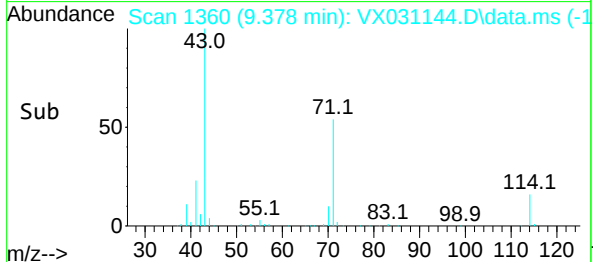

#62
4-Bromofluorobenzene
Concen: 48.740 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion: 95 Resp: 155964
Ion Ratio Lower Upper
95 100
174 85.1 0.0 149.0
176 83.8 0.0 146.0


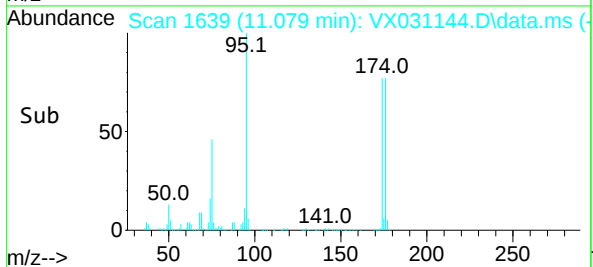

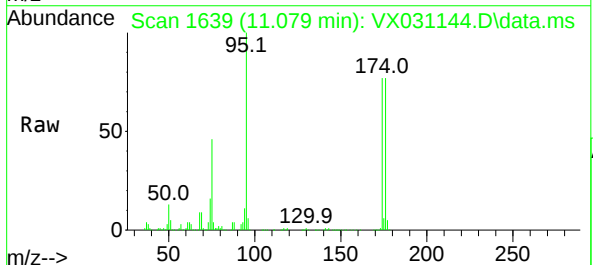




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion:117 Resp: 298927
Ion Ratio Lower Upper
117 100
82 49.8 42.7 64.1
119 32.5 25.4 38.2

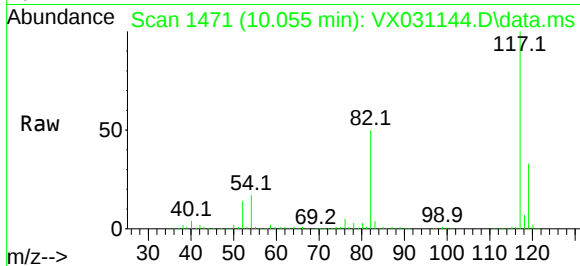

#68
m/p-Xylenes
Concen: 0.680 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion:106 Resp: 3261
Ion Ratio Lower Upper
106 100
91 181.3 158.2 237.4


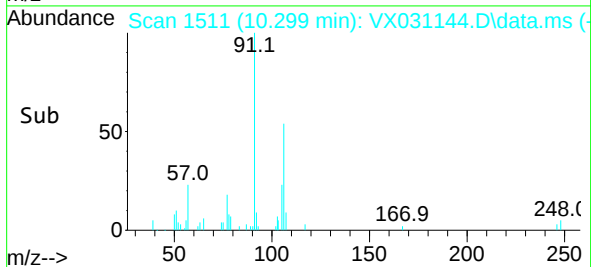

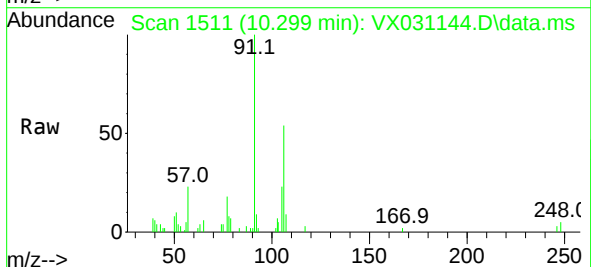




#69
o-Xylene
Concen: 0.433 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion:106 Resp: 2035
Ion Ratio Lower Upper
106 100
91 214.6 103.8 311.6

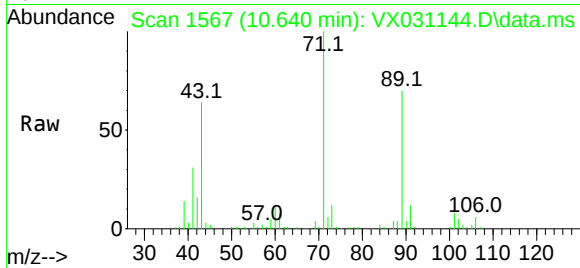

#70
Styrene
Concen: 0.451 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion:104 Resp: 3430
Ion Ratio Lower Upper
104 100
78 46.8 37.8 56.8
103 48.7 44.5 66.7

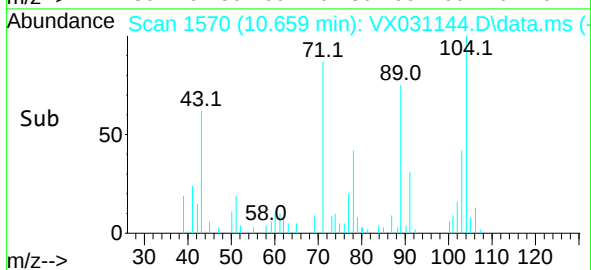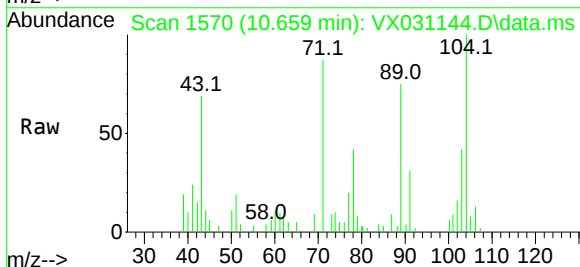



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30

Instrument :

MSVOA_X

ClientSampleId :

SB-14





Tgt Ion:152 Resp: 140419

Ion Ratio Lower Upper

152 100

115 57.0 40.5 121.5

150 159.4 0.0 347.0

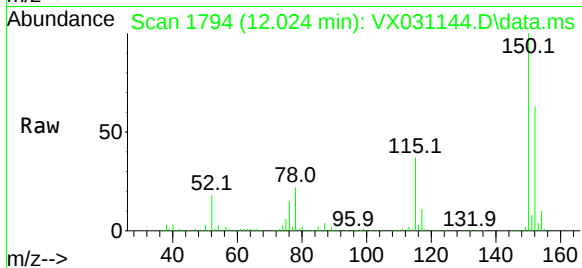

#74

N-ethyl acetate

Concen: 0.375 ug/l

RT: 10.768 min Scan# 1588

Delta R.T. -0.080 min

Lab File: VX031144.D

Acq: 06 Sep 2022 21:30

Tgt Ion: 43 Resp: 1282




Ion Ratio Lower Upper


43 100

70 0.0 32.3 48.5#

55 13.1 18.4 27.6#

61 0.0 19.2 28.8#



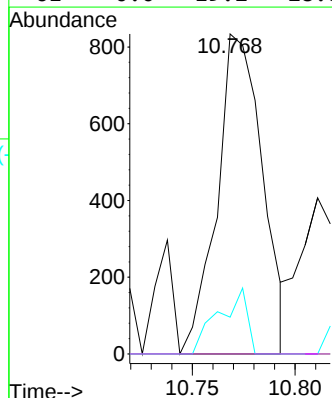
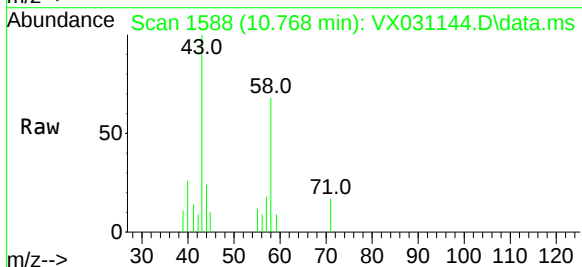




#76
1,2,3-Trichloropropane
Concen: 20.984 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion: 75 Resp: 69654
Ion Ratio Lower Upper
75 100
77 1.3 19.8 59.3#



#81
trans-1,4-Dichloro-2-butene
Concen: 65.947 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.055 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Tgt Ion: 75 Resp: 69654
Ion Ratio Lower Upper
75 100
53 0.1 74.2 111.4#
89 0.0 34.8 52.2#


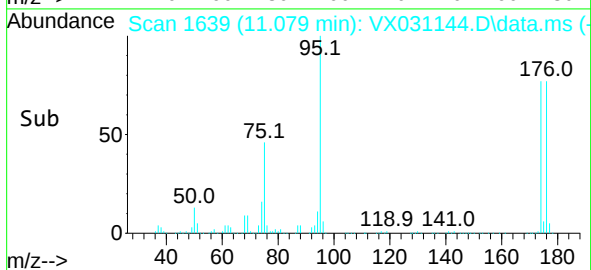

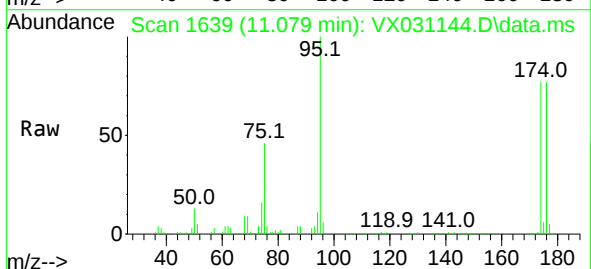




#84
1,2,4-Trimethylbenzene
Concen: 0.823 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30




Instrument :
MSVOA_X
ClientSampleId :
SB-14


Tgt Ion:105 Resp: 7793
Ion Ratio Lower Upper
105 100
120 12.5 22.9 68.8#

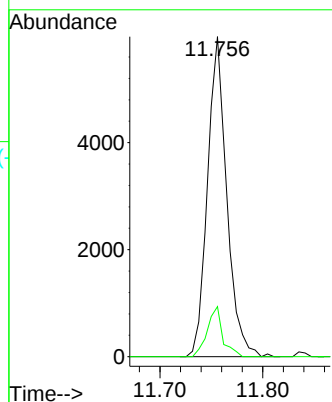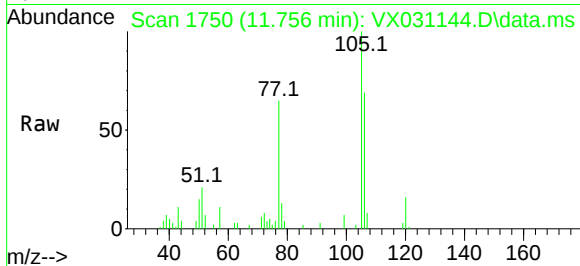

#85
sec-Butylbenzene
Concen: 0.628 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.140 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30


Tgt Ion:105 Resp: 7793
Ion Ratio Lower Upper
105 100
134 0.0 10.0 30.0#

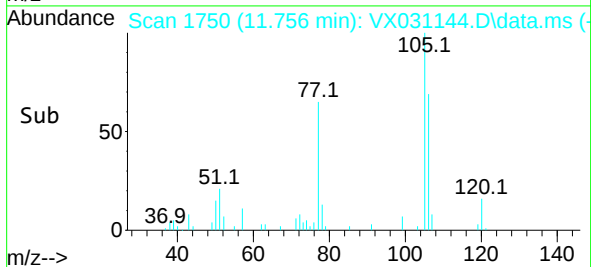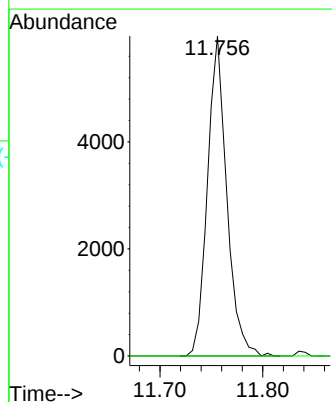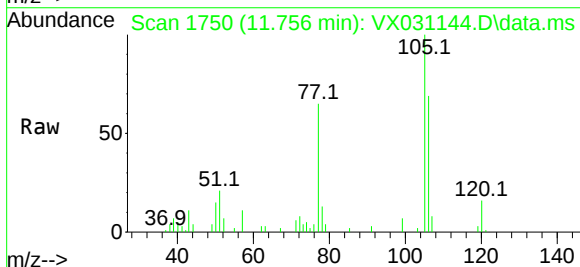

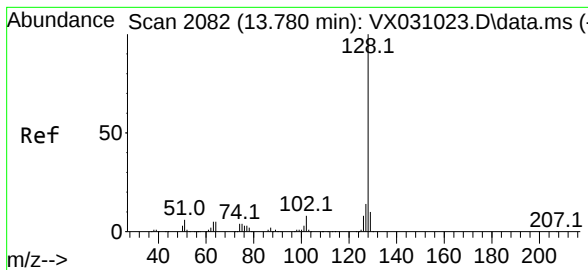

#95
Naphthalene
Concen: 5.637 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX031144.D
Acq: 06 Sep 2022 21:30

Instrument :
MSVOA_X
ClientSampleId :
SB-14

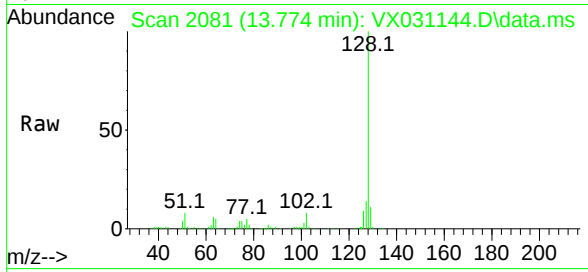

Tgt Ion:128 Resp: 71746

Ion	Ratio	Lower	Upper
128	100		
127	13.6	10.2	15.2
129	11.0	8.6	13.0

