
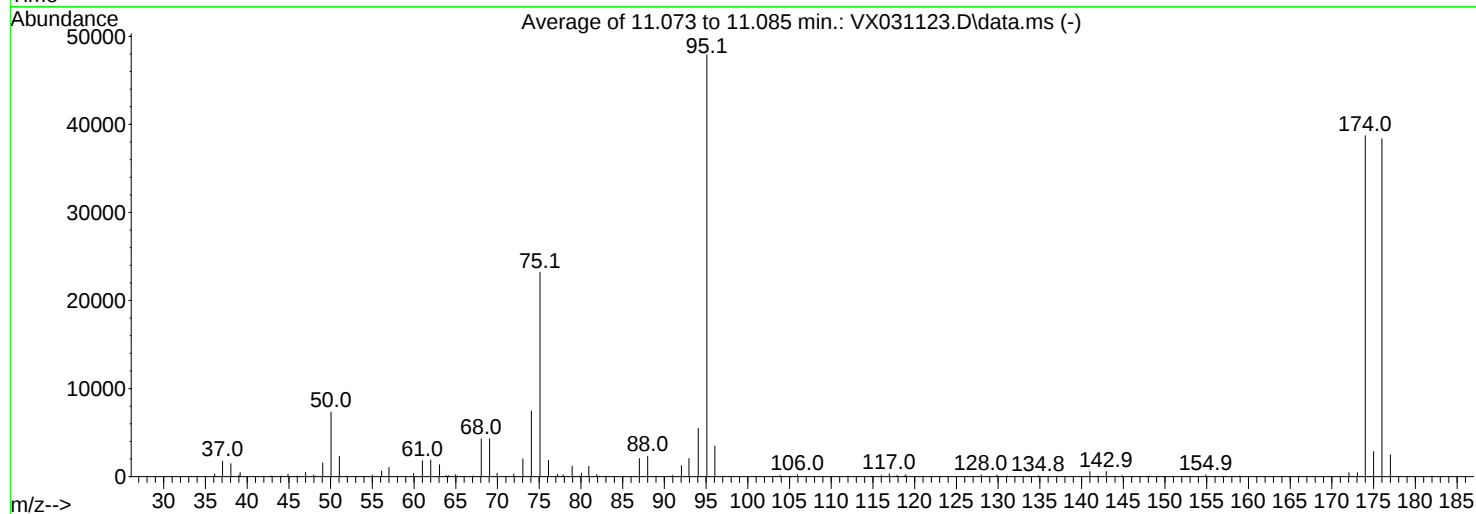


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090622\
Data File : VX031123.D
Acq On : 06 Sep 2022 11:39
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090122W.M
Title : SW846 8260
Last Update : Fri Sep 02 02:49:21 2022

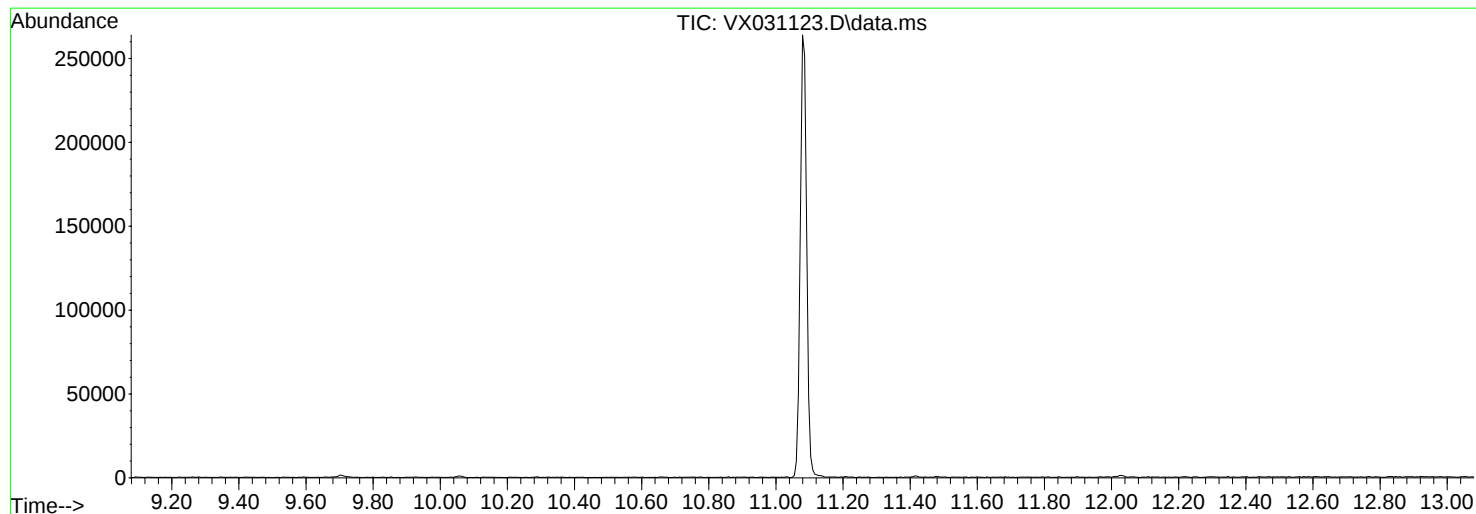

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.3	7339	PASS
75	95	30	60	48.4	23195	PASS
95	95	100	100	100.0	47896	PASS
96	95	5	9	7.2	3462	PASS
173	174	0.00	2	1.2	461	PASS
174	95	50	100	80.8	38720	PASS
175	174	5	9	7.4	2854	PASS
176	174	95	101	99.1	38379	PASS
177	176	5	9	6.5	2496	PASS