

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090623\
 Data File : VX037549.D
 Acq On : 06 Sep 2023 12:57
 Operator : JC/MD
 Sample : 04220-02DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW5DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Title : SW846 8260

Signal : TIC: VX037549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.575	69	80	81	rBV8	2257	6269	1.01%	0.170%
2	1.618	81	87	93	rVB8	2739	6966	1.12%	0.189%
3	2.971	297	309	323	rBV2	19305	57208	9.22%	1.555%
4	3.117	323	333	348	rVB	58278	136892	22.06%	3.720%
5	3.764	432	439	448	rBV2	2534	6544	1.05%	0.178%
6	4.587	562	574	591	rBV	30018	103510	16.68%	2.813%
7	5.013	636	644	663	rVB2	10130	33755	5.44%	0.917%
8	5.385	694	705	721	rBV	69517	207350	33.42%	5.635%
9	5.550	721	732	748	rVB2	132330	376882	60.75%	10.243%
10	5.958	789	799	808	rBV3	74260	197612	31.85%	5.371%
11	6.038	808	812	822	rVB3	5840	15010	2.42%	0.408%
12	6.251	839	847	854	rBV4	2582	6602	1.06%	0.179%
13	6.763	922	931	947	rBV	192799	462344	74.52%	12.565%
14	8.647	1234	1240	1250	rBV	394338	620406	100.00%	16.861%
15	9.494	1375	1379	1387	rVB	4471	6760	1.09%	0.184%
16	10.055	1465	1471	1481	rBV	388249	535994	86.39%	14.567%
17	11.079	1634	1639	1650	rBV	310116	399440	64.38%	10.856%
18	12.024	1788	1794	1807	rBV	387475	487968	78.65%	13.262%
19	12.244	1825	1830	1836	rVB2	9065	12026	1.94%	0.327%




Sum of corrected areas: 3679538

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090623\
Data File : VX037549.D
Acq On : 06 Sep 2023 12:57
Operator : JC/MD
Sample : 04220-02DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

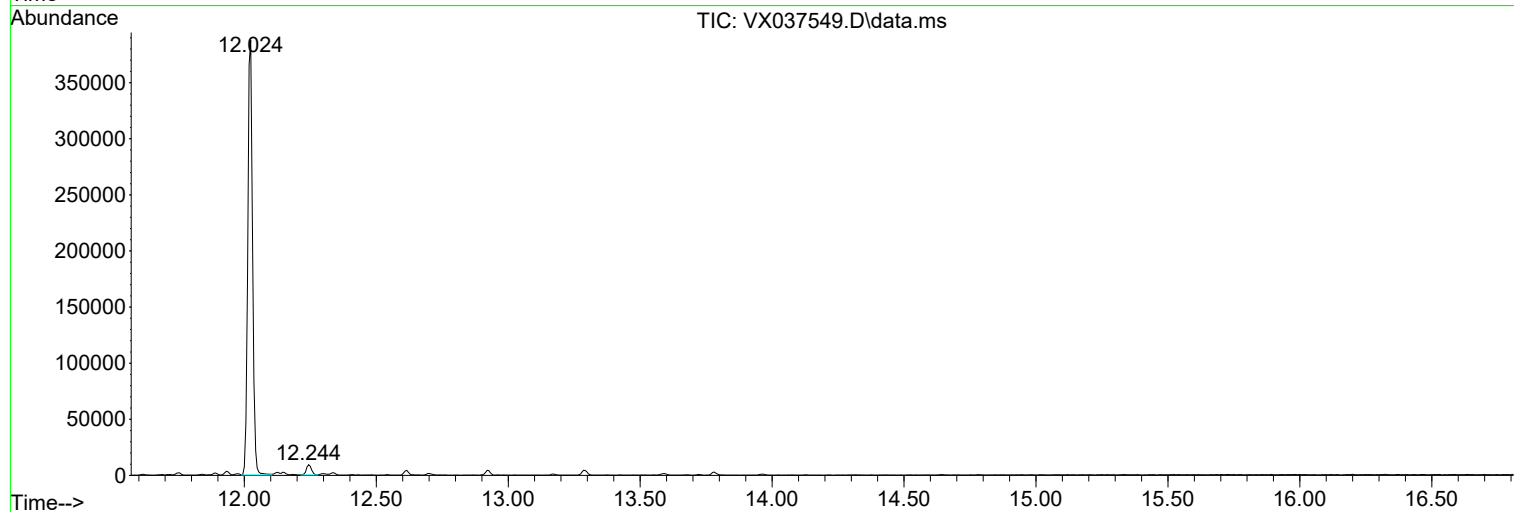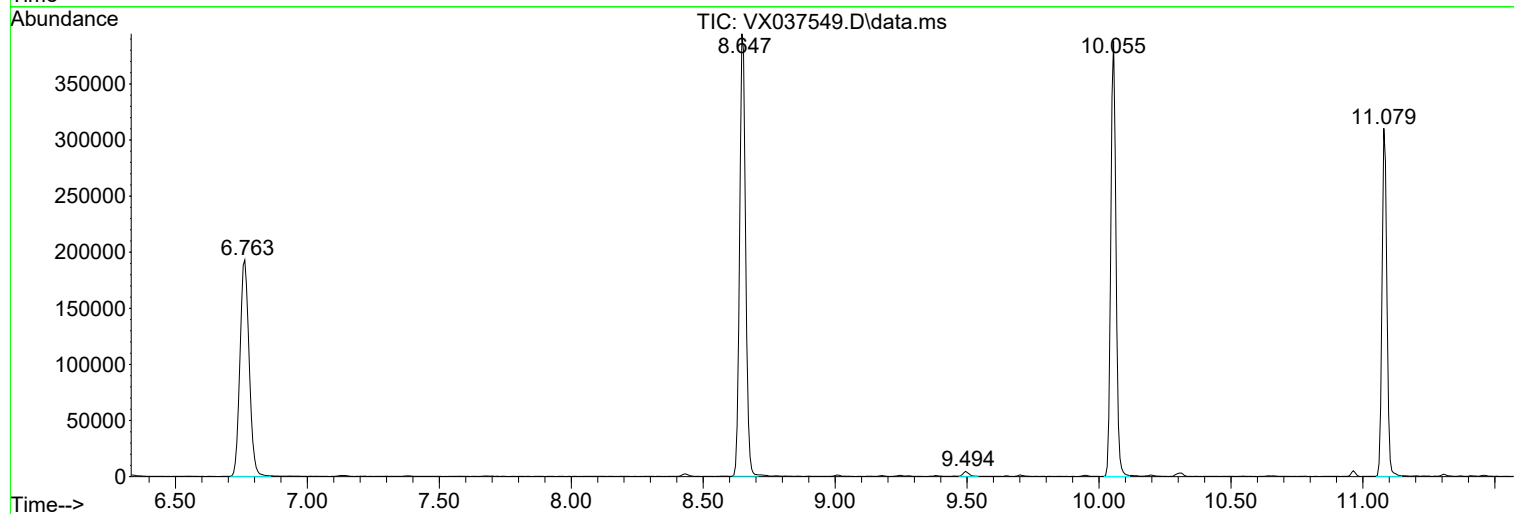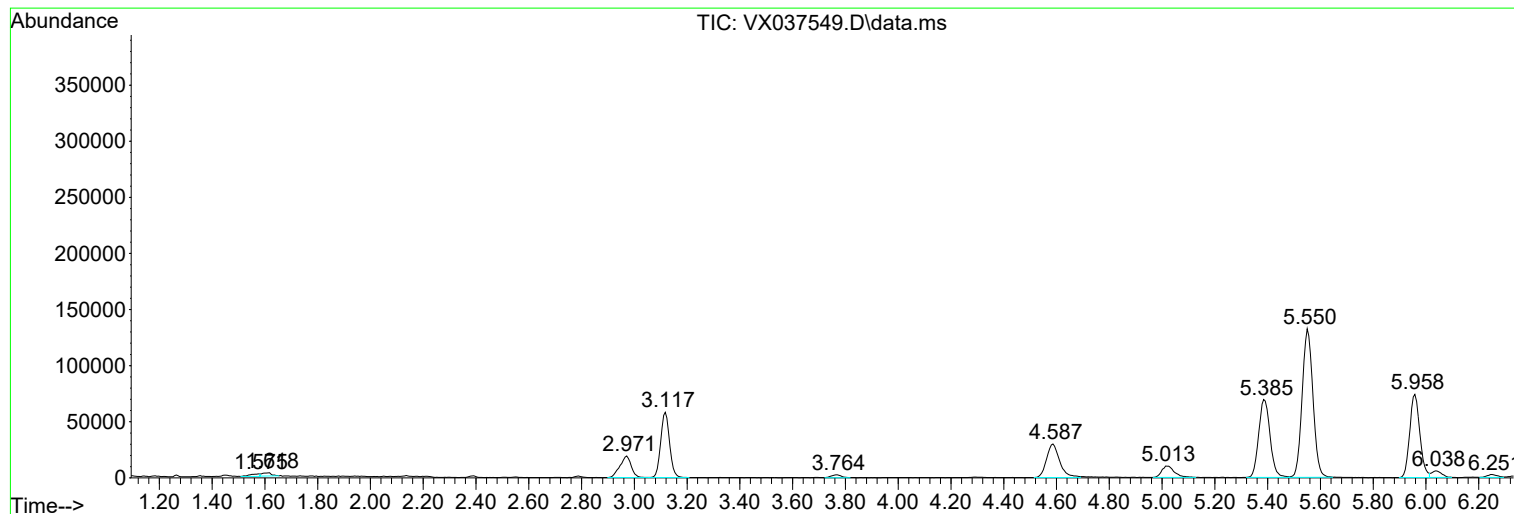

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090623\
Data File : VX037549.D
Acq On : 06 Sep 2023 12:57
Operator : JC/MD
Sample : 04220-02DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090623\
Data File : VX037549.D
Acq On : 06 Sep 2023 12:57
Operator : JC/MD
Sample : 04220-02DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc