

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090623\
 Data File : VX037553.D
 Acq On : 06 Sep 2023 14:35
 Operator : JC/MD
 Sample : 04220-03DL 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW7DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Title : SW846 8260

Signal : TIC: VX037553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.971	297	309	323	rBV2	53287	141138	16.00%	2.773%
2	3.117	323	333	350	rVB	383567	881925	100.00%	17.325%
3	4.586	561	574	598	rBV	60423	210153	23.83%	4.128%
4	5.019	635	645	658	rBV2	11667	37248	4.22%	0.732%
5	5.385	694	705	720	rBV2	69990	207526	23.53%	4.077%
6	5.550	722	732	748	rVB2	131938	372915	42.28%	7.326%
7	5.958	789	799	807	rBV	75875	197806	22.43%	3.886%
8	6.037	807	812	824	rVB	12698	34947	3.96%	0.687%
9	6.330	853	860	872	rVB2	6327	19002	2.15%	0.373%
10	6.763	920	931	951	rBV	194399	465569	52.79%	9.146%
11	8.647	1234	1240	1250	rBV	379483	616926	69.95%	12.119%
12	9.378	1355	1360	1368	rBV	10017	14468	1.64%	0.284%
13	9.494	1368	1379	1392	rBV	33403	53853	6.11%	1.058%
14	10.055	1465	1471	1486	rVV	400618	573549	65.03%	11.267%
15	10.195	1490	1494	1500	rBV	13236	18499	2.10%	0.363%
16	10.305	1506	1512	1518	rVB2	8341	13570	1.54%	0.267%
17	10.963	1614	1620	1626	rVB	15976	19550	2.22%	0.384%
18	11.079	1634	1639	1647	rBV	314733	403827	45.79%	7.933%
19	11.305	1671	1676	1684	rBV2	18384	24715	2.80%	0.486%
20	11.884	1766	1771	1779	rVB4	6168	9586	1.09%	0.188%
21	12.024	1789	1794	1801	rBV	404178	502549	56.98%	9.872%
22	12.097	1801	1806	1812	rVB3	5658	10267	1.16%	0.202%
23	12.189	1816	1821	1825	rBV	7042	8974	1.02%	0.176%
24	12.244	1825	1830	1837	rVB	47117	61063	6.92%	1.200%
25	12.542	1873	1879	1887	rBV3	6250	13254	1.50%	0.260%
26	12.615	1887	1891	1894	rBV	17032	19349	2.19%	0.380%
27	12.701	1900	1905	1912	rBV3	10344	14691	1.67%	0.289%
28	12.920	1934	1941	1945	rBV2	15040	22001	2.49%	0.432%
29	13.170	1978	1982	1987	rBV	11512	13698	1.55%	0.269%
30	13.292	1993	2002	2006	rBV2	33458	46054	5.22%	0.905%
31	13.512	2031	2038	2041	rBV3	6289	9486	1.08%	0.186%
32	13.774	2076	2081	2089	rBV	32291	42275	4.79%	0.830%
33	14.639	2219	2223	2233	rVB	8227	10134	1.15%	0.199%




Sum of corrected areas: 5090567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090623\
Data File : VX037553.D
Acq On : 06 Sep 2023 14:35
Operator : JC/MD
Sample : 04220-03DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

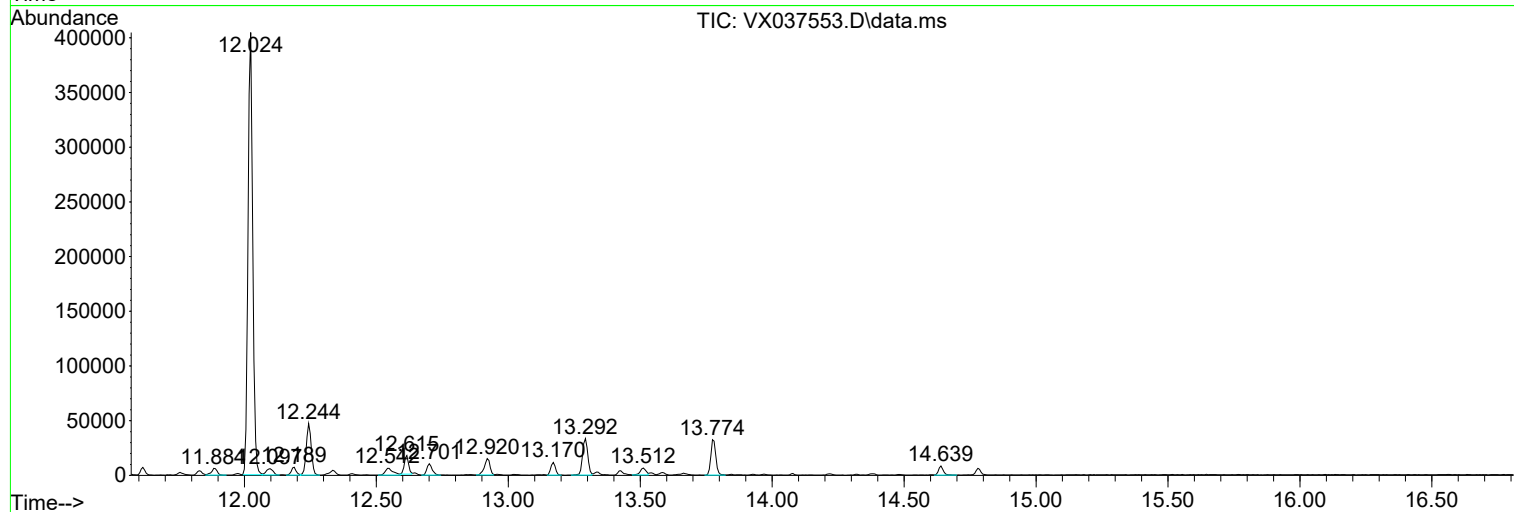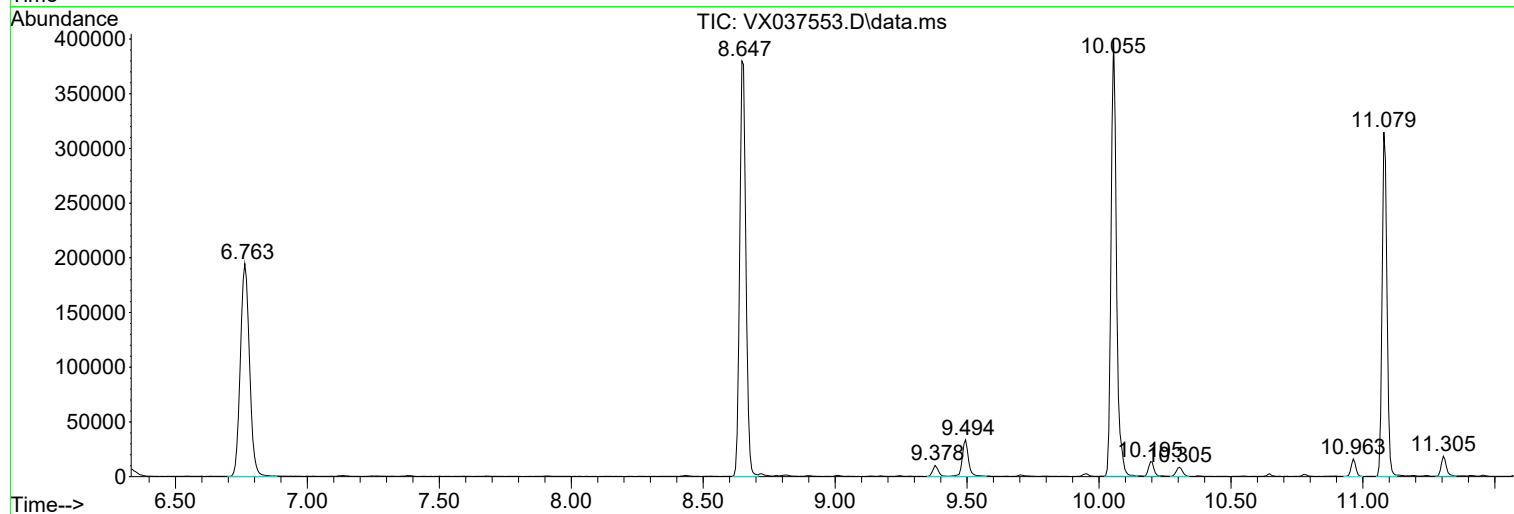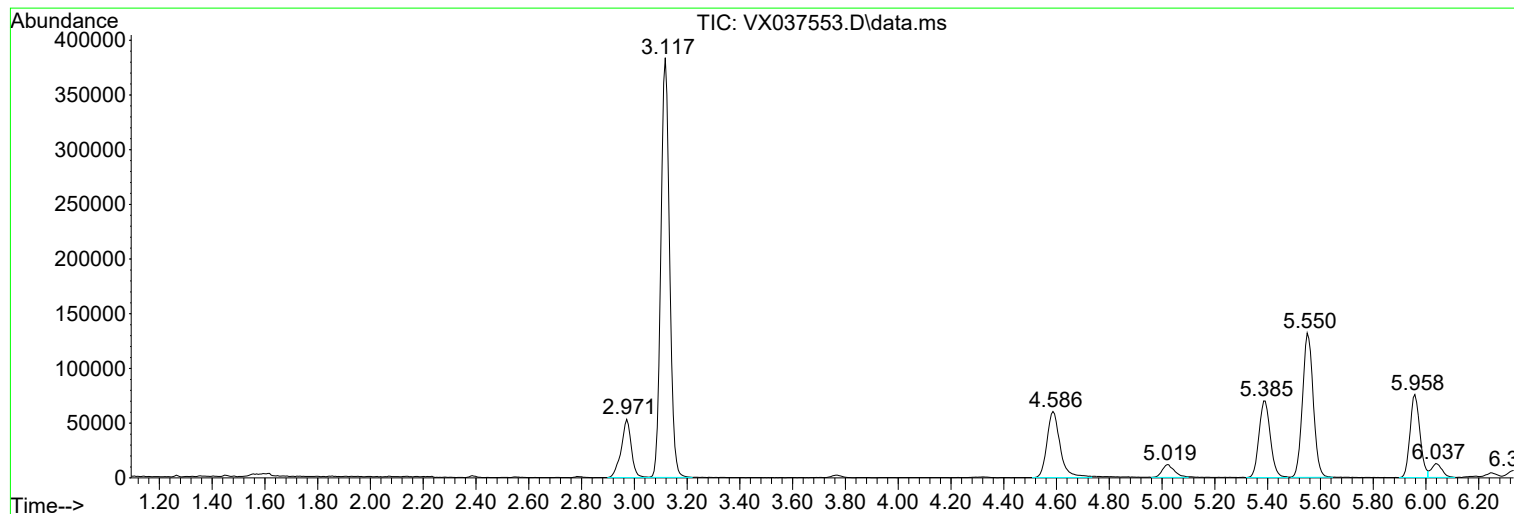

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090623\
Data File : VX037553.D
Acq On : 06 Sep 2023 14:35
Operator : JC/MD
Sample : 04220-03DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090623\
Data File : VX037553.D
Acq On : 06 Sep 2023 14:35
Operator : JC/MD
Sample : 04220-03DL 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------