

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX090718\
 Data File : VX004409.D
 Acq On : 07 Sep 2018 16:05
 Operator : JC/MD
 Sample : J4812-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB090518

Quant Time: Sep 08 04:03:56 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 23 05:39:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	321481	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	508997	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	494557	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	281065	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	216993	51.79	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.58%	
35) Dibromofluoromethane	5.49	113	191081	50.46	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.92%	
50) Toluene-d8	8.71	98	724690	50.70	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.40%	
62) 4-Bromofluorobenzene	11.14	95	260750	48.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.78%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX090718\
Data File : VX004409.D
Acq On : 07 Sep 2018 16:05
Operator : JC/MD
Sample : J4812-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB090518

Quant Time: Sep 08 04:03:56 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 23 05:39:44 2018
Response via : Initial Calibration

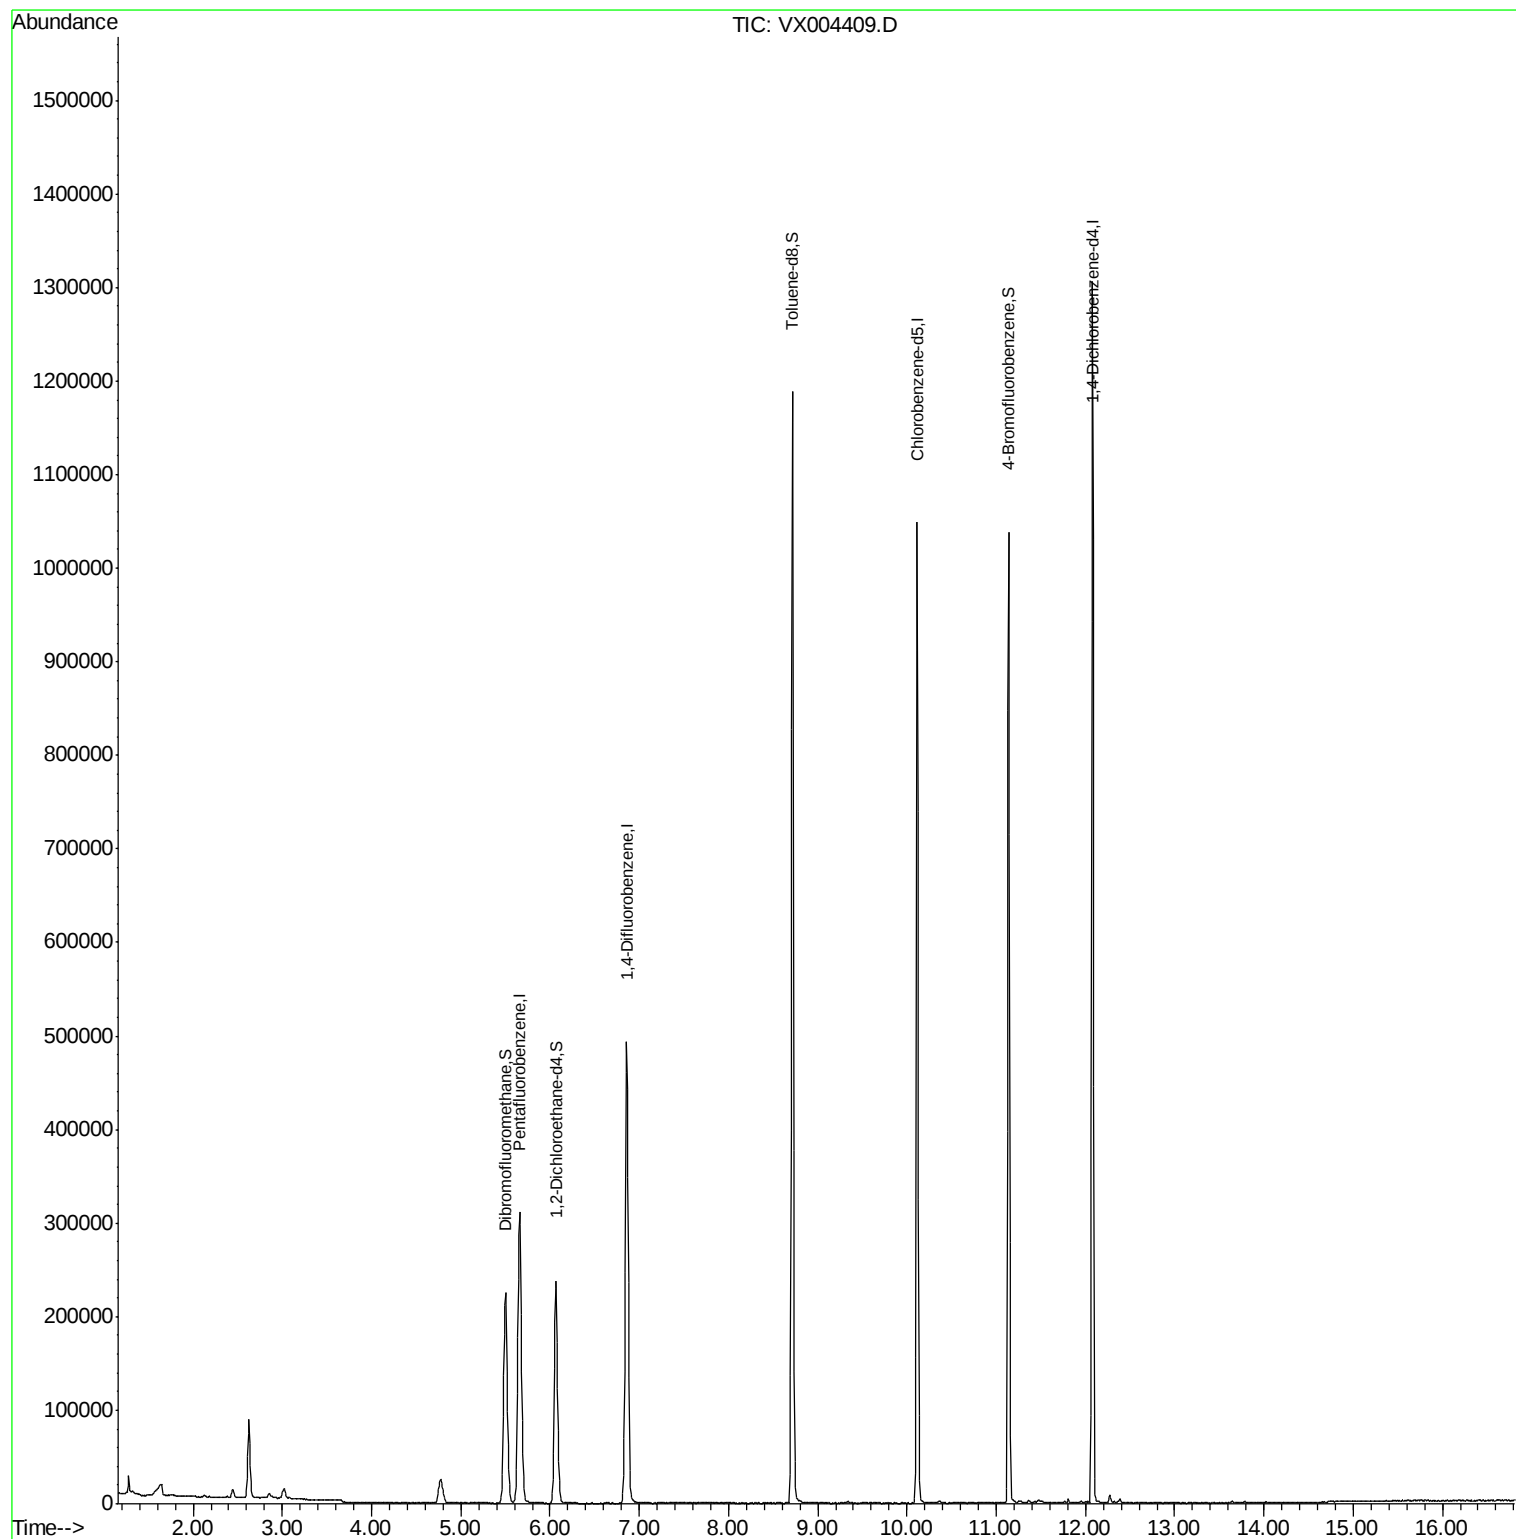

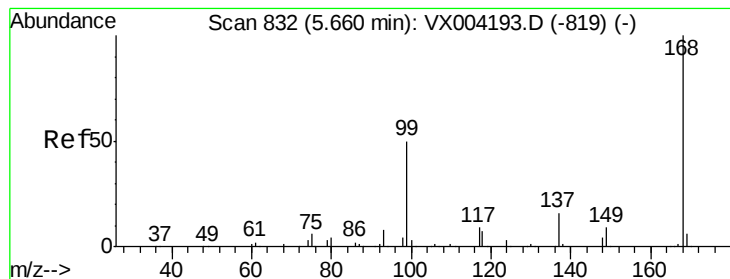

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.00 min

Lab File: VX004409.D

Acq: 07 Sep 2018 16:05

Instrument :

MSVOA_X

ClientSampleId :


FB090518

Tot Ion:168 Resp: 321481




Ion Ratio Lower Upper

168 100

99 51.8 39.9 59.9

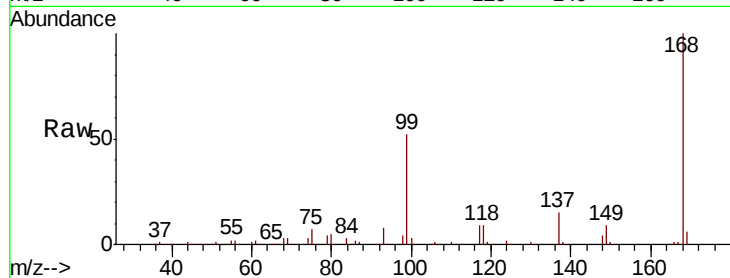

Abundance Ion 167.90 (167.60 to 168.60): VX004409.D (-690) (-)

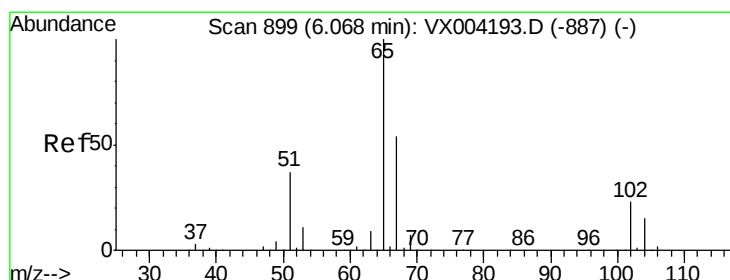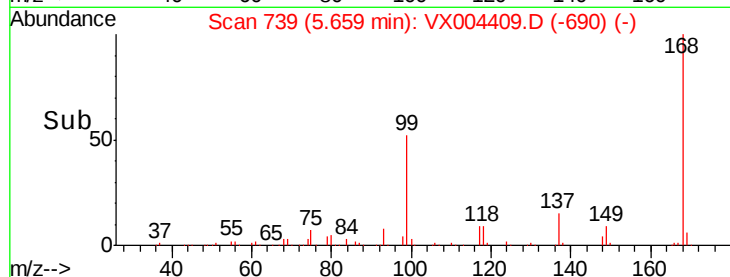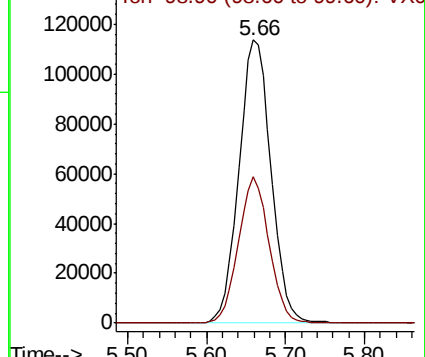

#33

1,2-Dichloroethane-d4

Concen: 51.79 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX004409.D


Acq: 07 Sep 2018 16:05

Tgt Ion: 65 Resp: 216993



Ion Ratio Lower Upper

65 100

67 54.0 0.0 106.8

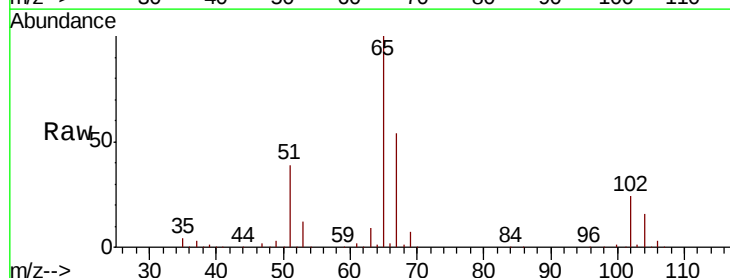

Abundance Ion 64.90 (64.60 to 65.60): VX004409.D (-757) (-)

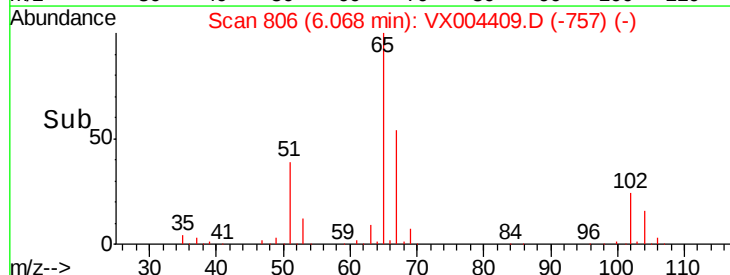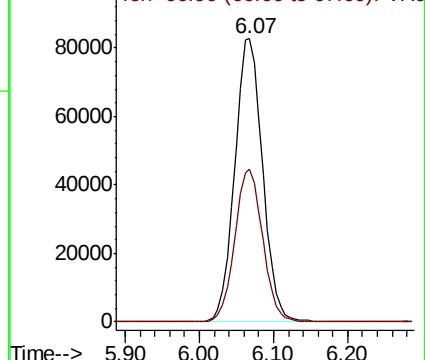







#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX004409.D
 Acq: 07 Sep 2018 16:05

Instrument :
 MSVOA_X
 ClientSampleId :
 FB090518

Tot Ion	Ratio	Lower	Upper
114	100		
63	19.5	0.0	39.0
88	15.3	0.0	30.4

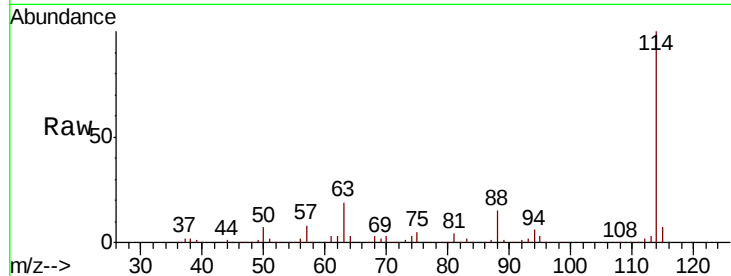


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 87.90 (87.60 to 88.60): VX0

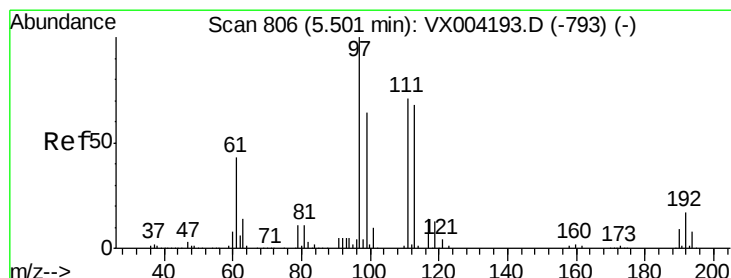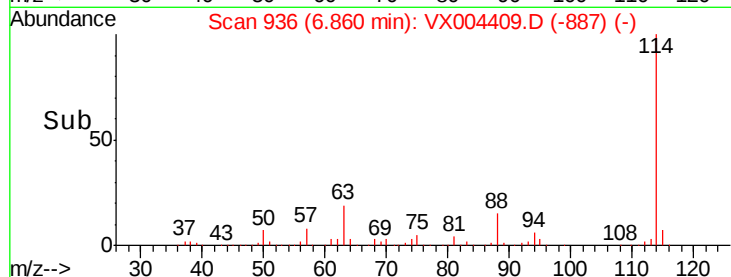
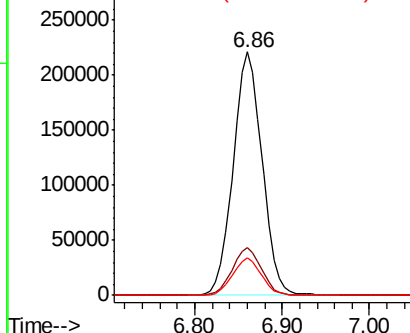



#35
 Dibromofluoromethane
 Concen: 50.46 ug/l
 RT: 5.49 min Scan# 712
 Delta R.T. -0.01 min
 Lab File: VX004409.D
 Acq: 07 Sep 2018 16:05

Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.4	82.4	123.6
192	24.3	19.4	29.2

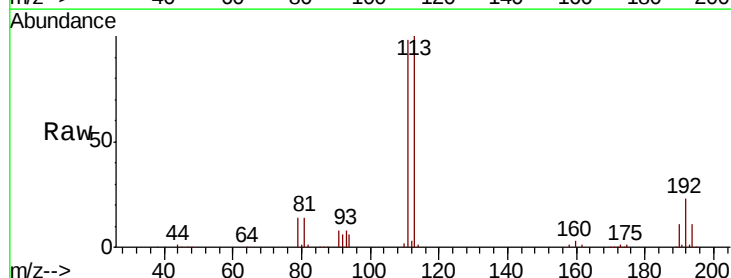

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

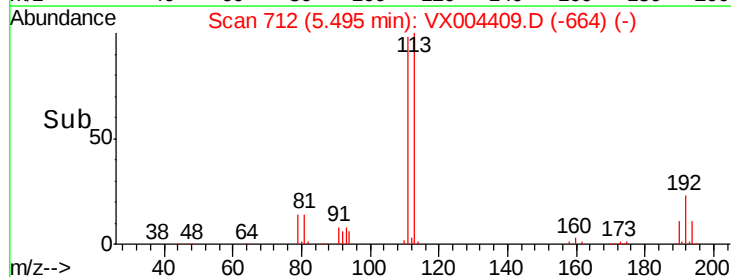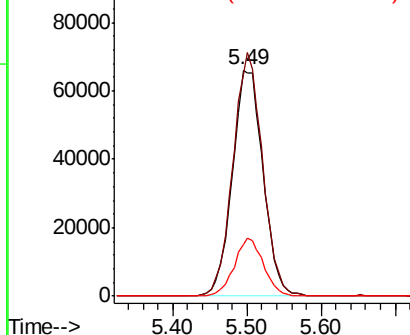

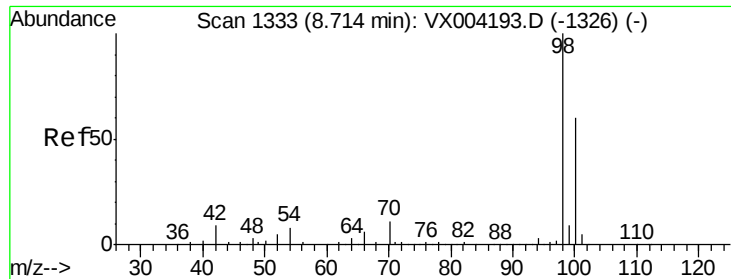

#50

Toluene-d8

Concen: 50.70 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX004409.D

Acq: 07 Sep 2018 16:05

Instrument :

MSVOA_X

ClientSampleId :


FB090518

Tot Ion: 98 Resp: 724690

Ion Ratio Lower Upper




98 100

100 66.2 52.9 79.3

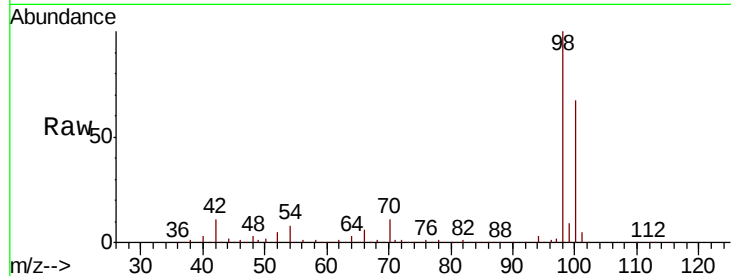

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

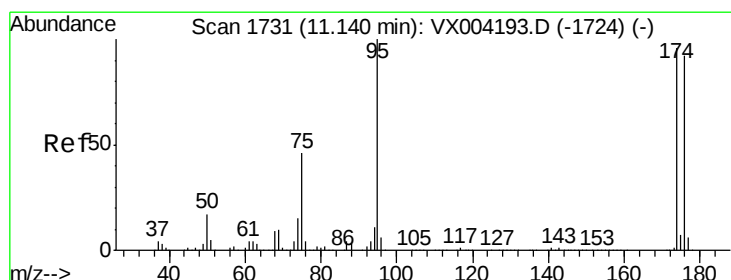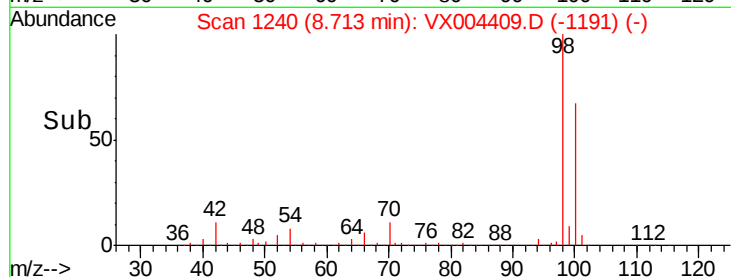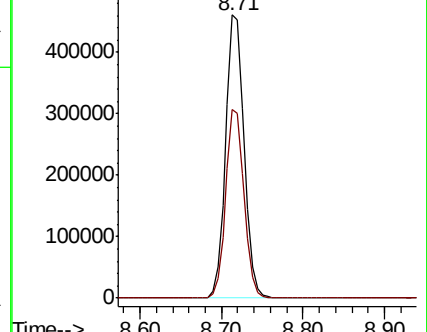

#62

4-Bromofluorobenzene

Concen: 48.89 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. -0.00 min

Lab File: VX004409.D

Acq: 07 Sep 2018 16:05


Tgt Ion: 95 Resp: 260750

Ion Ratio Lower Upper

95 100

174 91.0 0.0 185.2



176 88.8 0.0 178.6

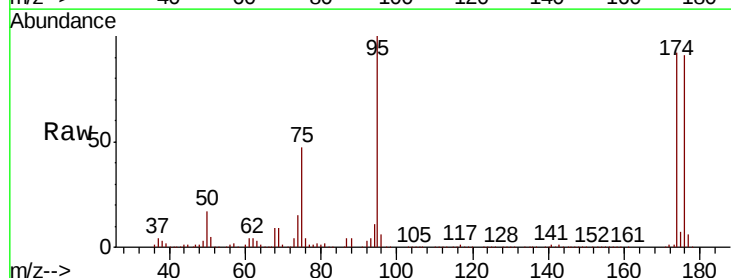


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

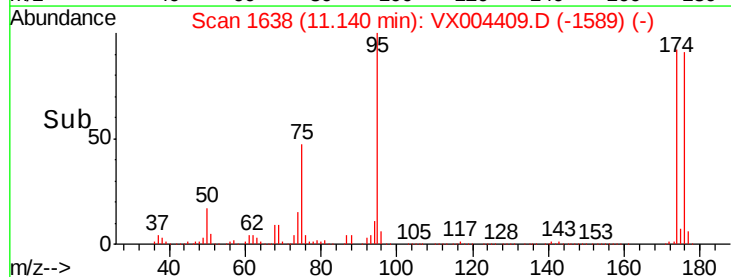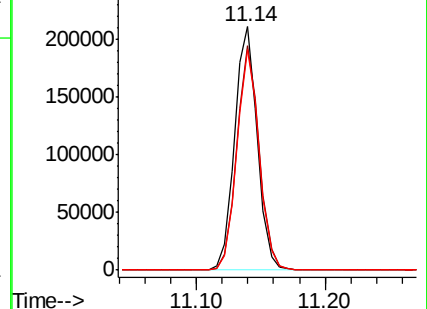


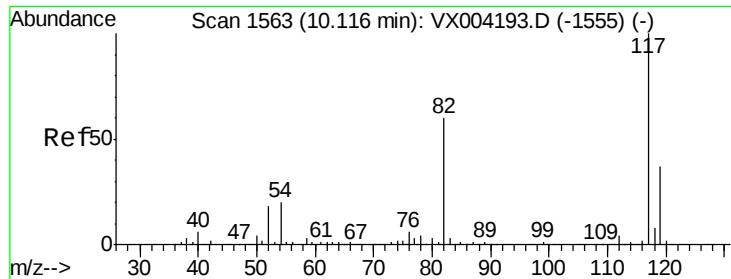




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. -0.00 min
Lab File: VX004409.D
Acq: 07 Sep 2018 16:05

Instrument :
MSVOA_X
ClientSampled :
FB090518

Tot Ion:117 Resp: 494557
Ion Ratio Lower Upper
117 100
82 52.4 47.8 71.6
119 31.8 29.3 43.9

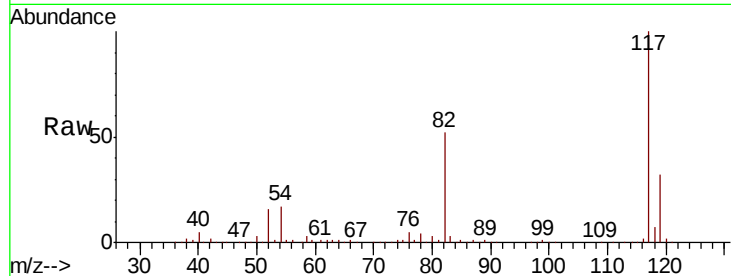


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

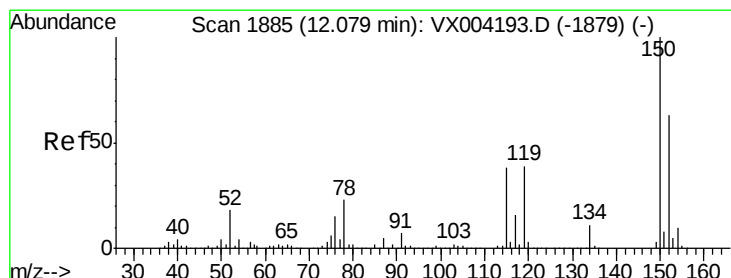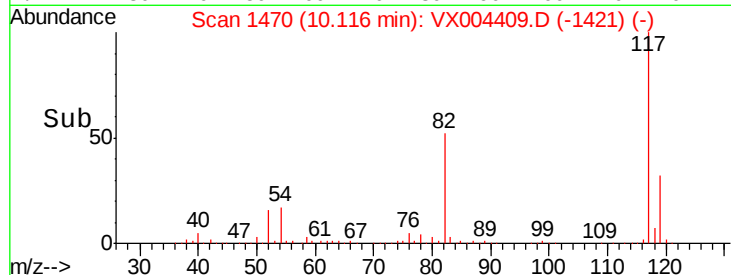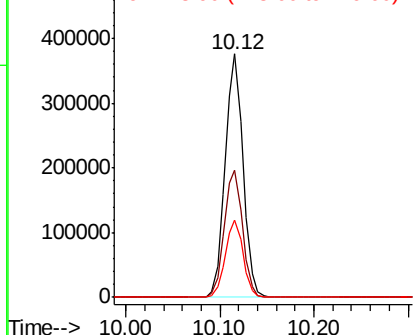

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX004409.D
Acq: 07 Sep 2018 16:05

Tgt Ion:152 Resp: 281065
Ion Ratio Lower Upper
152 100
115 54.9 39.0 117.0
150 155.6 0.0 351.0

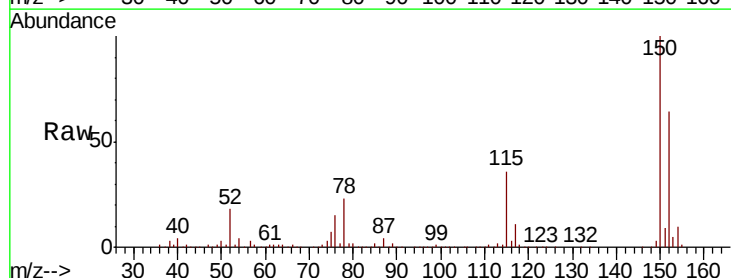

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

