


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090718\
Data File : VX004400.D
Acq On : 07 Sep 2018 09:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Title : SW846 8260
Last Update : Thu Aug 23 05:39:44 2018

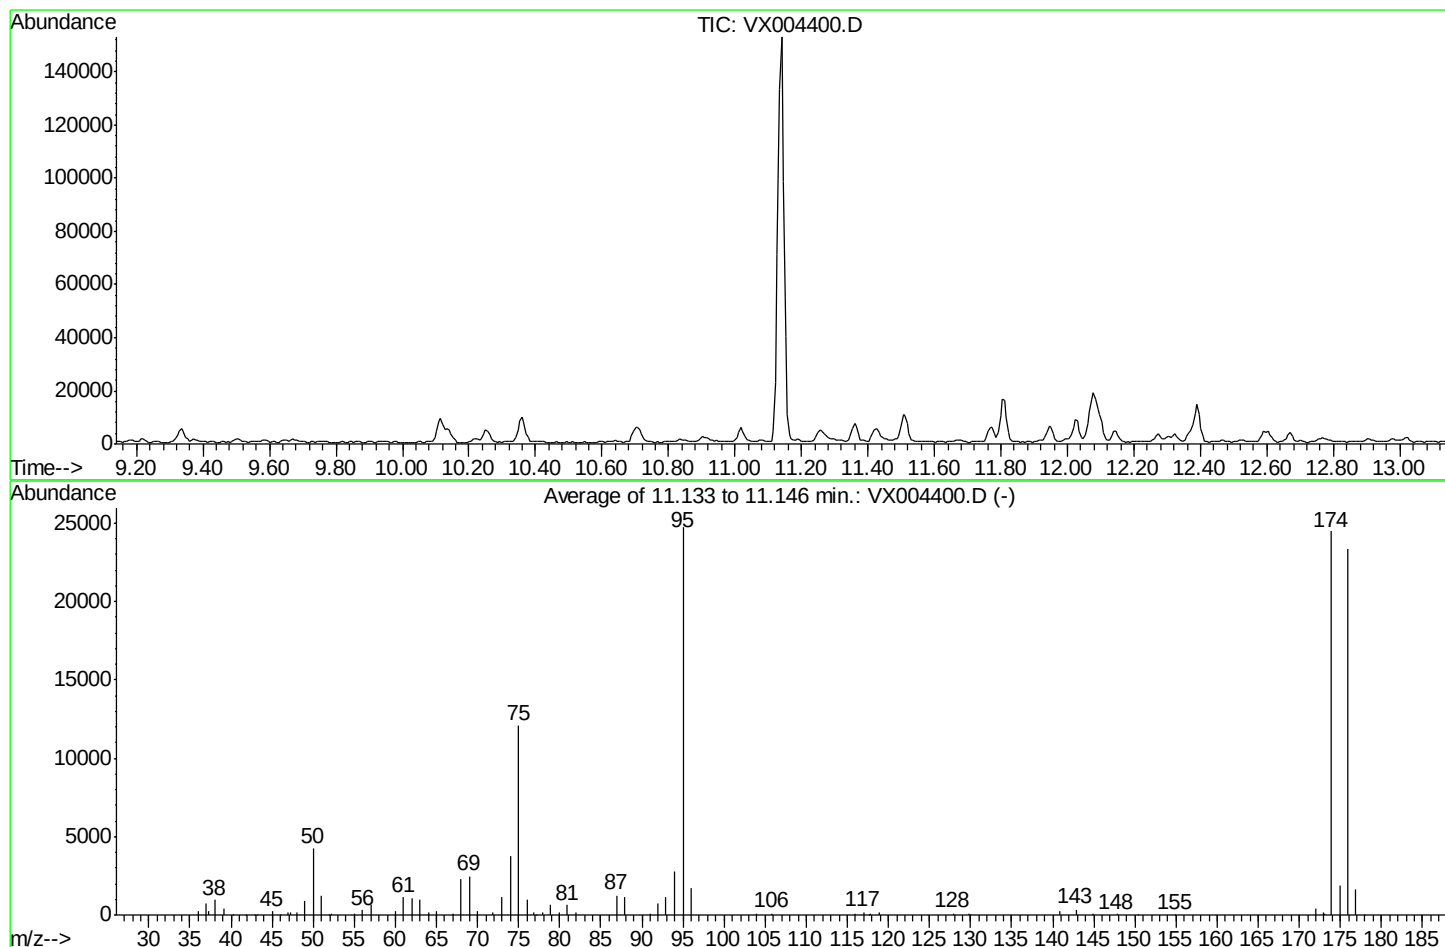

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	4230	PASS
75	95	30	60	48.9	12089	PASS
95	95	100	100	100.0	24741	PASS
96	95	5	9	7.0	1728	PASS
173	174	0.00	2	0.8	193	PASS
174	95	50	100	98.9	24472	PASS
175	174	5	9	7.6	1852	PASS
176	174	95	101	95.6	23402	PASS
177	176	5	9	6.9	1613	PASS