


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090718\
Data File : VX004421.D
Acq On : 07 Sep 2018 21:52
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Title : SW846 8260
Last Update : Thu Aug 23 05:39:44 2018

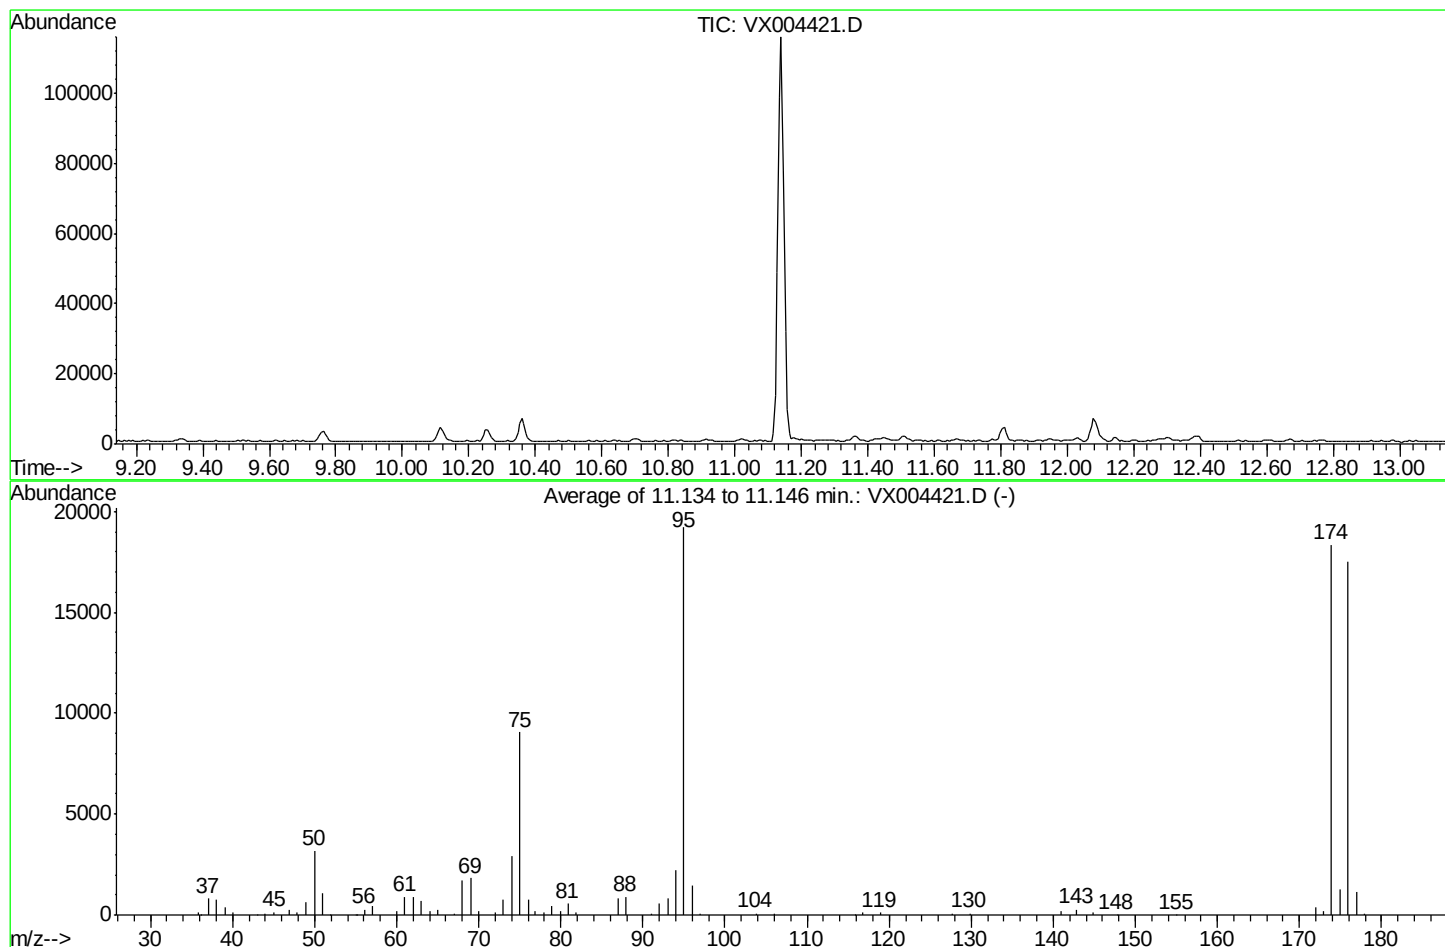

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	3188	PASS
75	95	30	60	47.2	9068	PASS
95	95	100	100	100.0	19222	PASS
96	95	5	9	7.5	1435	PASS
173	174	0.00	2	1.0	189	PASS
174	95	50	100	95.5	18355	PASS
175	174	5	9	7.1	1296	PASS
176	174	95	101	95.3	17496	PASS
177	176	5	9	6.6	1152	PASS