


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX090719\
Data File : VX012189.D
Acq On : 07 Sep 2019 21:13
Operator : SY/SP
Sample : BFB
Misc : 5.00µ/5.0mL/MSVOA X/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X090319S.M
Title : SW846 8260
Last Update : Tue Sep 03 15:26:48 2019

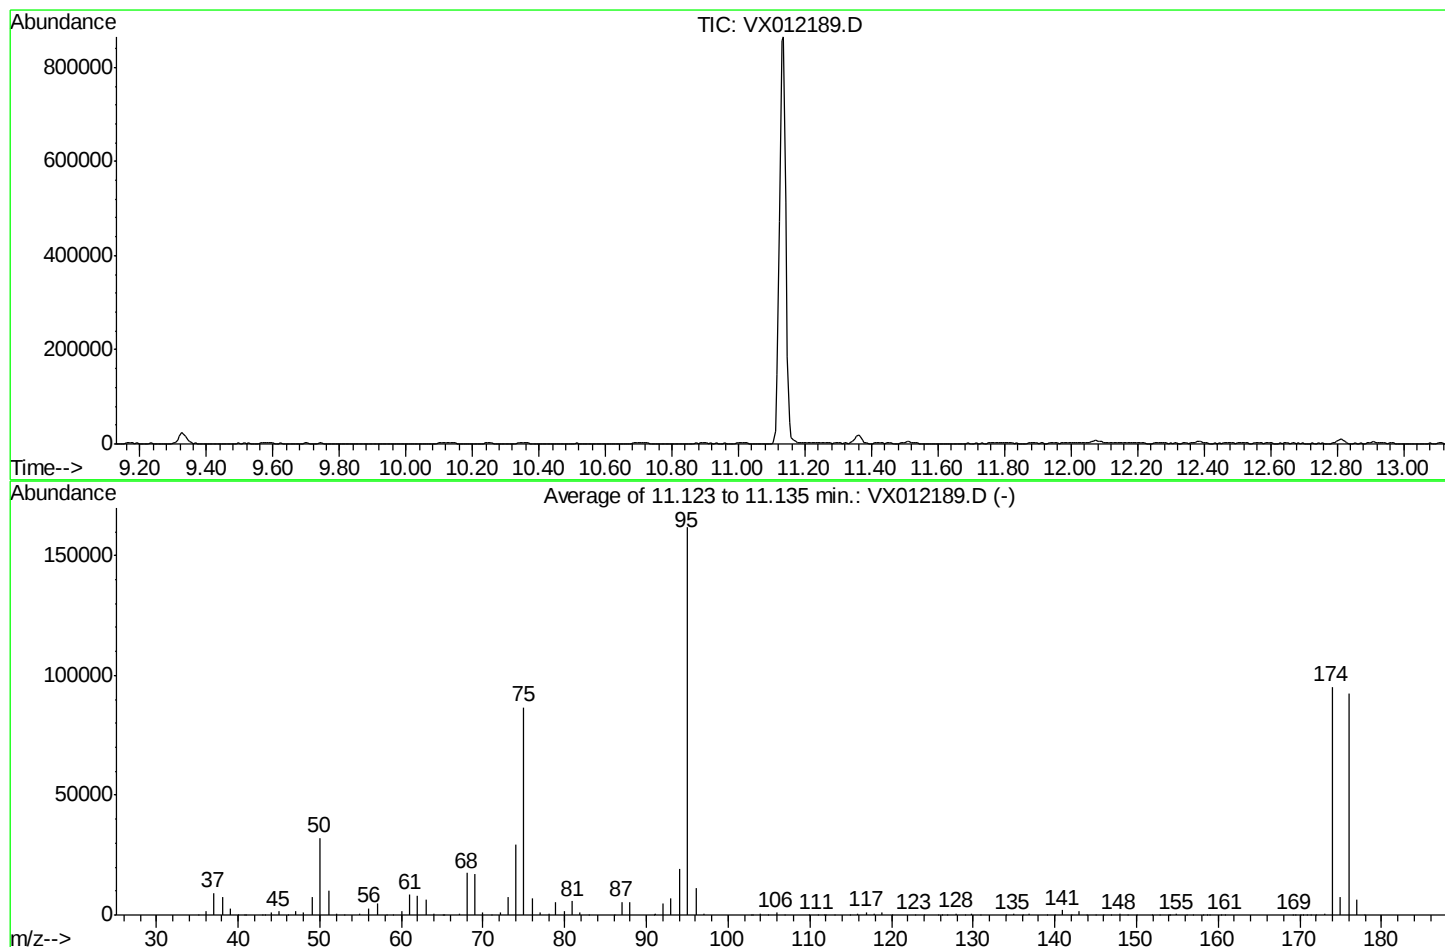

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	32304	PASS
75	95	30	60	53.6	86773	PASS
95	95	100	100	100.0	161789	PASS
96	95	5	9	6.9	11139	PASS
173	174	0.00	2	0.6	557	PASS
174	95	50	100	58.8	95208	PASS
175	174	5	9	8.0	7637	PASS
176	174	95	101	97.0	92328	PASS
177	176	5	9	6.7	6203	PASS