

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090721\
 Data File : VX024121.D
 Acq On : 07 Sep 2021 16:29
 Operator : JC/MD
 Sample : PB138939TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Sep 08 13:27:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 11:57:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	156027	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	262035	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	255348	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	109157	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	121569	55.826	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 111.660%			
35) Dibromofluoromethane	5.391	113	93385	53.845	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 107.680%			
50) Toluene-d8	8.653	98	349918	53.010	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 106.020%			
62) 4-Bromofluorobenzene	11.085	95	129929	53.469	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 106.940%			
Target Compounds					Qvalue	
5) Bromomethane	1.618	94	786	0.709	ug/l #	74
6) Chloroethane	1.715	64	126	2.299	ug/l #	43
10) Methyl Iodide	2.465	142	1446	0.663	ug/l #	84
11) Tert butyl alcohol	2.953	59	5305	12.046	ug/l #	75
13) Acrolein	2.239	56	82	0.313	ug/l #	1
16) Acetone	2.386	43	34844	35.786	ug/l #	87
17) Carbon Disulfide	2.514	76	1408	0.394	ug/l #	92
18) Methyl Acetate	2.715	43	1002	0.412	ug/l	90
20) Methylene Chloride	2.794	84	10351	5.565	ug/l	89
25) 2-Butanone	4.574	43	7766	5.266	ug/l #	86
29) Tetrahydrofuran	5.044	42	1469	1.538	ug/l #	55
31) Cyclohexane	5.562	56	3726	1.332	ug/l #	25
36) 1,1-Dichloropropene	5.556	75	12188	5.023	ug/l #	50
37) Ethyl Acetate	4.574	43	7766	2.604	ug/l #	67
38) Carbon Tetrachloride	5.562	117	16398	6.480	ug/l #	15
41) Methacrylonitrile	5.038	41	996	0.616	ug/l #	41
43) Isopropyl Acetate	6.348	43	19616	4.204	ug/l	93
48) Methyl methacrylate	7.806	41	112773	49.547	ug/l #	38
49) 1,4-Dioxane	7.799	88	158	3.285	ug/l #	1
51) 4-Methyl-2-Pentanone	8.555	43	78233	25.939	ug/l #	45
53) t-1,3-Dichloropropene	8.988	75	238	2.211	ug/l	100
54) cis-1,3-Dichloropropene	8.555	75	32801	11.285	ug/l #	67
56) Ethyl methacrylate	9.013	69	124	0.797	ug/l #	29
57) 1,3-Dichloropropane	9.482	76	19959	6.286	ug/l #	43
59) 2-Hexanone	9.488	43	297347	128.258	ug/l #	42
60) Dibromochloromethane	9.281	129	72	1.721	ug/l #	11
74) N-amyl acetate	10.768	43	789	0.210	ug/l #	38
76) 1,2,3-Trichloropropane	11.085	75	72205	28.356	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.457	105	4411	0.645	ug/l	92
81) trans-1,4-Dichloro-2-b...	11.085	75	72205	83.411	ug/l #	12
93) 1,2,4-Trichlorobenzene	13.591	180	507	0.234	ug/l	89
95) Naphthalene	13.780	128	1158	1.424	ug/l #	89
96) 1,2,3-Trichlorobenzene	13.969	180	524	0.243	ug/l	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX0090721\
Data File : VX024121.D
Acq On : 07 Sep 2021 16:29
Operator : JC/MD
Sample : PB138939TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Sep 08 13:27:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 11:57:51 2021
Response via : Initial Calibration




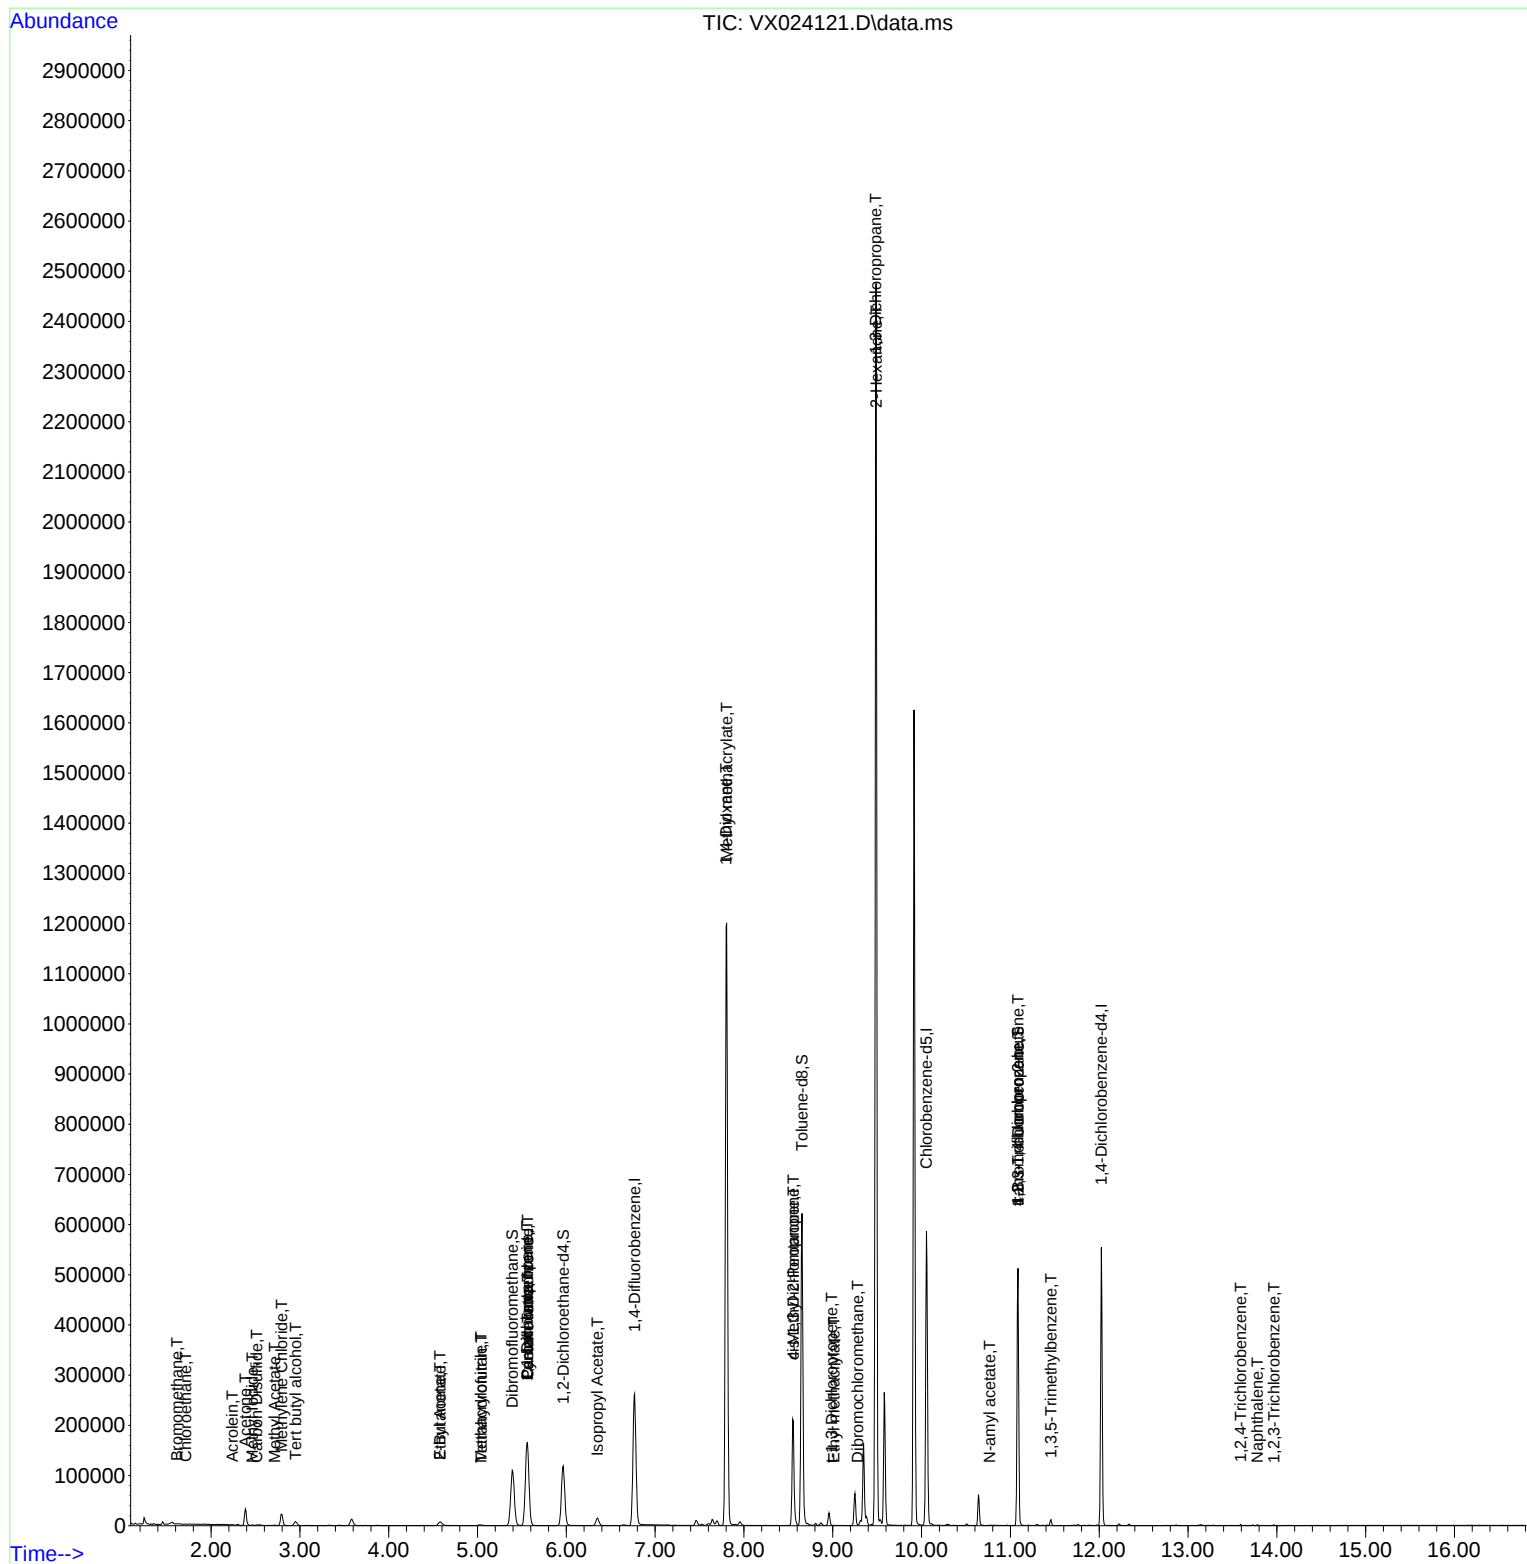




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:168 Resp: 156027
Ion Ratio Lower Upper
168 100
99 61.0 45.8 68.6

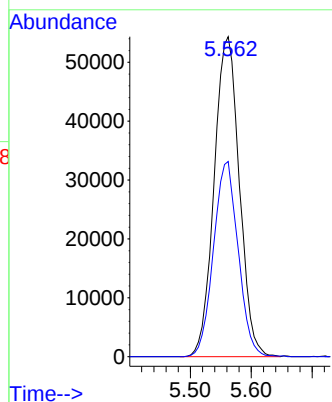


#5
Bromomethane
Concen: 0.709 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.019 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 94 Resp: 786
Ion Ratio Lower Upper
94 100
96 69.8 76.4 114.6#



Abundance Scan 97 (1.679 min): VX023756.D\data.ms (-90)


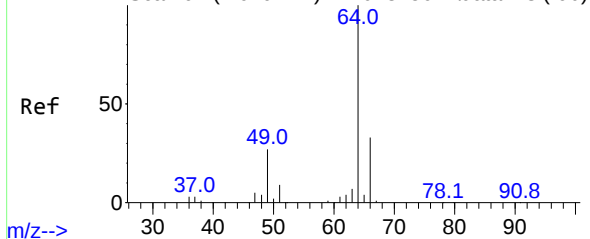


#6
Chloroethane
Concen: 2.299 ug/l
RT: 1.715 min Scan# 103
Delta R.T. 0.036 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29


Tgt Ion: 64 Resp: 126
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

Instrument :
MSVOA_X
ClientSampled :


Abundance Scan 103 (1.715 min): VX024121.D\data.ms

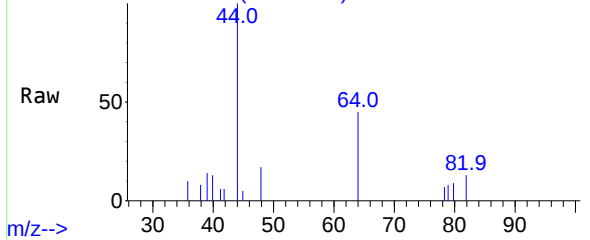

Abundance Scan 103 (1.715 min): VX024121.D\data.ms (-48)

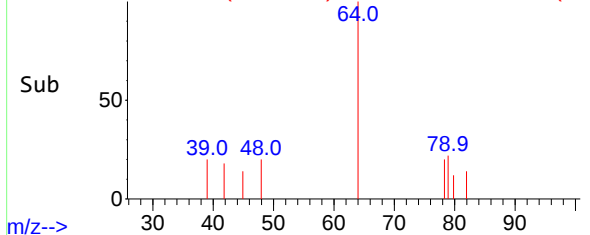



Abundance Scan 224 (2.453 min): VX023756.D\data.ms (-21)

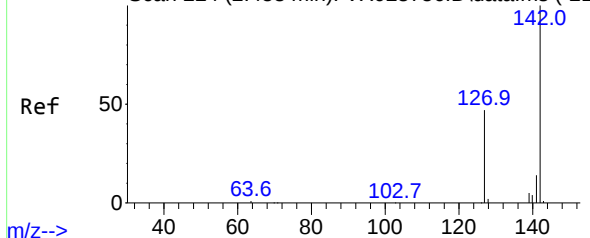


#10
Methyl Iodide
Concen: 0.663 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29


Tgt Ion: 142 Resp: 1446
Ion Ratio Lower Upper
142 100
127 51.1 33.3 49.9#
141 6.4 11.4 17.0#

Abundance Scan 226 (2.465 min): VX024121.D\data.ms

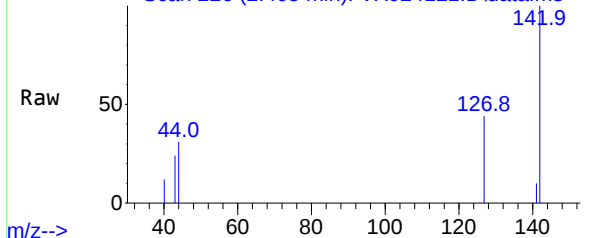

Abundance Scan 226 (2.465 min): VX024121.D\data.ms (-17)

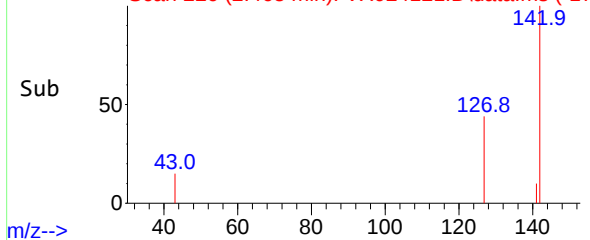







#11

Tert butyl alcohol
Concen: 12.046 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.030 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion: 59 Resp: 5305
Ion Ratio Lower Upper
59 100
57 0.5 7.8 11.8#




#13

Acrolein
Concen: 0.313 ug/l
RT: 2.239 min Scan# 189
Delta R.T. -0.006 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 56 Resp: 82
Ion Ratio Lower Upper
56 100
55 152.4 56.4 84.6#



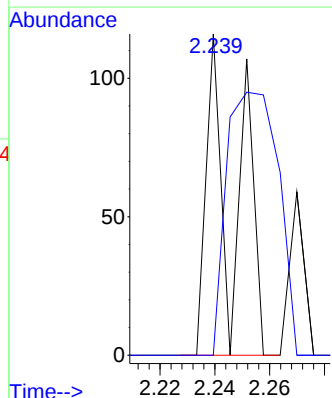





#16
Acetone
Concen: 35.786 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 34844
Ion Ratio Lower Upper
43 100
58 27.1 27.8 41.8#



#17
Carbon Disulfide
Concen: 0.394 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 76 Resp: 1408
Ion Ratio Lower Upper
76 100
78 6.2 7.2 10.8#


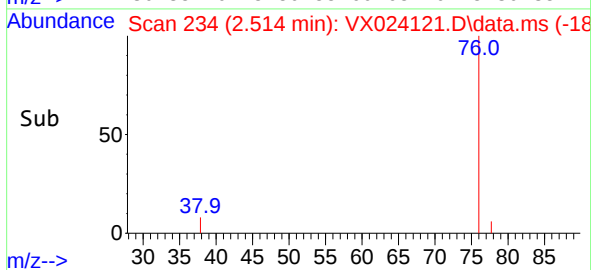






#18
Methyl Acetate
Concen: 0.412 ug/l
RT: 2.715 min Scan# 267
Delta R.T. -0.000 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 1002
Ion Ratio Lower Upper
43 100
74 22.4 21.9 32.9



#20
Methylene Chloride
Concen: 5.565 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 84 Resp: 10351
Ion Ratio Lower Upper
84 100
49 128.1 88.6 132.8
51 40.3 27.0 40.6
86 61.0 50.3 75.5



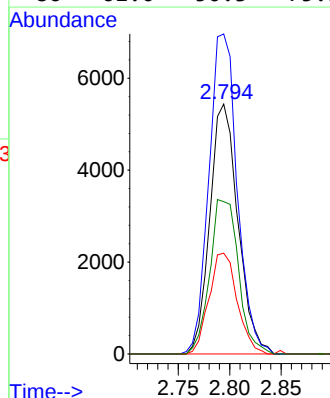





#25
2-Butanone
Concen: 5.266 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.006 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 7766
Ion Ratio Lower Upper
43 100
72 21.8 23.7 35.5#

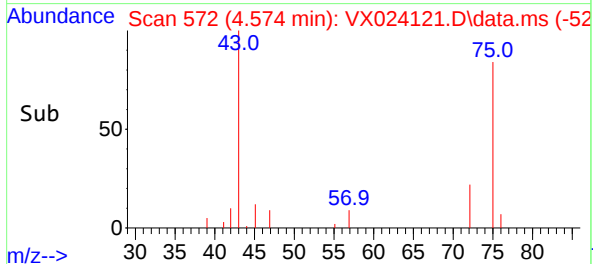

#29
Tetrahydrofuran
Concen: 1.538 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.025 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29


Tgt Ion: 42 Resp: 1469
Ion Ratio Lower Upper
42 100
72 37.4 41.7 62.5#
71 0.0 38.4 57.6#

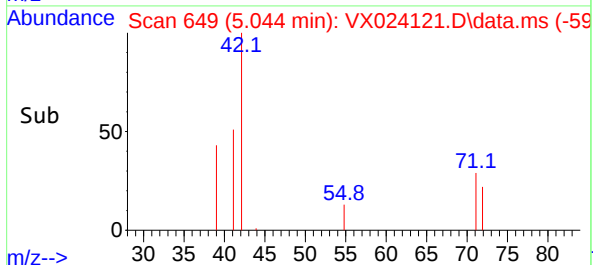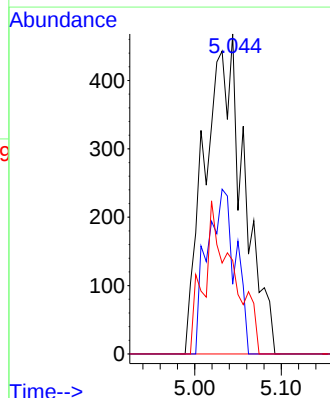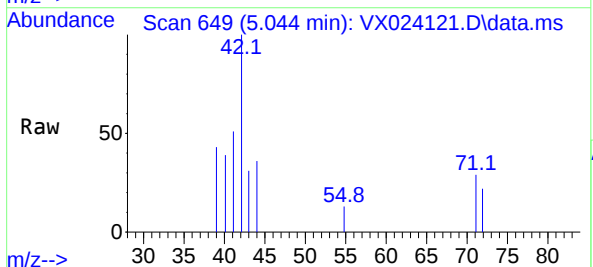






#31
Cyclohexane
Concen: 1.332 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.085 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29


Instrument :
MSVOA_X
ClientSampled :





Tgt Ion: 56 Resp: 3726
Ion Ratio Lower Upper
56 100
69 157.4 25.3 37.9#
84 108.8 71.4 107.0#




#33
1,2-Dichloroethane-d4
Concen: 55.826 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29



Tgt Ion: 65 Resp: 121569
Ion Ratio Lower Upper
65 100
67 49.5 0.0 105.4



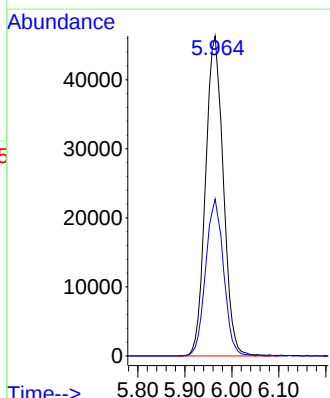





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:114 Resp: 262035
Ion Ratio Lower Upper
114 100
63 20.7 0.0 40.8
88 17.2 0.0 32.8



#35
Dibromofluoromethane
Concen: 53.845 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion:113 Resp: 93385
Ion Ratio Lower Upper
113 100
111 102.0 81.9 122.9
192 20.2 16.7 25.1


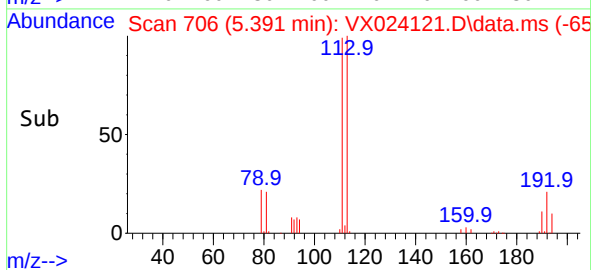






#36
1,1-Dichloropropene
Concen: 5.023 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.146 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 12188
Ion Ratio Lower Upper
75 100
110 10.4 18.1 54.4#
77 0.0 25.3 37.9#



#37
Ethyl Acetate
Concen: 2.604 ug/l
RT: 4.574 min Scan# 572
Delta R.T. -0.153 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29


Tgt Ion: 43 Resp: 7766
Ion Ratio Lower Upper
43 100
61 1.8 12.8 19.2#
70 0.0 10.5 15.7#

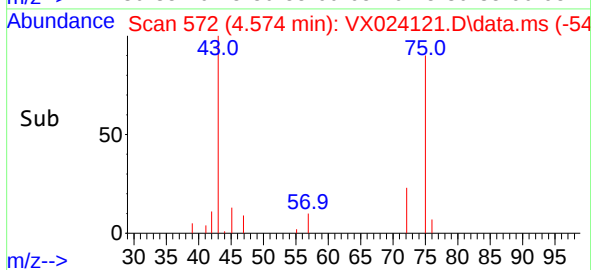



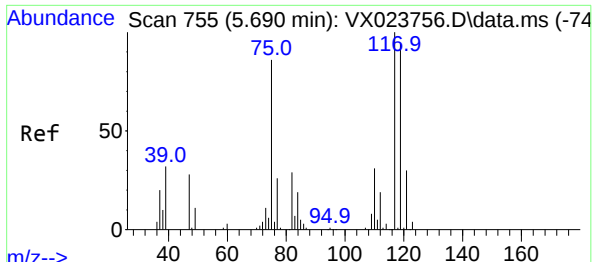


#38
Carbon Tetrachloride
Concen: 6.480 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29


Instrument :
MSVOA_X
ClientSampled :

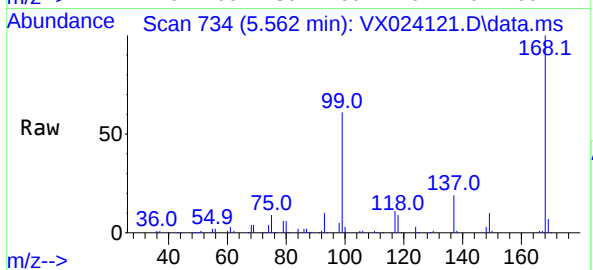



Tgt Ion:117 Resp: 16398
Ion Ratio Lower Upper
117 100
119 3.3 76.2 114.2#
121 0.0 24.8 37.2#

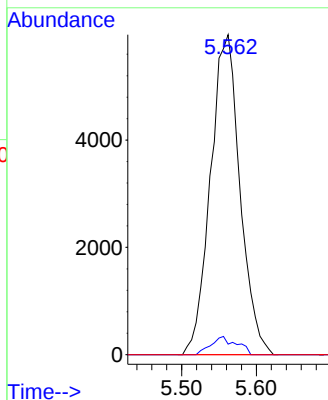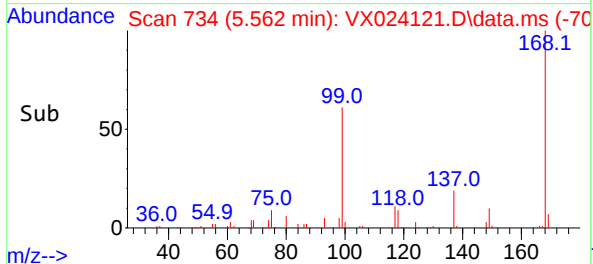


#41
Methacrylonitrile
Concen: 0.616 ug/l
RT: 5.038 min Scan# 648
Delta R.T. 0.104 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

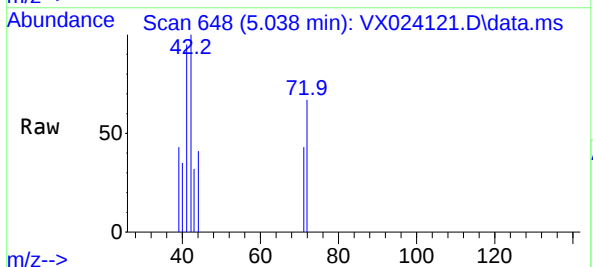

Tgt Ion: 41 Resp: 996
Ion Ratio Lower Upper
41 100
39 46.0 42.5 63.7
67 0.0 65.0 97.6#
52 0.0 25.3 37.9#



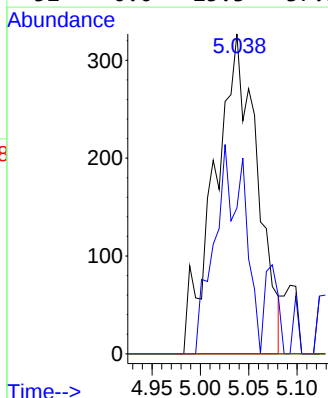
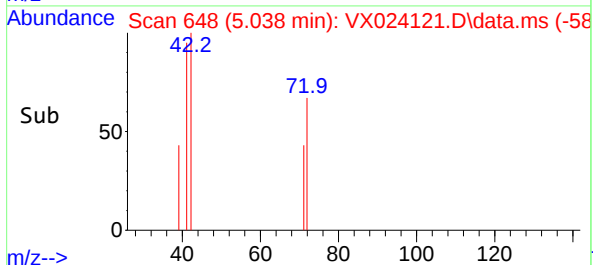




#43
Isopropyl Acetate
Concen: 4.204 ug/l
RT: 6.348 min Scan# 863
Delta R.T. -0.006 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 19616
Ion Ratio Lower Upper
43 100
61 19.2 18.2 27.4
87 13.2 12.5 18.7

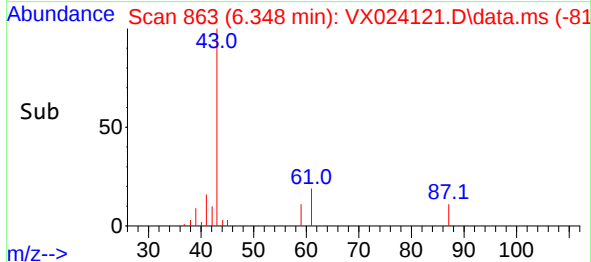

#48
Methyl methacrylate
Concen: 49.547 ug/l
RT: 7.806 min Scan# 1102
Delta R.T. 0.104 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 41 Resp: 112773
Ion Ratio Lower Upper
41 100
69 0.1 76.0 114.0#
39 55.1 44.6 67.0


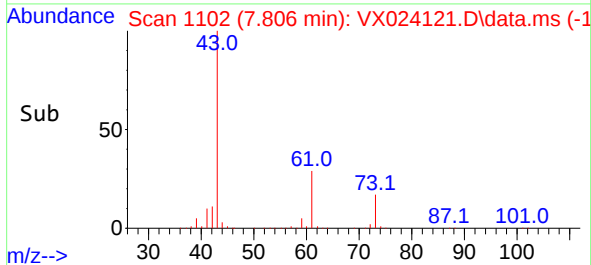

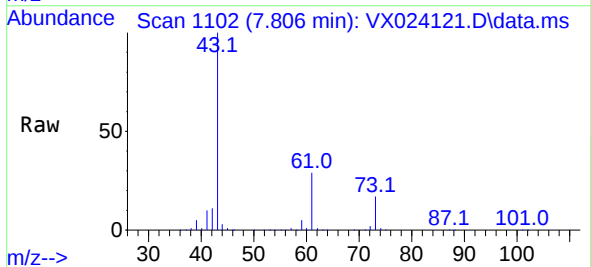


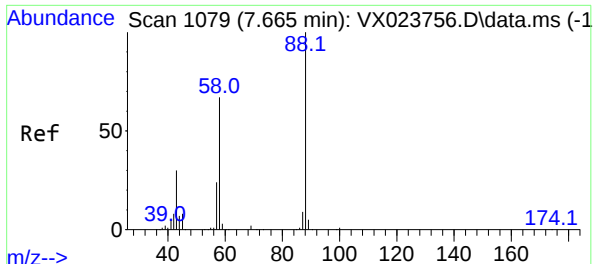

#49
1,4-Dioxane
Concen: 3.285 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.134 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 88 Resp: 158
Ion Ratio Lower Upper
88 100
43 708068.4 23.2 34.8#
58 2985.4 55.0 82.4#

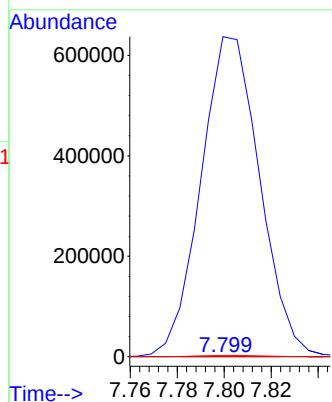

#50
Toluene-d8
Concen: 53.010 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 98 Resp: 349918
Ion Ratio Lower Upper
98 100
100 64.0 51.9 77.9


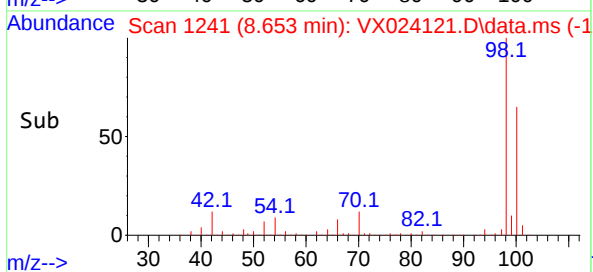
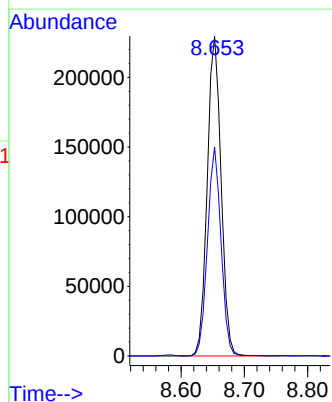
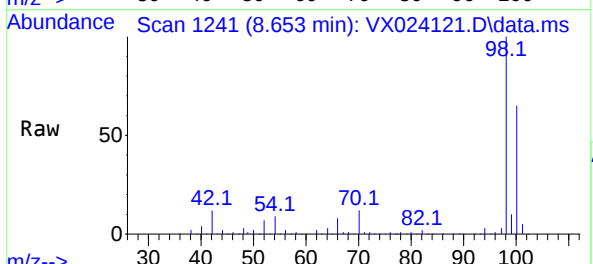


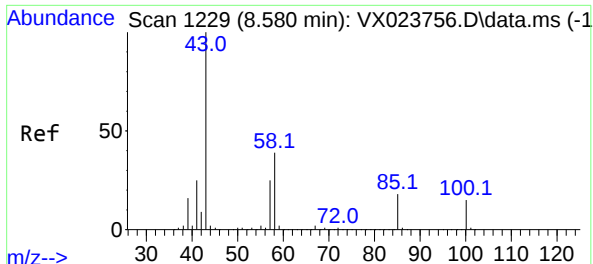

#51
4-Methyl-2-Pentanone
Concen: 25.939 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. -0.025 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 78233
Ion Ratio Lower Upper
43 100
58 8.5 35.4 53.0#

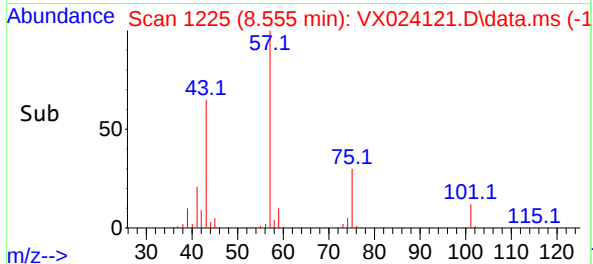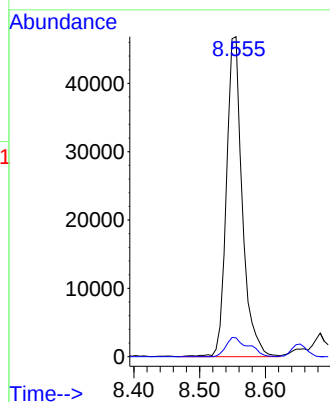

#53
t-1,3-Dichloropropene
Concen: 2.211 ug/l
RT: 8.988 min Scan# 1296
Delta R.T. 0.006 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 75 Resp: 238
Ion Ratio Lower Upper
75 100
77 31.1 24.9 37.3




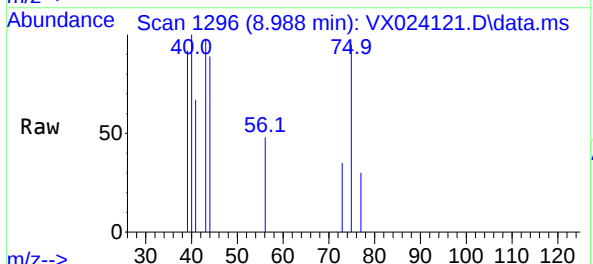




#54
cis-1,3-Dichloropropene
Concen: 11.285 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. 0.183 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 32801
Ion Ratio Lower Upper
75 100
77 0.3 25.7 38.5#
39 33.7 35.1 52.7#

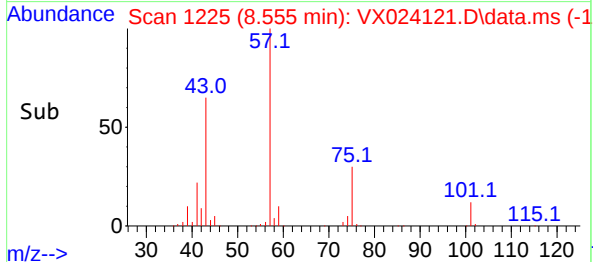

#56
Ethyl methacrylate
Concen: 0.797 ug/l
RT: 9.013 min Scan# 1300
Delta R.T. -0.109 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 69 Resp: 124
Ion Ratio Lower Upper
69 100
41 0.0 46.8 70.2#
39 0.0 24.7 37.1#


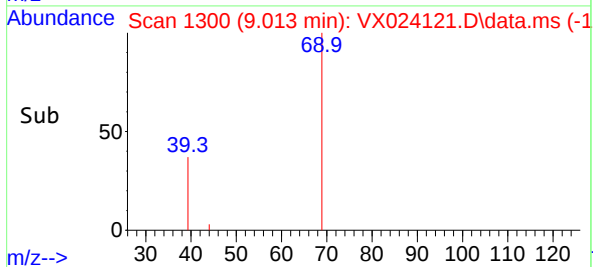

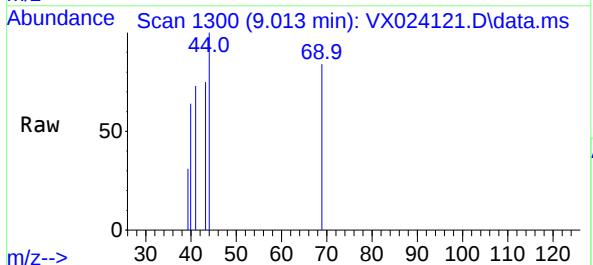




#57
1,3-Dichloropropane
Concen: 6.286 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.171 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 76 Resp: 19959
Ion Ratio Lower Upper
76 100
78 0.5 26.2 39.2#

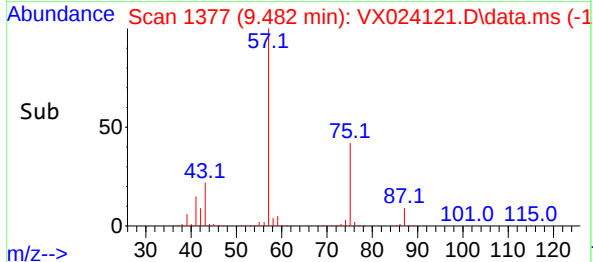

#59
2-Hexanone
Concen: 128.258 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.055 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 43 Resp: 297347
Ion Ratio Lower Upper
43 100
58 17.5 30.9 92.8#

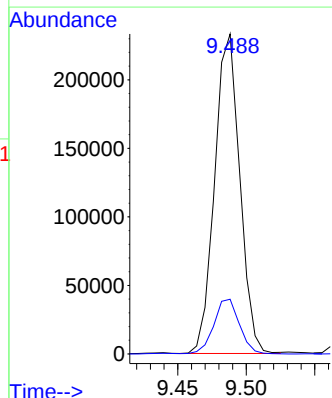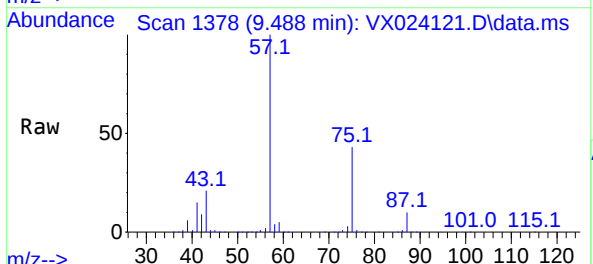



#60

Dibromochloromethane

Concen: 1.721 ug/l

RT: 9.281 min Scan# 1344

Delta R.T. -0.244 min

Lab File: VX024121.D





Acq: 07 Sep 2021 16:29

Tgt Ion:129 Resp: 72

Ion Ratio Lower Upper

129 100

127 0.0 38.4 115.2#

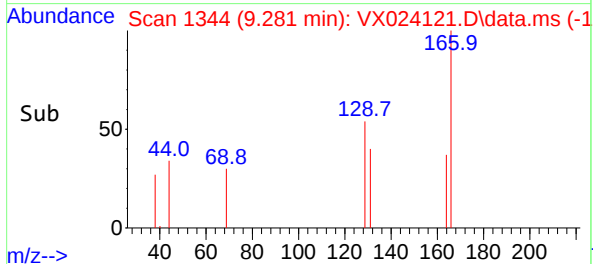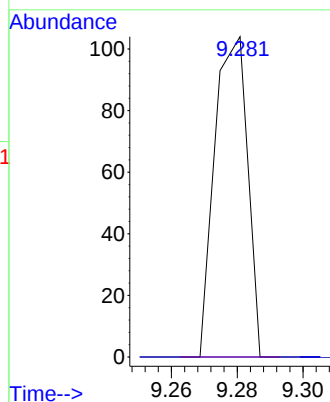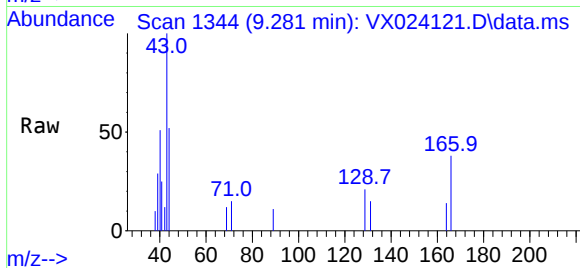

#62

4-Bromofluorobenzene

Concen: 53.469 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.000 min

Lab File: VX024121.D

Acq: 07 Sep 2021 16:29




Tgt Ion: 95 Resp: 129929


Ion Ratio Lower Upper

95 100

174 81.2 0.0 154.6

176 78.3 0.0 155.8


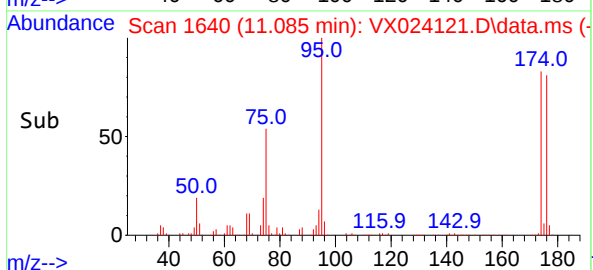

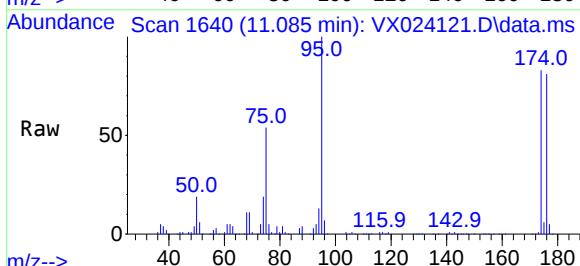




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:117 Resp: 255348
Ion Ratio Lower Upper
117 100
82 58.2 47.4 71.2
119 32.7 26.6 39.8

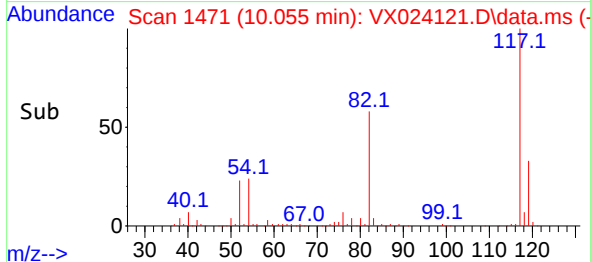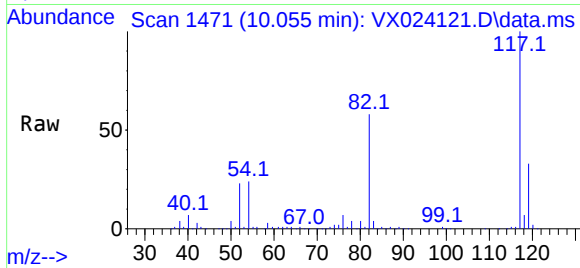

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29


Tgt Ion:152 Resp: 109157
Ion Ratio Lower Upper
152 100
115 61.1 41.1 123.3
150 156.8 0.0 349.0

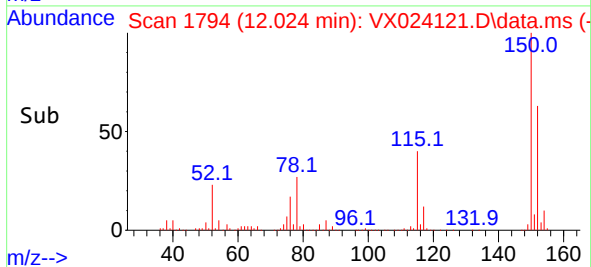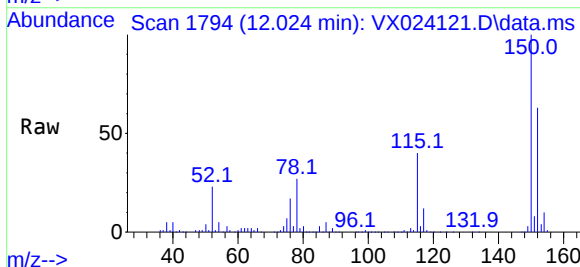






#74
N-amy1 acetate
Concen: 0.210 ug/l
RT: 10.768 min Scan# 1588
Delta R.T. -0.080 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Instrument :
MSVOA_X
ClientSampled :



Tgt Ion: 43 Resp: 789




Ion	Ratio	Lower	Upper
43	100		
70	0.0	39.0	58.6#
55	0.0	21.5	32.3#
61	0.0	22.1	33.1#

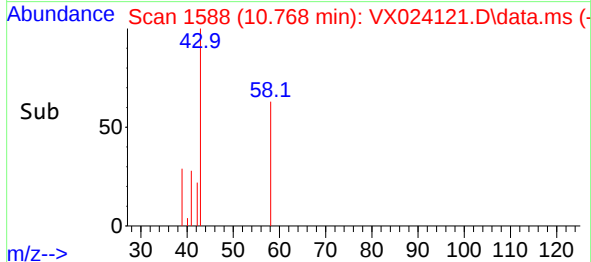


#76
1,2,3-Trichloropropane
Concen: 28.356 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 75 Resp: 72205


Ion	Ratio	Lower	Upper
75	100		
77	1.2	19.1	57.5#

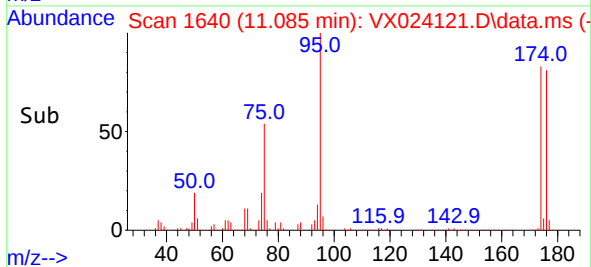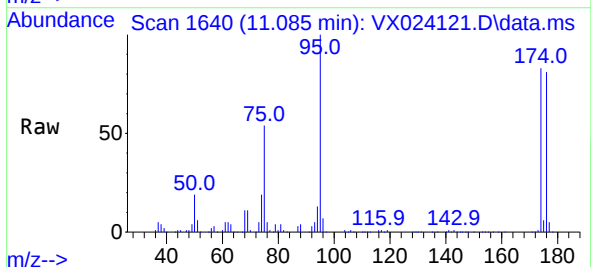


Abundance Scan 1700 (11.451 min): VX023756.D\data.ms (-

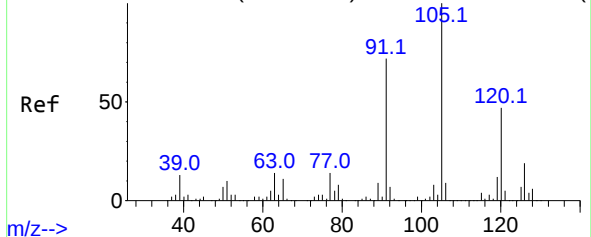


m/z--> Abundance Scan 1701 (11.457 min): VX024121.D\data.ms (-

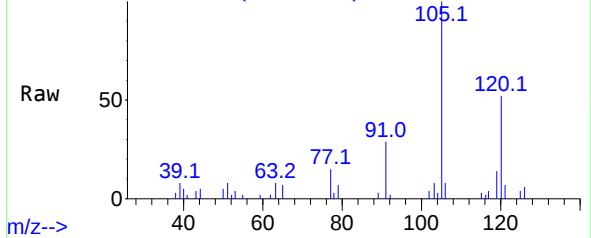


m/z--> Abundance Scan 1701 (11.457 min): VX024121.D\data.ms (-

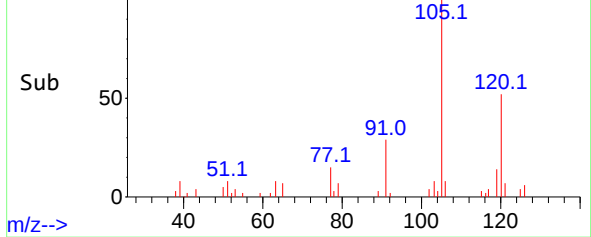


m/z--> Abundance Scan 1630 (11.024 min): VX023756.D\data.ms (-

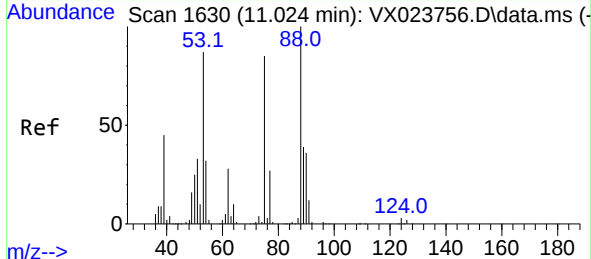

m/z--> Abundance Scan 1640 (11.085 min): VX024121.D\data.ms (-

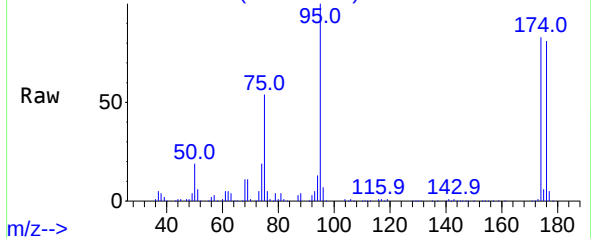

m/z--> Abundance Scan 1640 (11.085 min): VX024121.D\data.ms (-

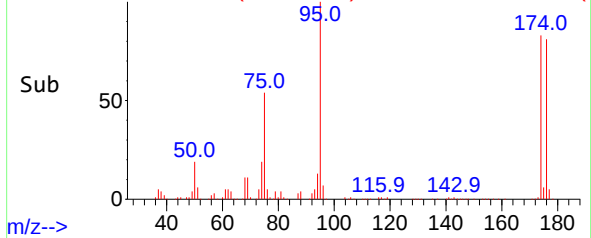

m/z--> Abundance Scan 1640 (11.085 min): VX024121.D\data.ms (-




m/z--> Abundance Scan 1640 (11.085 min): VX024121.D\data.ms (-



m/z--> Abundance Scan 1640 (11.085 min): VX024121.D\data.ms (-




m/z--> Abundance Scan 1640 (11.085 min): VX024121.D\data.ms (-



m/z--> Abundance Scan 1640 (11.085 min): VX024121.D\data.ms (-


#80
1,3,5-Trimethylbenzene
Concen: 0.645 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion:105 Resp: 4411
Ion Ratio Lower Upper
105 100
120 53.0 23.8 71.5

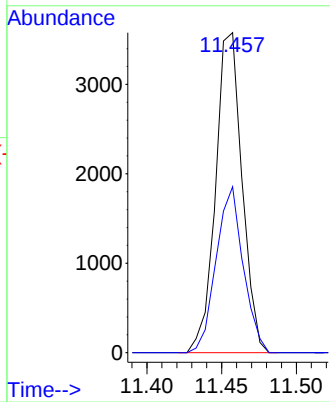


#81
trans-1,4-Dichloro-2-butene
Concen: 83.411 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion: 75 Resp: 72205
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.1 37.9 56.9#







Instrument :
MSVOA_X
ClientSampled :



#93
1,2,4-Trichlorobenzene
Concen: 0.234 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.000 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:180 Resp: 507
Ion Ratio Lower Upper
180 100
182 104.5 47.7 143.1
145 20.3 15.0 45.0

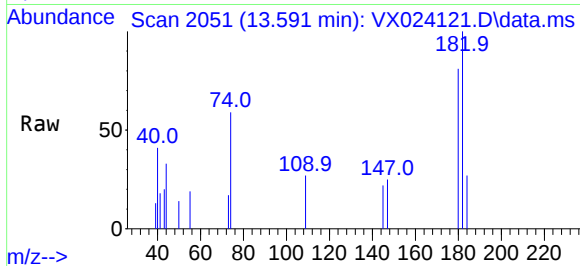

#95
Naphthalene
Concen: 1.424 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Tgt Ion:128 Resp: 1158
Ion Ratio Lower Upper
128 100
127 9.4 10.3 15.5#
129 5.6 8.8 13.2#

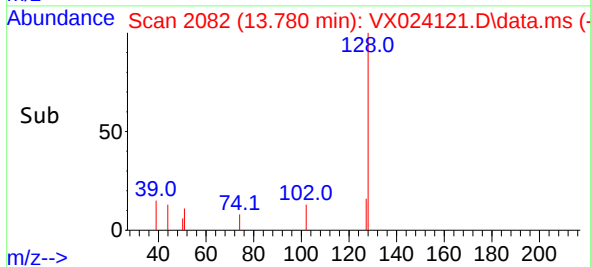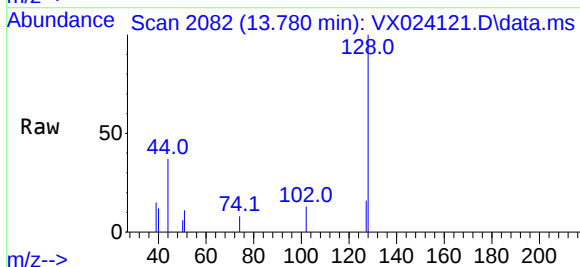



#96
1,2,3-Trichlorobenzene
Concen: 0.243 ug/l
RT: 13.969 min Scan# 2113
Delta R.T. 0.006 min
Lab File: VX024121.D
Acq: 07 Sep 2021 16:29

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:180 Resp: 524
Ion Ratio Lower Upper
180 100
182 76.5 47.6 142.9
145 26.3 16.1 48.3

