

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090722\  
 Data File : VX031157.D  
 Acq On : 07 Sep 2022 13:48  
 Operator : JC/MD  
 Sample : IBLK  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK

Quant Time: Sep 07 23:24:26 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X090722W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Sep 07 23:22:41 2022  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc      | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|-----------|--------|----------|
| -----                         |                |      |            |           |        |          |
| Internal Standards            |                |      |            |           |        |          |
| 1) Pentafluorobenzene         | 5.556          | 168  | 85829      | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.763          | 114  | 148015     | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 10.055         | 117  | 127967     | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024         | 152  | 56814      | 50.000    | ug/l   | 0.00     |
|                               |                |      |            |           |        |          |
| System Monitoring Compounds   |                |      |            |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 5.958          | 65   | 62040      | 30.531    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = | 61.060%#  |        |          |
| 35) Dibromofluoromethane      | 5.391          | 113  | 47626      | 29.527    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = | 59.060%#  |        |          |
| 50) Toluene-d8                | 8.653          | 98   | 172516     | 29.438    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = | 58.880%#  |        |          |
| 62) 4-Bromofluorobenzene      | 11.079         | 95   | 65647      | 30.568    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = | 61.140%#  |        |          |
|                               |                |      |            |           |        |          |
| Target Compounds              |                |      |            |           | Qvalue |          |
| 5) Bromomethane               | 1.617          | 94   | 204        | 0.255     | ug/l # | 77       |
| 10) Methyl Iodide             | 2.453          | 142  | 627        | 0.329     | ug/l # | 80       |
| 11) Tert butyl alcohol        | 2.946          | 59   | 1837       | Below Cal | #      | 74       |
| 15) Acrylonitrile             | 3.075          | 53   | 358        | 0.463     | ug/l # | 67       |
| 16) Acetone                   | 2.392          | 43   | 340        | 0.483     | ug/l # | 40       |
| 17) Carbon Disulfide          | 2.514          | 76   | 2237       | 0.628     | ug/l # | 89       |
| 21) trans-1,2-Dichloroethene  | 3.093          | 96   | 534        | 0.333     | ug/l # | 39       |
| 25) 2-Butanone                | 4.586          | 43   | 294        | 0.282     | ug/l # | 48       |
| 38) Carbon Tetrachloride      | 5.550          | 117  | 9440       | 3.714     | ug/l # | 18       |
| 68) m/p-Xylenes               | 10.305         | 106  | 913        | 0.361     | ug/l   | 75       |
| 76) 1,2,3-Trichloropropane    | 11.079         | 75   | 37719      | 24.326    | ug/l # | 37       |
| 77) Bromobenzene              | 11.201         | 156  | 234        | 0.218     | ug/l   | 76       |
| 78) n-propylbenzene           | 11.305         | 91   | 1412       | 0.251     | ug/l   | 92       |
| 79) 2-Chlorotoluene           | 11.366         | 91   | 752        | 0.216     | ug/l   | 77       |
| 81) trans-1,4-Dichloro-2-b... | 11.079         | 75   | 37719      | 78.450    | ug/l # | 12       |
| 82) 4-Chlorotoluene           | 11.457         | 91   | 1342       | 0.333     | ug/l   | 98       |
| 85) sec-Butylbenzene          | 11.896         | 105  | 1224       | 0.242     | ug/l   | 93       |
| 86) p-Isopropyltoluene        | 12.006         | 119  | 820        | 0.200     | ug/l # | 48       |
| 87) 1,3-Dichlorobenzene       | 11.969         | 146  | 718        | 0.360     | ug/l # | 84       |
| 88) 1,4-Dichlorobenzene       | 12.036         | 146  | 1031       | 0.503     | ug/l # | 24       |
| 89) n-Butylbenzene            | 12.335         | 91   | 1221       | 0.346     | ug/l   | 94       |
| 91) 1,2-Dichlorobenzene       | 12.341         | 146  | 600        | 0.307     | ug/l   | 81       |
| 93) 1,2,4-Trichlorobenzene    | 13.585         | 180  | 748        | 0.655     | ug/l   | 81       |
| 94) Hexachlorobutadiene       | 13.725         | 225  | 408        | 0.841     | ug/l   | 97       |
| 95) Naphthalene               | 13.780         | 128  | 2456       | 0.549     | ug/l # | 92       |
| 96) 1,2,3-Trichlorobenzene    | 13.963         | 180  | 589        | 0.506     | ug/l   | 79       |
| -----                         |                |      |            |           |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090722\  
Data File : VX031157.D  
Acq On : 07 Sep 2022 13:48  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Quant Time: Sep 07 23:24:26 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X090722W.M  
Quant Title : SW846 8260  
QLast Update : Wed Sep 07 23:22:41 2022  
Response via : Initial Calibration




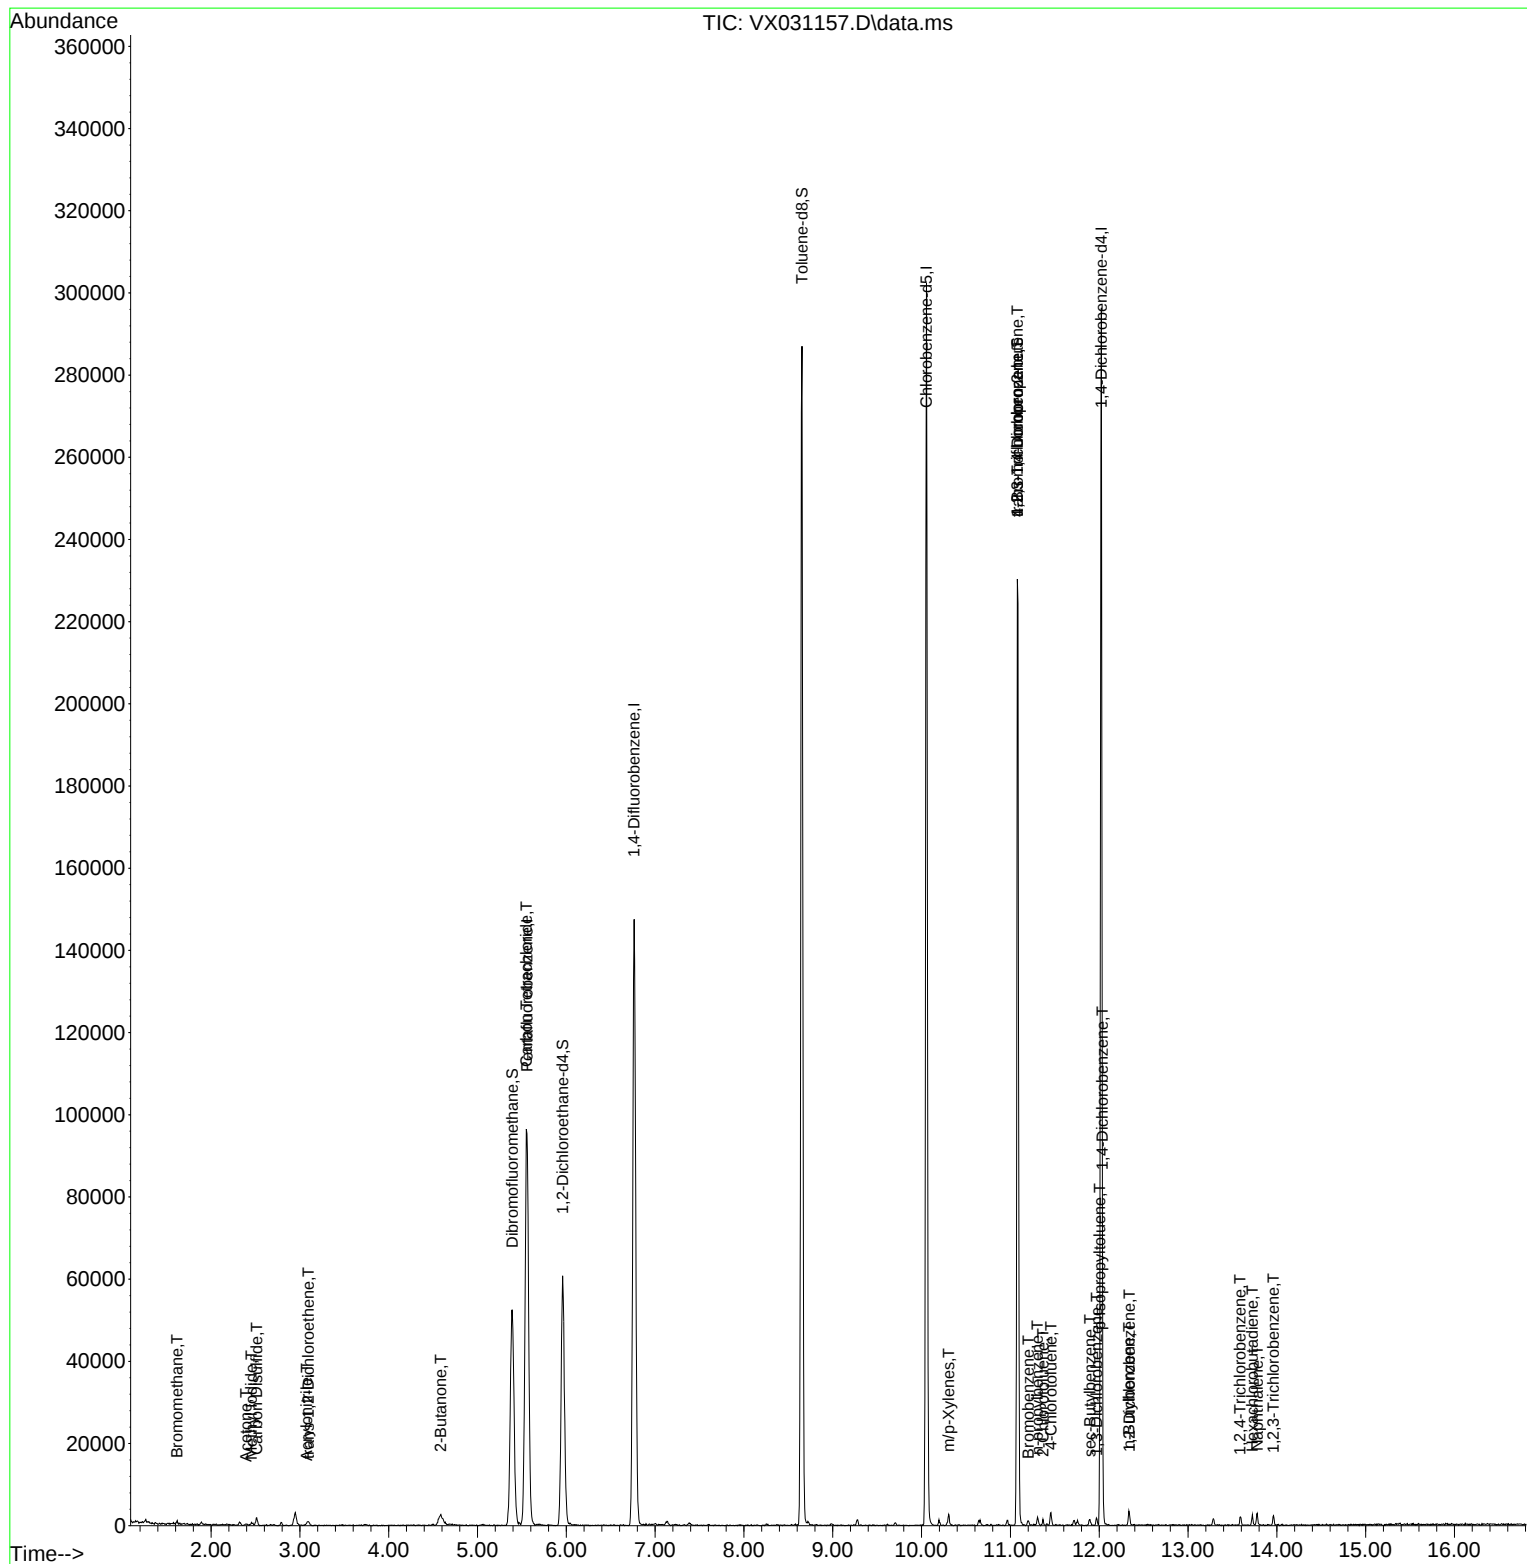




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.556 min Scan# 71  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion:168 Resp: 85829  
Ion Ratio Lower Upper  
168 100  
99 65.3 44.0 66.0

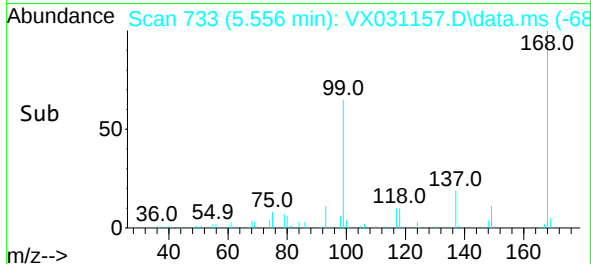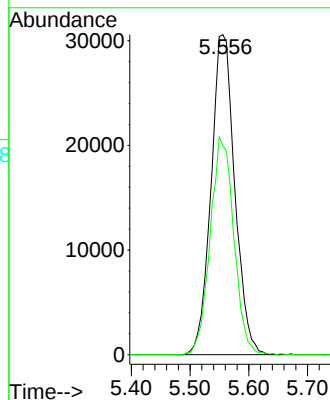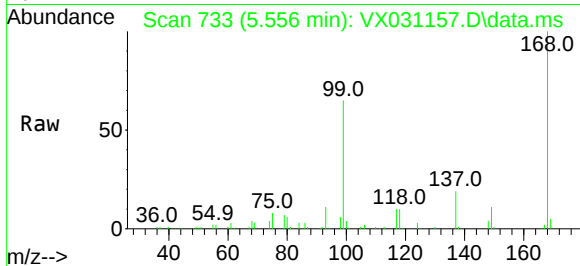

#5  
Bromomethane  
Concen: 0.255 ug/l  
RT: 1.617 min Scan# 87  
Delta R.T. 0.006 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48


Tgt Ion: 94 Resp: 204  
Ion Ratio Lower Upper  
94 100  
96 118.5 76.9 115.3#

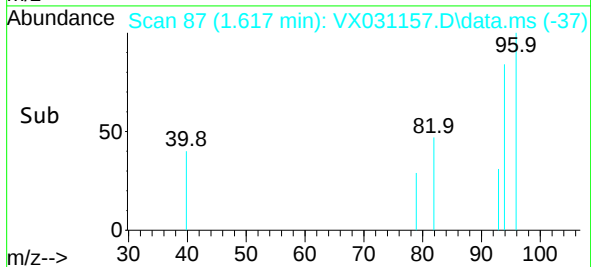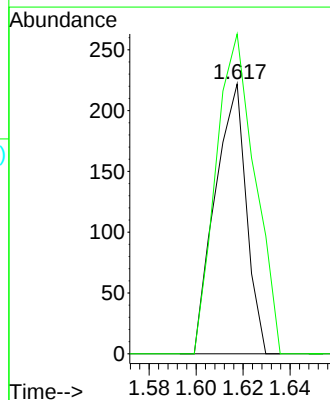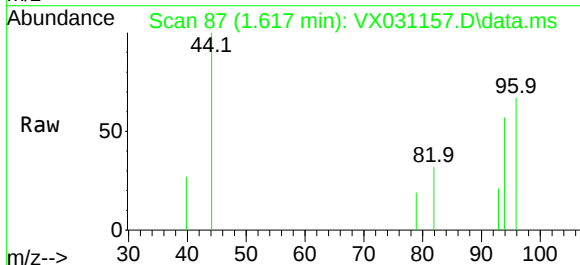



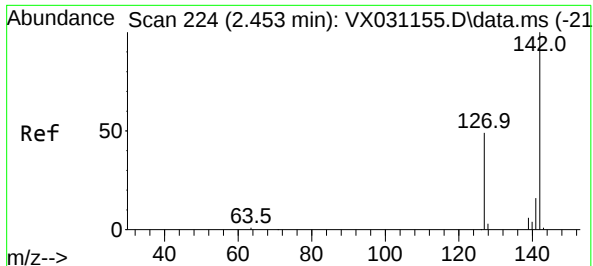


#10  
Methyl Iodide  
Concen: 0.329 ug/l  
RT: 2.453 min Scan# 21  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48


Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

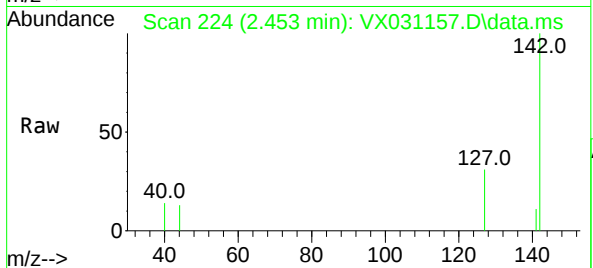



Tgt Ion:142 Resp: 627  
Ion Ratio Lower Upper  
142 100  
127 50.2 30.2 45.2#  
141 7.0 11.3 16.9#

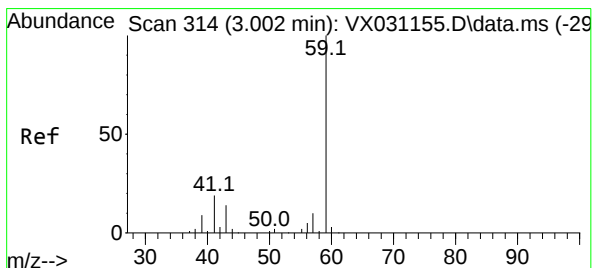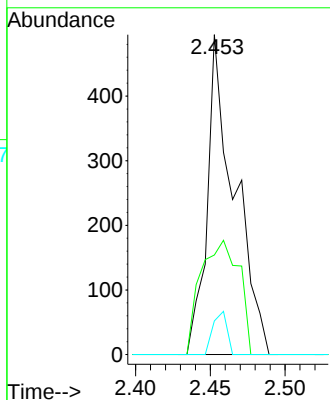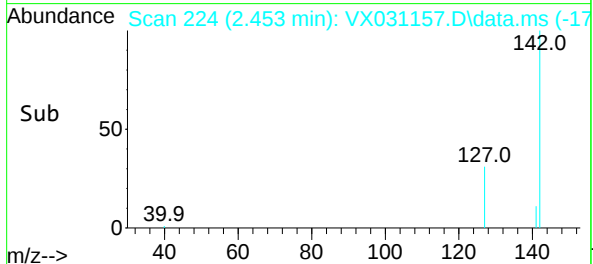


#11  
Tert butyl alcohol  
Concen: Below Cal  
RT: 2.946 min Scan# 305  
Delta R.T. -0.055 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48

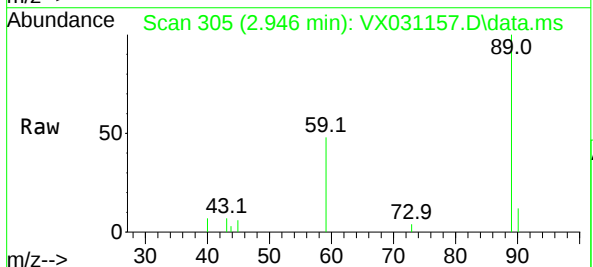

Tgt Ion: 59 Resp: 1837  
Ion Ratio Lower Upper  
59 100  
57 0.0 7.4 11.2#

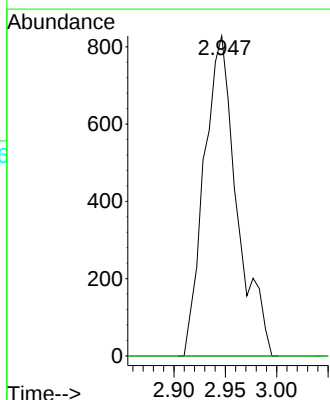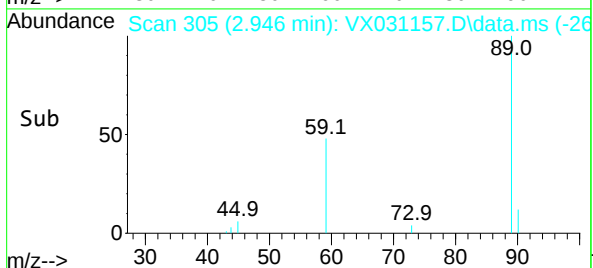



#15

Acrylonitrile

Concen: 0.463 ug/l

RT: 3.075 min Scan# 31

Delta R.T. 0.006 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48

Instrument :

MSVOA\_X

ClientSampleId :

IBLK





Tgt Ion: 53 Resp: 358

Ion Ratio Lower Upper

53 100

52 62.0 65.4 98.0#

51 0.0 27.7 41.5#

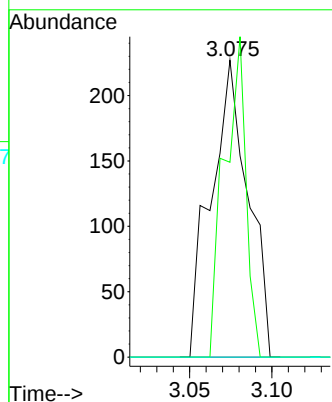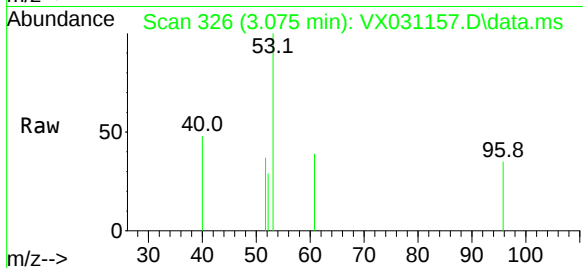

#16

Acetone

Concen: 0.483 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX031157.D




Acq: 07 Sep 2022 13:48


Tgt Ion: 43 Resp: 340

Ion Ratio Lower Upper

43 100

58 0.0 27.7 41.5#

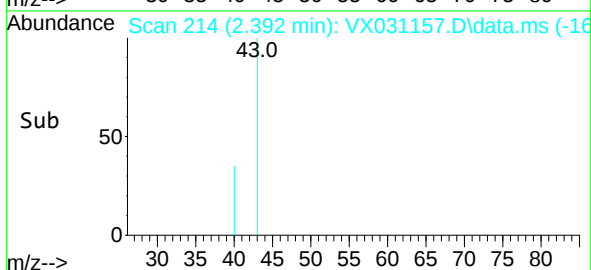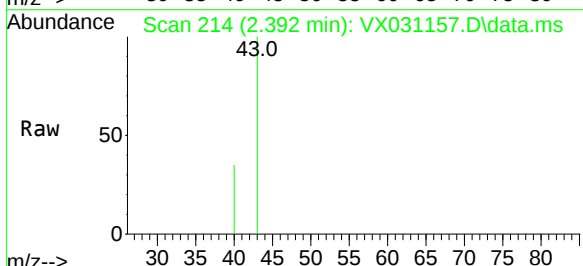

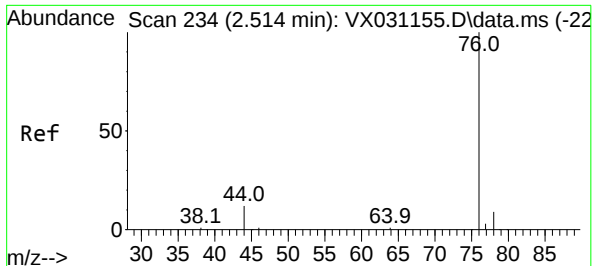

#17

Carbon Disulfide

Concen: 0.628 ug/l

RT: 2.514 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48

Instrument :

MSVOA\_X

ClientSampleId :





IBLK

Tgt Ion: 76 Resp: 2237

Ion Ratio Lower Upper

76 100

78 5.5 7.8 11.6#

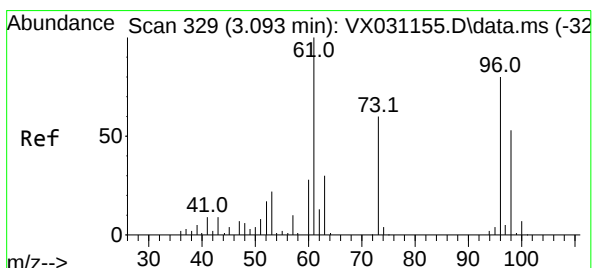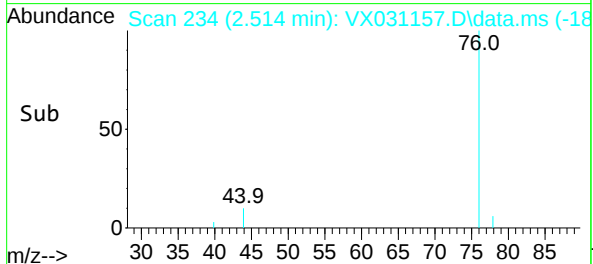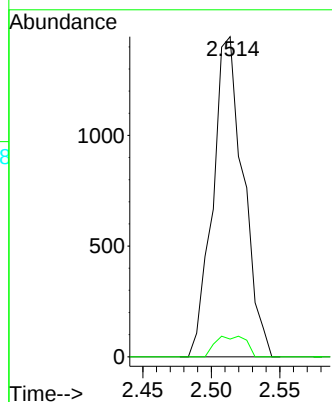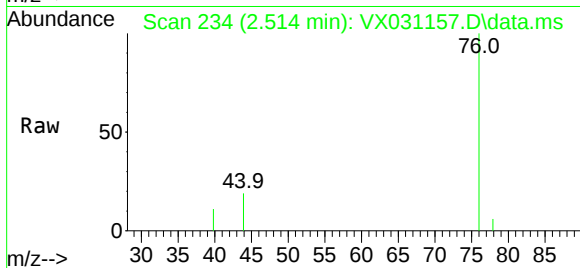

#21

trans-1,2-Dichloroethene

Concen: 0.333 ug/l

RT: 3.093 min Scan# 329

Delta R.T. -0.000 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48




Tgt Ion: 96 Resp: 534


Ion Ratio Lower Upper

96 100

61 49.7 105.6 158.4#

98 30.7 50.1 75.1#


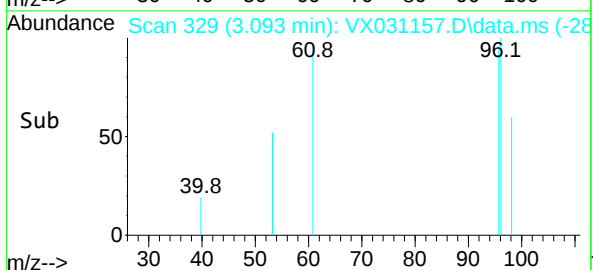

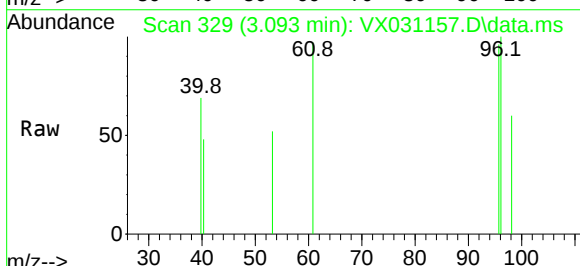




#25  
2-Butanone  
Concen: 0.282 ug/l  
RT: 4.586 min Scan# 51  
Delta R.T. 0.018 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 43 Resp: 294  
Ion Ratio Lower Upper  
43 100  
72 0.0 21.7 32.5#

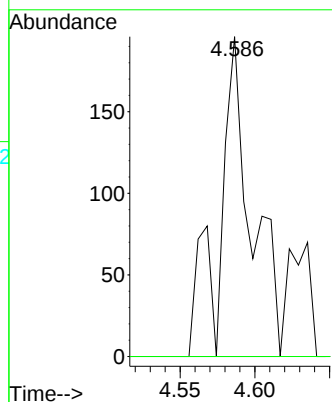

#33  
1,2-Dichloroethane-d4  
Concen: 30.531 ug/l  
RT: 5.958 min Scan# 799  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48

Tgt Ion: 65 Resp: 62040  
Ion Ratio Lower Upper  
65 100  
67 49.7 0.0 109.6


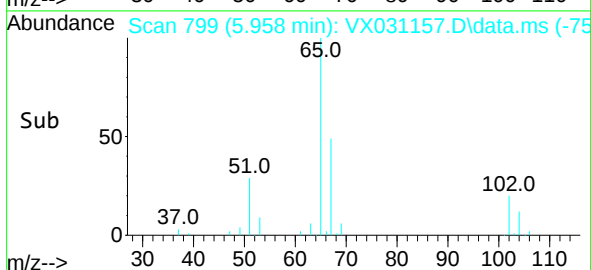




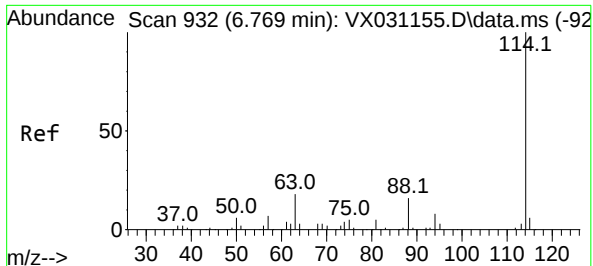

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.763 min Scan# 911  
Delta R.T. -0.006 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion:114 Resp: 148015  
Ion Ratio Lower Upper  
114 100  
63 20.3 0.0 38.4  
88 16.8 0.0 31.8

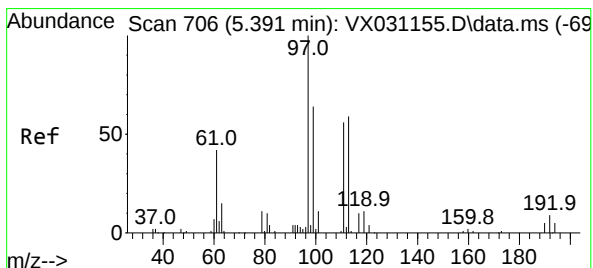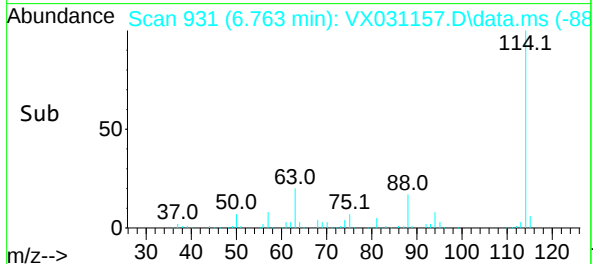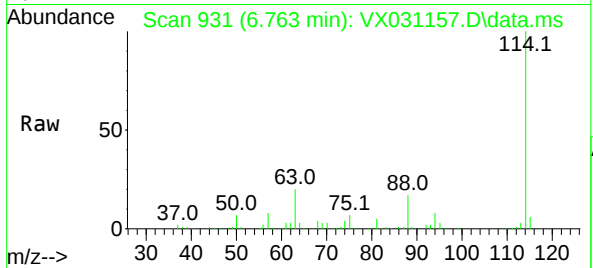

#35  
Dibromofluoromethane  
Concen: 29.527 ug/l  
RT: 5.391 min Scan# 706  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48


Tgt Ion:113 Resp: 47626  
Ion Ratio Lower Upper  
113 100  
111 103.6 83.2 124.8  
192 16.9 14.8 22.2

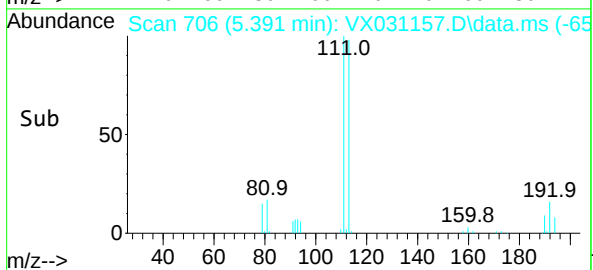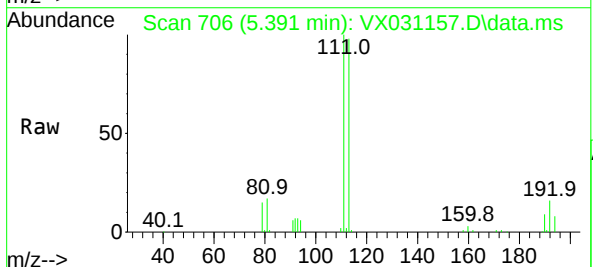



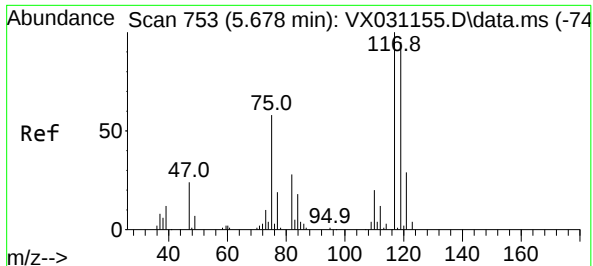


#38  
Carbon Tetrachloride  
Concen: 3.714 ug/l  
RT: 5.550 min Scan# 71  
Delta R.T. -0.128 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK



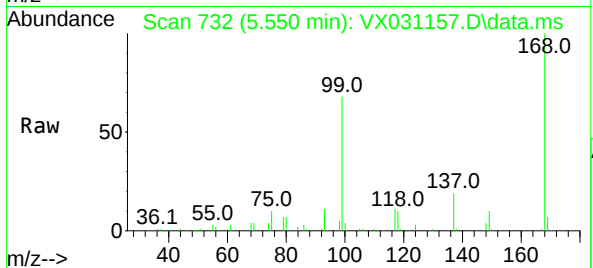



Tgt Ion:117 Resp: 9440  
Ion Ratio Lower Upper  
117 100  
119 5.5 74.1 111.1#  
121 0.0 25.8 38.8#

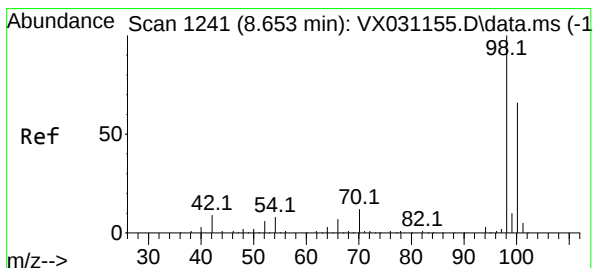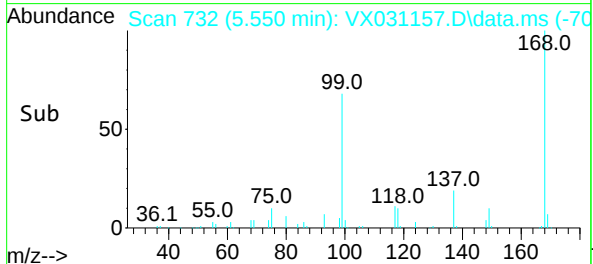

#50  
Toluene-d8  
Concen: 29.438 ug/l  
RT: 8.653 min Scan# 1241  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48

Tgt Ion: 98 Resp: 172516  
Ion Ratio Lower Upper  
98 100  
100 63.8 52.3 78.5

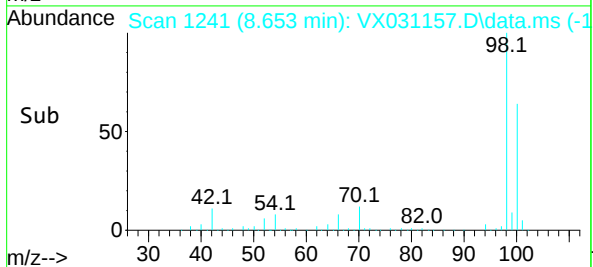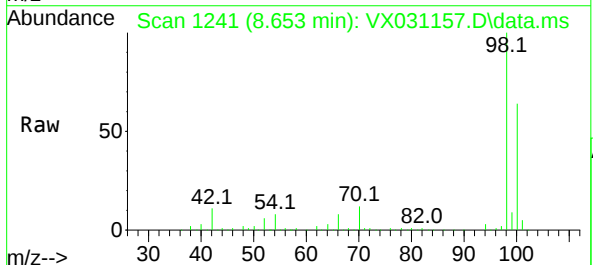



#62

4-Bromofluorobenzene

Concen: 30.568 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48

Instrument :

MSVOA\_X

ClientSampleId :

IBLK





Tgt Ion: 95 Resp: 65647

Ion Ratio Lower Upper

95 100

174 64.7 0.0 149.0

176 62.8 0.0 146.0

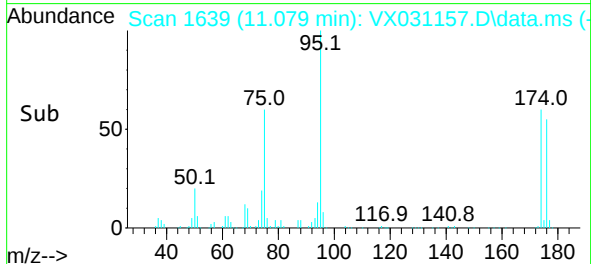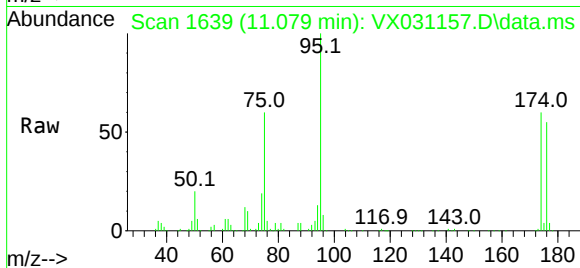

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48




Tgt Ion: 117 Resp: 127967


Ion Ratio Lower Upper

117 100

82 61.5 42.7 64.1

119 31.5 25.4 38.2


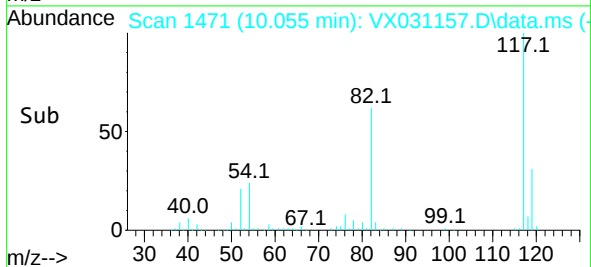

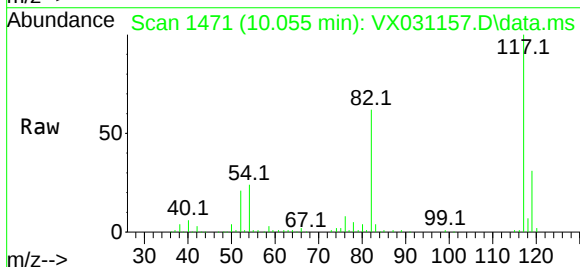




#68  
m/p-Xylenes  
Concen: 0.361 ug/l  
RT: 10.305 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion:106 Resp: 913  
Ion Ratio Lower Upper  
106 100  
91 159.6 158.2 237.4

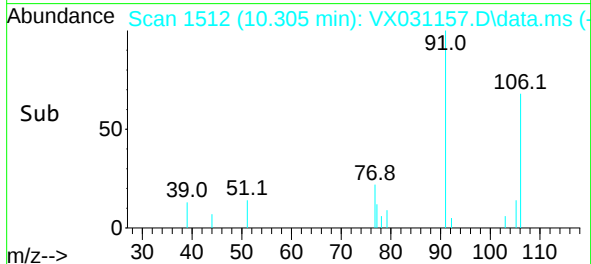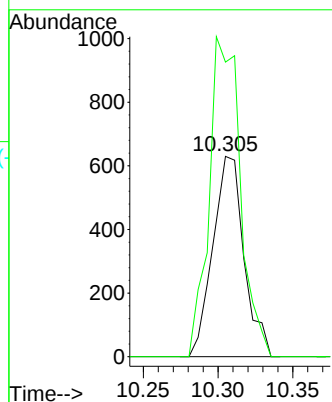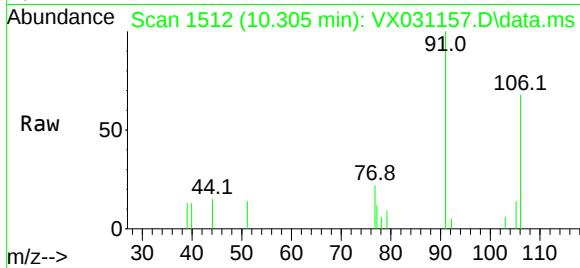

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 1794  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48

Tgt Ion:152 Resp: 56814  
Ion Ratio Lower Upper  
152 100  
115 66.4 40.5 121.5  
150 152.0 0.0 347.0

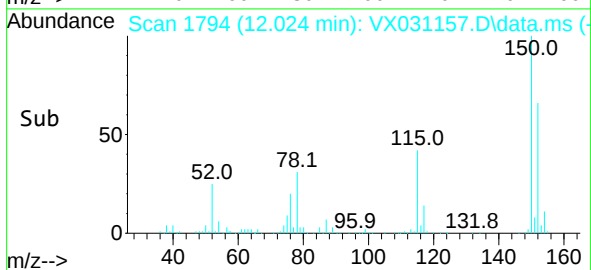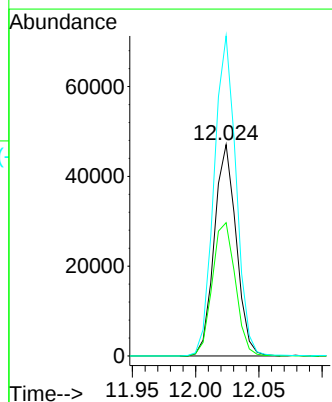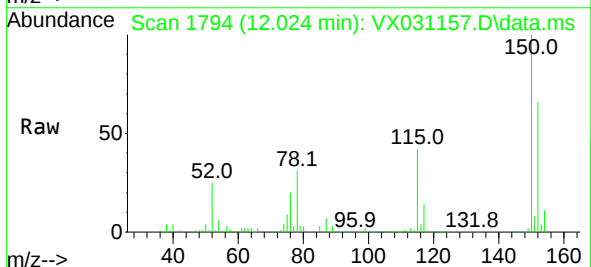



#76

1,2,3-Trichloropropane

Concen: 24.326 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48

Instrument :

MSVOA\_X

ClientSampleId :





IBLK

Tgt Ion: 75 Resp: 37719

Ion Ratio Lower Upper

75 100

77 1.1 19.8 59.3#

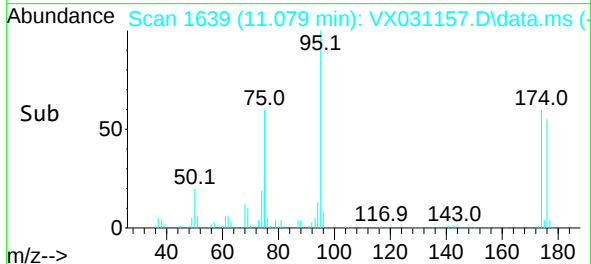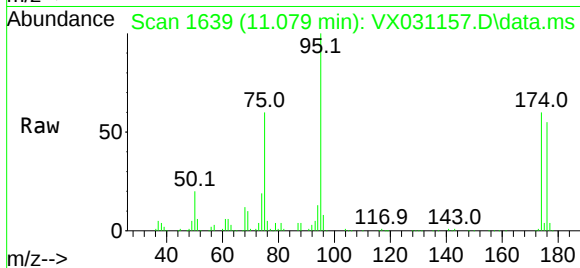

#77

Bromobenzene

Concen: 0.218 ug/l

RT: 11.201 min Scan# 1659

Delta R.T. -0.000 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48




Tgt Ion: 156 Resp: 234


Ion Ratio Lower Upper

156 100

77 209.8 82.7 247.9

158 103.0 47.5 142.5

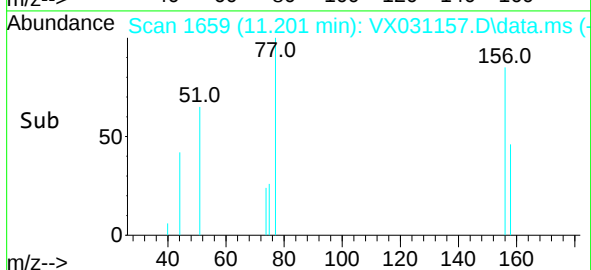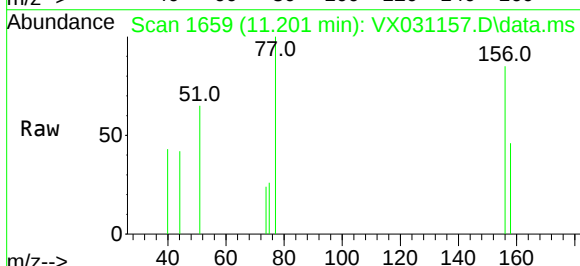



#78

n-propylbenzene

Concen: 0.251 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48

Instrument :

MSVOA\_X

ClientSampleId :





IBLK

Tgt Ion: 91 Resp: 1412

Ion Ratio Lower Upper

91 100

120 19.3 11.6 34.8

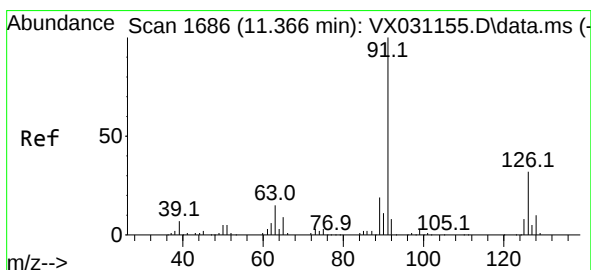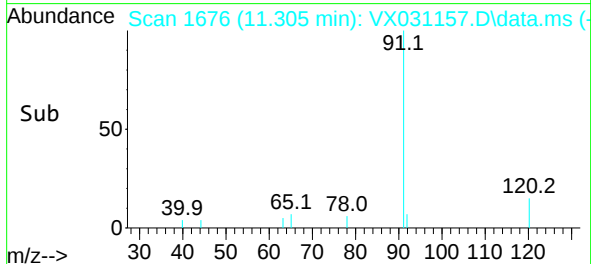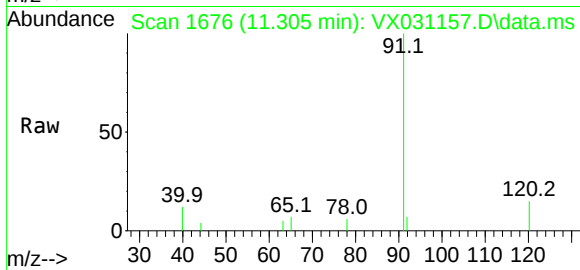

#79

2-Chlorotoluene

Concen: 0.216 ug/l

RT: 11.366 min Scan# 1686

Delta R.T. -0.000 min

Lab File: VX031157.D




Acq: 07 Sep 2022 13:48


Tgt Ion: 91 Resp: 752

Ion Ratio Lower Upper

91 100

126 21.8 17.4 52.3


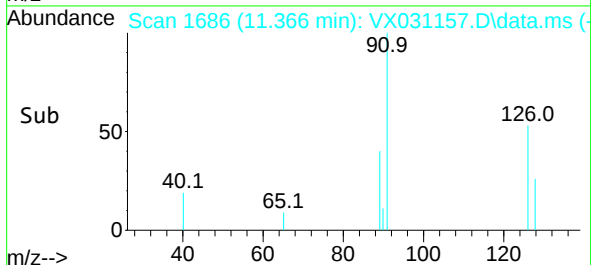

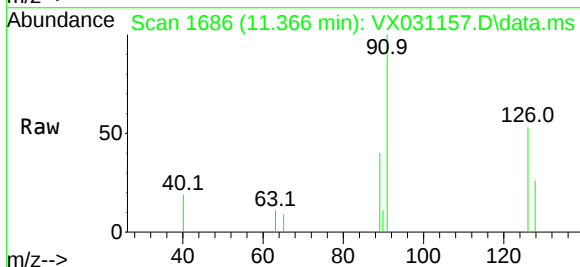


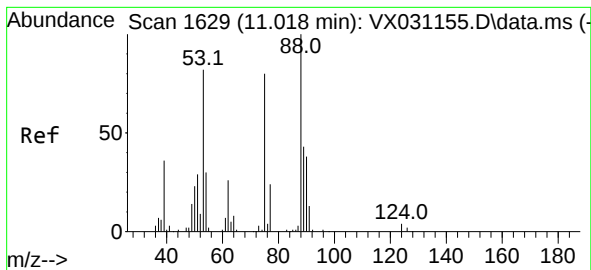

#81  
trans-1,4-Dichloro-2-butene  
Concen: 78.450 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.061 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 75 Resp: 37719  
Ion Ratio Lower Upper  
75 100  
53 0.0 74.2 111.4#  
89 0.0 34.8 52.2#

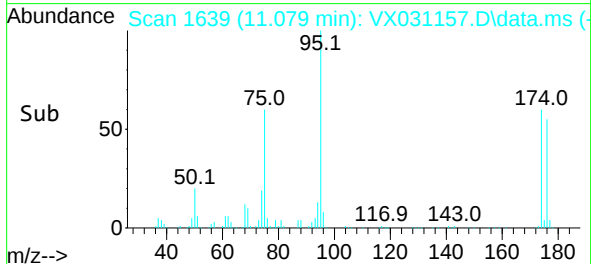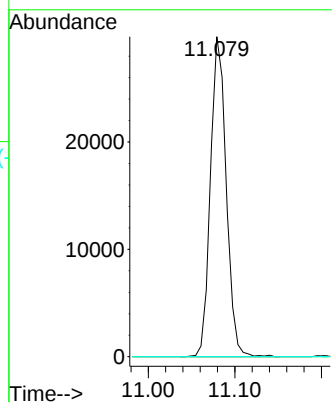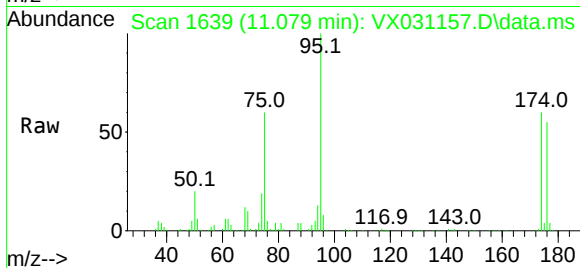

#82  
4-Chlorotoluene  
Concen: 0.333 ug/l  
RT: 11.457 min Scan# 1701  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48

Tgt Ion: 91 Resp: 1342  
Ion Ratio Lower Upper  
91 100  
126 31.8 15.3 45.9


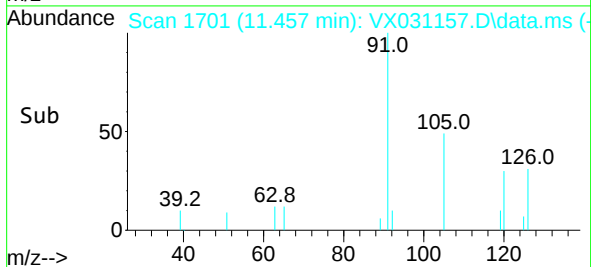
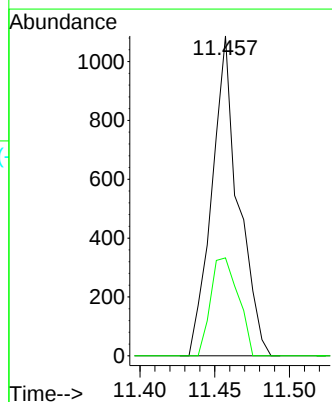
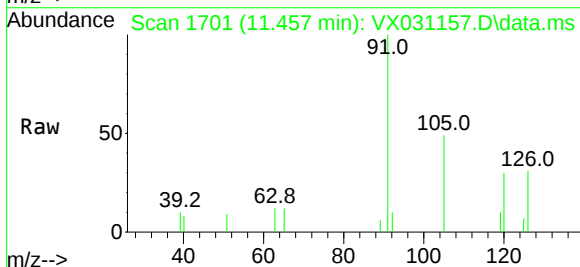




#85  
 sec-Butylbenzene  
 Concen: 0.242 ug/l  
 RT: 11.896 min Scan# 1773  
 Delta R.T. 0.006 min  
 Lab File: VX031157.D  
 Acq: 07 Sep 2022 13:48




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK


Tgt Ion:105 Resp: 1224  
 Ion Ratio Lower Upper  
 105 100  
 134 16.9 10.0 30.0

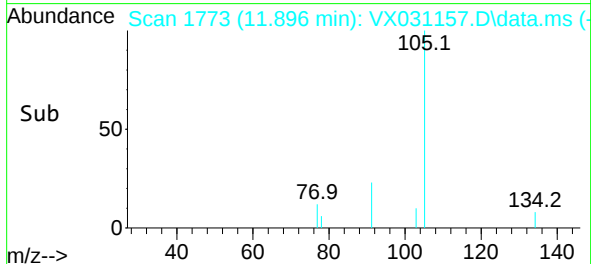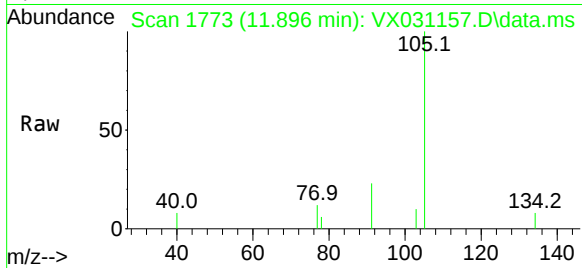

#86  
 p-Isopropyltoluene  
 Concen: 0.200 ug/l  
 RT: 12.006 min Scan# 1791  
 Delta R.T. -0.006 min  
 Lab File: VX031157.D  
 Acq: 07 Sep 2022 13:48


Tgt Ion:119 Resp: 820  
 Ion Ratio Lower Upper  
 119 100  
 134 41.2 13.9 41.6  
 91 64.1 11.8 35.3#

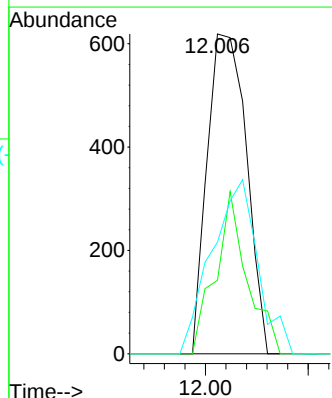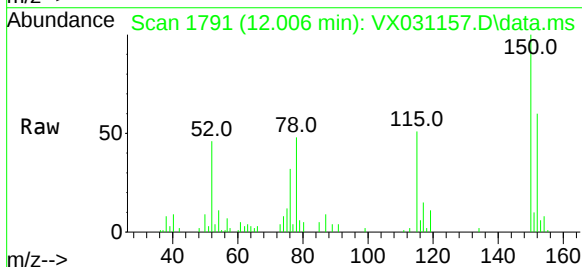






#87  
1,3-Dichlorobenzene  
Concen: 0.360 ug/l  
RT: 11.969 min Scan# 1785  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK



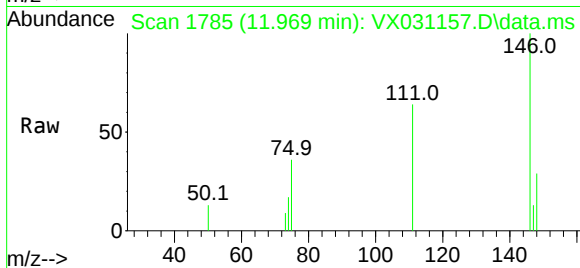



Tgt Ion:146 Resp: 718  
Ion Ratio Lower Upper  
146 100  
111 63.4 20.3 60.8#  
148 65.3 31.8 95.3

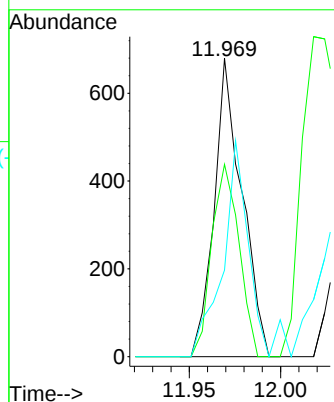

#88  
1,4-Dichlorobenzene  
Concen: 0.503 ug/l  
RT: 12.036 min Scan# 1796  
Delta R.T. -0.006 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48

Tgt Ion:146 Resp: 1031  
Ion Ratio Lower Upper  
146 100  
111 130.6 20.3 60.9#  
148 90.7 32.3 96.8

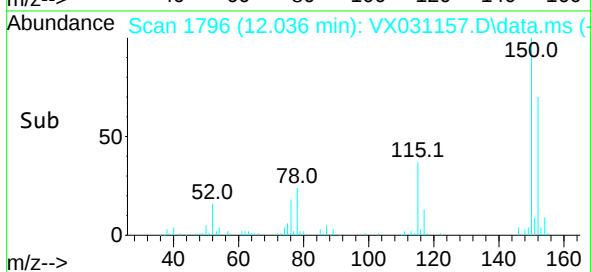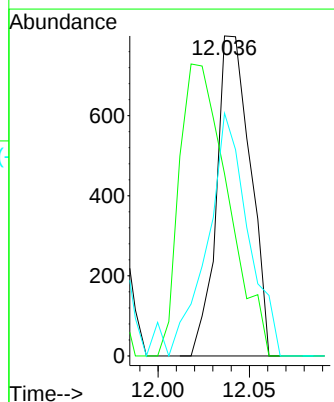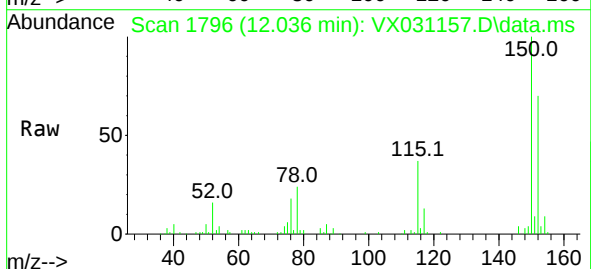



#89

n-Butylbenzene

Concen: 0.346 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. -0.000 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48

Instrument :

MSVOA\_X

ClientSampleId :

IBLK





Tgt Ion: 91 Resp: 1221

Ion Ratio Lower Upper

91 100

92 51.0 26.2 78.5

134 17.0 12.6 37.8

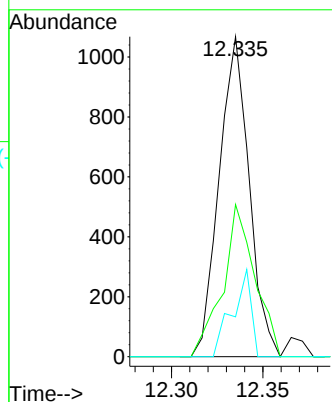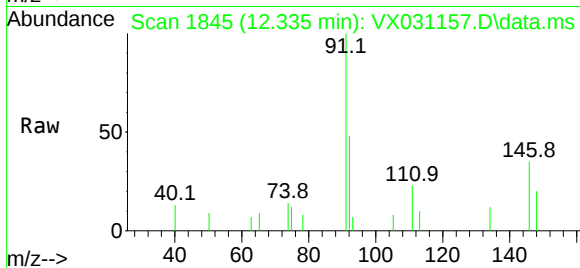

#91

1,2-Dichlorobenzene

Concen: 0.307 ug/l

RT: 12.341 min Scan# 1846

Delta R.T. 0.006 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48




Tgt Ion:146 Resp: 600


Ion Ratio Lower Upper

146 100

111 42.2 20.7 62.1

148 40.0 32.0 96.2


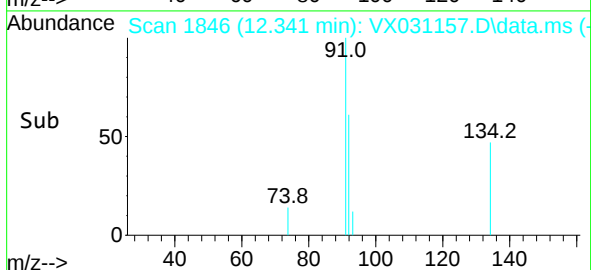

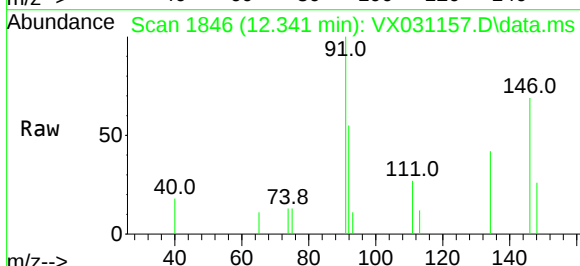




#93  
1,2,4-Trichlorobenzene  
Concen: 0.655 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


|             |       |             |
|-------------|-------|-------------|
| Tgt Ion:180 | Resp: | 748         |
| Ion         | Ratio | Lower Upper |
| 180         | 100   |             |
| 182         | 79.5  | 48.2 144.6  |
| 145         | 44.3  | 15.9 47.6   |

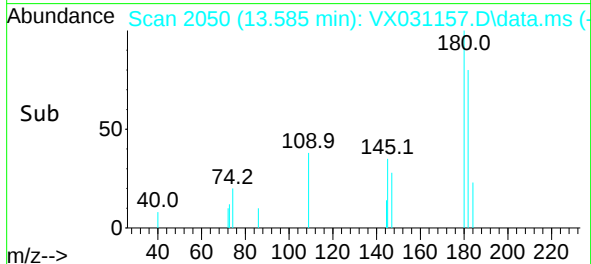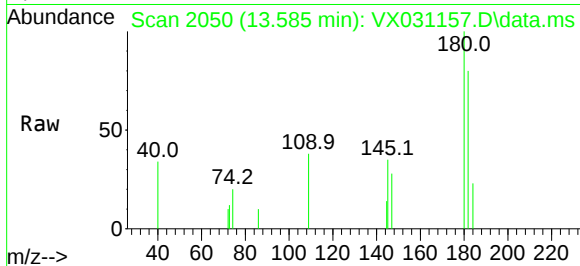

#94  
Hexachlorobutadiene  
Concen: 0.841 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. -0.000 min  
Lab File: VX031157.D  
Acq: 07 Sep 2022 13:48

|             |       |             |
|-------------|-------|-------------|
| Tgt Ion:225 | Resp: | 408         |
| Ion         | Ratio | Lower Upper |
| 225         | 100   |             |
| 223         | 58.8  | 30.6 91.6   |
| 227         | 61.0  | 31.9 95.9   |

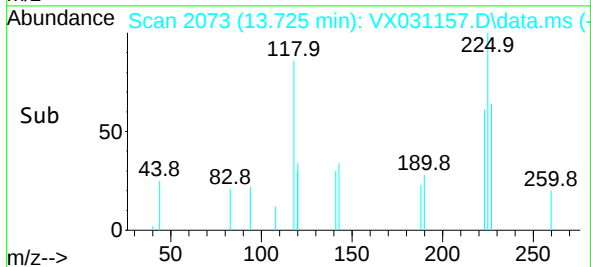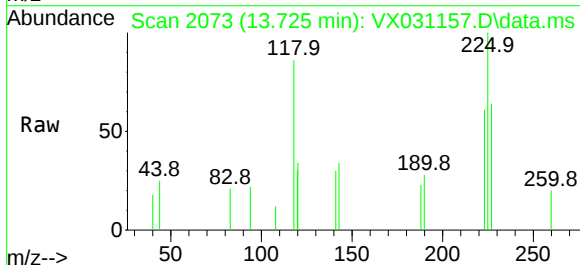



#95

Naphthalene

Concen: 0.549 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48





Instrument :

MSVOA\_X

ClientSampleId :

IBLK

|             |       |           |
|-------------|-------|-----------|
| Tgt Ion:128 | Resp: | 2456      |
| Ion Ratio   | Lower | Upper     |
| 128         | 100   |           |
| 127         | 11.7  | 10.2 15.2 |
| 129         | 5.7   | 8.6 13.0  |

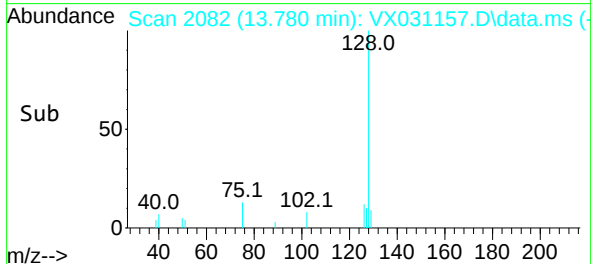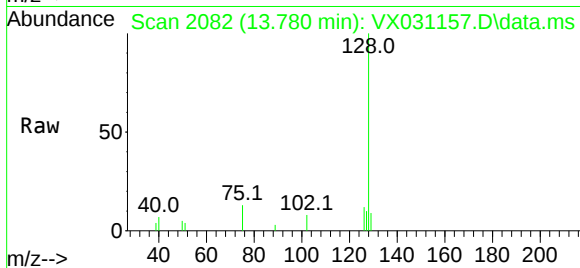

#96

1,2,3-Trichlorobenzene

Concen: 0.506 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX031157.D

Acq: 07 Sep 2022 13:48

|             |       |            |
|-------------|-------|------------|
| Tgt Ion:180 | Resp: | 589        |
| Ion Ratio   | Lower | Upper      |
| 180         | 100   |            |
| 182         | 115.4 | 47.0 141.0 |
| 145         | 44.0  | 17.0 50.9  |

