

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090722\
 Data File : VX031194.D
 Acq On : 08 Sep 2022 06:28
 Operator : JC/MD
 Sample : N4446-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IDW-WATER-LIQUID

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M

Title : SW846 8260

Signal : TIC: VX031194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	694	706	720	rBV2	86317	249649	36.15%	8.306%
2	5.555	722	733	745	rVB2	88101	251773	36.45%	8.377%
3	5.958	787	799	812	rBV	100051	263180	38.11%	8.756%
4	6.763	922	931	945	rBV	135277	322351	46.67%	10.725%
5	8.652	1234	1241	1248	rBV	440378	690652	100.00%	22.979%
6	8.726	1248	1253	1260	rVB2	4652	8355	1.21%	0.278%
7	10.055	1465	1471	1482	rBV	285622	372893	53.99%	12.406%
8	10.195	1490	1494	1501	rBV	8085	11383	1.65%	0.379%
9	10.305	1507	1512	1521	rBV	10793	14987	2.17%	0.499%
10	10.646	1563	1568	1573	rBV	13661	18448	2.67%	0.614%
11	11.079	1634	1639	1650	rVB	356903	469666	68.00%	15.626%
12	12.024	1788	1794	1803	rBV	266374	332304	48.11%	11.056%




Sum of corrected areas: 3005641

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090722\
Data File : VX031194.D
Acq On : 08 Sep 2022 06:28
Operator : JC/MD
Sample : N4446-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IDW-WATER-LIQUID

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

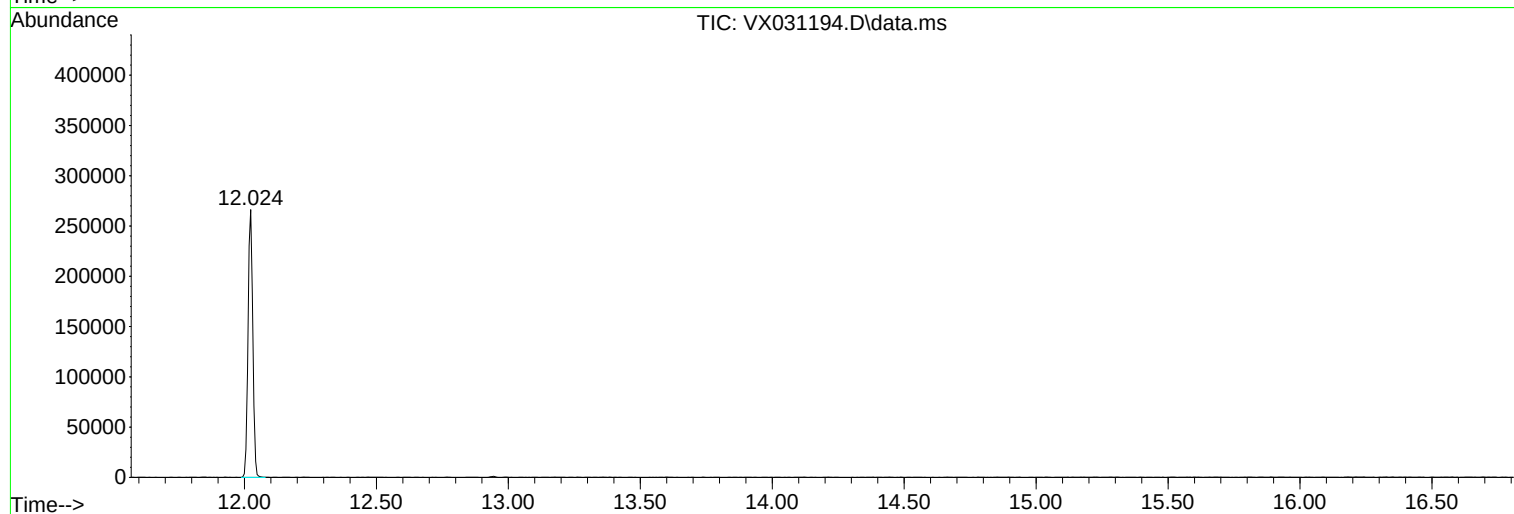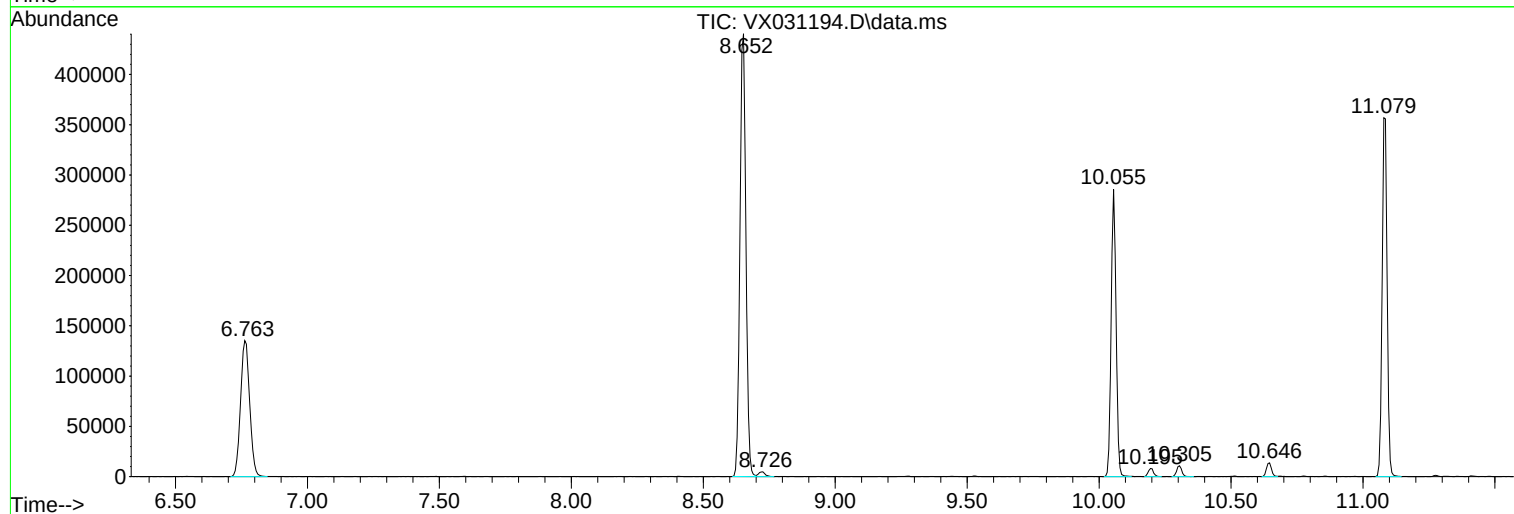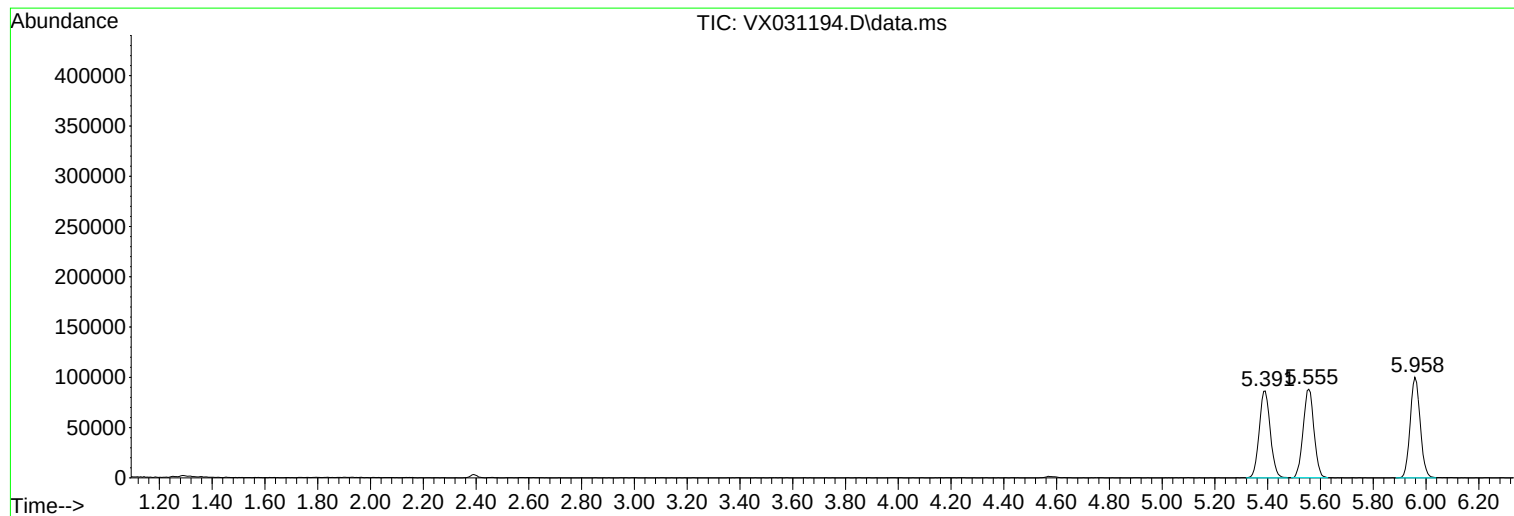

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090722\
Data File : VX031194.D
Acq On : 08 Sep 2022 06:28
Operator : JC/MD
Sample : N4446-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IDW-WATER-LIQUID

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090722\
Data File : VX031194.D
Acq On : 08 Sep 2022 06:28
Operator : JC/MD
Sample : N4446-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IDW-WATER-LIQUID

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------