



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090722\
Data File : VX031159.D
Acq On : 07 Sep 2022 14:55
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Title : SW846 8260
Last Update : Wed Sep 07 23:22:41 2022

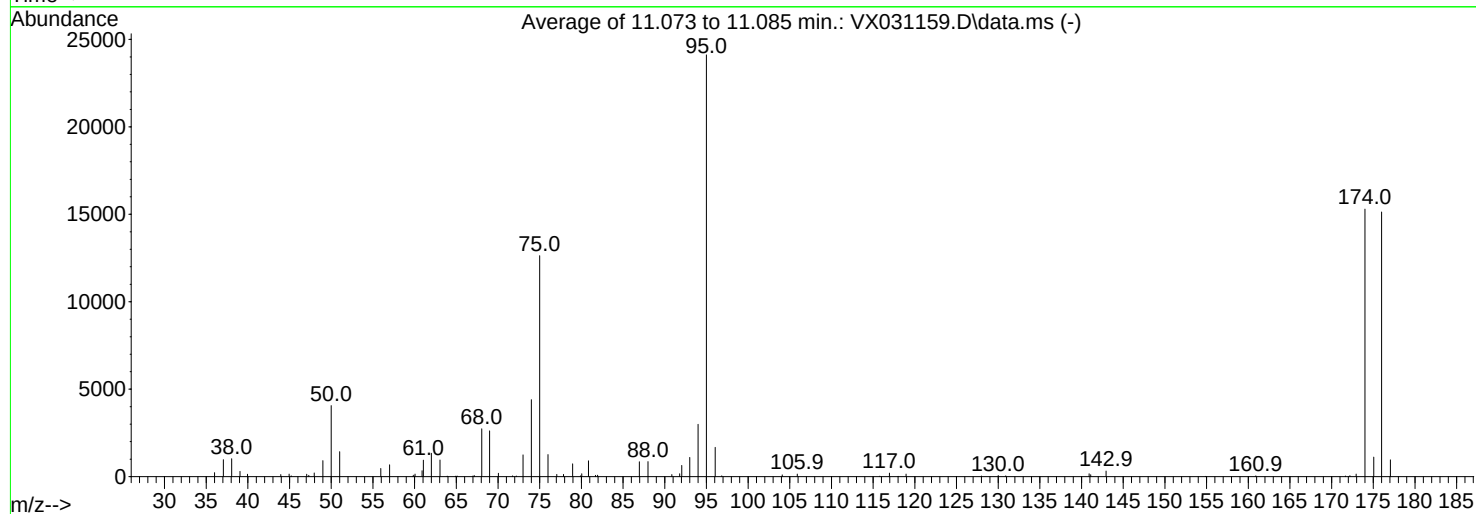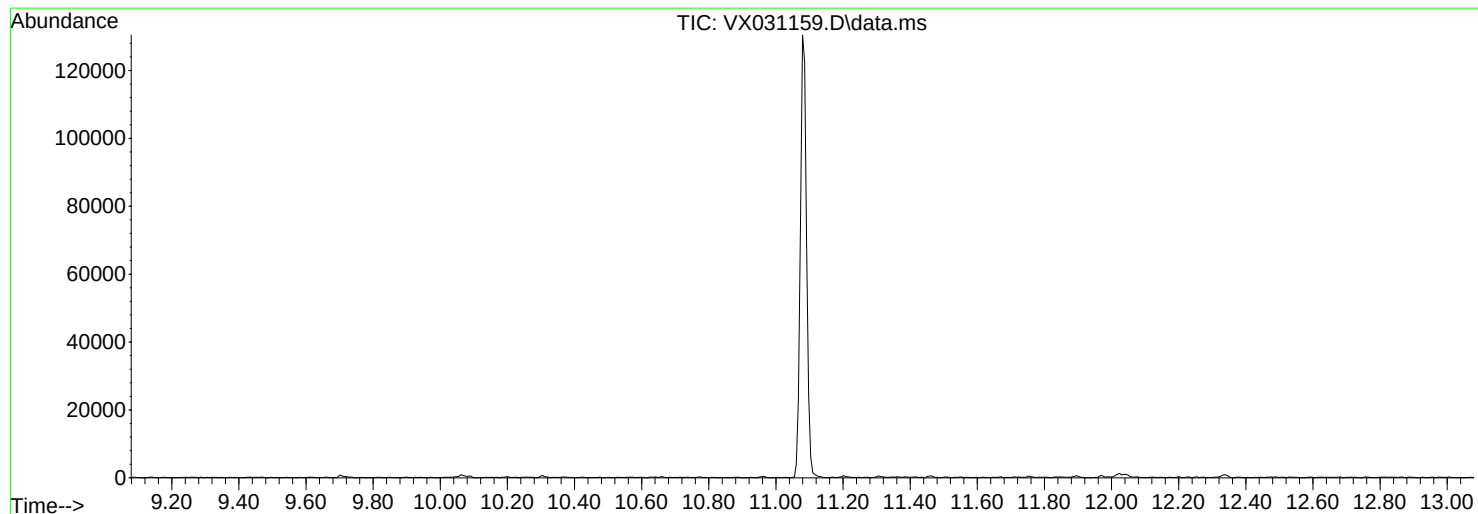

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	4061	PASS
75	95	30	60	52.4	12637	PASS
95	95	100	100	100.0	24117	PASS
96	95	5	9	7.0	1677	PASS
173	174	0.00	2	0.9	143	PASS
174	95	50	100	63.4	15296	PASS
175	174	5	9	7.3	1114	PASS
176	174	95	101	98.9	15135	PASS
177	176	5	9	6.4	964	PASS