
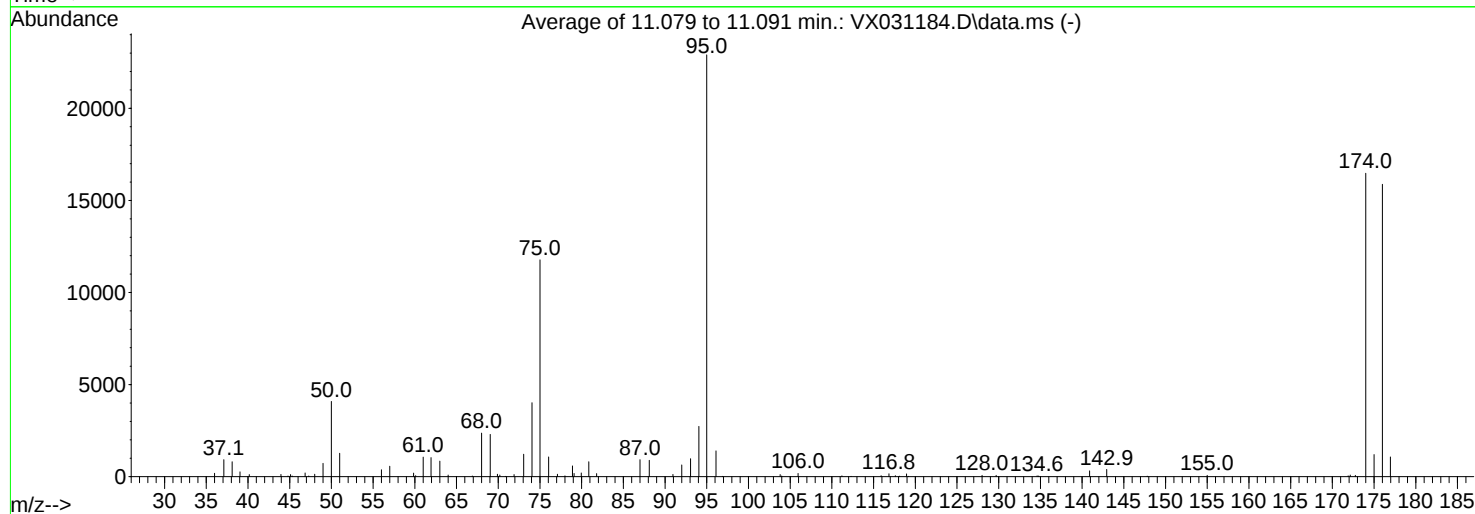


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090722\
Data File : VX031184.D
Acq On : 08 Sep 2022 02:12
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Title : SW846 8260
Last Update : Wed Sep 07 23:22:41 2022

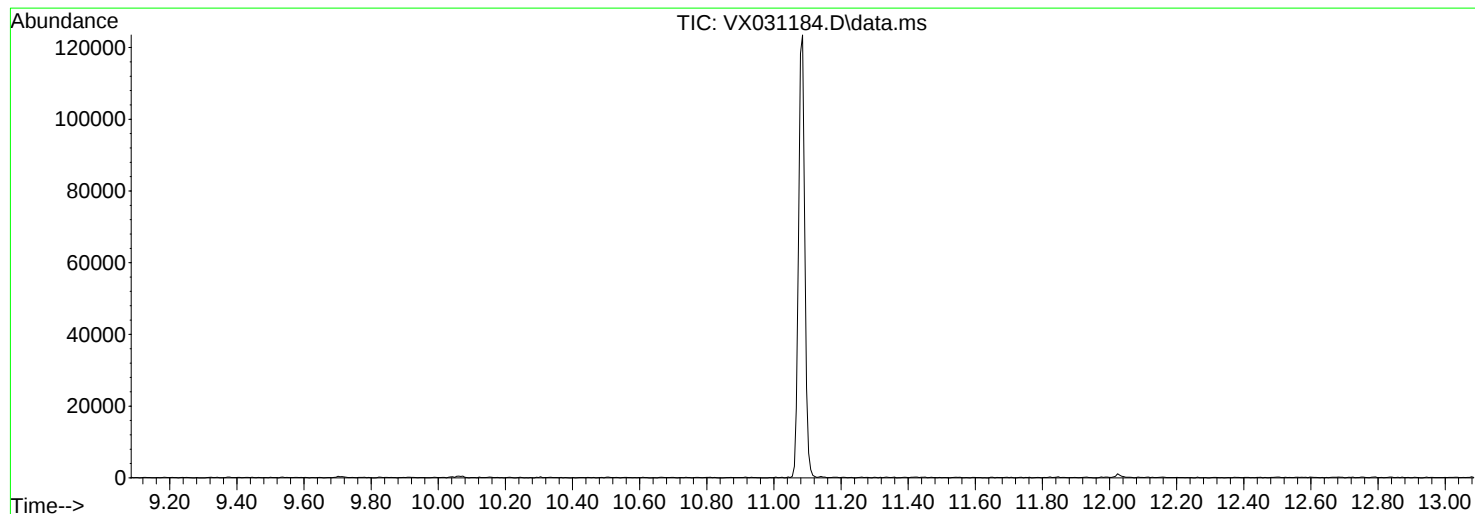

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	4080	PASS
75	95	30	60	51.4	11775	PASS
95	95	100	100	100.0	22907	PASS
96	95	5	9	6.1	1396	PASS
173	174	0.00	2	0.4	69	PASS
174	95	50	100	71.9	16474	PASS
175	174	5	9	7.3	1198	PASS
176	174	95	101	96.4	15875	PASS
177	176	5	9	6.7	1071	PASS