

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX090819\
 Data File : VX012216.D
 Acq On : 08 Sep 2019 12:01
 Operator : SY/SP
 Sample : K4661-01
 Misc : 6.42g/5.0mL/MSVOA X/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 HD-01-090519

Quant Time: Sep 09 02:10:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X090319S.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 03 15:26:48 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	149075	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	258635	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	230336	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	103503	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	104345	50.73	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.46%	
35) Dibromofluoromethane	5.48	113	77734	48.87	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.74%	
50) Toluene-d8	8.71	98	305695	52.38	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.76%	
62) 4-Bromofluorobenzene	11.13	95	123758	45.59	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.18%	
Target Compounds						
					Qvalue	
16) Acetone	2.43	43	20582	41.863	ug/l	94
20) Methylene Chloride	2.84	84	10709	5.424	ug/l	96
29) Tetrahydrofuran	5.12	42	3104	8.232	ug/l #	89
52) Toluene	8.78	92	14781	3.474	ug/l	94
67) Ethyl Benzene	10.25	91	11837	1.429	ug/l	99
68) m/p-Xylenes	10.36	106	19956	6.538	ug/l	88
69) o-Xylene	10.70	106	18519	6.257	ug/l	88
80) 1,3,5-Trimethylbenzene	11.50	105	37408	5.621	ug/l	93
84) 1,2,4-Trimethylbenzene	11.80	105	100980	14.763	ug/l	93
89) n-Butylbenzene	12.38	91	19352	2.780	ug/l #	39
95) Naphthalene	13.83	128	777469	164.657	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX090819\
Data File : VX012216.D
Acq On : 08 Sep 2019 12:01
Operator : SY/SP
Sample : K4661-01
Misc : 6.42g/5.0mL/MSVOA X/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
HD-01-090519

Quant Time: Sep 09 02:10:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X090319S.M
Quant Title : SW846 8260
QLast Update : Tue Sep 03 15:26:48 2019
Response via : Initial Calibration

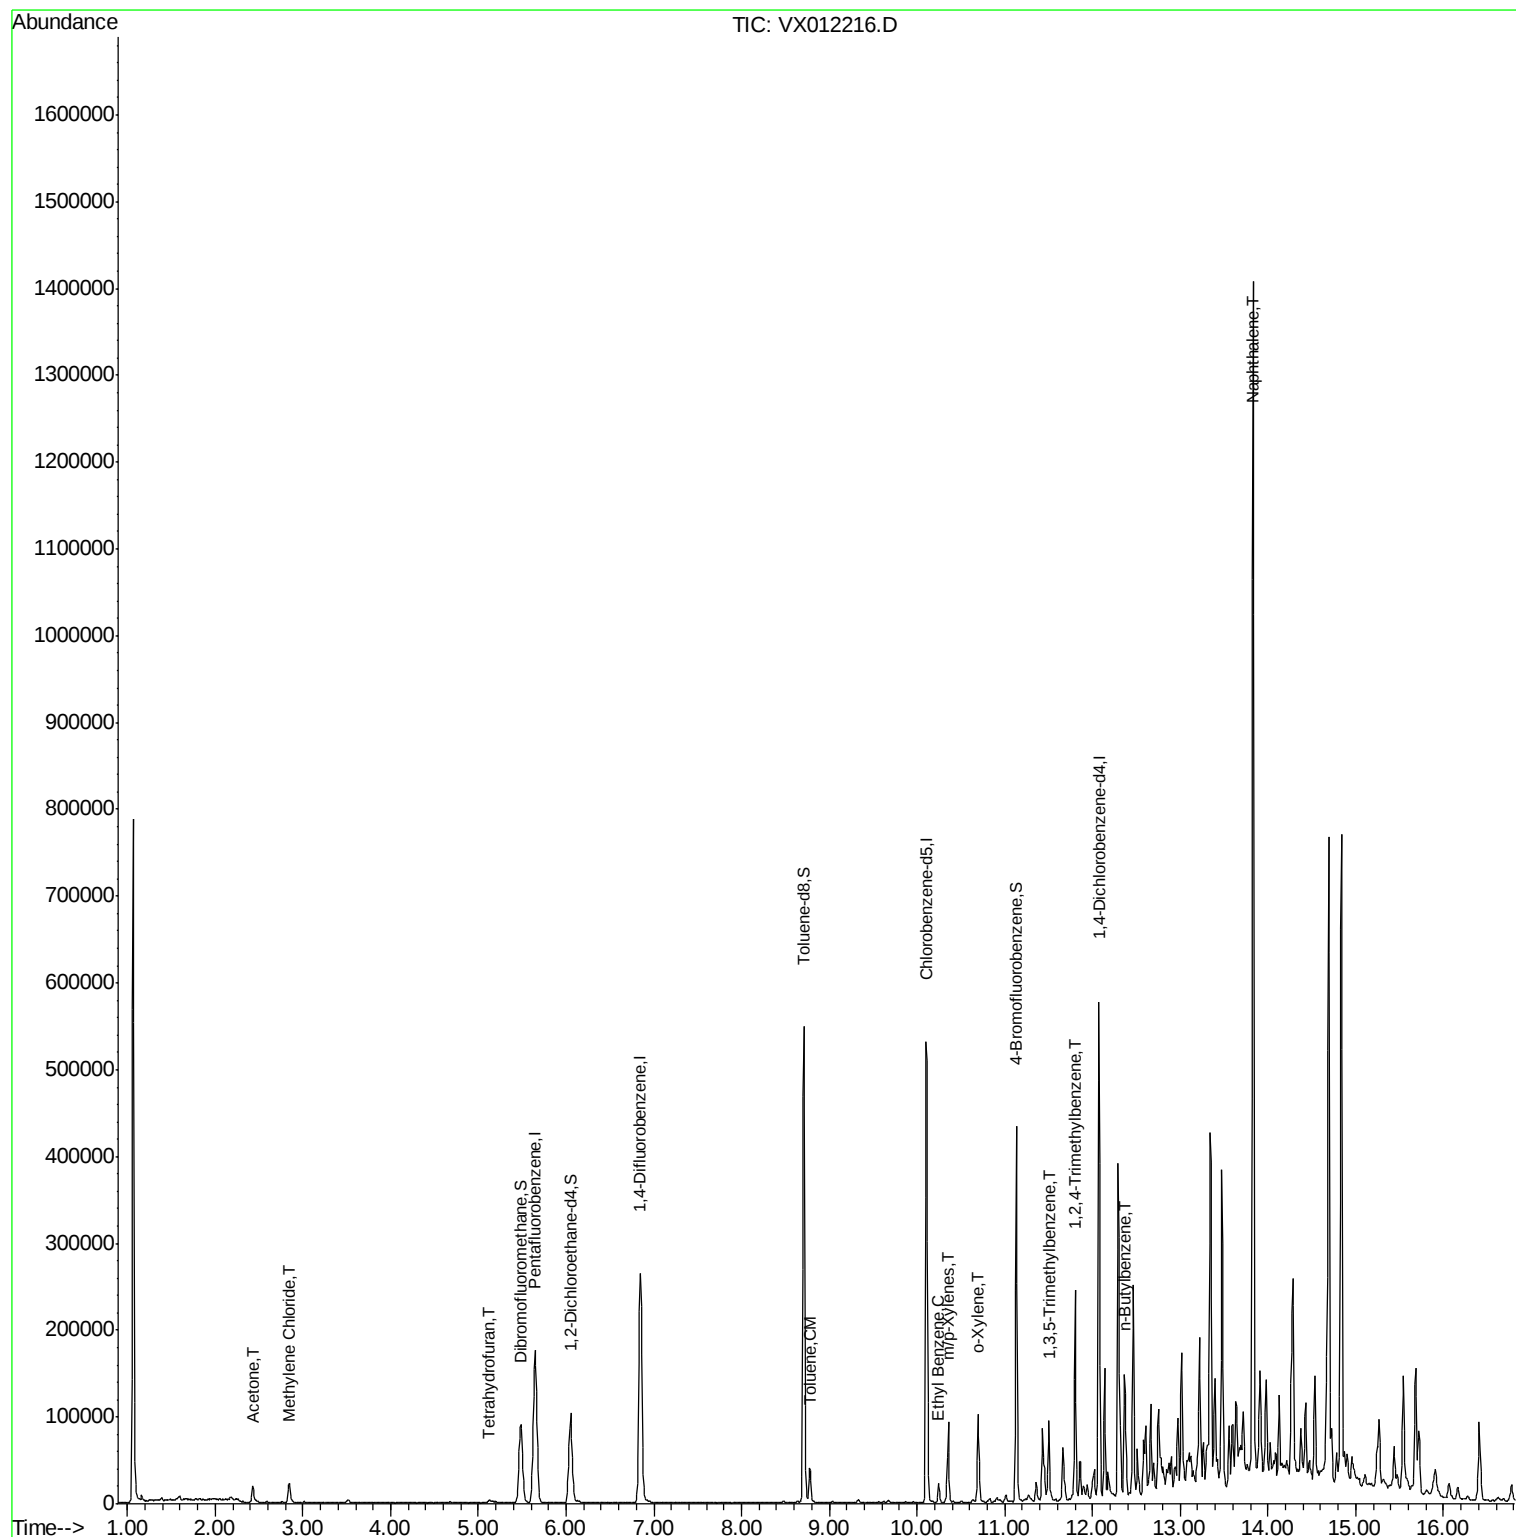

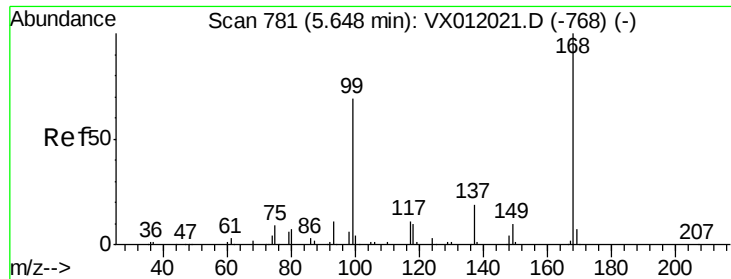

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.00 min

Lab File: VX012216.D

Acq: 08 Sep 2019 12:01

Instrument :

MSVOA_X

ClientSampleId :





HD-01-090519

Tot Ion:168 Resp: 149075

Ion Ratio Lower Upper

168 100

99 69.2 37.6 56.4#

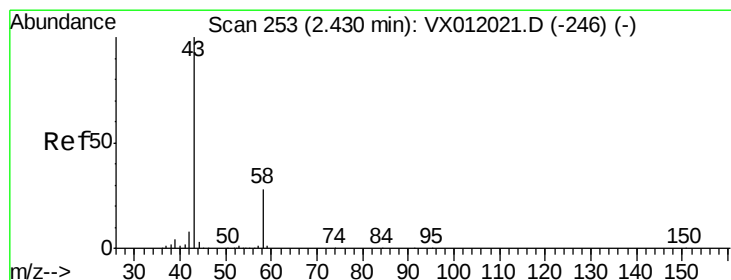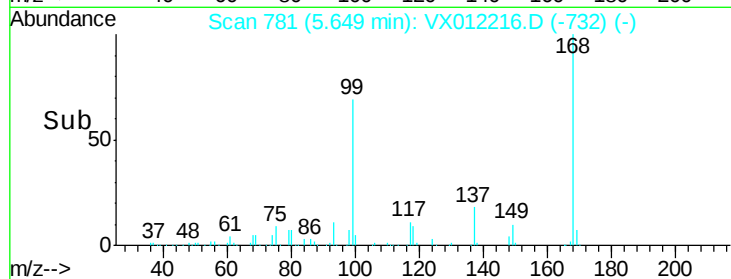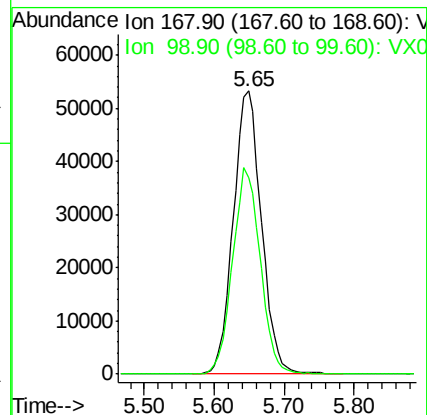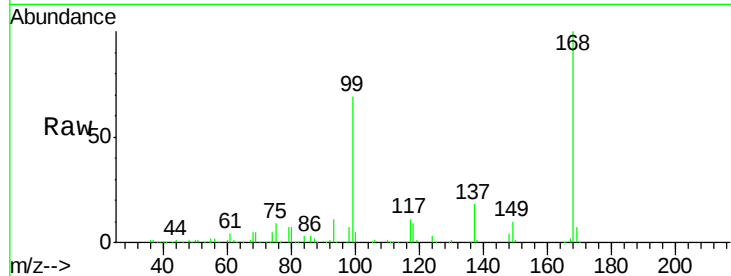

#16

Acetone

Concen: 41.863 ug/l

RT: 2.43 min Scan# 253

Delta R.T. -0.00 min

Lab File: VX012216.D




Acq: 08 Sep 2019 12:01


Tgt Ion: 43 Resp: 20582

Ion Ratio Lower Upper

43 100

58 25.6 22.8 34.2



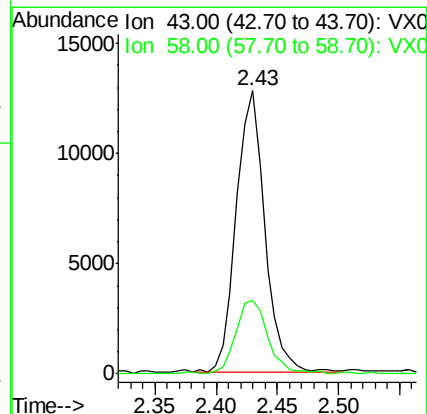



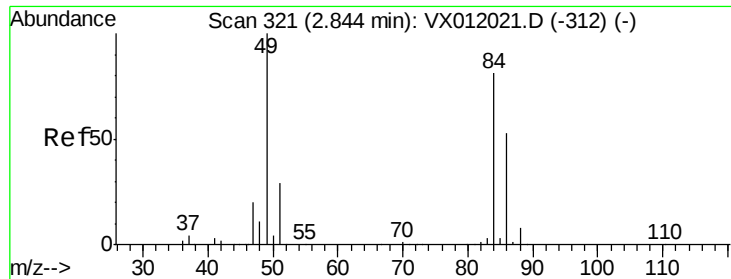

#20
Methvlene Chloride
Concen: 5.424 ug/l
RT: 2.84 min Scan# 321
Delta R.T. -0.00 min
Lab File: VX012216.D
Acq: 08 Sep 2019 12:01




Instrument :
MSVOA_X
ClientSampled :
HD-01-090519


Tot Ion:	84	Resp:	10709
Ion	Ratio	Lower	Upper
84	100		
49	124.3	95.8	143.8
51	39.9	28.6	43.0
86	64.7	50.9	76.3

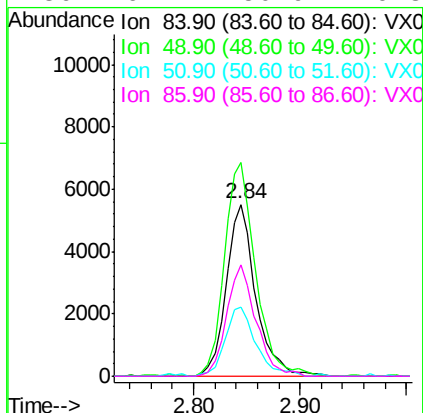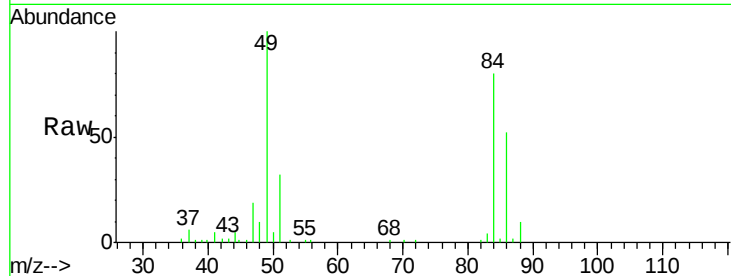

#29
Tetrahydrofuran
Concen: 8.232 ug/l
RT: 5.12 min Scan# 694
Delta R.T. 0.01 min
Lab File: VX012216.D
Acq: 08 Sep 2019 12:01

Tgt Ion:	42	Resp:	3104
Ion	Ratio	Lower	Upper
42	100		
72	34.7	37.0	55.4#
71	45.0	33.8	50.8

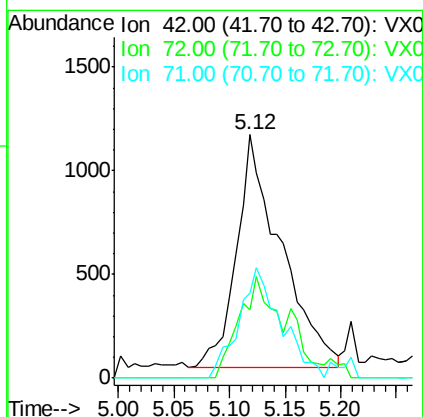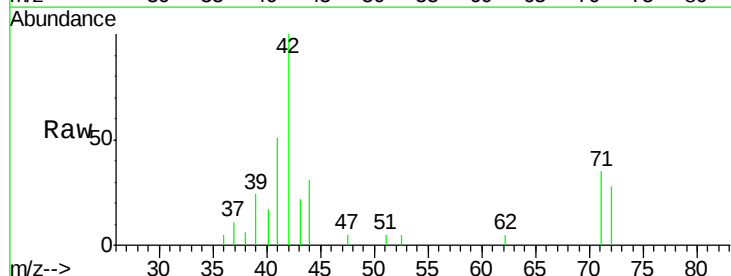

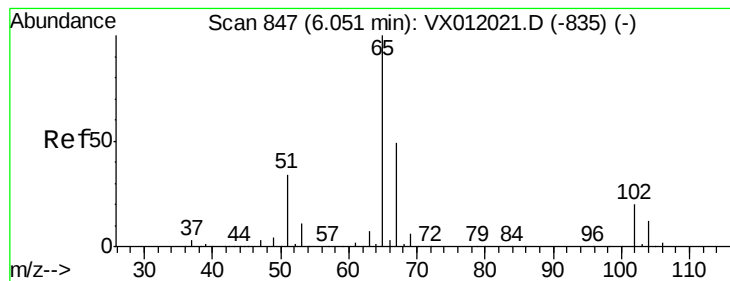

#33

1,2-Dichloroethane-d4

Concen: 50.728 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX012216.D

Acq: 08 Sep 2019 12:01

Instrument :

MSVOA_X

ClientSampleId :


HD-01-090519

Tot Ion: 65 Resp: 104345

Ion Ratio Lower Upper




65 100

67 49.3 0.0 102.0

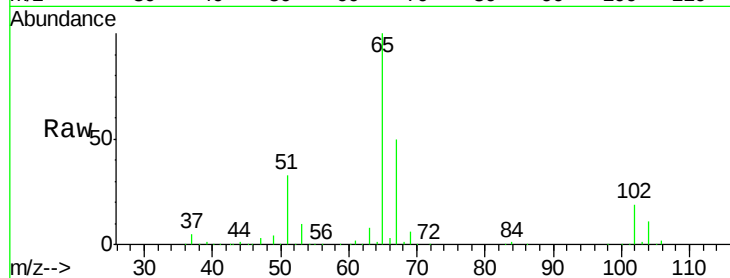

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

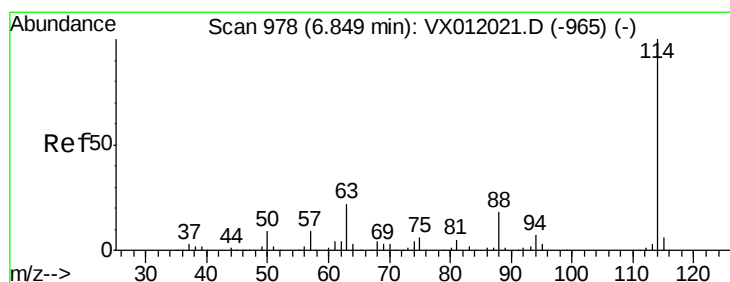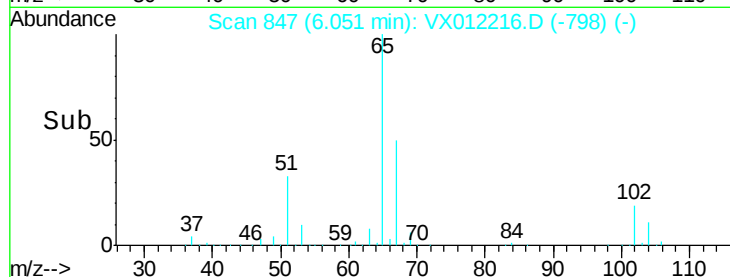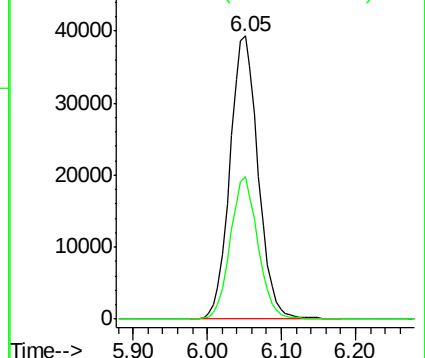

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 977

Delta R.T. -0.01 min

Lab File: VX012216.D

Acq: 08 Sep 2019 12:01


Tgt Ion: 114 Resp: 258635

Ion Ratio Lower Upper

114 100

63 22.3 0.0 37.4



88 17.9 0.0 29.6

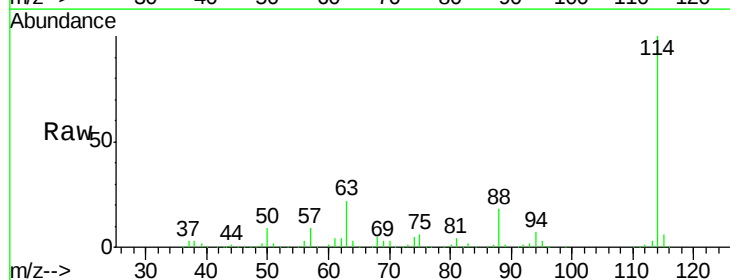


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

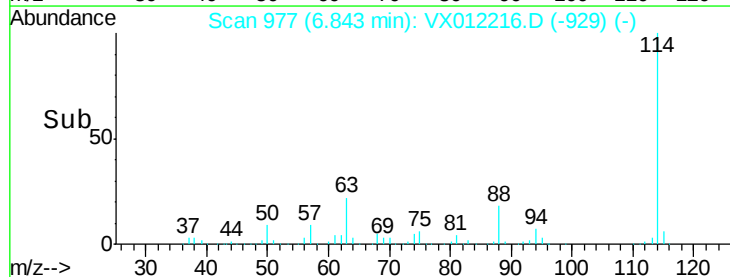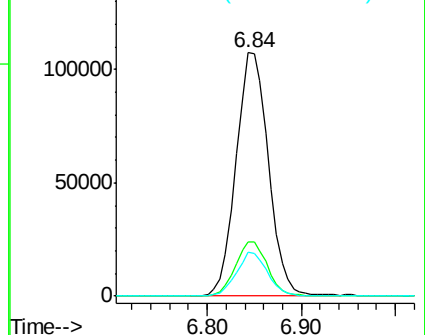







#35
 Dibromofluoromethane
 Concen: 48.873 ug/l
 RT: 5.48 min Scan# 754
 Delta R.T. -0.00 min
 Lab File: VX012216.D
 Acq: 08 Sep 2019 12:01

Instrument :
 MSVOA_X
 ClientSampleId :
 HD-01-090519

Tot Ion:113 Resp: 77734
 Ion Ratio Lower Upper
 113 100
 111 102.0 81.7 122.5
 192 16.8 22.5 33.7#

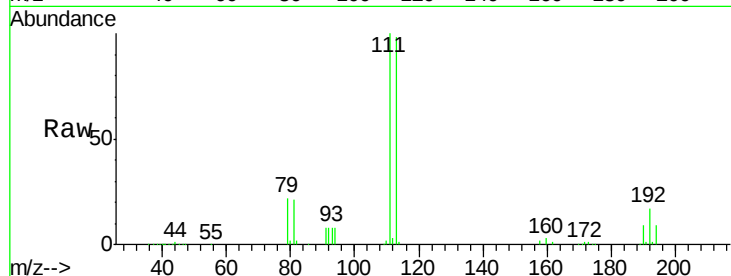


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V


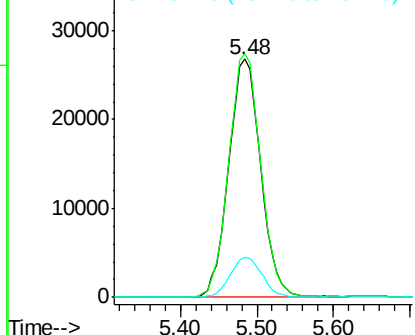



#50
 Toluene-d8
 Concen: 52.376 ug/l
 RT: 8.71 min Scan# 1283
 Delta R.T. -0.00 min
 Lab File: VX012216.D
 Acq: 08 Sep 2019 12:01

Tgt Ion: 98 Resp: 305695
 Ion Ratio Lower Upper
 98 100
 100 67.1 53.3 79.9



Abundance Ion 98.00 (97.70 to 98.70): VX0
 Ion 100.00 (99.70 to 100.70): V

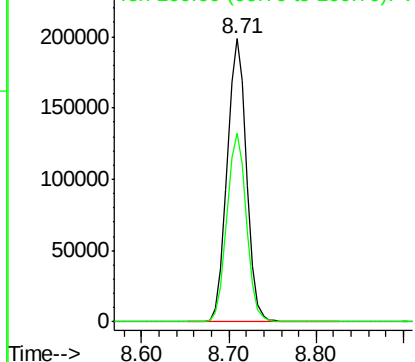

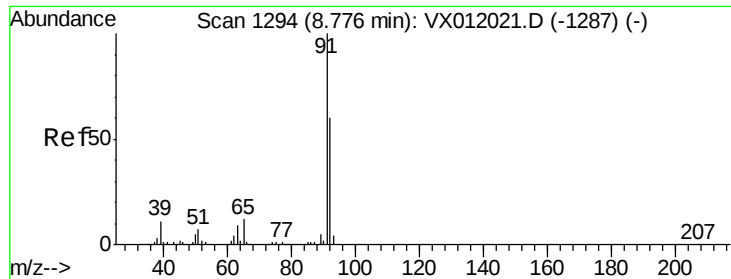

#52

Toluene

Concen: 3.474 ug/l

RT: 8.78 min Scan# 1294

Delta R.T. -0.00 min

Lab File: VX012216.D

Acq: 08 Sep 2019 12:01

Instrument :

MSVOA_X

ClientSampleId :





HD-01-090519

Tot Ion: 92 Resp: 14781

Ion Ratio Lower Upper

92 100

91 161.3 136.0 204.0

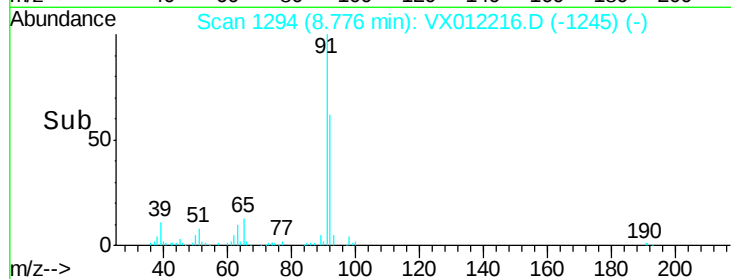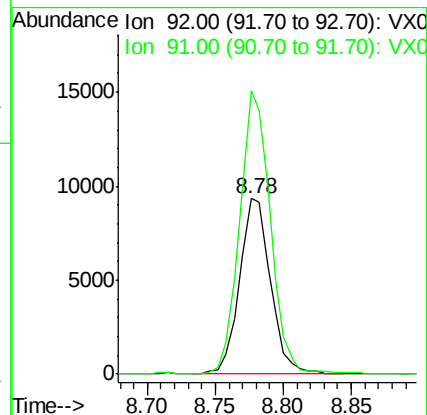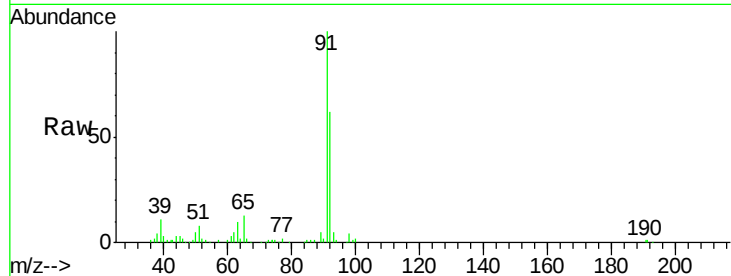

#62

4-Bromofluorobenzene

Concen: 45.594 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.01 min

Lab File: VX012216.D

Acq: 08 Sep 2019 12:01




Tgt Ion: 95 Resp: 123758


Ion Ratio Lower Upper

95 100

174 65.6 0.0 205.4

176 61.8 0.0 201.8



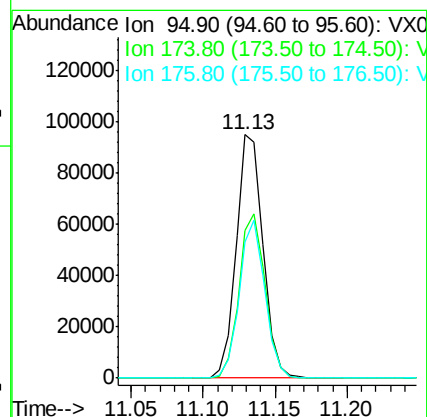



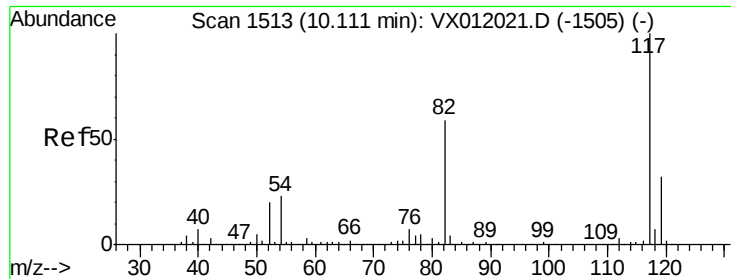

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1513
Delta R.T. -0.00 min
Lab File: VX012216.D
Acq: 08 Sep 2019 12:01




Instrument :
MSVOA_X
ClientSampleId :
HD-01-090519


Tot Ion:117 Resp: 230336
Ion Ratio Lower Upper
117 100
82 57.3 39.4 59.0
119 31.6 26.1 39.1

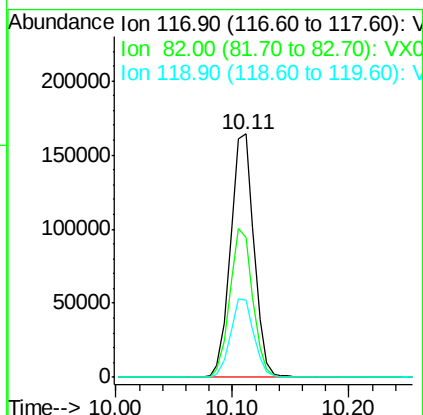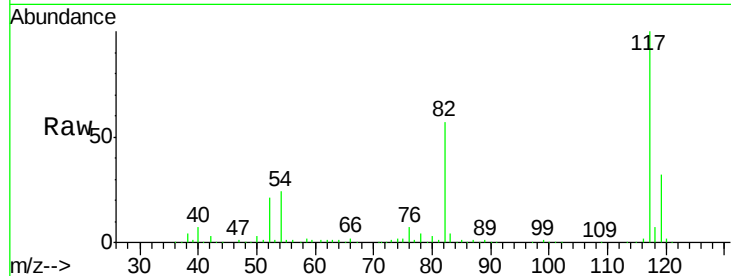

#67
Ethyl Benzene
Concen: 1.429 ug/l
RT: 10.25 min Scan# 1535
Delta R.T. -0.00 min
Lab File: VX012216.D
Acq: 08 Sep 2019 12:01

Tgt Ion: 91 Resp: 11837
Ion Ratio Lower Upper
91 100
106 31.6 25.8 38.8


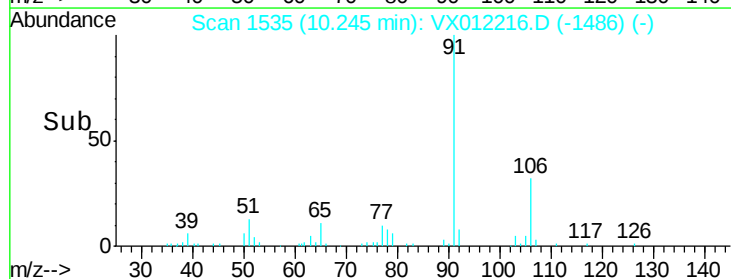
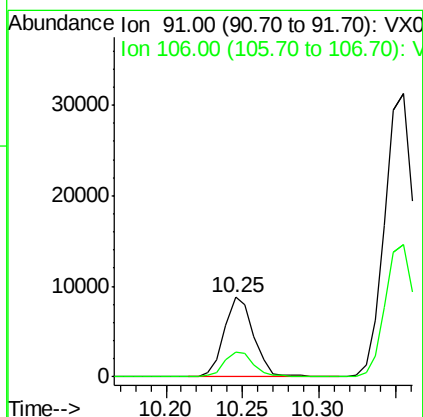





#68
m/p-Xylenes
Concen: 6.538 ug/l
RT: 10.36 min Scan# 1553
Delta R.T. -0.00 min
Lab File: VX012216.D
Acq: 08 Sep 2019 12:01




Instrument :
MSVOA_X
ClientSampleId :
HD-01-090519


Tot Ion:106 Resp: 19956
Ion Ratio Lower Upper
106 100
91 214.5 157.5 236.3

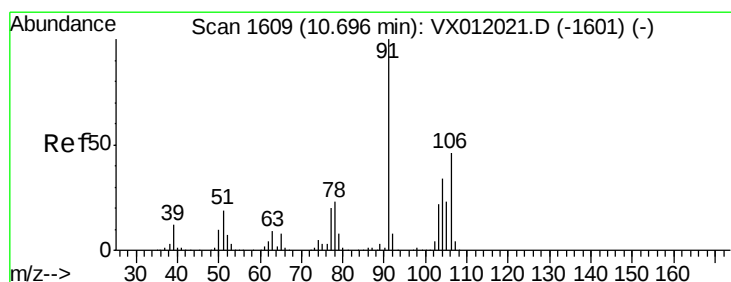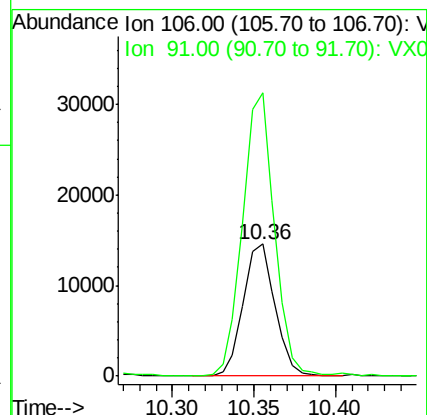

#69
o-Xylene
Concen: 6.257 ug/l
RT: 10.70 min Scan# 1609
Delta R.T. -0.00 min
Lab File: VX012216.D
Acq: 08 Sep 2019 12:01

Tgt Ion:106 Resp: 18519
Ion Ratio Lower Upper
106 100
91 226.2 103.5 310.3

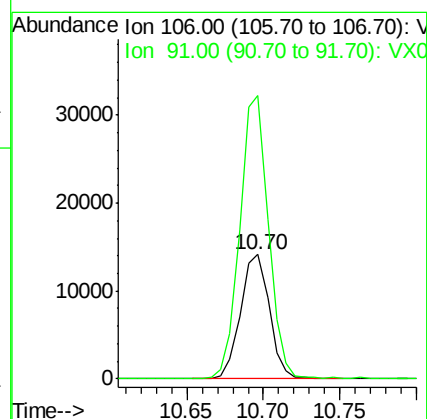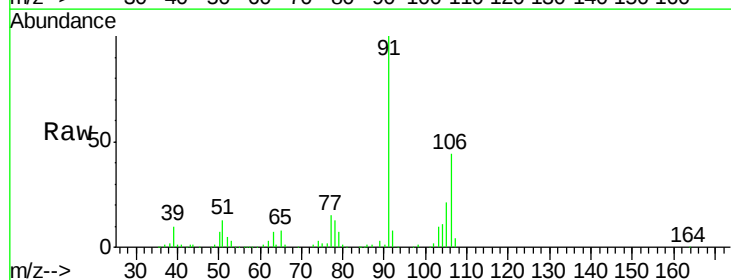

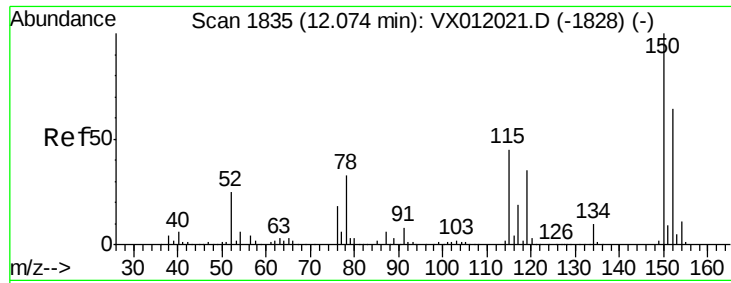

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.07 min Scan# 1835

Delta R.T. -0.00 min

Lab File: VX012216.D

Acq: 08 Sep 2019 12:01

Instrument :

MSVOA_X

ClientSampleId :

HD-01-090519


Tot Ion:152 Resp: 103503

Ion Ratio Lower Upper

152 100

115 65.7 36.4 109.3




150 158.3 0.0 341.2

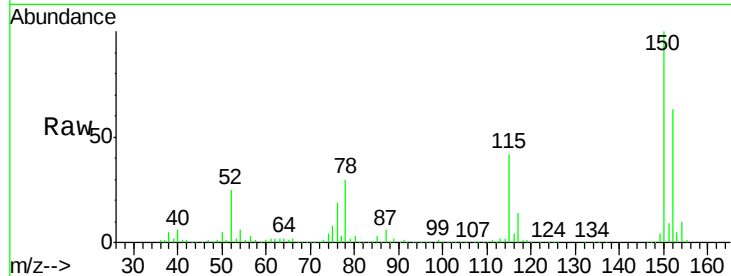

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

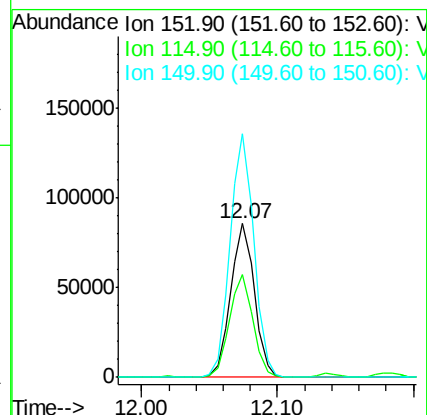

#80

1,3,5-Trimethylbenzene

Concen: 5.621 ug/l

RT: 11.50 min Scan# 1741

Delta R.T. -0.00 min

Lab File: VX012216.D


Acq: 08 Sep 2019 12:01

Tgt Ion:105 Resp: 37408

Ion Ratio Lower Upper



105 100


120 46.3 25.8 77.3



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

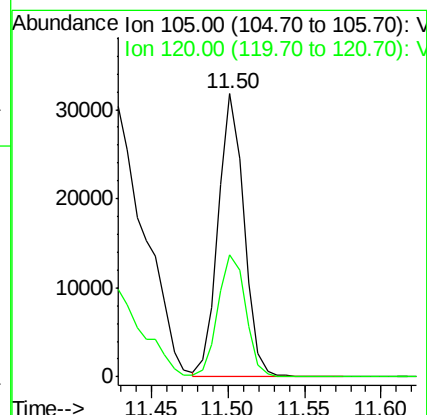


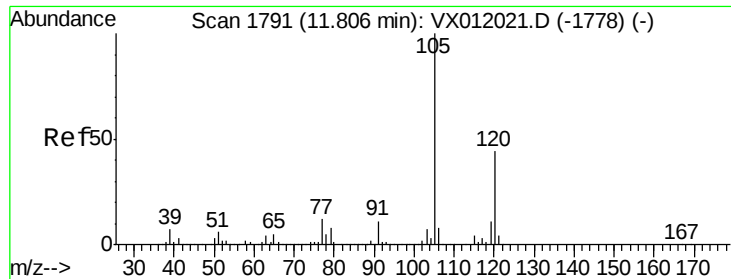




#84
 1,2,4-Trimethylbenzene
 Concen: 14.763 ug/l
 RT: 11.80 min Scan# 1790
 Delta R.T. -0.00 min
 Lab File: VX012216.D
 Acq: 08 Sep 2019 12:01

Instrument :
 MSVOA_X
 ClientSampleId :
 HD-01-090519

Tot Ion:105 Resp: 100980
 Ion Ratio Lower Upper
 105 100
 120 42.7 23.6 70.8

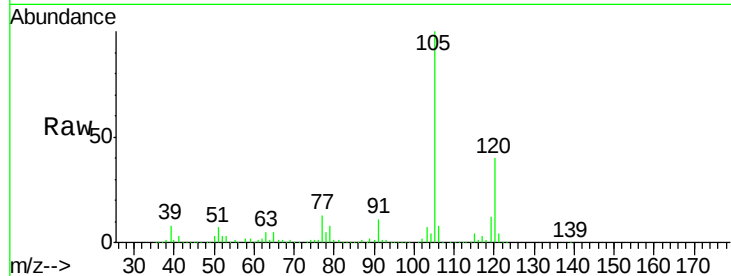


Abundance Ion 105.00 (104.70 to 105.70): V
 Ion 120.00 (119.70 to 120.70): V


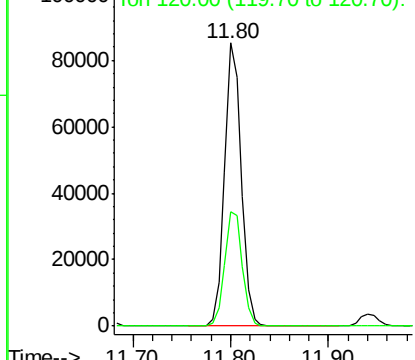



#89
 n-Butylbenzene
 Concen: 2.780 ug/l
 RT: 12.38 min Scan# 1885
 Delta R.T. -0.01 min
 Lab File: VX012216.D
 Acq: 08 Sep 2019 12:01

Tgt Ion: 91 Resp: 19352
 Ion Ratio Lower Upper
 91 100
 92 32.4 27.6 82.8
 134 93.9 15.4 46.1#



Abundance Ion 91.00 (90.70 to 91.70): VX0
 Ion 92.00 (91.70 to 92.70): VX0
 Ion 134.00 (133.70 to 134.70): V

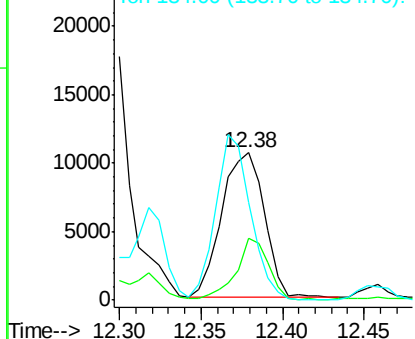




#95
Naphthalene
Concen: 164.657 ug/l
RT: 13.83 min Scan# 2123
Delta R.T. -0.00 min
Lab File: VX012216.D
Acq: 08 Sep 2019 12:01

Instrument :
MSVOA_X
ClientSampleId :
HD-01-090519

Tot Ion	Ratio	Lower	Upper
128	100		
127	13.0	10.5	15.7
129	11.2	8.8	13.2

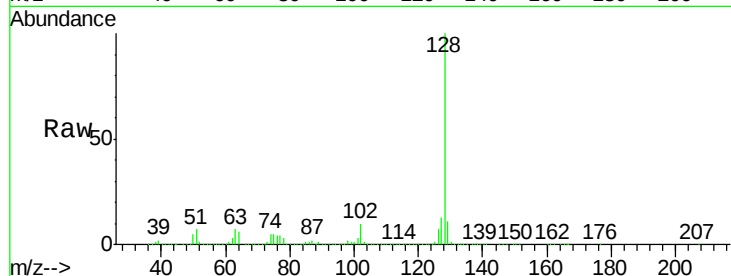

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

