

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX090820\
 Data File : VX018288.D
 Acq On : 08 Sep 2020 20:13
 Operator : JC/SP
 Sample : PB131451ZHE#09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB131451ZHE#09

Quant Time: Sep 09 02:34:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082120W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 21 03:03:56 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	470365	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	765396	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	793563	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	382719	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	340095	52.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.16%	
35) Dibromofluoromethane	5.47	113	271342	52.05	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.10%	
50) Toluene-d8	8.70	98	975895	50.26	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.52%	
62) 4-Bromofluorobenzene	11.12	95	370704	48.53	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.06%	
Target Compounds						
16) Acetone	2.42	43	28747	11.298	ug/l	95
18) Methyl Acetate	2.75	43	6265	1.020	ug/l	91
20) Methylene Chloride	2.84	84	19636	2.669	ug/l	95
43) Isopropyl Acetate	6.42	43	112197	8.472	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX090820\
Data File : VX018288.D
Acq On : 08 Sep 2020 20:13
Operator : JC/SP
Sample : PB131451ZHE#09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB131451ZHE#09

Quant Time: Sep 09 02:34:01 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X082120W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 21 03:03:56 2020
Response via : Initial Calibration

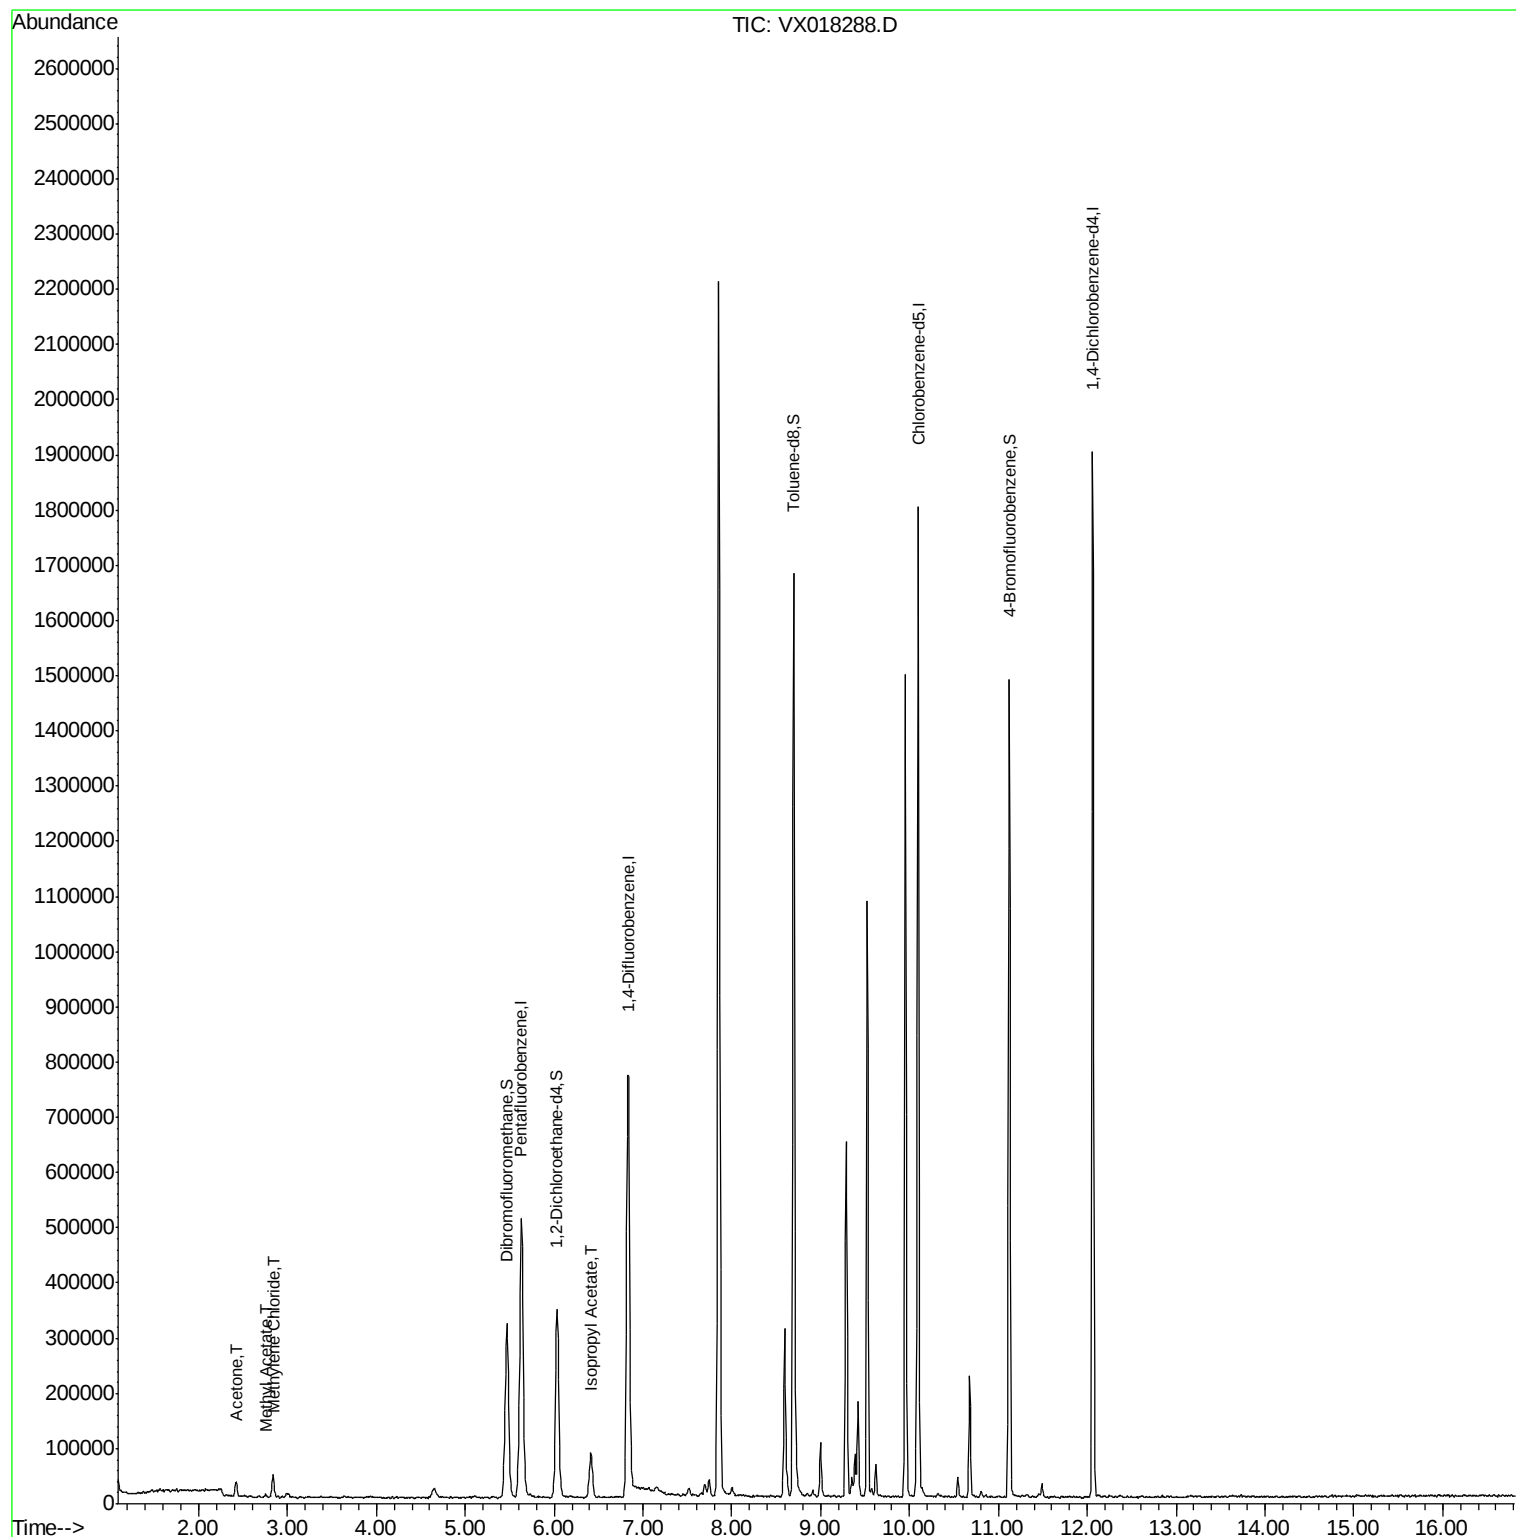

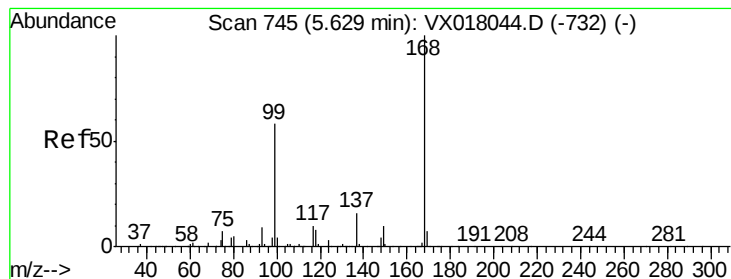

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 746

Delta R.T. 0.01 min

Lab File: VX018288.D

Acq: 08 Sep 2020 20:13

Instrument :

MSVOA_X

ClientSampleId :


PB131451ZHE#09

Tgt Ion:168 Resp: 470365

Ion Ratio Lower Upper

168 100

99 59.7 46.3 69.5

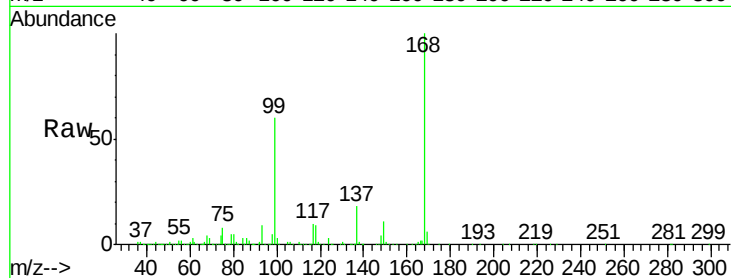

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63



150000

100000

50000

0

Time-->

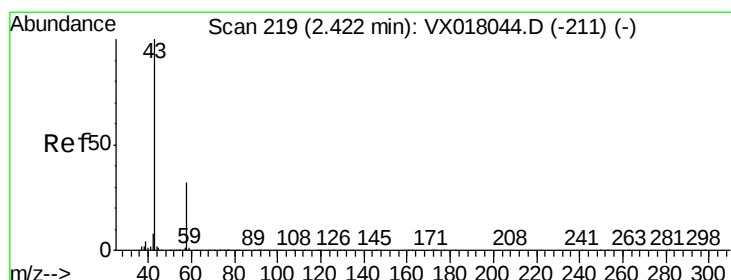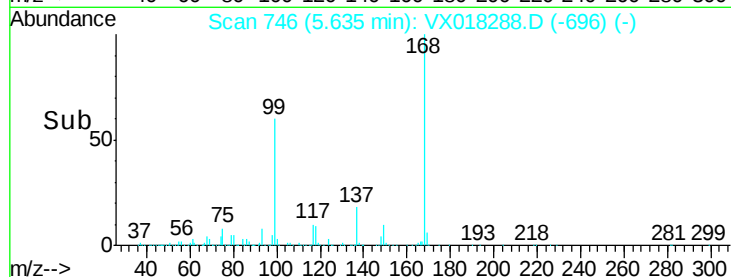

#16

Acetone

Concen: 11.298 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX018288.D


Acq: 08 Sep 2020 20:13

Tgt Ion: 43 Resp: 28747

Ion Ratio Lower Upper

43 100

58 29.1 25.5 38.3

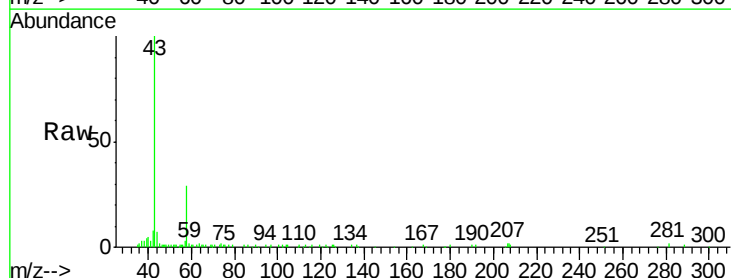

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

20000


15000


10000

5000

0

Time-->




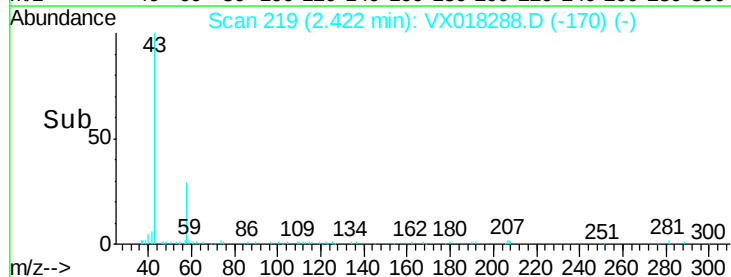


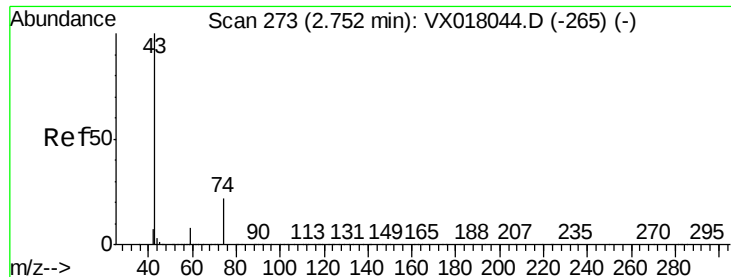

#18
Methyl Acetate
Concen: 1.020 ug/l
RT: 2.75 min Scan# 273
Delta R.T. -0.00 min
Lab File: VX018288.D
Acq: 08 Sep 2020 20:13




Instrument :
MSVOA_X
ClientSampleId :
PB131451ZHE#09

Tgt Ion: 43 Resp: 6265
Ion Ratio Lower Upper
43 100
74 27.0 18.2 27.4

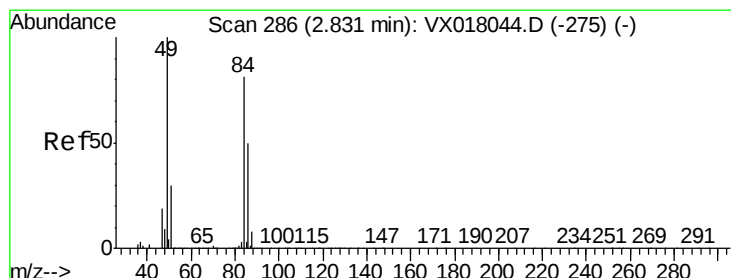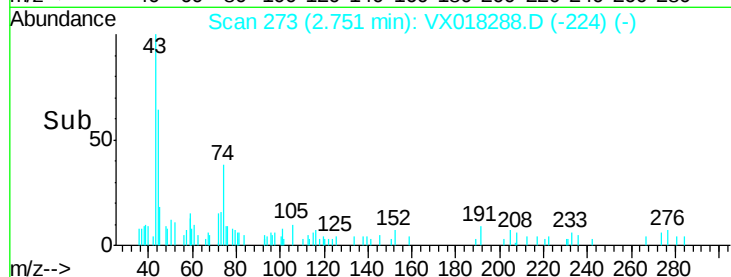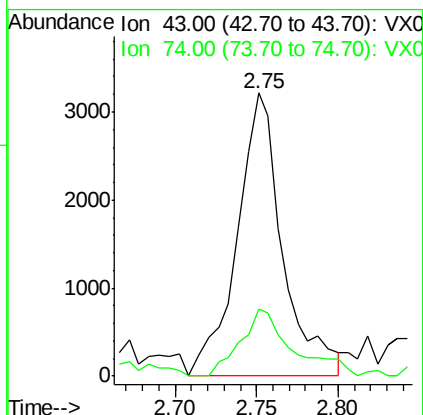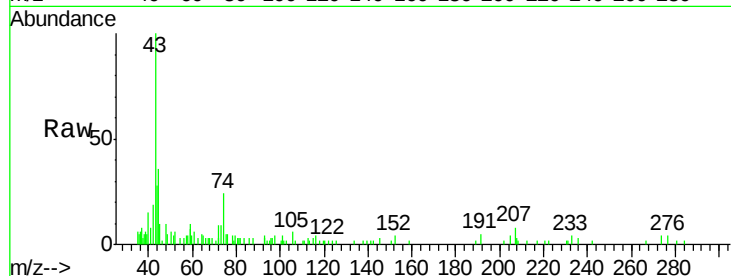

#20
Methylene Chloride
Concen: 2.669 ug/l
RT: 2.84 min Scan# 287
Delta R.T. 0.01 min
Lab File: VX018288.D
Acq: 08 Sep 2020 20:13

Tgt Ion: 84 Resp: 19636
Ion Ratio Lower Upper
84 100
49 118.6 98.6 148.0
51 42.5 29.6 44.4
86 60.2 49.8 74.6


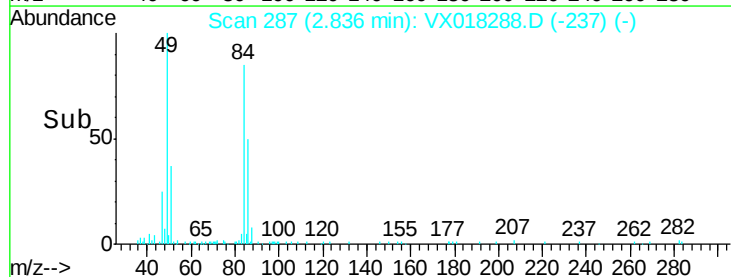
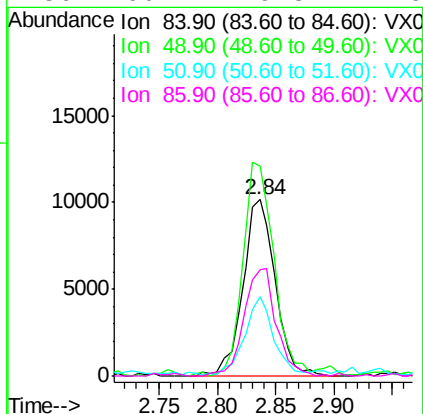
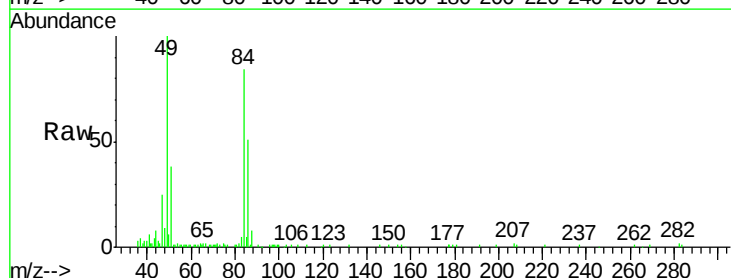




#33
 1,2-Dichloroethane-d4
 Concen: 52.083 ug/l
 RT: 6.03 min Scan# 811
 Delta R.T. -0.00 min
 Lab File: VX018288.D
 Acq: 08 Sep 2020 20:13




Instrument :
 MSVOA_X
 ClientSampleId :
 PB131451ZHE#09


Tgt Ion: 65 Resp: 340095
 Ion Ratio Lower Upper
 65 100
 67 51.2 0.0 105.8

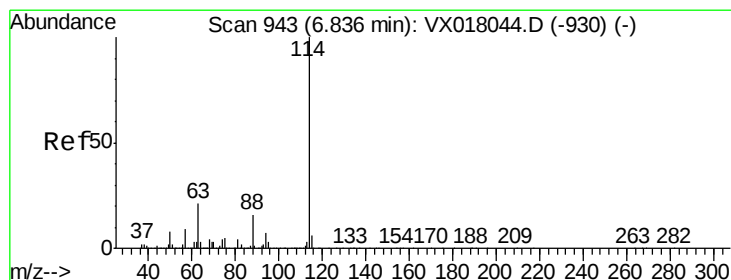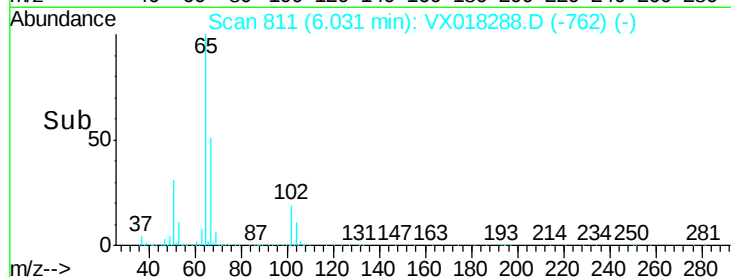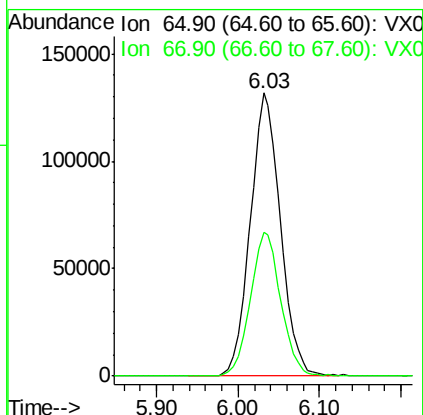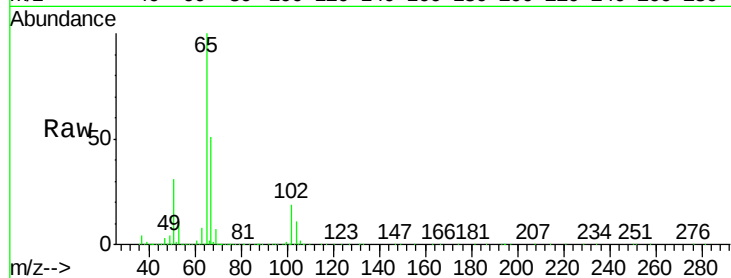

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.84 min Scan# 943
 Delta R.T. -0.00 min
 Lab File: VX018288.D
 Acq: 08 Sep 2020 20:13

Tgt Ion: 114 Resp: 765396
 Ion Ratio Lower Upper
 114 100
 63 20.8 0.0 42.6
 88 15.3 0.0 31.8

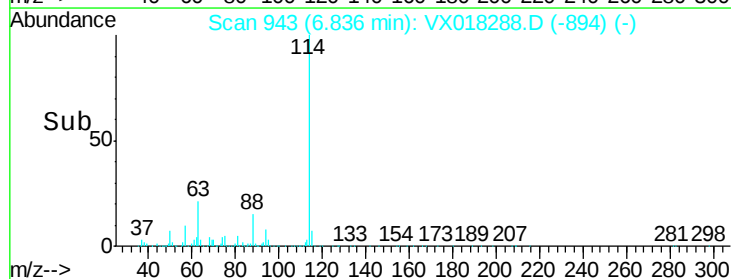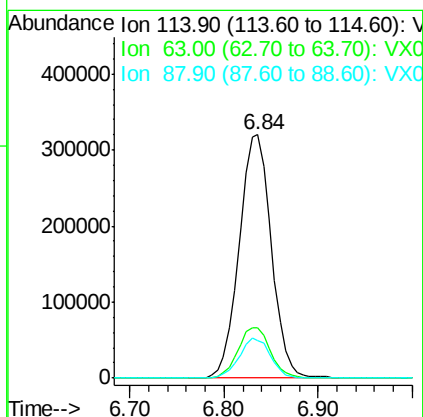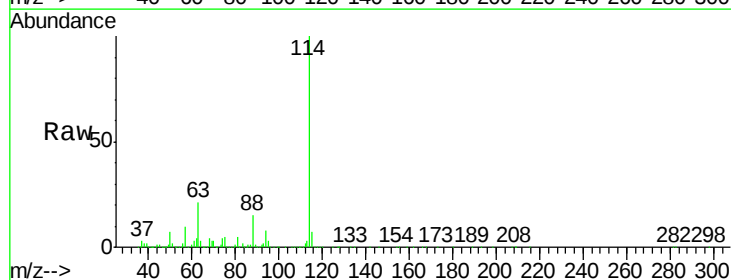

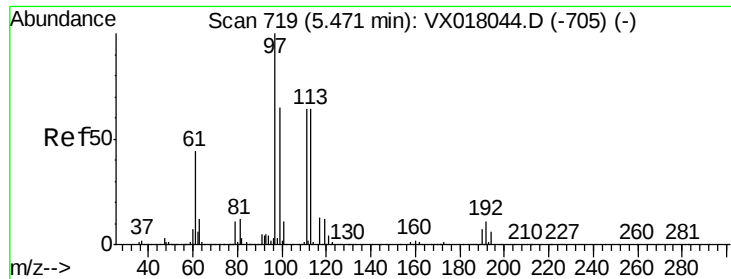

#35

Dibromofluoromethane

Concen: 52.054 ug/l

RT: 5.47 min Scan# 719

Delta R.T. -0.00 min

Lab File: VX018288.D

Acq: 08 Sep 2020 20:13

Instrument :

MSVOA_X

ClientSampleId :

PB131451ZHE#09


Tgt Ion:113 Resp: 271342

Ion Ratio Lower Upper

113 100

111 101.8 81.6 122.4




192 20.2 15.8 23.8

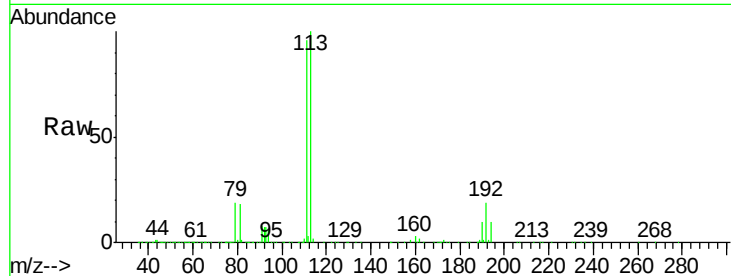

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

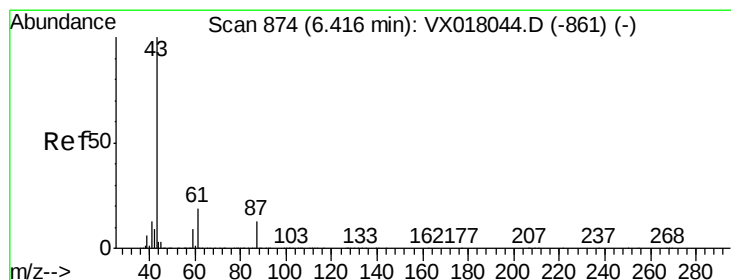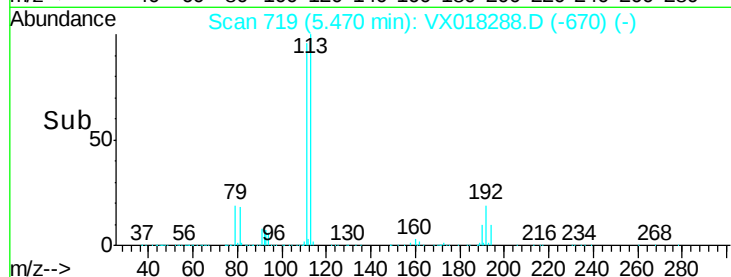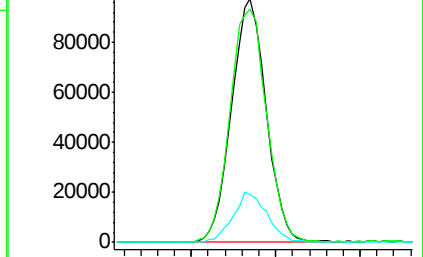

#43

Isopropyl Acetate

Concen: 8.472 ug/l

RT: 6.42 min Scan# 874

Delta R.T. -0.00 min

Lab File: VX018288.D

Acq: 08 Sep 2020 20:13


Tgt Ion: 43 Resp: 112197

Ion Ratio Lower Upper

43 100

61 19.9 15.7 23.5



87 13.0 10.3 15.5

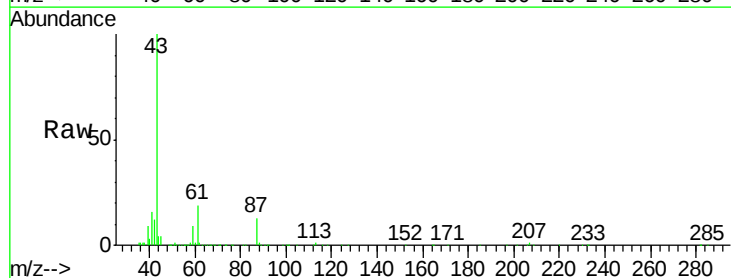


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

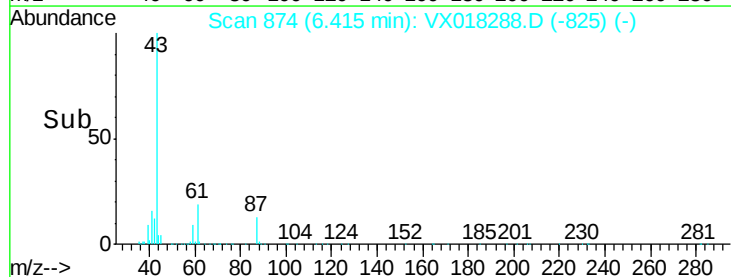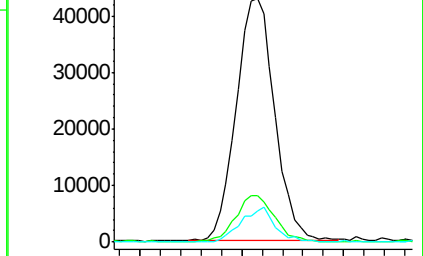

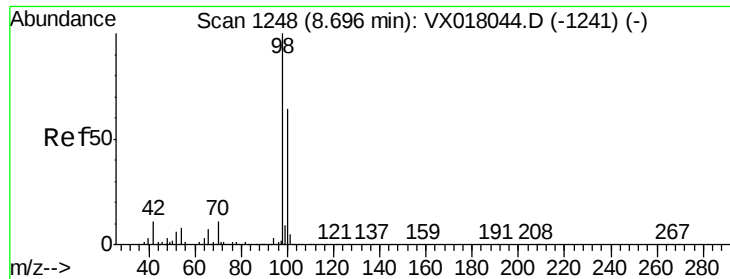

#50

Toluene-d8

Concen: 50.265 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX018288.D

Acq: 08 Sep 2020 20:13

Instrument :

MSVOA_X

ClientSampleId :





PB131451ZHE#09

Tgt Ion: 98 Resp: 975895

Ion Ratio Lower Upper

98 100

100 65.3 52.2 78.4

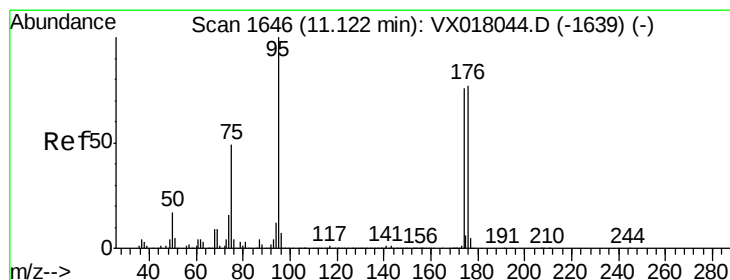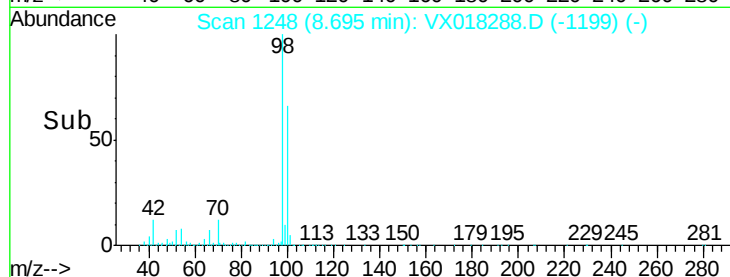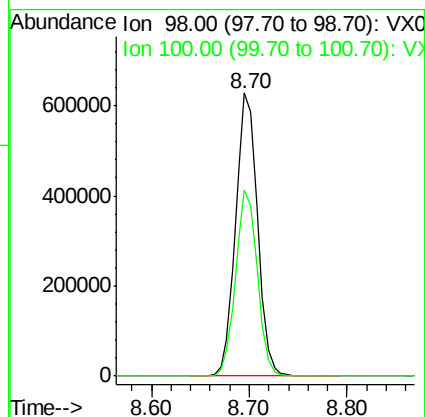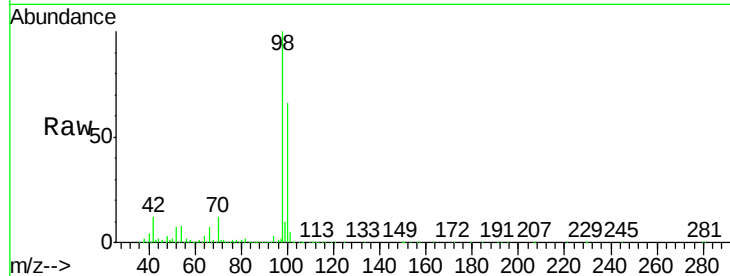

#62

4-Bromofluorobenzene

Concen: 48.530 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX018288.D

Acq: 08 Sep 2020 20:13




Tgt Ion: 95 Resp: 370704


Ion Ratio Lower Upper

95 100

174 81.9 0.0 160.2

176 77.9 0.0 155.8


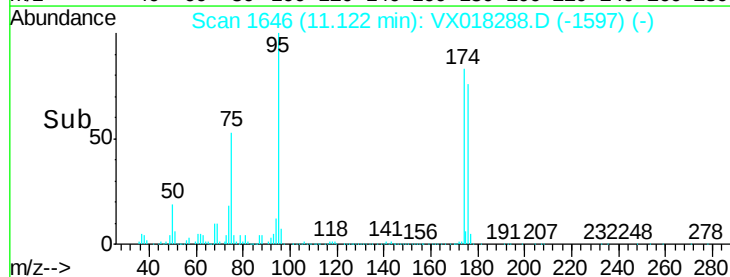
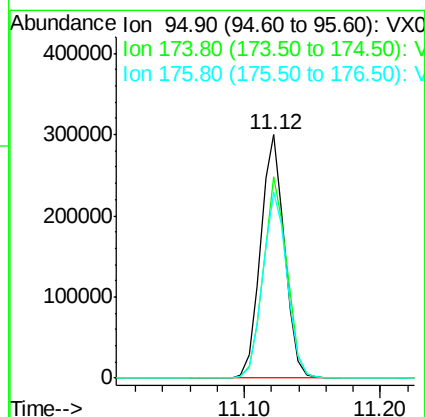
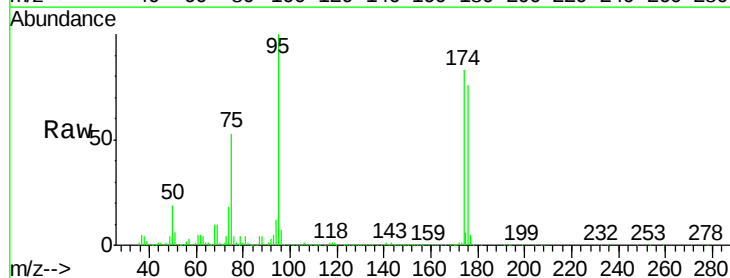


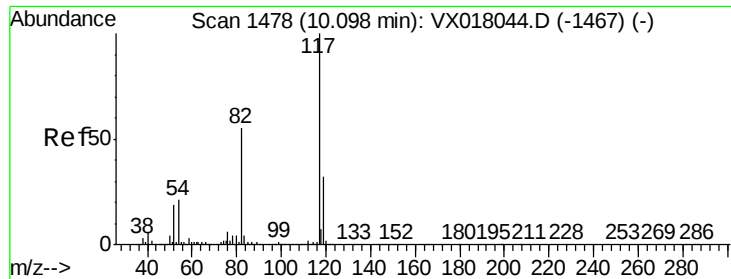

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX018288.D
Acq: 08 Sep 2020 20:13

Instrument :
MSVOA_X
ClientSampleId :
PB131451ZHE#09

Tgt Ion:117 Resp: 793563
Ion Ratio Lower Upper
117 100
82 53.2 44.2 66.2
119 31.7 25.7 38.5

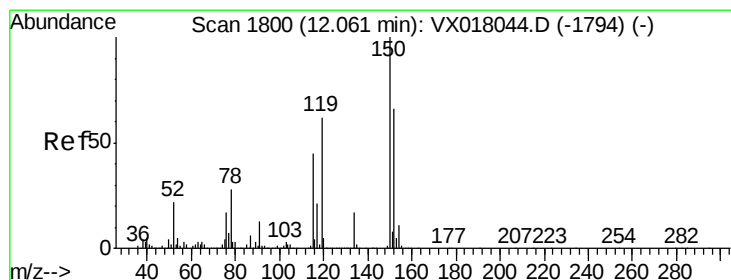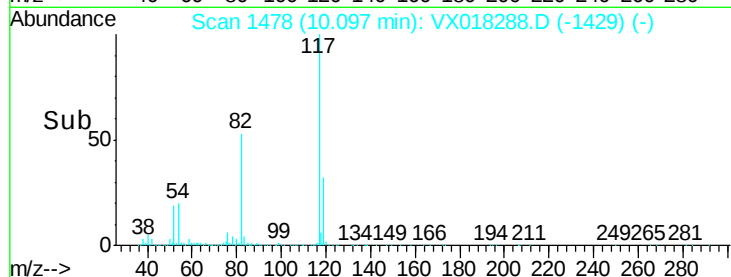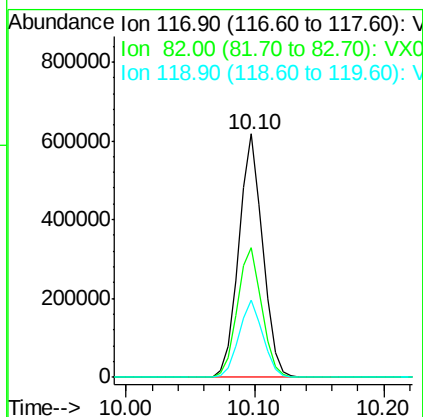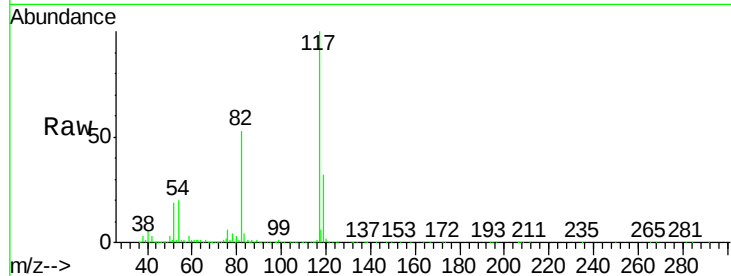

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX018288.D
Acq: 08 Sep 2020 20:13

Tgt Ion:152 Resp: 382719
Ion Ratio Lower Upper
152 100
115 61.6 41.5 124.5
150 160.0 0.0 343.8

