


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX090820\
 Data File : VX018262.D
 Acq On : 08 Sep 2020 09:37
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082120W.M
 Title : SW846 8260
 Last Update : Fri Aug 21 03:03:56 2020

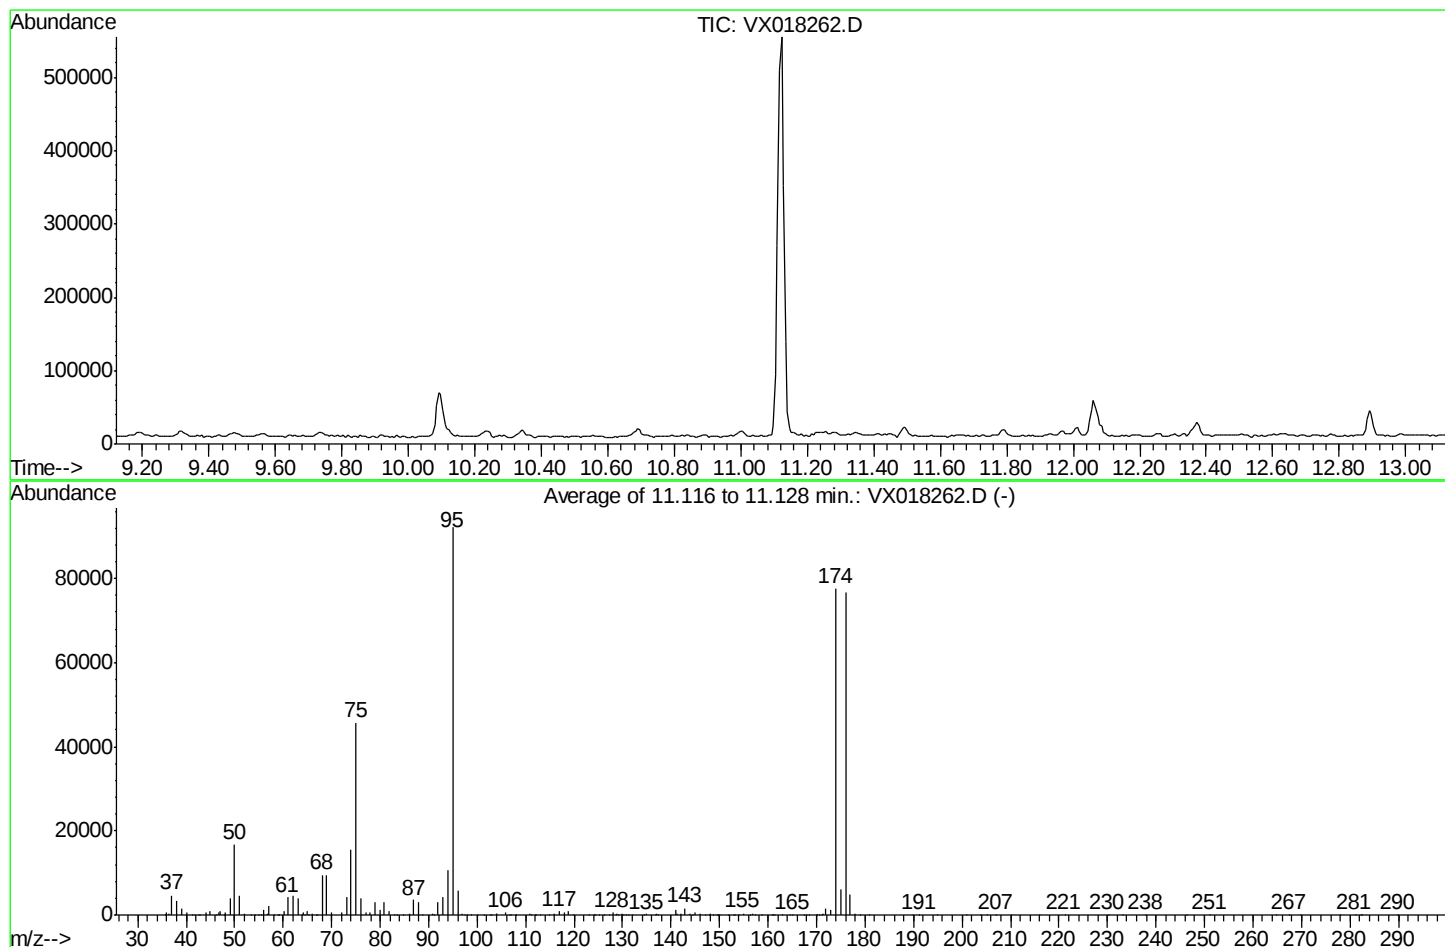

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	16660	PASS
75	95	30	60	49.6	45670	PASS
95	95	100	100	100.0	92149	PASS
96	95	5	9	6.3	5793	PASS
173	174	0.00	2	1.7	1286	PASS
174	95	50	100	84.1	77538	PASS
175	174	5	9	7.9	6120	PASS
176	174	95	101	98.8	76613	PASS
177	176	5	9	6.6	5029	PASS