


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX090820\
Data File : VX018290.D
Acq On : 08 Sep 2020 21:21
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082120W.M
Title : SW846 8260
Last Update : Fri Aug 21 03:03:56 2020

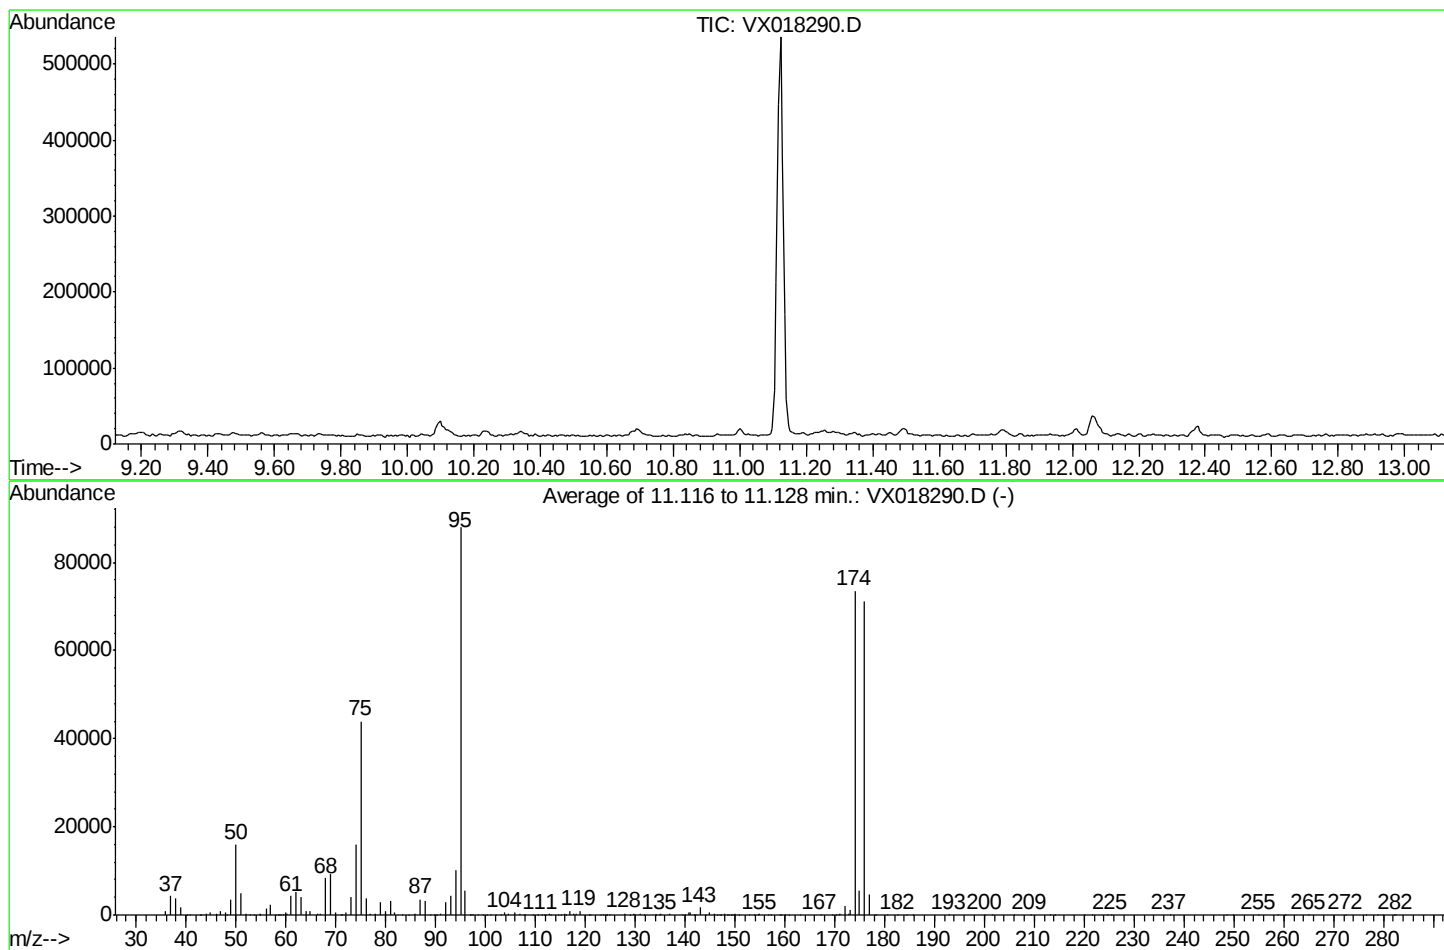

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	15938	PASS
75	95	30	60	50.0	43969	PASS
95	95	100	100	100.0	87978	PASS
96	95	5	9	6.4	5604	PASS
173	174	0.00	2	1.4	1060	PASS
174	95	50	100	83.6	73546	PASS
175	174	5	9	7.3	5391	PASS
176	174	95	101	96.7	71125	PASS
177	176	5	9	6.6	4701	PASS