

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090821\
 Data File : VX024131.D
 Acq On : 08 Sep 2021 12:33
 Operator : JC/MD
 Sample : M3675-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-VPB-RW7-GW-720-722

Quant Time: Sep 09 05:43:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 11:57:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	146046	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	245903	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	225369	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	87102	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	112682	55.281	ug/l	0.00
Spiked Amount	50.000	Range 78 - 117	Recovery	= 110.560%		
35) Dibromofluoromethane	5.391	113	85719	52.667	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	= 105.340%		
50) Toluene-d8	8.653	98	314428	50.758	ug/l	0.00
Spiked Amount	50.000	Range 92 - 112	Recovery	= 101.520%		
62) 4-Bromofluorobenzene	11.085	95	107386	47.091	ug/l	0.00
Spiked Amount	50.000	Range 83 - 123	Recovery	= 94.180%		
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.172	85	365	0.237	ug/l	78
3) Chloromethane	1.294	50	491	0.290	ug/l #	86
5) Bromomethane	1.630	94	595	0.574	ug/l	97
6) Chloroethane	1.666	64	65	2.263	ug/l #	43
9) 1,1,2-Trichlorotrifluo...	2.331	101	19206	13.101	ug/l	97
10) Methyl Iodide	2.465	142	855	0.419	ug/l #	88
11) Tert butyl alcohol	2.971	59	250	0.606	ug/l #	73
12) 1,1-Dichloroethene	2.325	96	16473	11.753	ug/l	98
16) Acetone	2.392	43	6583	7.223	ug/l #	82
17) Carbon Disulfide	2.520	76	819	0.245	ug/l #	75
20) Methylene Chloride	2.794	84	402	0.231	ug/l #	75
24) 1,1-Dichloroethane	3.623	63	3120	1.090	ug/l #	94
25) 2-Butanone	4.586	43	801	0.580	ug/l	92
27) cis-1,2-Dichloroethene	4.501	96	4178	2.345	ug/l	96
28) Bromochloromethane	5.111	49	331	0.254	ug/l #	9
30) Chloroform	5.111	83	3263	1.076	ug/l	99
31) Cyclohexane	5.556	56	3322	1.269	ug/l #	28
32) 1,1,1-Trichloroethane	5.397	97	2747	1.058	ug/l #	49
36) 1,1-Dichloropropene	5.562	75	11745	5.158	ug/l #	50
37) Ethyl Acetate	4.586	43	801	0.286	ug/l #	64
38) Carbon Tetrachloride	5.690	117	5818	2.450	ug/l #	93
39) Methylcyclohexane	7.135	83	5603	2.021	ug/l #	1
42) 1,2-Dichloroethane	6.104	62	930	0.351	ug/l #	73
44) Trichloroethene	7.135	130	448689	241.213	ug/l	100
49) 1,4-Dioxane	7.683	88	388	8.595	ug/l #	83
51) 4-Methyl-2-Pentanone	8.653	43	1630	0.576	ug/l #	1
55) 1,1,2-Trichloroethane	9.159	97	1727	0.961	ug/l #	86
60) Dibromochloromethane	9.281	129	171	1.771	ug/l #	11
76) 1,2,3-Trichloropropane	11.085	75	57881	28.487	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	57881	83.795	ug/l #	12
95) Naphthalene	13.780	128	280	1.325	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090821\
Data File : VX024131.D
Acq On : 08 Sep 2021 12:33
Operator : JC/MD
Sample : M3675-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722

Quant Time: Sep 09 05:43:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 11:57:51 2021
Response via : Initial Calibration




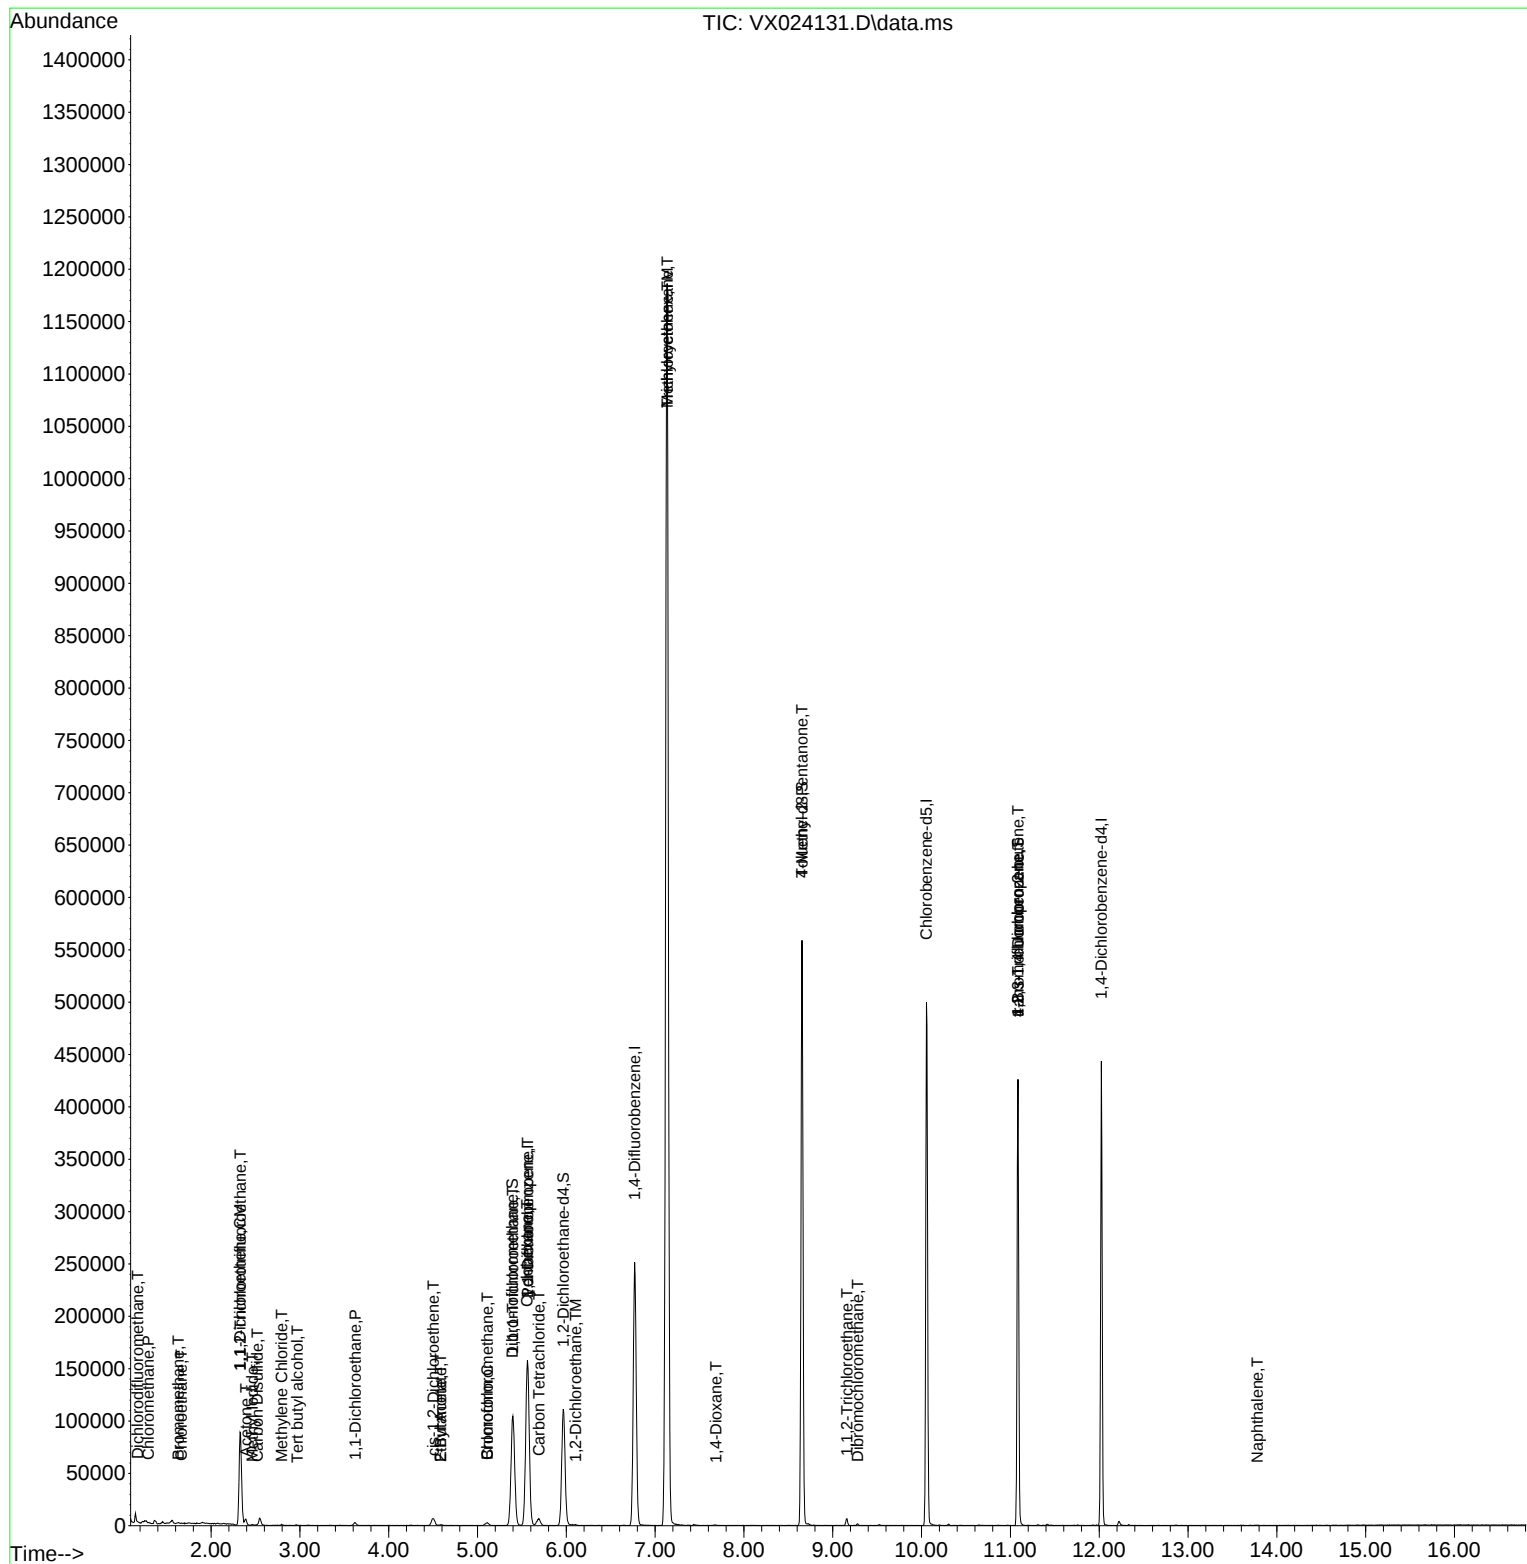


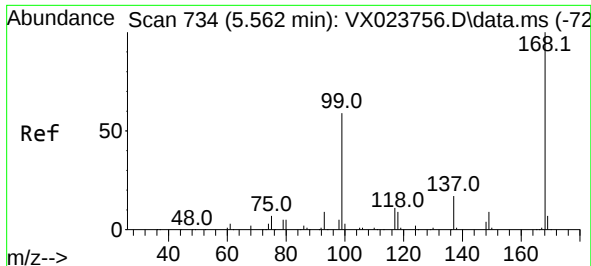

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion:168 Resp: 146046
Ion Ratio Lower Upper
168 100
99 61.3 45.8 68.6

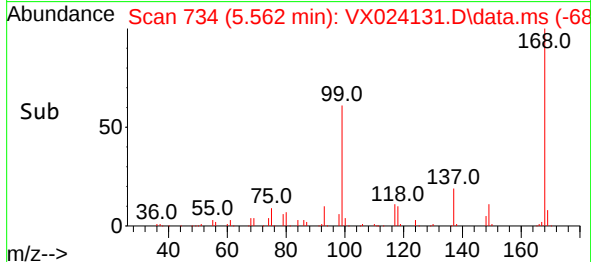

#2
Dichlorodifluoromethane
Concen: 0.237 ug/l
RT: 1.172 min Scan# 14
Delta R.T. -0.001 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 85 Resp: 365
Ion Ratio Lower Upper
85 100
87 20.3 16.4 49.2


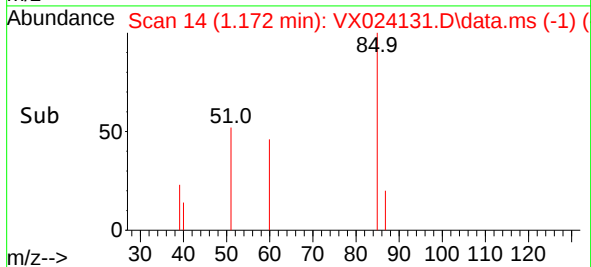

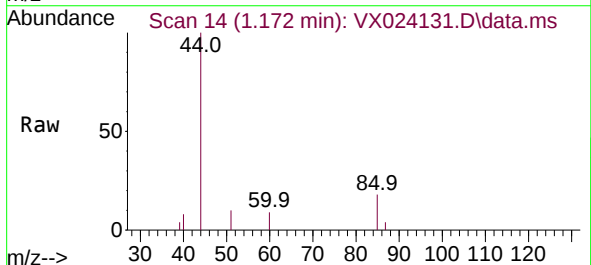


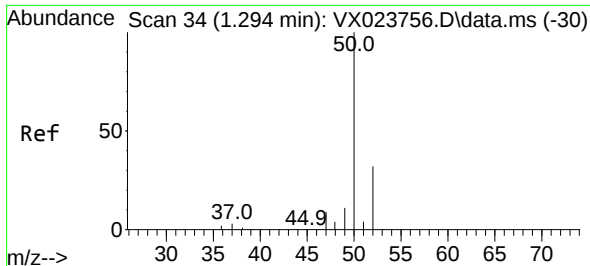

#3
Chloromethane
Concen: 0.290 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion: 50 Resp: 491
Ion Ratio Lower Upper
50 100
52 25.3 26.4 39.6#

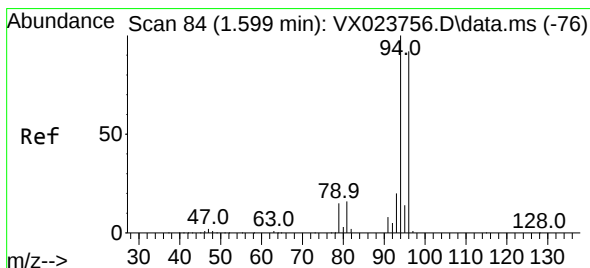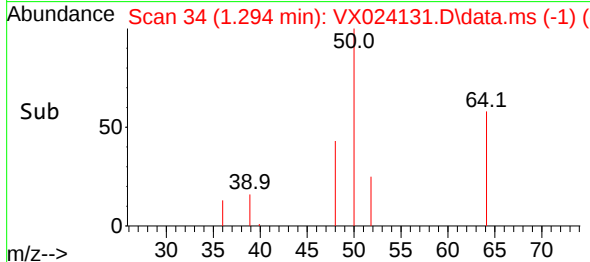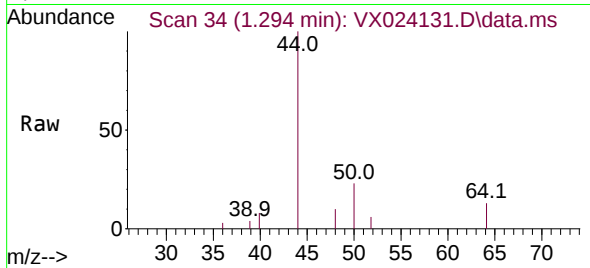

#5
Bromomethane
Concen: 0.574 ug/l
RT: 1.630 min Scan# 89
Delta R.T. 0.031 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 94 Resp: 595
Ion Ratio Lower Upper
94 100
96 92.5 76.4 114.6


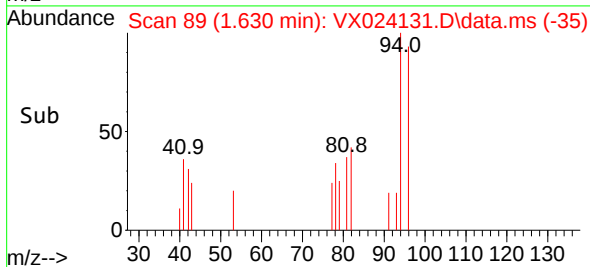

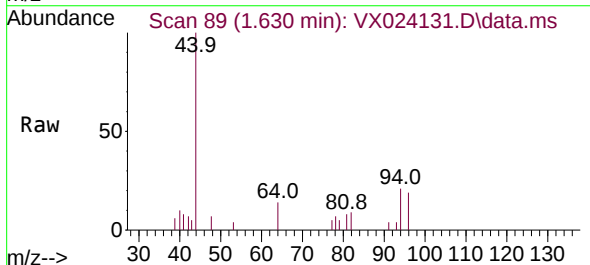


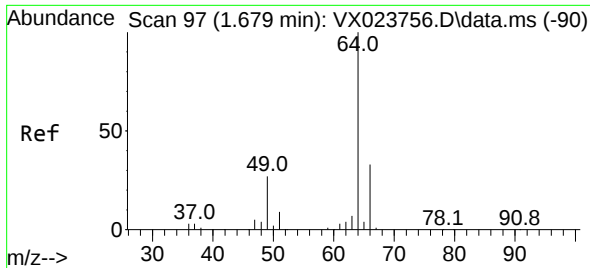

#6
Chloroethane
Concen: 2.263 ug/l
RT: 1.666 min Scan# 95
Delta R.T. -0.013 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion: 64 Resp: 65
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

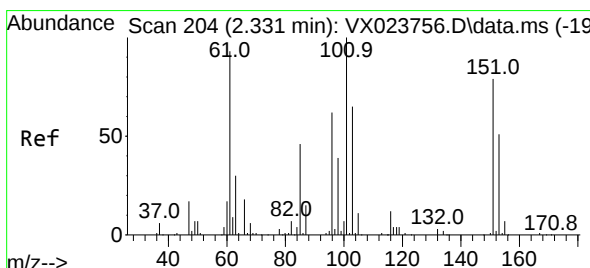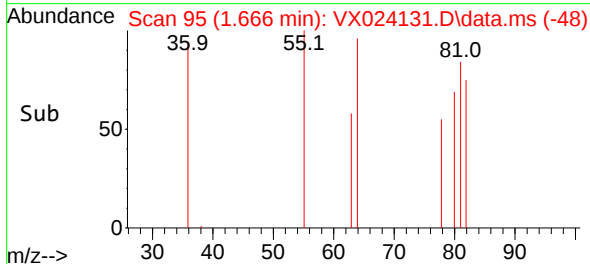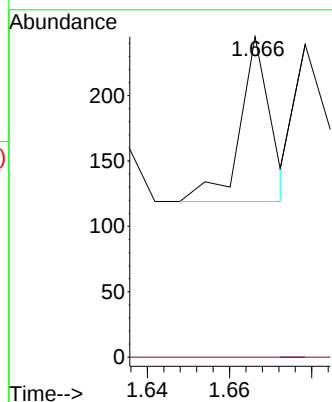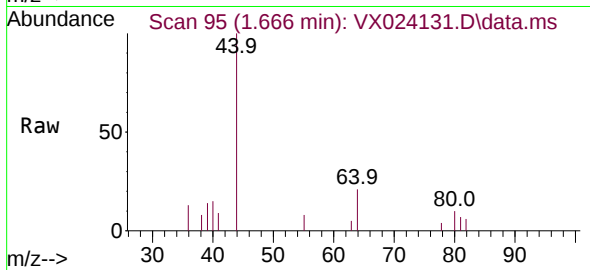

#9
1,1,2-Trichlorotrifluoroethane
Concen: 13.101 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33


Tgt Ion: 101 Resp: 19206
Ion Ratio Lower Upper
101 100
85 46.2 34.9 52.3
151 78.9 61.4 92.2

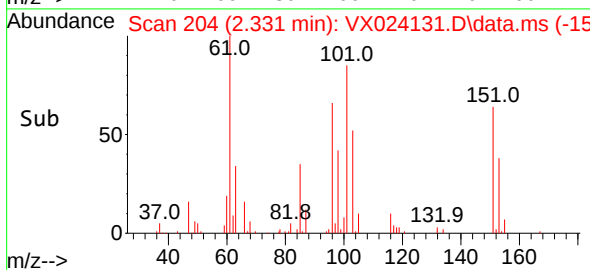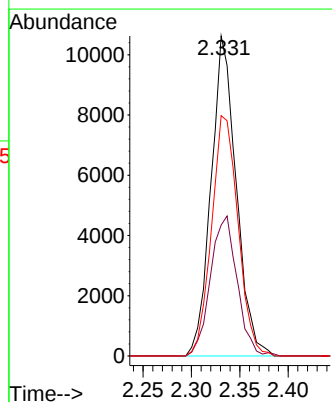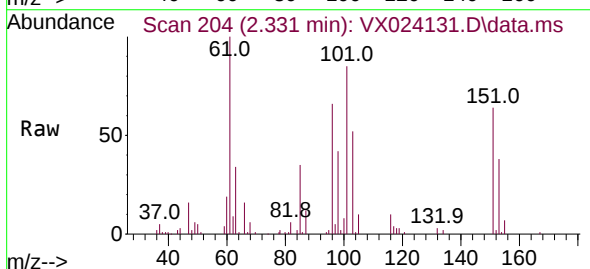






#10
Methyl Iodide
Concen: 0.419 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722







Tgt Ion:142 Resp: 855
Ion Ratio Lower Upper
142 100
127 48.7 33.3 49.9
141 8.5 11.4 17.0#

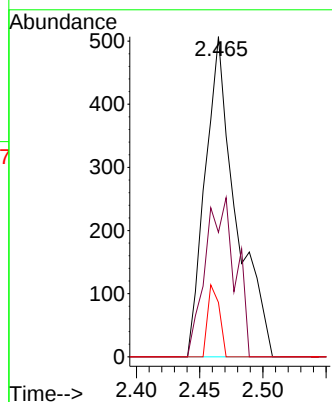

#11
Tert butyl alcohol
Concen: 0.606 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.012 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 59 Resp: 250
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

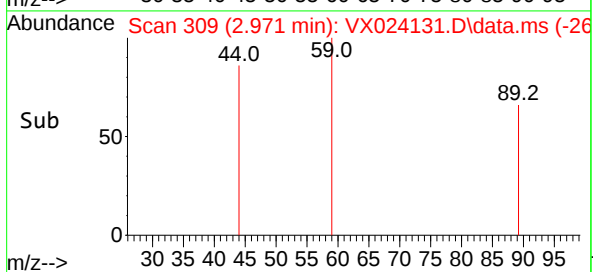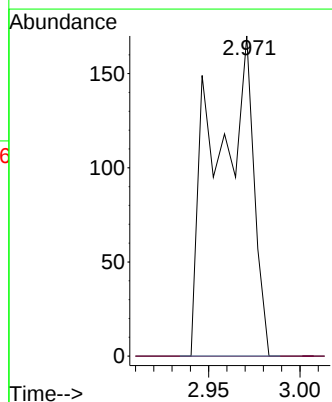



#12

1,1-Dichloroethene

Concen: 11.753 ug/l

RT: 2.325 min Scan# 203

Delta R.T. 0.006 min

Lab File: VX024131.D

Acq: 08 Sep 2021 12:33





Tgt Ion: 96 Resp: 16473

Ion Ratio Lower Upper

96 100

61 158.5 124.6 187.0

98 63.1 50.6 76.0

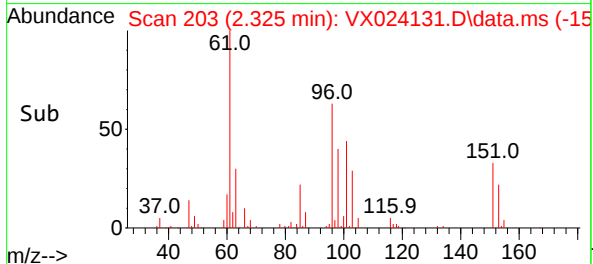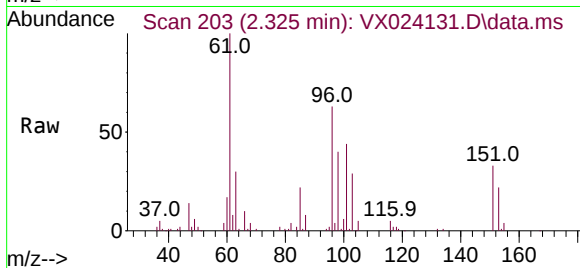

#16

Acetone

Concen: 7.223 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX024131.D




Acq: 08 Sep 2021 12:33


Tgt Ion: 43 Resp: 6583

Ion Ratio Lower Upper

43 100


58 24.3 27.8 41.8#

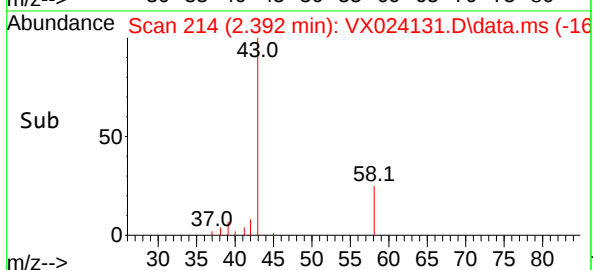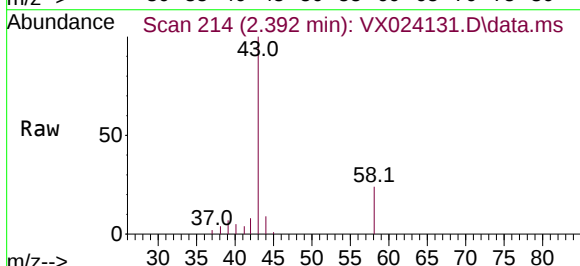






#17
Carbon Disulfide
Concen: 0.245 ug/l
RT: 2.520 min Scan# 235
Delta R.T. 0.006 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722







Tgt Ion: 76 Resp: 819
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

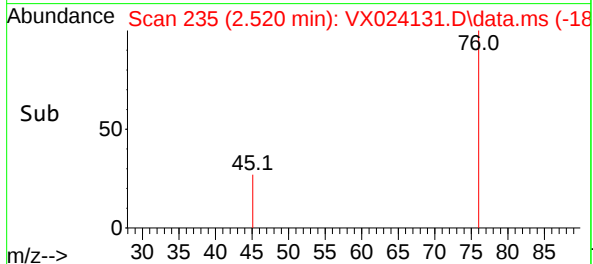

#20
Methylene Chloride
Concen: 0.231 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 84 Resp: 402
Ion Ratio Lower Upper
84 100
49 75.2 88.6 132.8#
51 40.4 27.0 40.6
86 50.0 50.3 75.5#

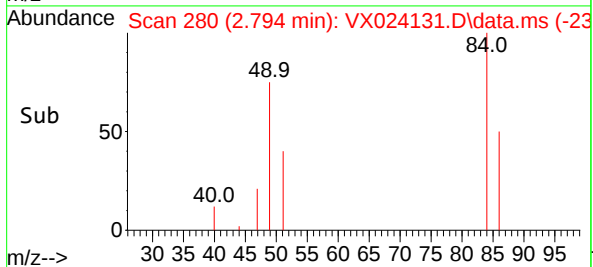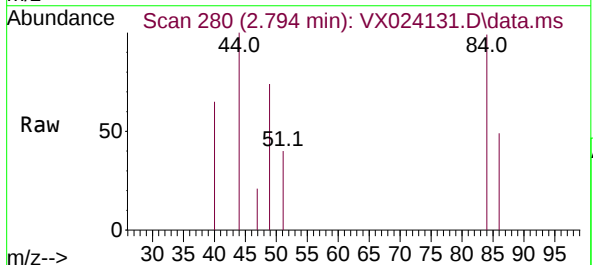



#24

1,1-Dichloroethane

Concen: 1.090 ug/l

RT: 3.623 min Scan# 416

Delta R.T. 0.006 min

Lab File: VX024131.D

Acq: 08 Sep 2021 12:33





Tgt Ion: 63	Resp: 3120
Ion Ratio	Lower Upper
63 100	
98 7.6	3.8 11.2
100 0.0	2.5 7.5#

Instrument :

MSVOA_X

ClientSampleId :

BP-TT-VPB-RW7-GW-720-722

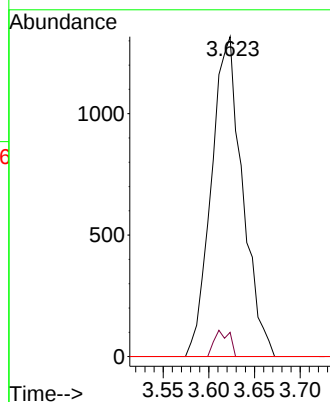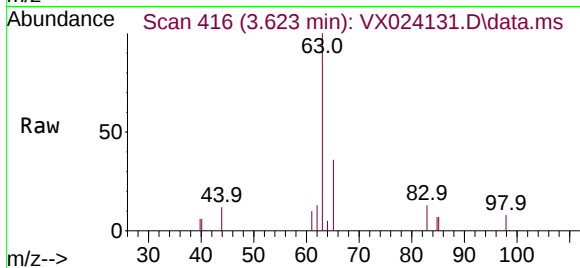

#25

2-Butanone

Concen: 0.580 ug/l




RT: 4.586 min Scan# 574


Delta R.T. 0.018 min

Lab File: VX024131.D

Acq: 08 Sep 2021 12:33

Tgt Ion: 43	Resp: 801
Ion Ratio	Lower Upper
43 100	
72 33.9	23.7 35.5

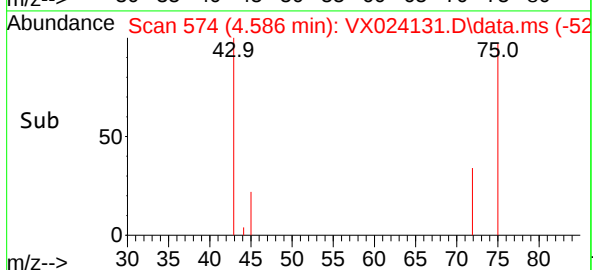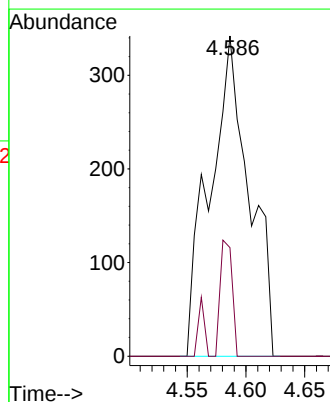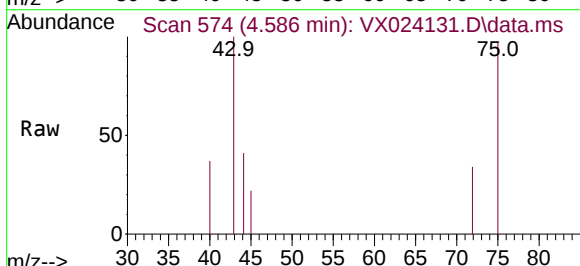



#27

cis-1,2-Dichloroethene

Concen: 2.345 ug/l

RT: 4.501 min Scan# 560

Delta R.T. 0.000 min

Lab File: VX024131.D

Acq: 08 Sep 2021 12:33

Tgt Ion: 96 Resp: 4178





Ion	Ratio	Lower	Upper
96	100		
61	136.9	0.0	285.6
98	66.6	0.0	129.6

Instrument :

MSVOA_X

ClientSampleId :

BP-TT-VPB-RW7-GW-720-722

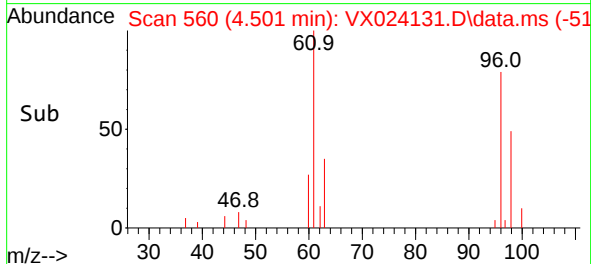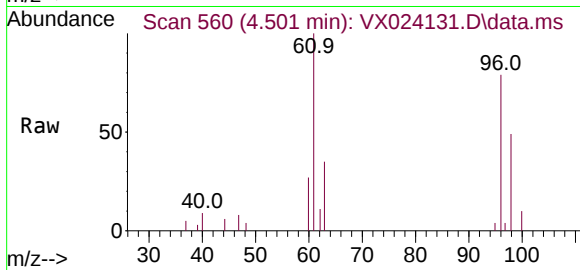

#28

Bromochloromethane

Concen: 0.254 ug/l

RT: 5.111 min Scan# 660




Delta R.T. 0.201 min


Lab File: VX024131.D

Acq: 08 Sep 2021 12:33

Tgt Ion: 49 Resp: 331

Ion	Ratio	Lower	Upper
49	100		
129	0.0	0.0	4.0
130	0.0	68.2	102.2#


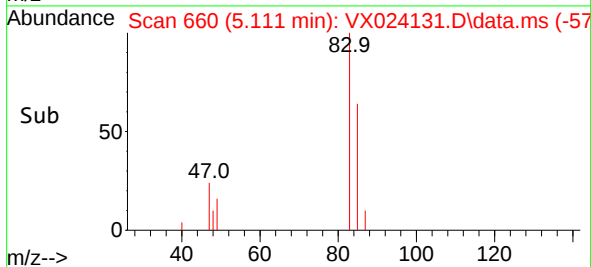

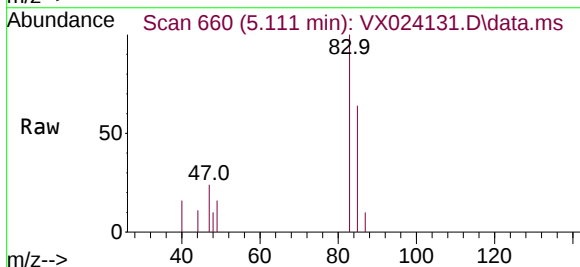




#30
Chloroform
Concen: 1.076 ug/l
RT: 5.111 min Scan# 660
Delta R.T. 0.006 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion: 83 Resp: 3263
Ion Ratio Lower Upper
83 100
85 63.9 52.0 78.0

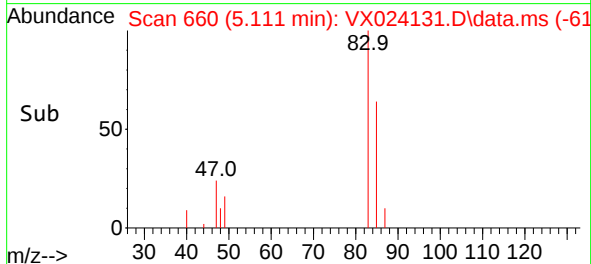

#31
Cyclohexane
Concen: 1.269 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.079 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 56 Resp: 3322
Ion Ratio Lower Upper
56 100
69 154.9 25.3 37.9#
84 107.2 71.4 107.0#

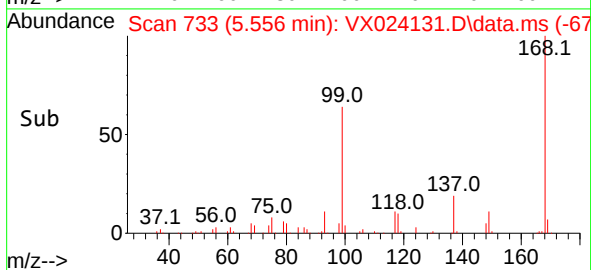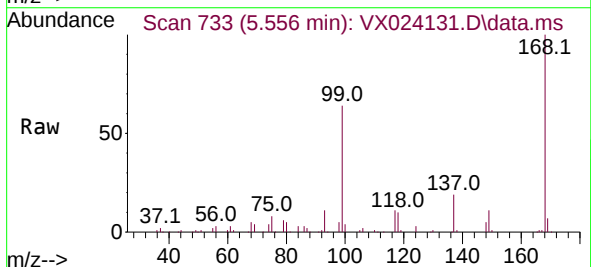







#32

1,1,1-Trichloroethane
Concen: 1.058 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722




Tgt Ion: 97 Resp: 2747
Ion Ratio Lower Upper
97 100
99 0.0 51.5 77.3#
61 46.2 34.2 51.4

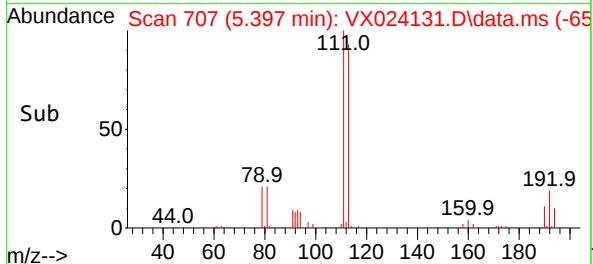


#33

1,2-Dichloroethane-d4
Concen: 55.281 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 65 Resp: 112682
Ion Ratio Lower Upper
65 100
67 49.9 0.0 105.4


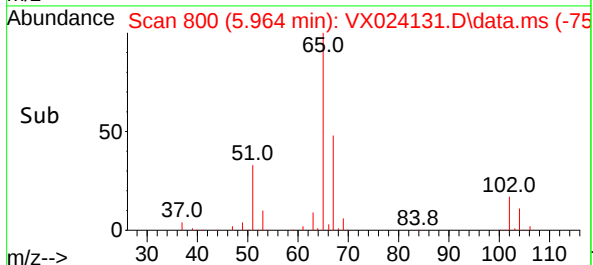

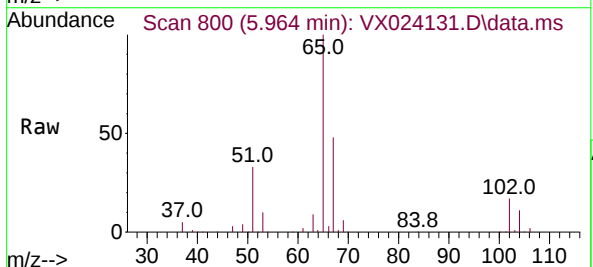




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion:	114	Resp:	245903
Ion Ratio	Lower	Upper	
114	100		
63	20.3	0.0	40.8
88	16.7	0.0	32.8

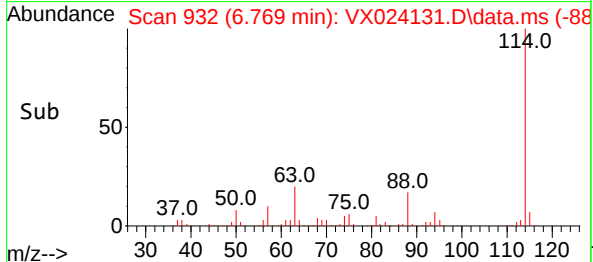

#35
Dibromofluoromethane
Concen: 52.667 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion:	113	Resp:	85719
Ion Ratio	Lower	Upper	
113	100		
111	104.2	81.9	122.9
192	20.3	16.7	25.1


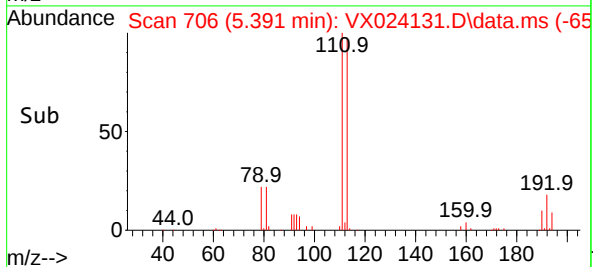

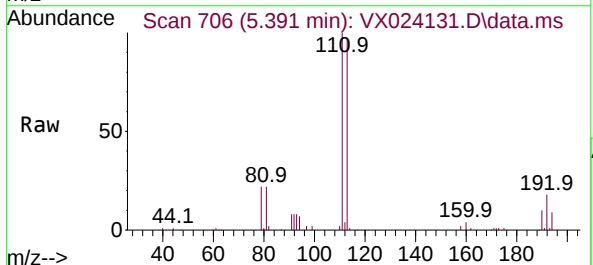


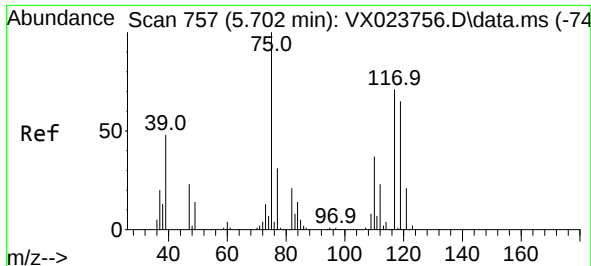

#36
1,1-Dichloropropene
Concen: 5.158 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.140 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion: 75 Resp: 11745
Ion Ratio Lower Upper
75 100
110 10.2 18.1 54.4#
77 0.0 25.3 37.9#

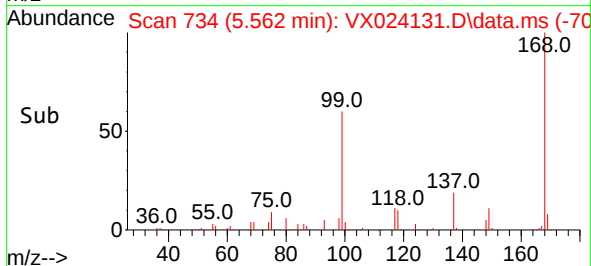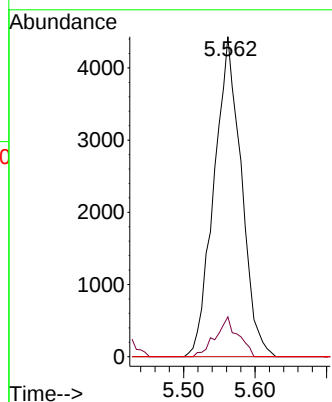

#37
Ethyl Acetate
Concen: 0.286 ug/l
RT: 4.586 min Scan# 574
Delta R.T. -0.141 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 43 Resp: 801
Ion Ratio Lower Upper
43 100
61 0.0 12.8 19.2#
70 0.0 10.5 15.7#


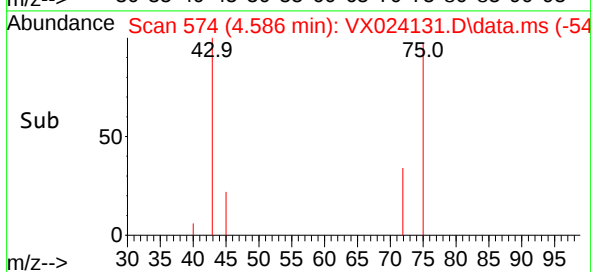
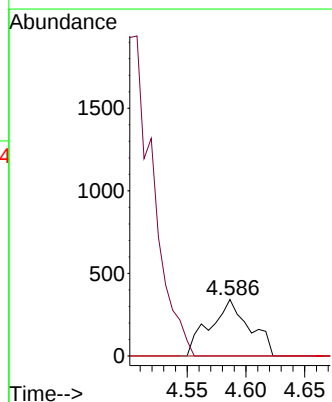
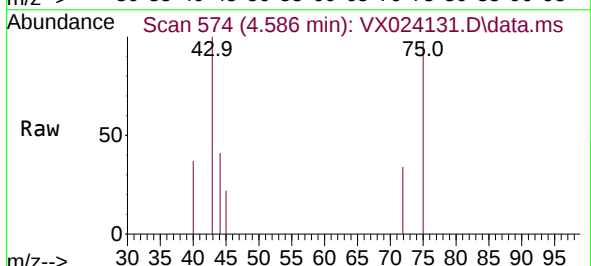




#38
Carbon Tetrachloride
Concen: 2.450 ug/l
RT: 5.690 min Scan# 755
Delta R.T. -0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion:117 Resp: 5818
Ion Ratio Lower Upper
117 100
119 99.9 76.2 114.2
121 39.0 24.8 37.2#

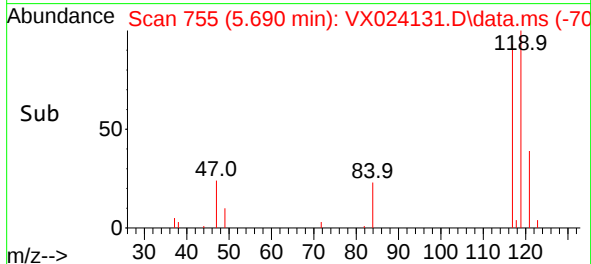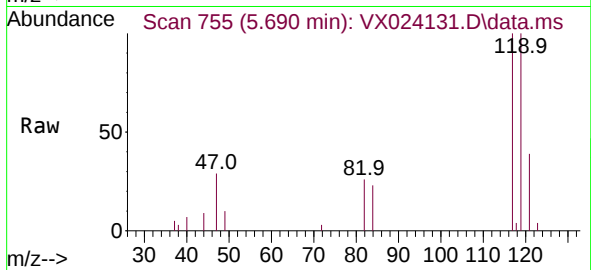

#39
Methylcyclohexane
Concen: 2.021 ug/l
RT: 7.135 min Scan# 992
Delta R.T. -0.250 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 83 Resp: 5603
Ion Ratio Lower Upper
83 100
55 0.0 58.9 88.3#
98 199.3 38.1 57.1#

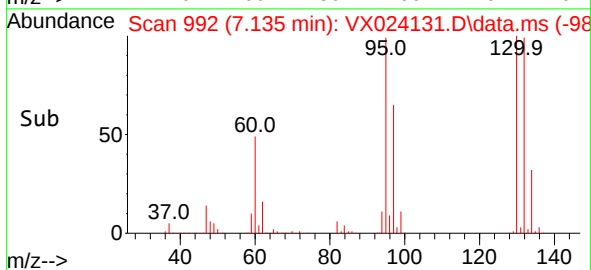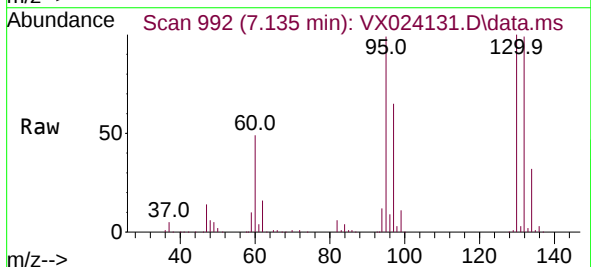

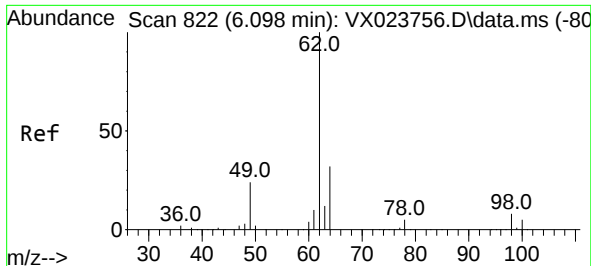

#42

1,2-Dichloroethane

Concen: 0.351 ug/l

RT: 6.104 min Scan# 823

Delta R.T. 0.006 min

Lab File: VX024131.D





Acq: 08 Sep 2021 12:33

Tgt Ion: 62 Resp: 930

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.2

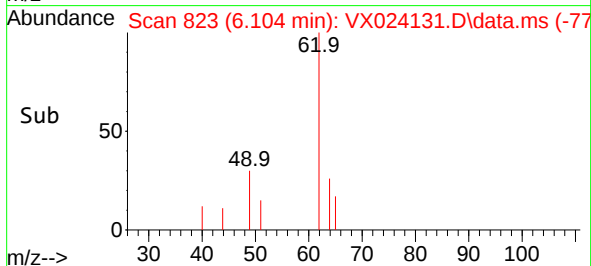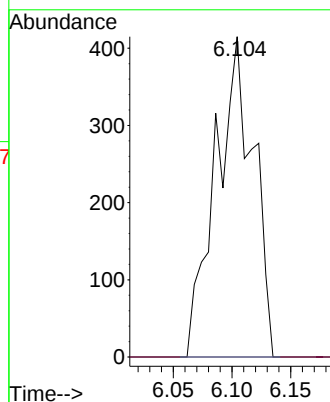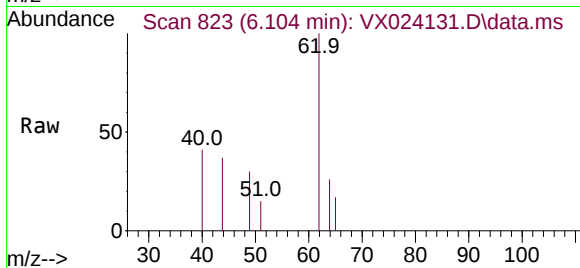

#44

Trichloroethene

Concen: 241.213 ug/l

RT: 7.135 min Scan# 992

Delta R.T. 0.006 min

Lab File: VX024131.D




Acq: 08 Sep 2021 12:33


Tgt Ion: 130 Resp: 448689

Ion Ratio Lower Upper

130 100

95 98.6 0.0 198.0


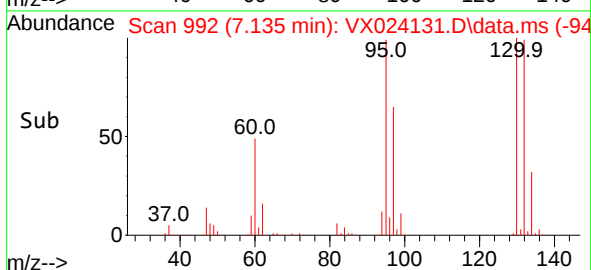

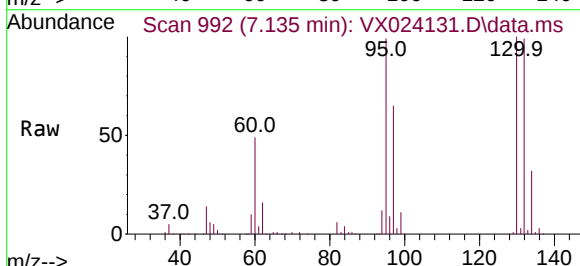


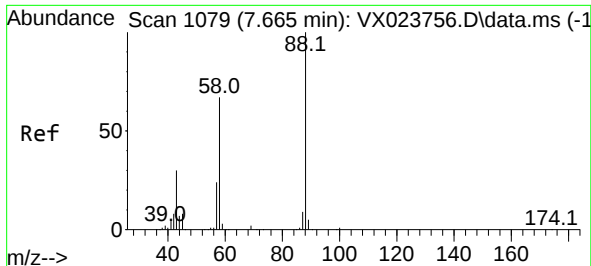

#49
1,4-Dioxane
Concen: 8.595 ug/l
RT: 7.683 min Scan# 1082
Delta R.T. 0.018 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion: 88 Resp: 388
Ion Ratio Lower Upper
88 100
43 29.4 23.2 34.8
58 49.5 55.0 82.4#

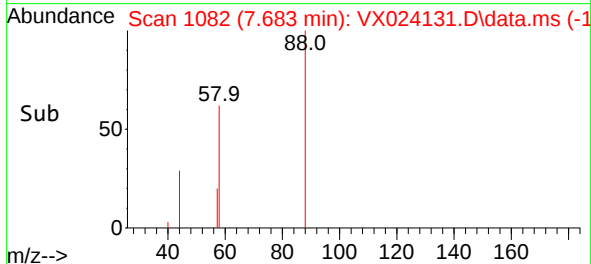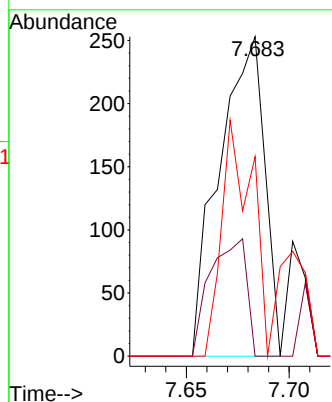

#50
Toluene-d8
Concen: 50.758 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 98 Resp: 314428
Ion Ratio Lower Upper
98 100
100 63.1 51.9 77.9


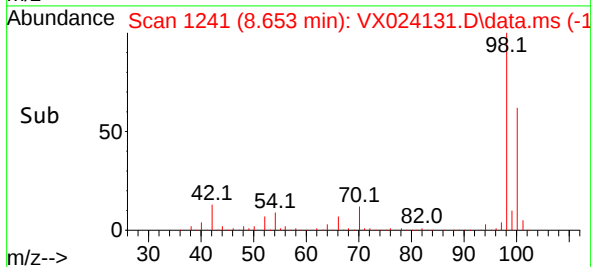
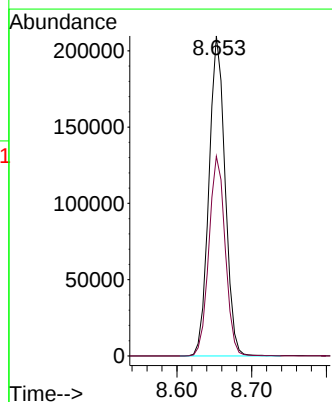
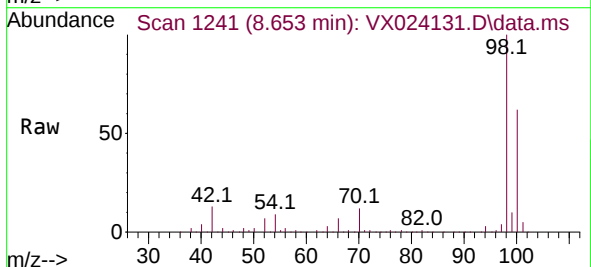




#51
4-Methyl-2-Pentanone
Concen: 0.576 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.073 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion: 43 Resp: 1630
Ion Ratio Lower Upper
43 100
58 171.8 35.4 53.0#

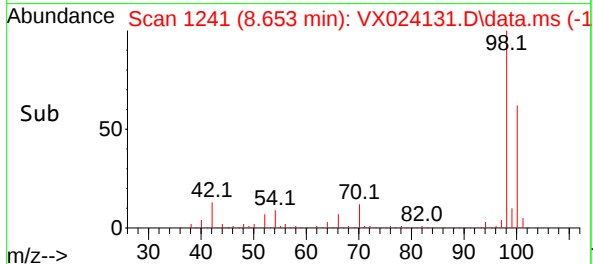

#55
1,1,2-Trichloroethane
Concen: 0.961 ug/l
RT: 9.159 min Scan# 1324
Delta R.T. -0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 97 Resp: 1727
Ion Ratio Lower Upper
97 100
83 68.9 69.3 103.9#
85 50.2 44.3 66.5
99 54.1 50.3 75.5


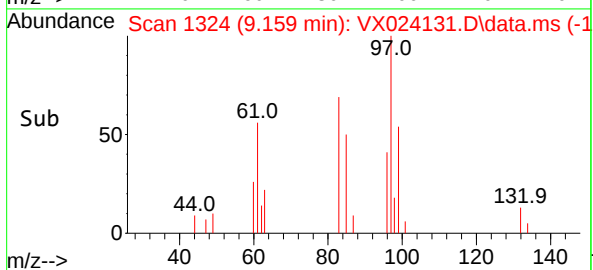

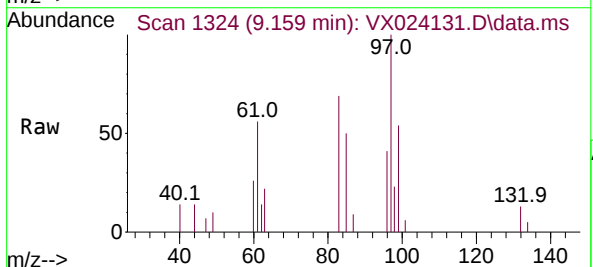




#60
Dibromochloromethane
Concen: 1.771 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.244 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion:129 Resp: 171
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#

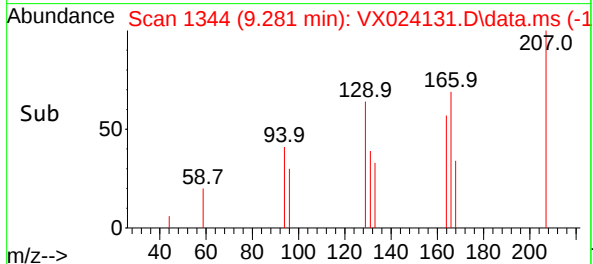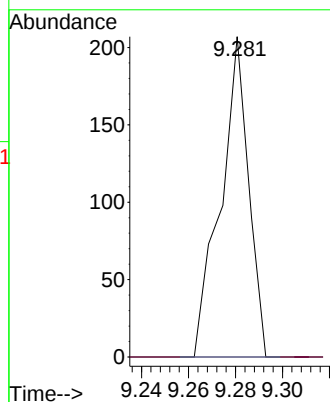

#62
4-Bromofluorobenzene
Concen: 47.091 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion: 95 Resp: 107386
Ion Ratio Lower Upper
95 100
174 80.7 0.0 154.6
176 78.3 0.0 155.8


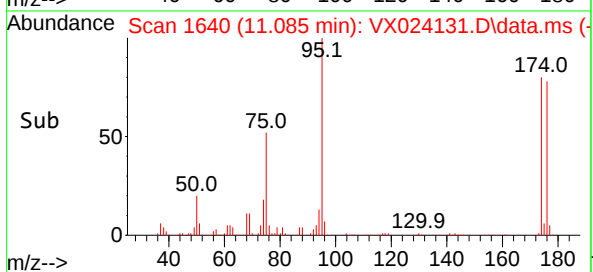
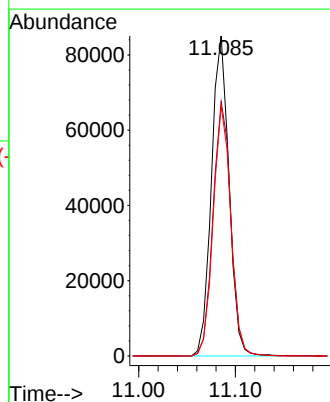
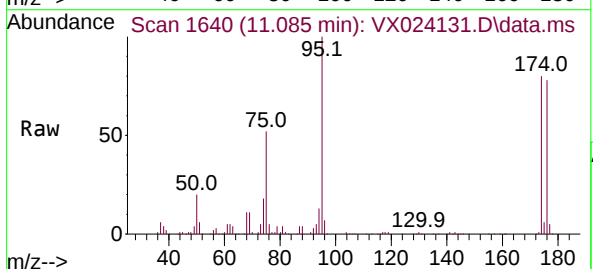




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion:117 Resp: 225369
Ion Ratio Lower Upper
117 100
82 57.0 47.4 71.2
119 31.5 26.6 39.8

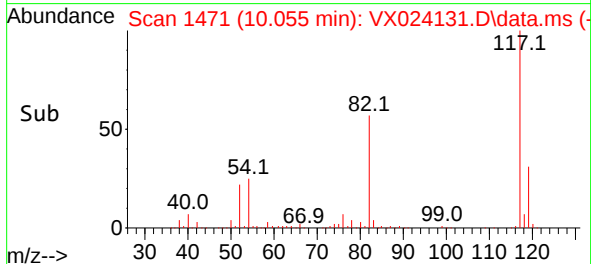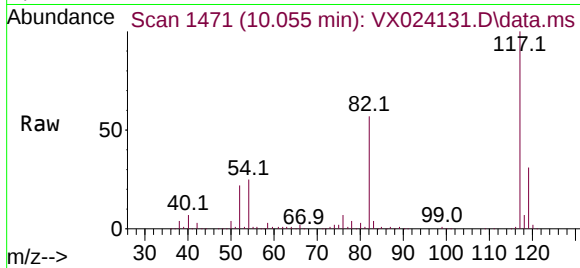

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Tgt Ion:152 Resp: 87102
Ion Ratio Lower Upper
152 100
115 60.0 41.1 123.3
150 156.5 0.0 349.0


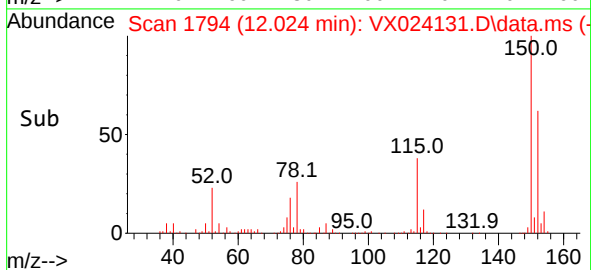

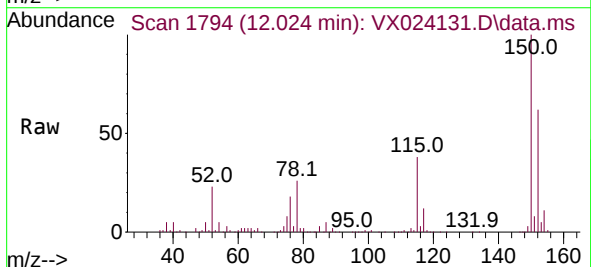


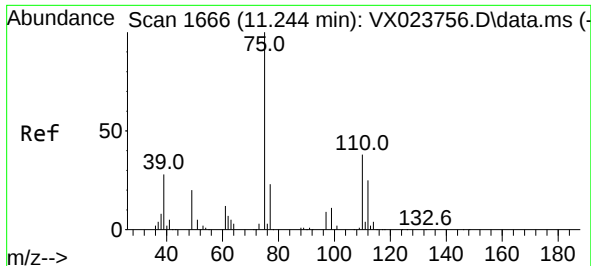

#76
1,2,3-Trichloropropane
Concen: 28.487 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722


Tgt Ion: 75 Resp: 57881
Ion Ratio Lower Upper
75 100
77 1.0 19.1 57.5#

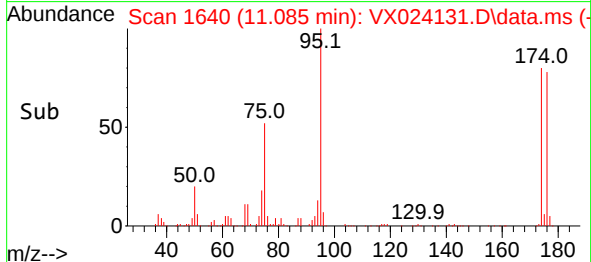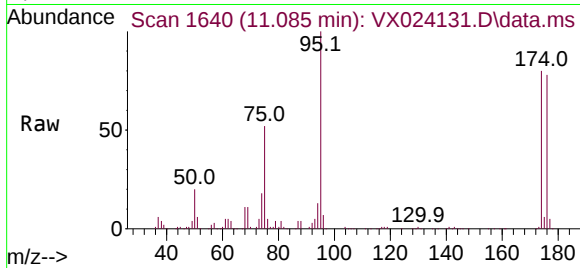

#81
trans-1,4-Dichloro-2-butene
Concen: 83.795 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33


Tgt Ion: 75 Resp: 57881
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

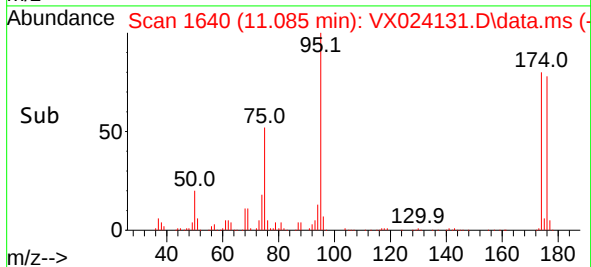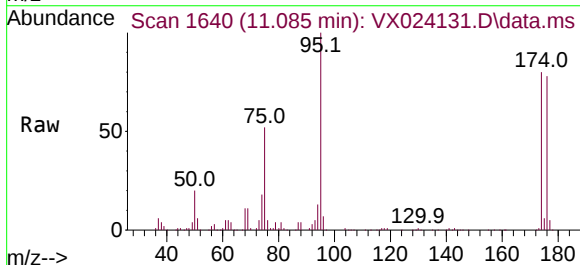

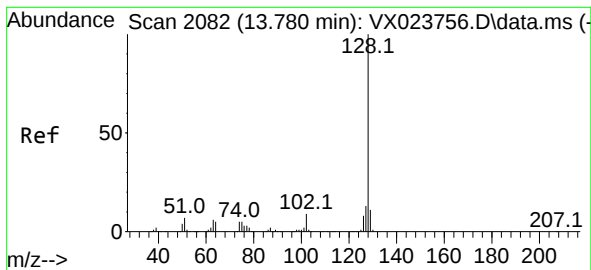

#95
Naphthalene
Concen: 1.325 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX024131.D
Acq: 08 Sep 2021 12:33

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-720-722

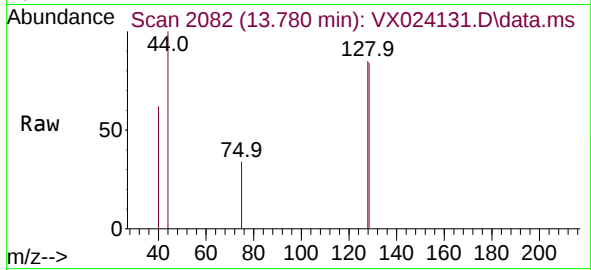

Tgt Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.3	15.5#
129	0.0	8.8	13.2#

