

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090821\
 Data File : VX024130.D
 Acq On : 08 Sep 2021 12:09
 Operator : JC/MD
 Sample : M3675-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-VPB-RW7-GW-705-707

Quant Time: Sep 09 05:43:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 11:57:51 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	142032	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	240529	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	217521	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	90163	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	113862	57.439	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	114.880%
35) Dibromofluoromethane	5.397	113	87817	55.161	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	110.320%
50) Toluene-d8	8.653	98	318813	52.616	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	105.240%
62) 4-Bromofluorobenzene	11.085	95	111246	49.873	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.740%
Target Compounds						
						Qvalue
16) Acetone	2.392	43	6755	7.621	ug/l #	81
17) Carbon Disulfide	2.514	76	1325	0.408	ug/l	100
44) Trichloroethene	7.135	130	12292	6.756	ug/l	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090821\
Data File : VX024130.D
Acq On : 08 Sep 2021 12:09
Operator : JC/MD
Sample : M3675-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-705-707

Quant Time: Sep 09 05:43:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 11:57:51 2021
Response via : Initial Calibration




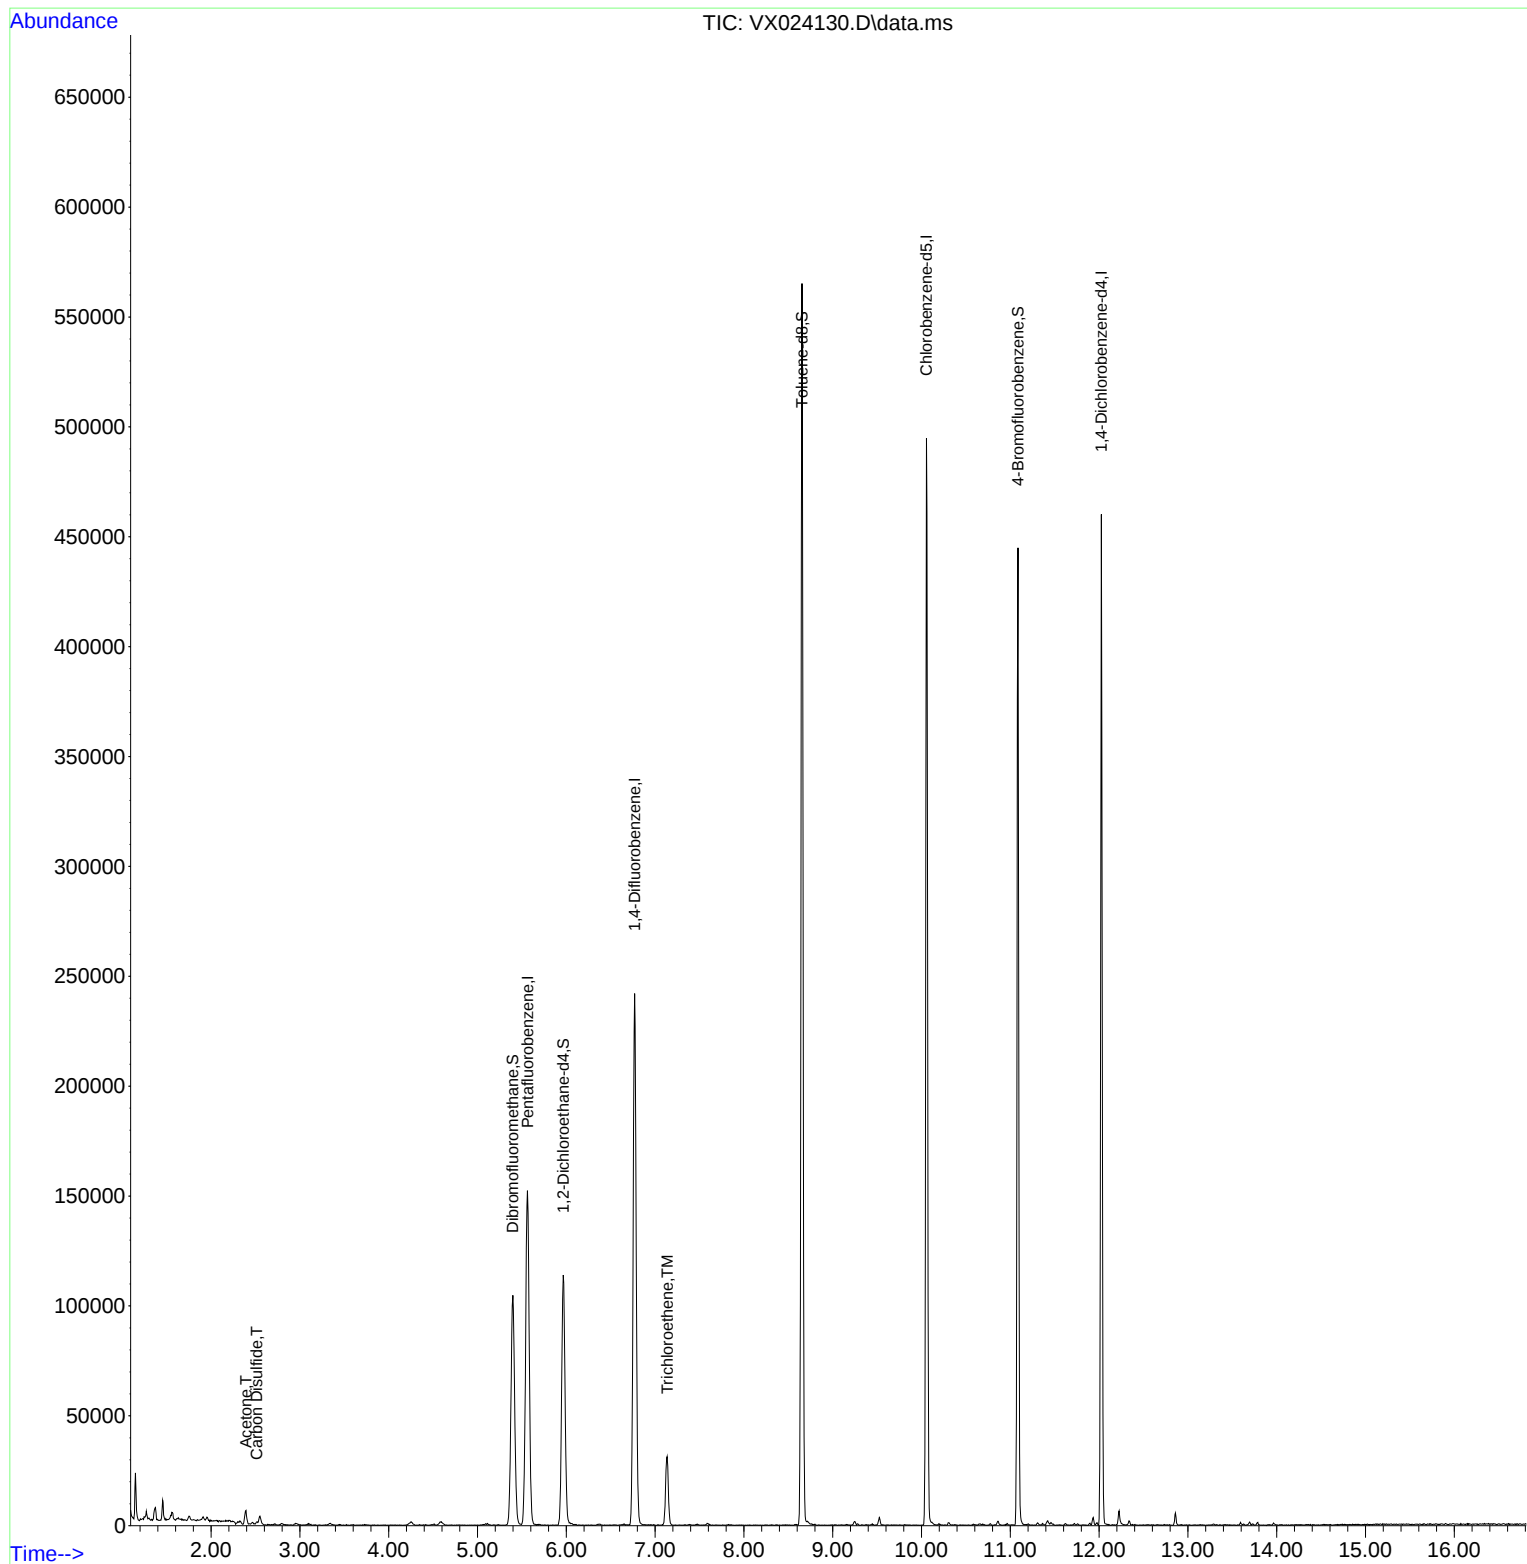


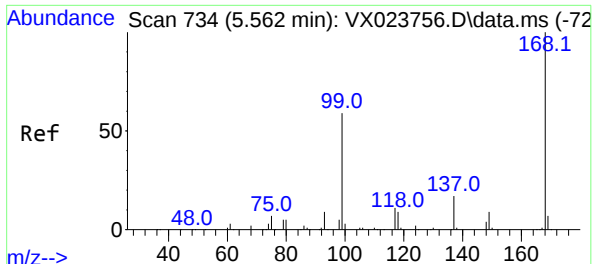

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-705-707


Tgt Ion:168 Resp: 142032
Ion Ratio Lower Upper
168 100
99 58.3 45.8 68.6

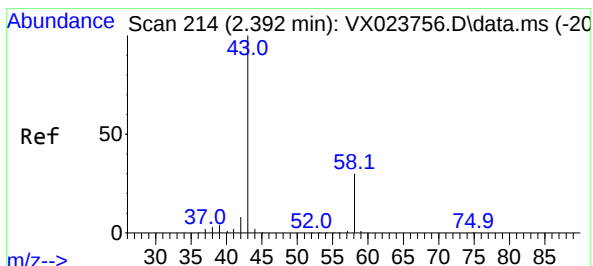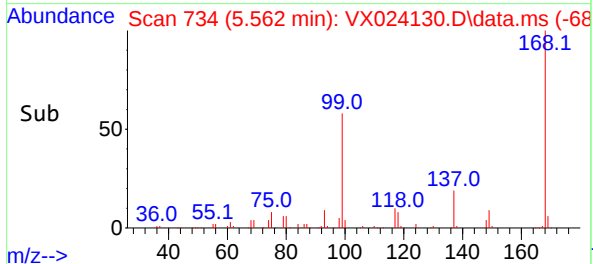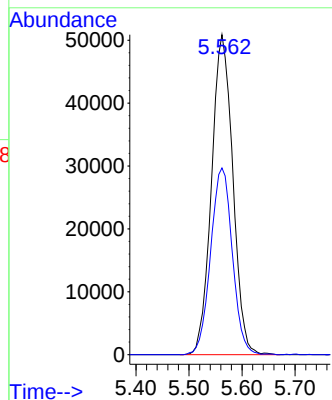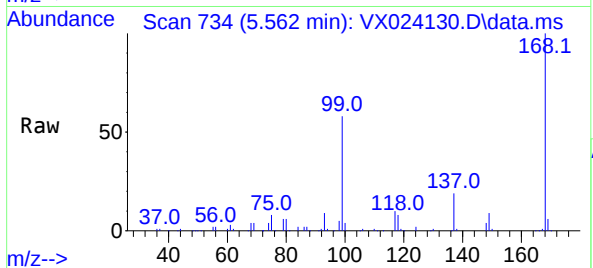

#16
Acetone
Concen: 7.621 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09

Tgt Ion: 43 Resp: 6755
Ion Ratio Lower Upper
43 100
58 23.9 27.8 41.8#


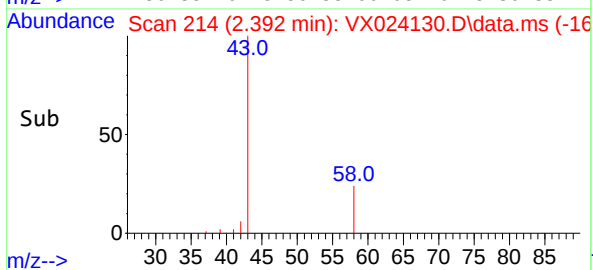
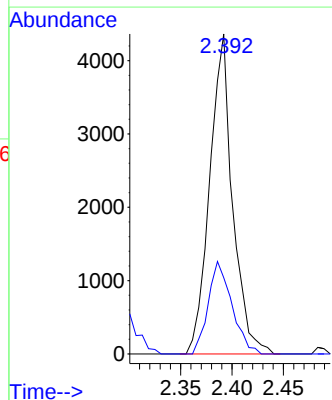
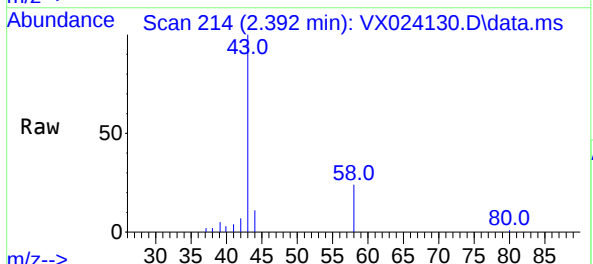


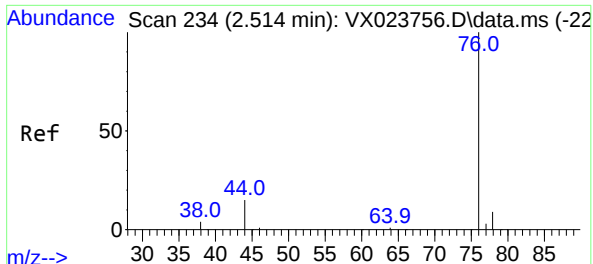

#17
Carbon Disulfide
Concen: 0.408 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-705-707


Tgt Ion: 76 Resp: 1325
Ion Ratio Lower Upper
76 100
78 8.8 7.2 10.8

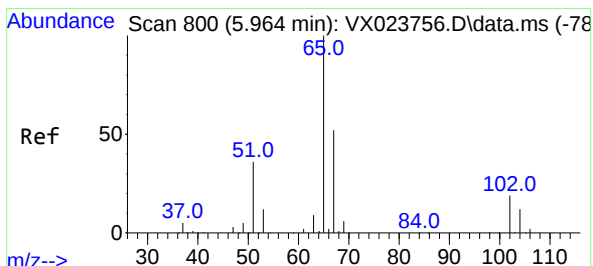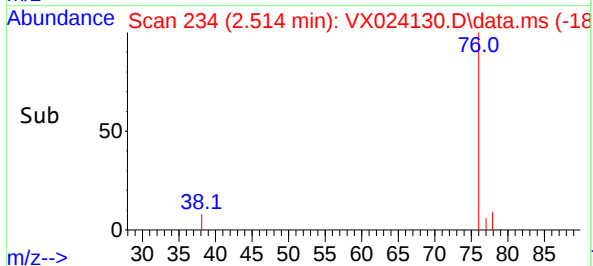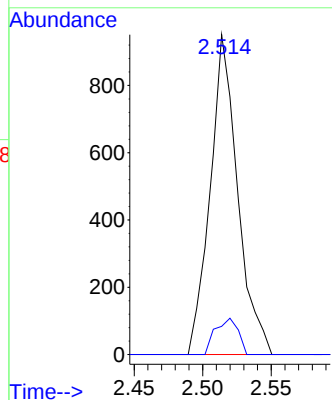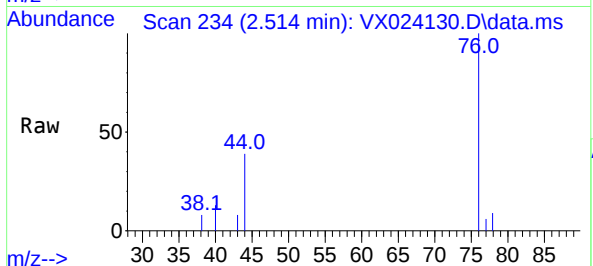

#33
1,2-Dichloroethane-d4
Concen: 57.439 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09

Tgt Ion: 65 Resp: 113862
Ion Ratio Lower Upper
65 100
67 50.6 0.0 105.4

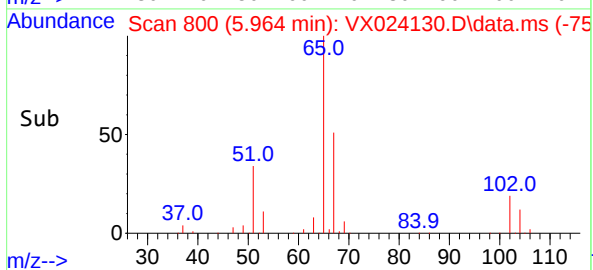
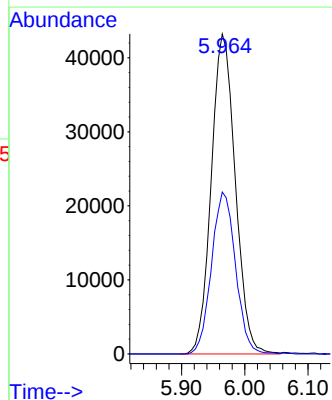
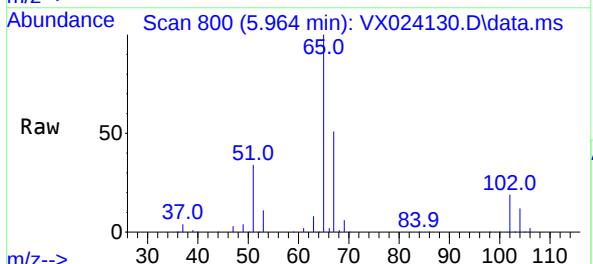


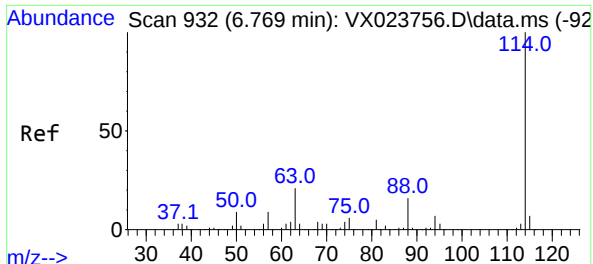

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-705-707


Tgt Ion:114 Resp: 240529
Ion Ratio Lower Upper
114 100
63 22.8 0.0 40.8
88 15.4 0.0 32.8

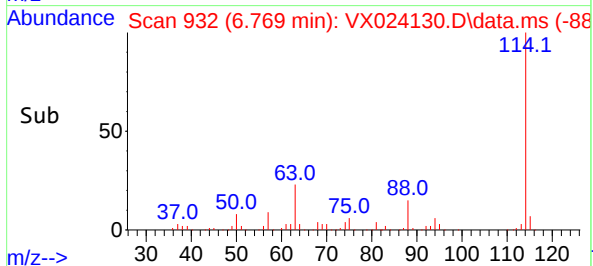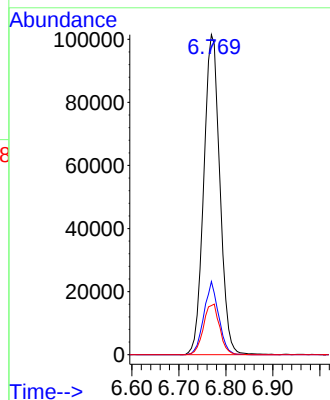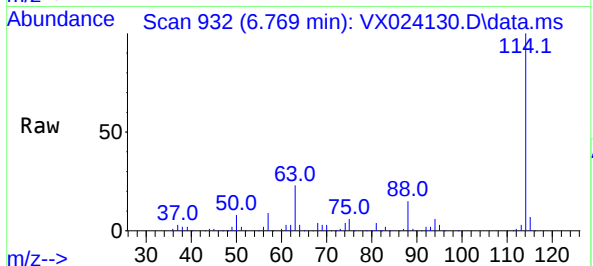

#35
Dibromofluoromethane
Concen: 55.161 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09

Tgt Ion:113 Resp: 87817
Ion Ratio Lower Upper
113 100
111 104.1 81.9 122.9
192 19.8 16.7 25.1


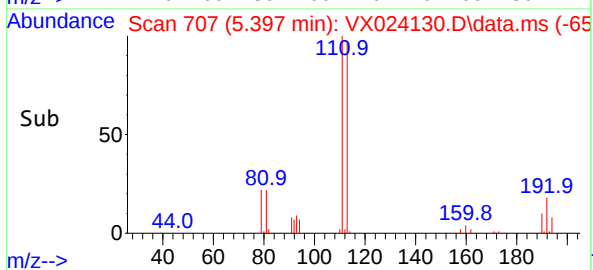
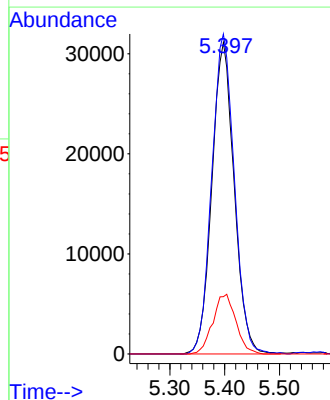
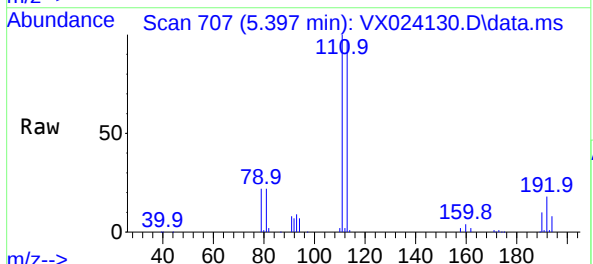


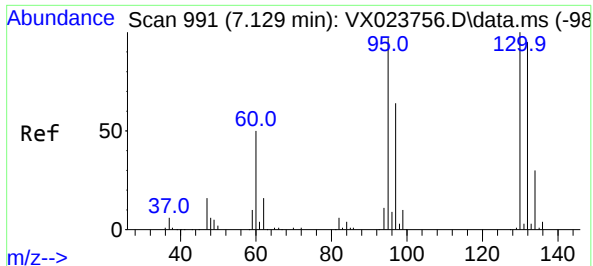

#44
Trichloroethene
Concen: 6.756 ug/l
RT: 7.135 min Scan# 992
Delta R.T. 0.006 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-705-707


Tgt Ion:130 Resp: 12292
Ion Ratio Lower Upper
130 100
95 87.2 0.0 198.0

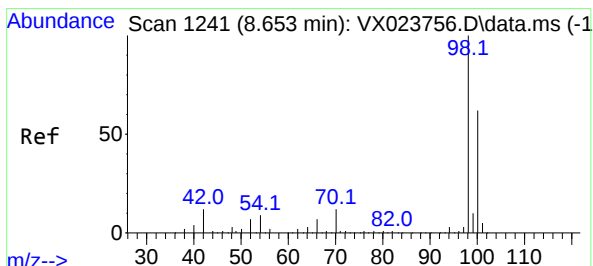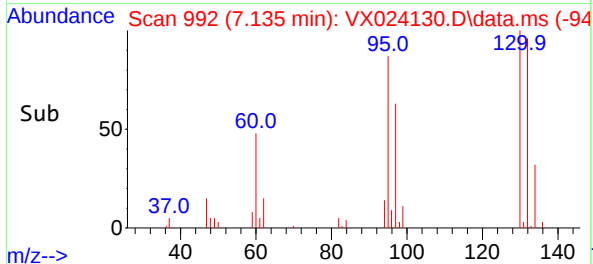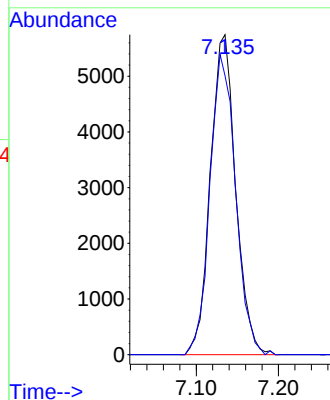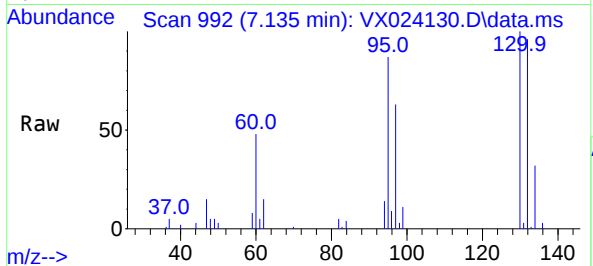

#50
Toluene-d8
Concen: 52.616 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09

Tgt Ion: 98 Resp: 318813
Ion Ratio Lower Upper
98 100
100 63.8 51.9 77.9

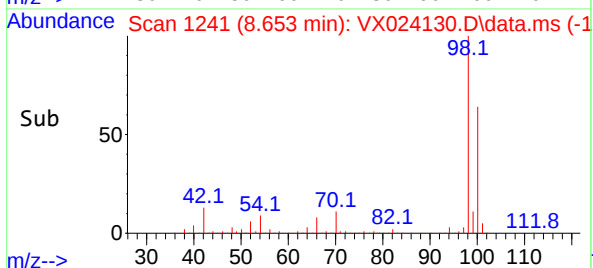
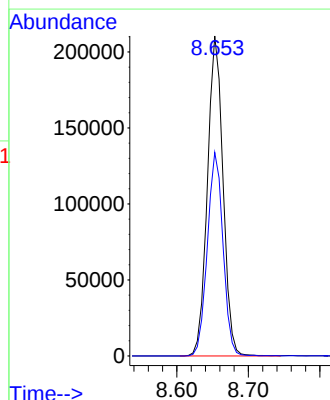
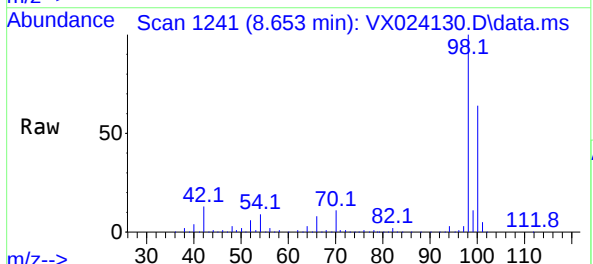


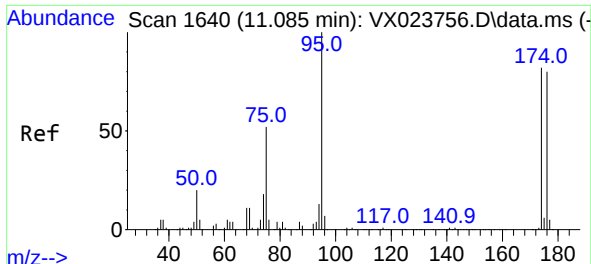

#62
4-Bromofluorobenzene
Concen: 49.873 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-705-707

Tgt Ion: 95 Resp: 111246
Ion Ratio Lower Upper
95 100
174 81.0 0.0 154.6
176 78.7 0.0 155.8

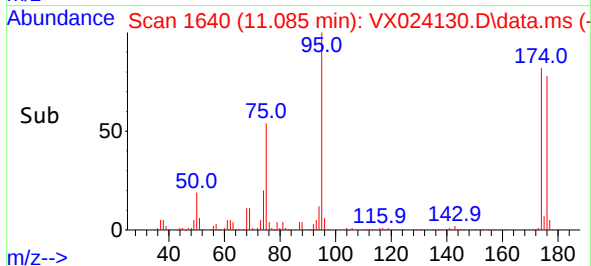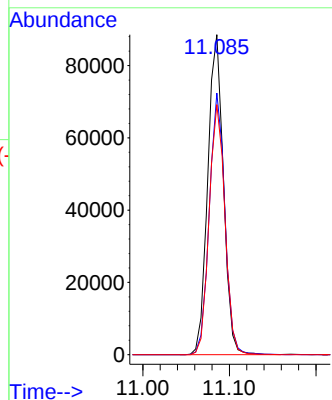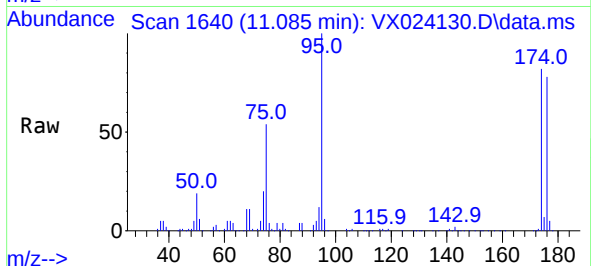

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09

Tgt Ion: 117 Resp: 217521
Ion Ratio Lower Upper
117 100
82 60.5 47.4 71.2
119 31.9 26.6 39.8

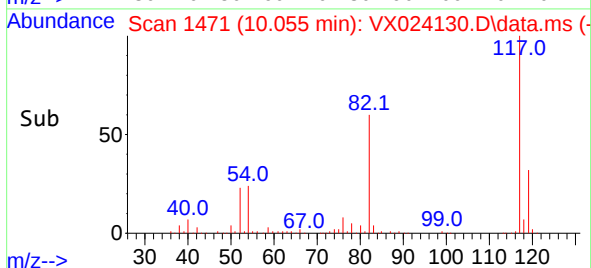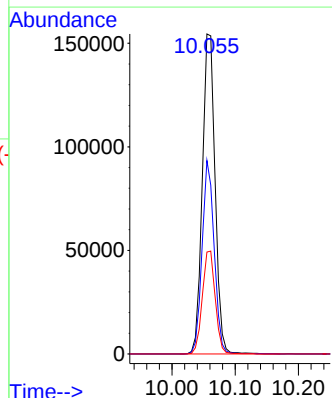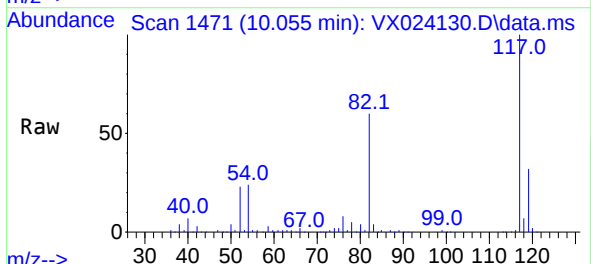



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024130.D
Acq: 08 Sep 2021 12:09

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-GW-705-707

Tgt Ion:	152	Resp:	90163
Ion	Ratio	Lower	Upper
152	100		
115	59.6	41.1	123.3
150	155.4	0.0	349.0

