

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090821\  
 Data File : VX024133.D  
 Acq On : 08 Sep 2021 13:25  
 Operator : JC/MD  
 Sample : M3675-01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BP-TT-VPB-RW7-TB-20210901

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081721W.M

Title : SW846 8260

Signal : TIC: VX024133.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.586       | 567           | 574         | 587          | rVB      | 4034           | 13222         | 1.46%           | 0.284%        |
| 2         | 5.397       | 695           | 707         | 721          | rBV      | 109306         | 310328        | 34.38%          | 6.667%        |
| 3         | 5.562       | 721           | 734         | 746          | rVV      | 161700         | 453527        | 50.25%          | 9.744%        |
| 4         | 5.964       | 789           | 800         | 818          | rBV      | 116504         | 309991        | 34.34%          | 6.660%        |
| 5         | 6.769       | 921           | 932         | 943          | rBV      | 260622         | 612254        | 67.83%          | 13.154%       |
| 6         | 8.653       | 1234          | 1241        | 1252         | rBV      | 594735         | 902585        | 100.00%         | 19.391%       |
| 7         | 10.055      | 1465          | 1471        | 1480         | rBV      | 547788         | 755649        | 83.72%          | 16.235%       |
| 8         | 11.085      | 1634          | 1640        | 1653         | rBV      | 501028         | 626729        | 69.44%          | 13.465%       |
| 9         | 12.024      | 1789          | 1794        | 1803         | rBV      | 536596         | 670280        | 74.26%          | 14.400%       |




Sum of corrected areas: 4654565

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090821\  
Data File : VX024133.D  
Acq On : 08 Sep 2021 13:25  
Operator : JC/MD  
Sample : M3675-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BP-TT-VPB-RW7-TB-20210901

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

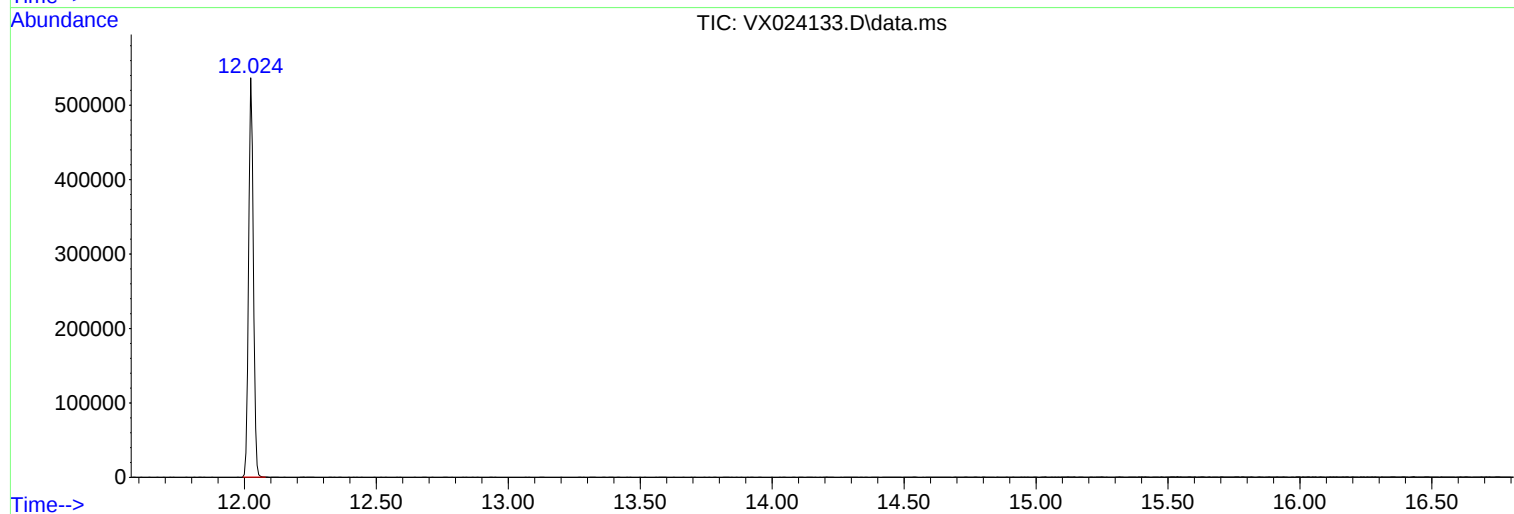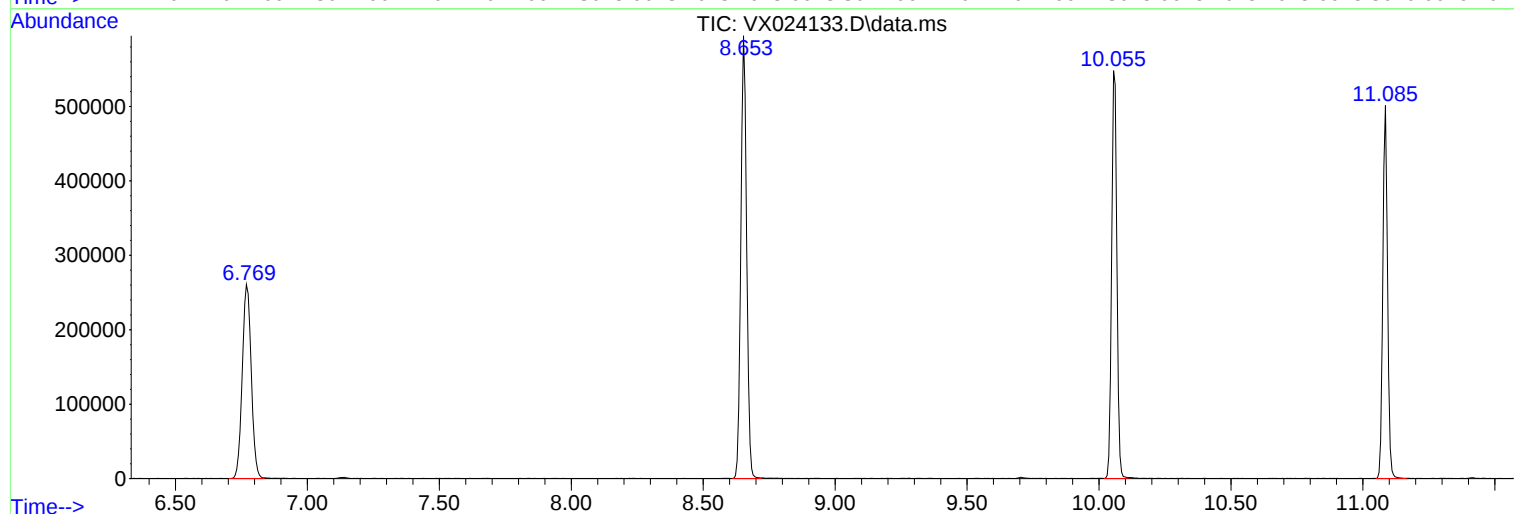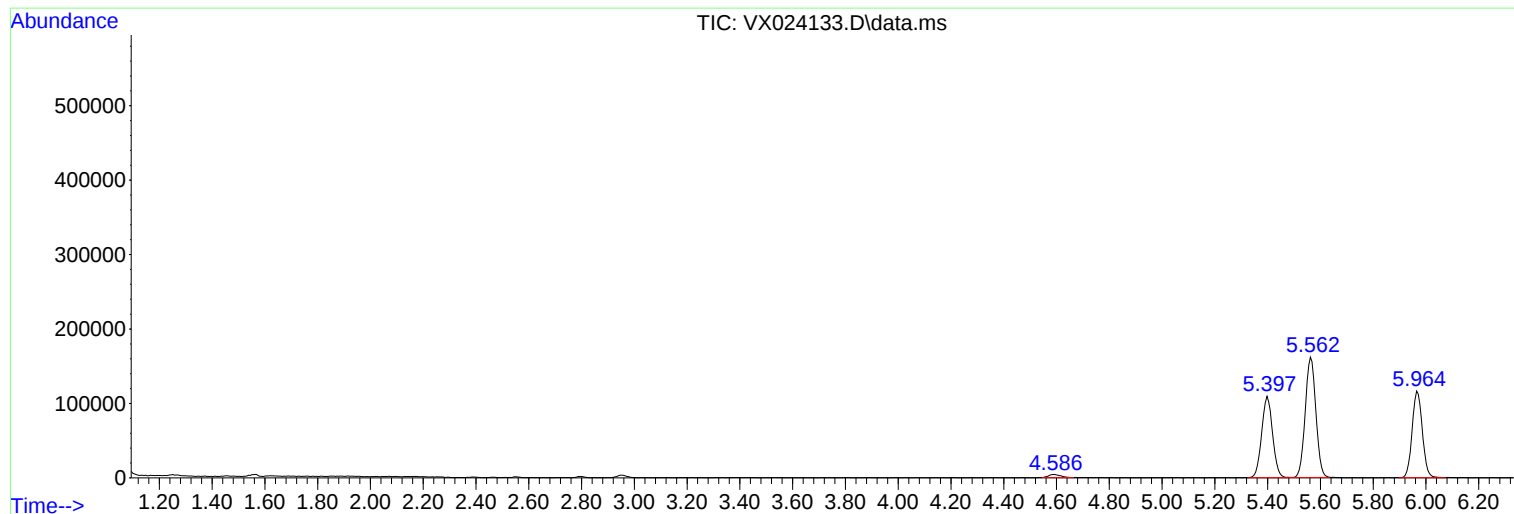

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090821\  
Data File : VX024133.D  
Acq On : 08 Sep 2021 13:25  
Operator : JC/MD  
Sample : M3675-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BP-TT-VPB-RW7-TB-20210901

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090821\  
Data File : VX024133.D  
Acq On : 08 Sep 2021 13:25  
Operator : JC/MD  
Sample : M3675-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BP-TT-VPB-RW7-TB-20210901

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|