

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090822\
 Data File : VX031218.D
 Acq On : 08 Sep 2022 17:50
 Operator : JC/MD
 Sample : N4490-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-14-A-SP

Quant Time: Sep 08 18:55:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 07 23:22:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	64524	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	120889	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	104784	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	47897	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	85711	56.107	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 112.220%			
35) Dibromofluoromethane	5.385	113	61953	47.028	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 94.060%			
50) Toluene-d8	8.653	98	215453	45.015	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 90.020%			
62) 4-Bromofluorobenzene	11.079	95	81792	46.631	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 93.260%			
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.947	59	1887	Below Cal	#	74
16) Acetone	2.380	43	16513	31.219	ug/l	# 83
17) Carbon Disulfide	2.508	76	1050	0.392	ug/l	# 74
18) Methyl Acetate	2.709	43	564	0.412	ug/l	# 71
20) Methylene Chloride	2.788	84	5139	4.134	ug/l	# 88
25) 2-Butanone	4.562	43	4541	5.796	ug/l	# 80
31) Cyclohexane	5.556	56	1722	1.009	ug/l	# 22
36) 1,1-Dichloropropene	5.556	75	6371	3.229	ug/l	# 49
37) Ethyl Acetate	4.727	43	8695	4.968	ug/l	# 98
38) Carbon Tetrachloride	5.562	117	8359	4.027	ug/l	# 17
40) Benzene	6.050	78	4067	0.759	ug/l	# 92
43) Isopropyl Acetate	6.349	43	38969	14.122	ug/l	# 95
48) Methyl methacrylate	7.799	41	31472	23.422	ug/l	# 43
51) 4-Methyl-2-Pentanone	8.549	43	30258	17.907	ug/l	# 52
52) Toluene	8.726	92	1618	0.458	ug/l	# 97
54) cis-1,3-Dichloropropene	8.549	75	14969	6.588	ug/l	# 63
57) 1,3-Dichloropropane	9.488	76	1414	0.563	ug/l	# 42
59) 2-Hexanone	9.378	43	29596	23.162	ug/l	# 24
68) m/p-Xylenes	10.299	106	606	0.292	ug/l	# 53
69) o-Xylene	10.647	106	824	0.398	ug/l	# 81
76) 1,2,3-Trichloropropane	11.079	75	46180	35.328	ug/l	# 37
80) 1,3,5-Trimethylbenzene	11.451	105	11048	3.160	ug/l	# 95
81) trans-1,4-Dichloro-2-b...	11.079	75	46180	113.928	ug/l	# 12
82) 4-Chlorotoluene	11.457	91	1673	0.492	ug/l	# 44
84) 1,2,4-Trimethylbenzene	11.756	105	3329	0.979	ug/l	# 93
85) sec-Butylbenzene	11.756	105	3329	0.780	ug/l	# 56
86) p-Isopropyltoluene	11.976	119	2704	0.784	ug/l	# 97
89) n-Butylbenzene	12.323	91	1724	0.580	ug/l	# 1
90) Hexachloroethane	12.567	117	804	1.357	ug/l	# 16
92) 1,2-Dibromo-3-Chloropr...	12.969	75	134	0.376	ug/l	# 1
95) Naphthalene	13.780	128	2774	0.735	ug/l	# 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090822\
Data File : VX031218.D
Acq On : 08 Sep 2022 17:50
Operator : JC/MD
Sample : N4490-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Quant Time: Sep 08 18:55:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 07 23:22:41 2022
Response via : Initial Calibration

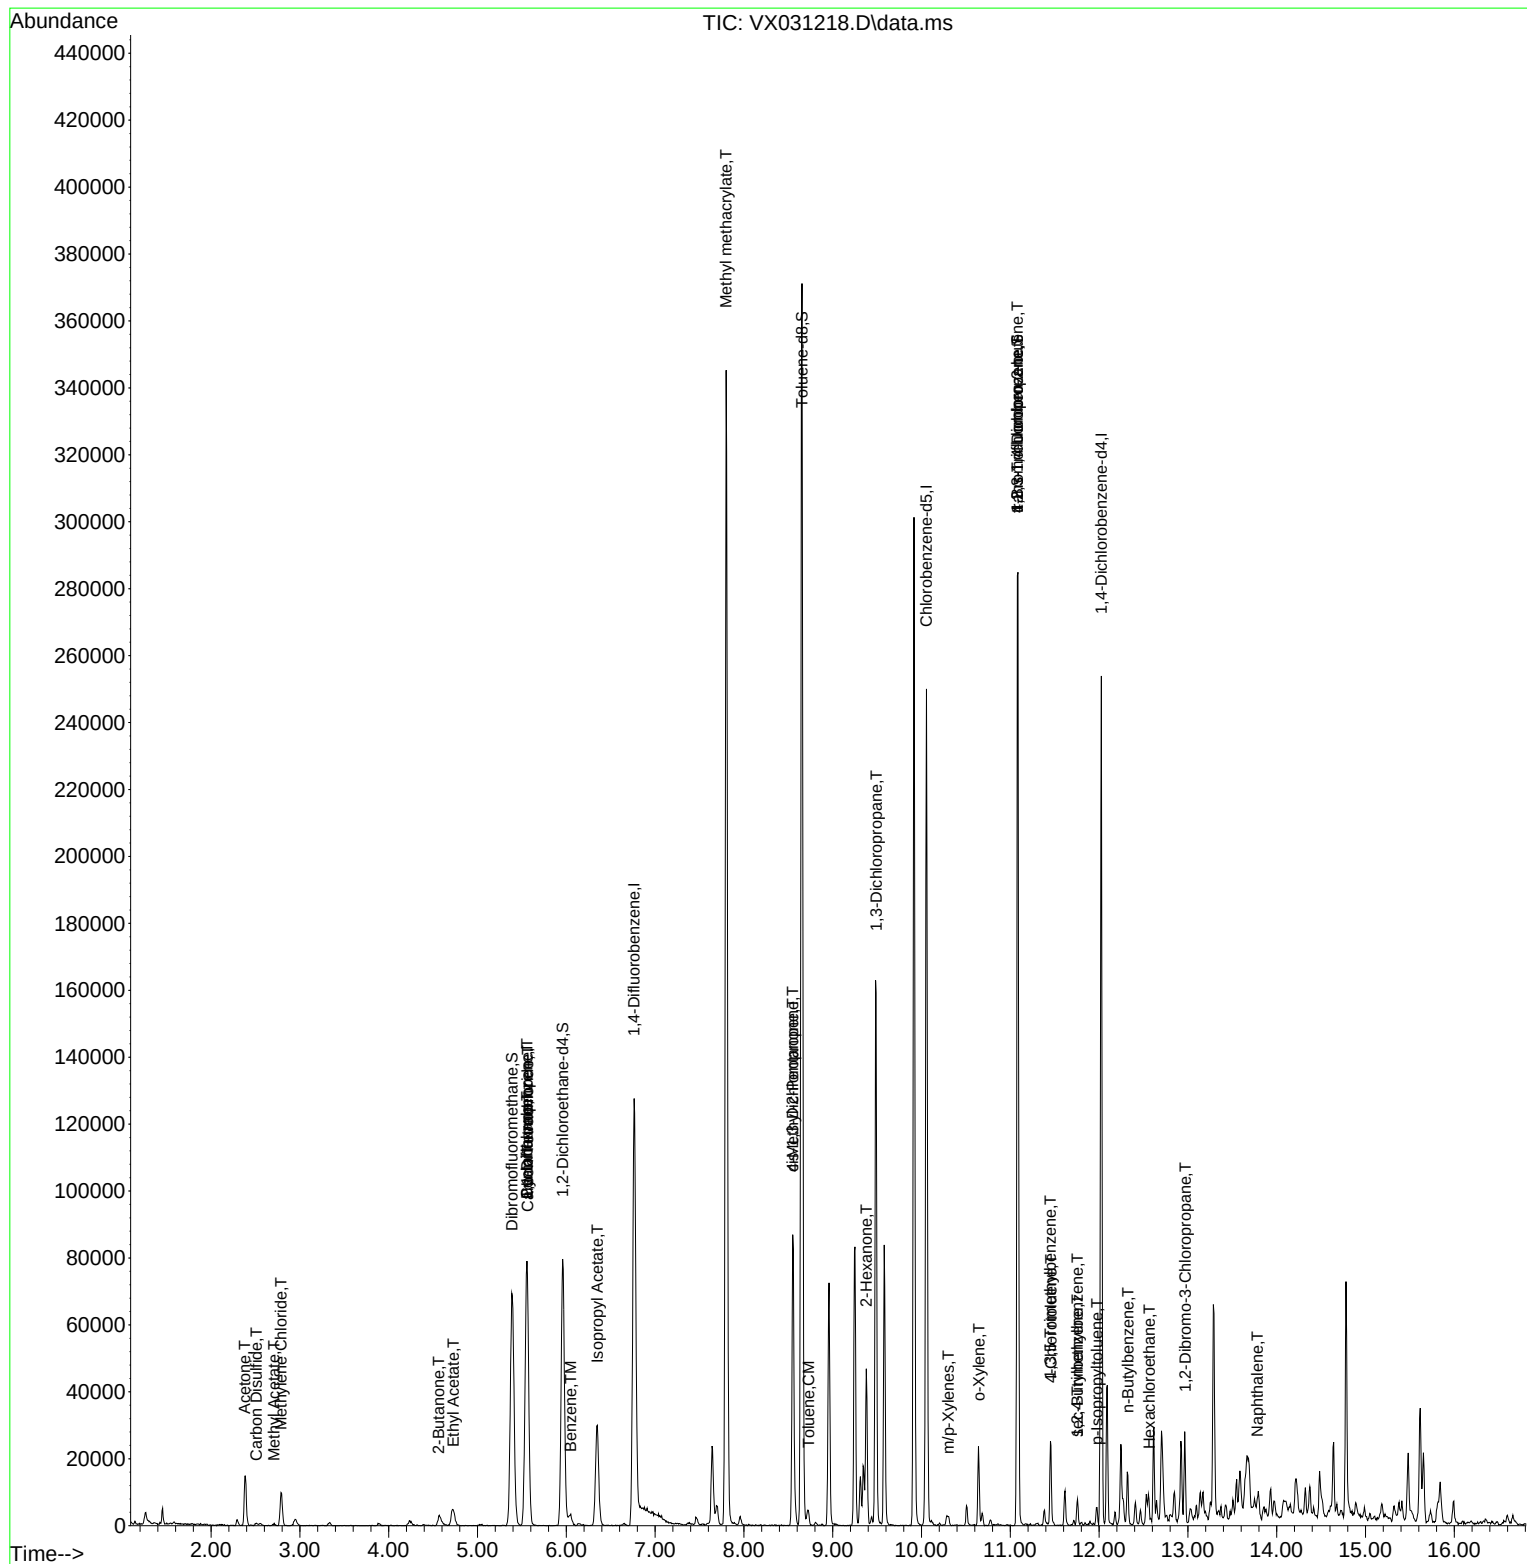



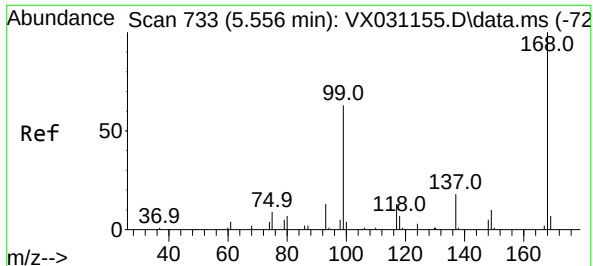


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP



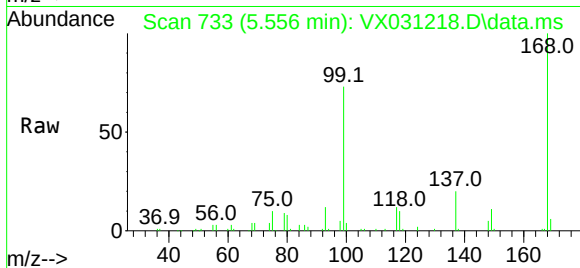



Tgt Ion:168 Resp: 64524
Ion Ratio Lower Upper
168 100
99 72.8 44.0 66.0#

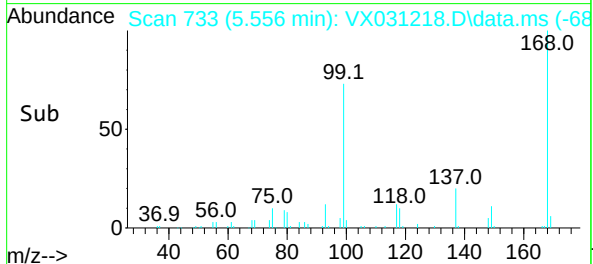

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.947 min Scan# 305
Delta R.T. -0.055 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Tgt Ion: 59 Resp: 1887
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#


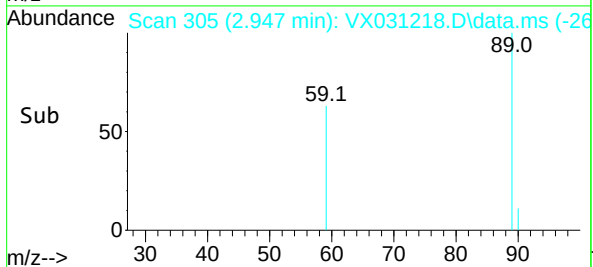

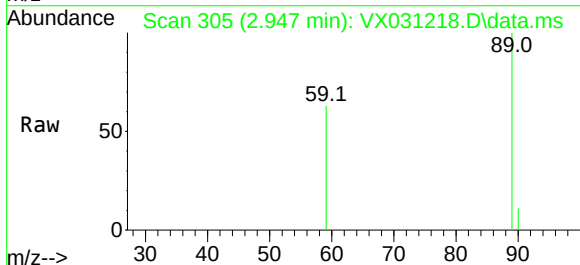


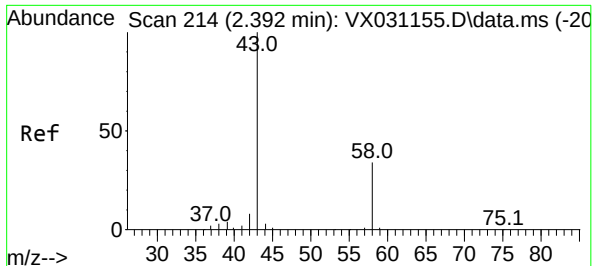

#16
Acetone
Concen: 31.219 ug/l
RT: 2.380 min Scan# 214
Delta R.T. -0.012 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50




Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Tgt Ion: 43 Resp: 16513
Ion Ratio Lower Upper
43 100
58 24.8 27.7 41.5#

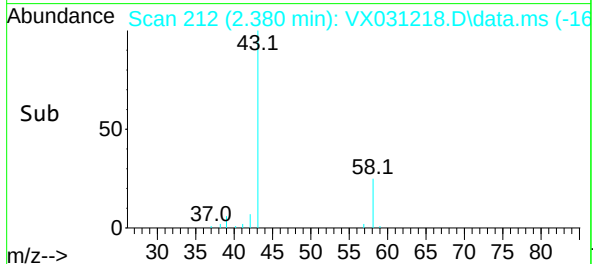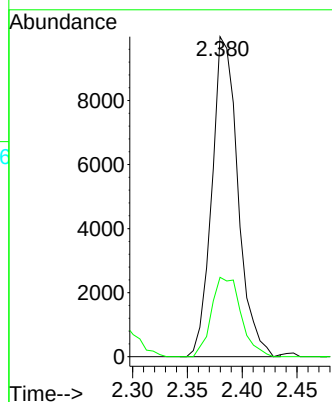

#17
Carbon Disulfide
Concen: 0.392 ug/l
RT: 2.508 min Scan# 233
Delta R.T. -0.006 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Tgt Ion: 76 Resp: 1050
Ion Ratio Lower Upper
76 100
78 0.0 7.8 11.6#


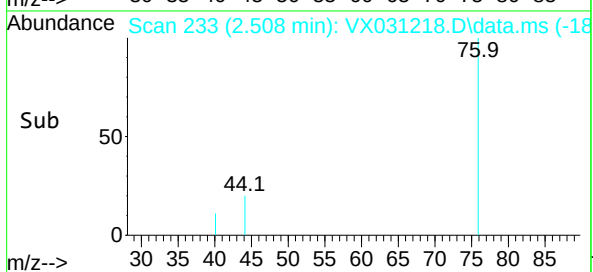
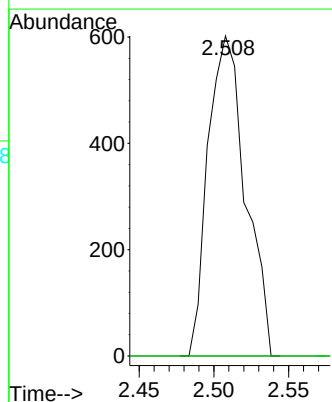
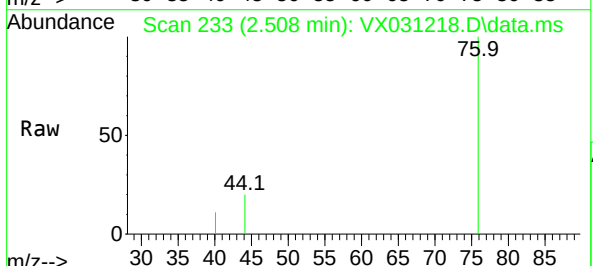




#18
Methyl Acetate
Concen: 0.412 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.000 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50




Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Tgt Ion: 43 Resp: 564
Ion Ratio Lower Upper
43 100
74 10.1 19.4 29.2#

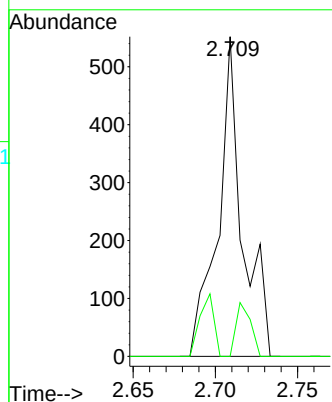

#20
Methylene Chloride
Concen: 4.134 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Tgt Ion: 84 Resp: 5139
Ion Ratio Lower Upper
84 100
49 99.4 93.8 140.6
51 32.4 29.4 44.0
86 68.2 51.0 76.4


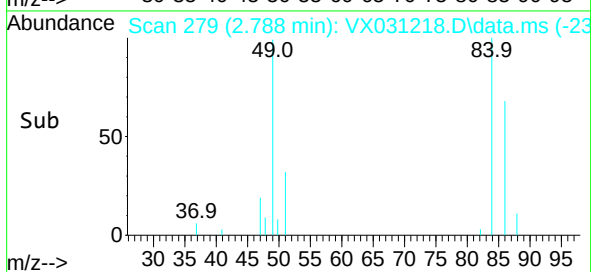




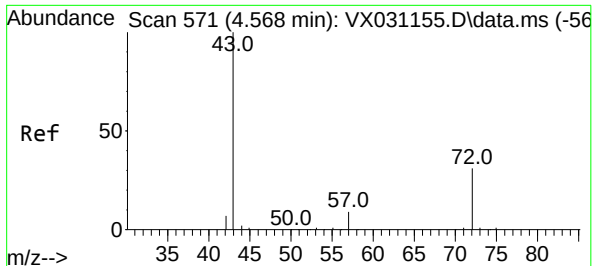

#25
2-Butanone
Concen: 5.796 ug/l
RT: 4.562 min Scan# 51
Delta R.T. -0.006 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50




Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Tgt Ion: 43 Resp: 4541
Ion Ratio Lower Upper
43 100
72 37.4 21.7 32.5#

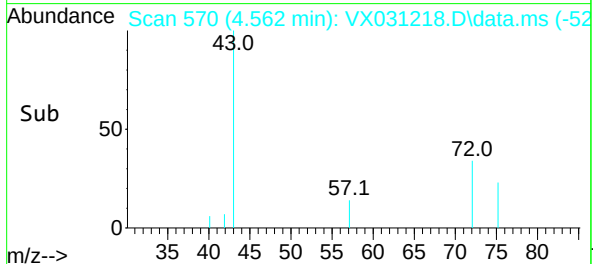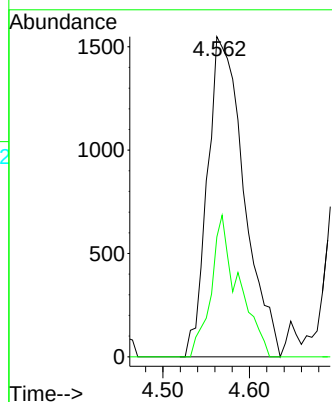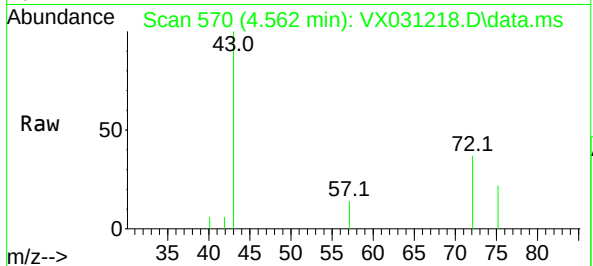

#31
Cyclohexane
Concen: 1.009 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.085 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Tgt Ion: 56 Resp: 1722
Ion Ratio Lower Upper
56 100
69 146.2 25.4 38.0#
84 113.9 68.9 103.3#

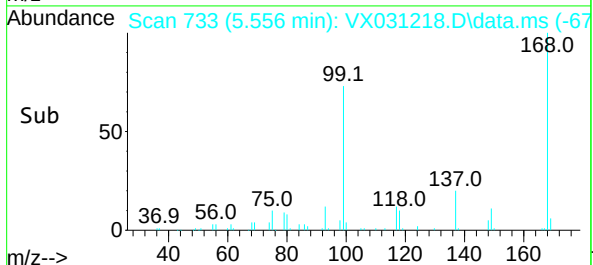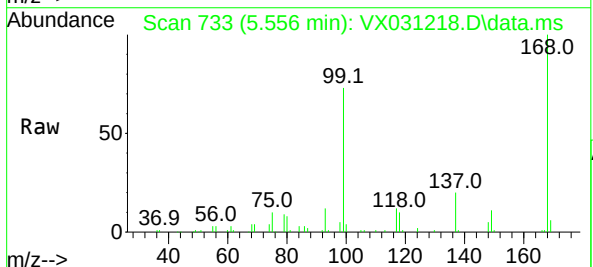

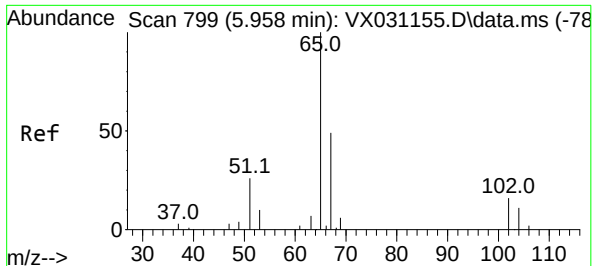

#33

1,2-Dichloroethane-d4

Concen: 56.107 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50

Instrument :

MSVOA_X

ClientSampleId :





WC-14-A-SP

Tgt Ion: 65 Resp: 85711

Ion Ratio Lower Upper

65 100

67 48.3 0.0 109.6

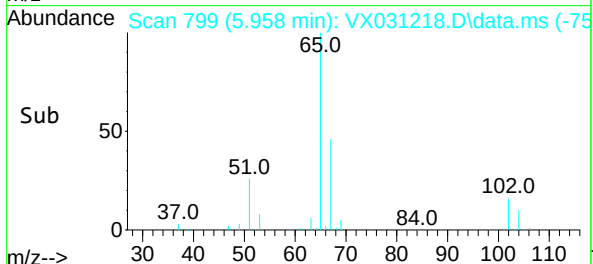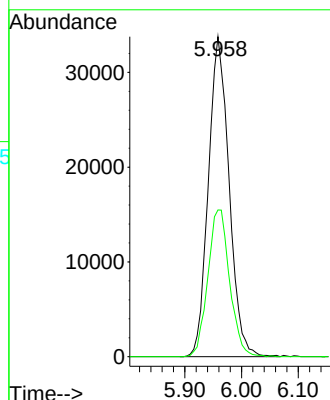

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50




Tgt Ion: 114 Resp: 120889


Ion Ratio Lower Upper

114 100

63 20.7 0.0 38.4

88 18.3 0.0 31.8


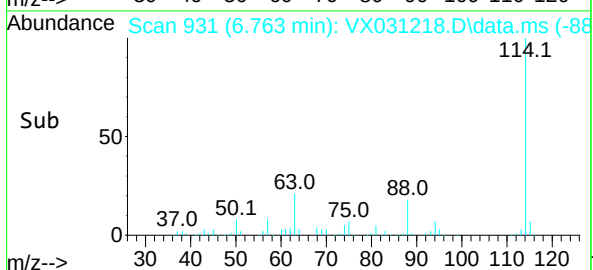
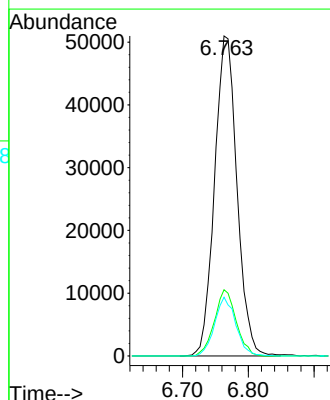
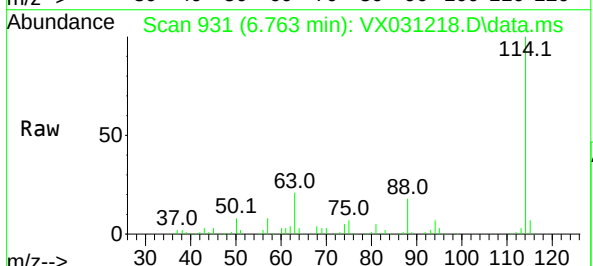




#35
Dibromofluoromethane
Concen: 47.028 ug/l
RT: 5.385 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50




Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Tgt Ion:113 Resp: 61953
Ion Ratio Lower Upper
113 100
111 100.3 83.2 124.8
192 16.3 14.8 22.2

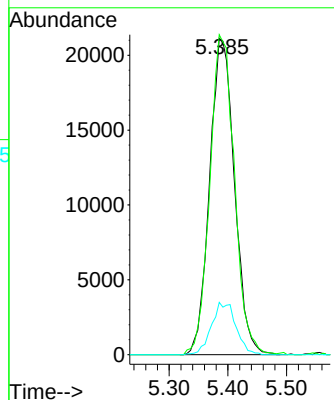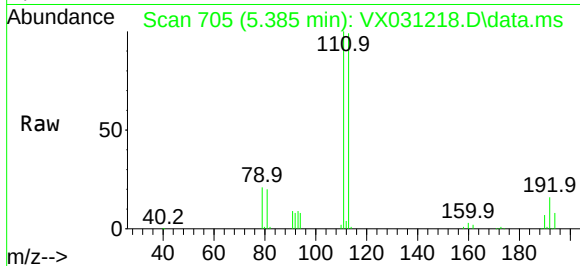

#36
1,1-Dichloropropene
Concen: 3.229 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Tgt Ion: 75 Resp: 6371
Ion Ratio Lower Upper
75 100
110 9.9 19.3 57.9#
77 0.0 24.4 36.6#

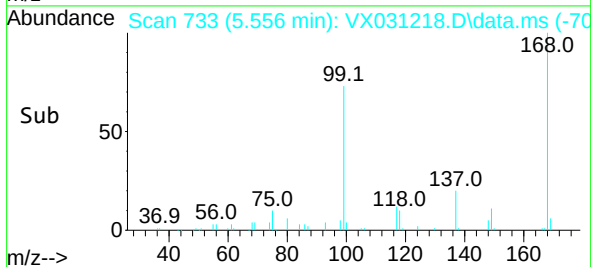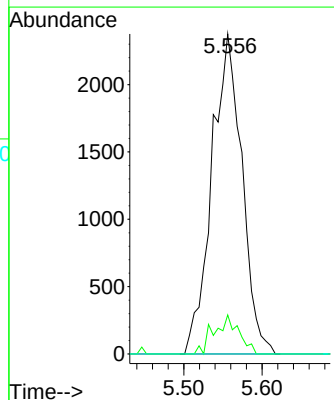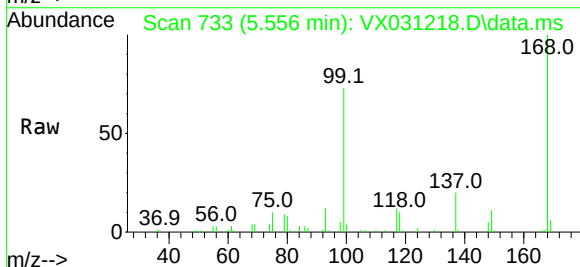



#37

Ethyl Acetate

Concen: 4.968 ug/l

RT: 4.727 min Scan# 595

Delta R.T. 0.012 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50





Instrument :

MSVOA_X

ClientSampleId :

WC-14-A-SP

Tgt Ion:	43	Resp:	8695
Ion	Ratio	Lower	Upper
43	100		
61	14.3	11.7	17.5
70	13.1	9.3	13.9

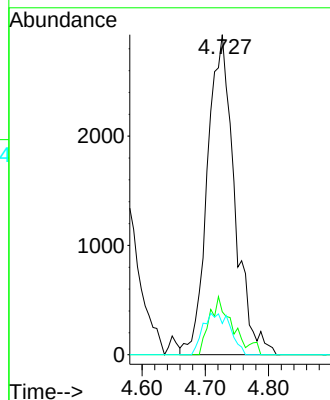

#38

Carbon Tetrachloride

Concen: 4.027 ug/l




RT: 5.562 min Scan# 734


Delta R.T. -0.116 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50

Tgt Ion:	117	Resp:	8359
Ion	Ratio	Lower	Upper
117	100		
119	4.8	74.1	111.1#
121	0.0	25.8	38.8#

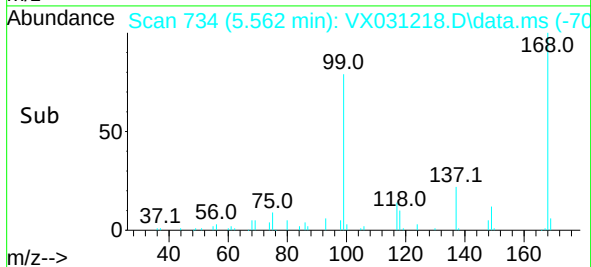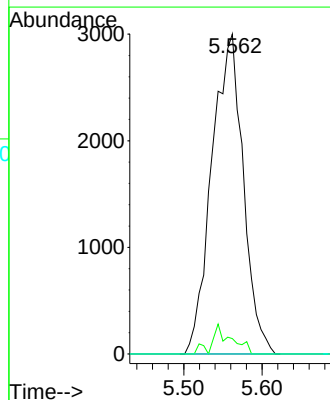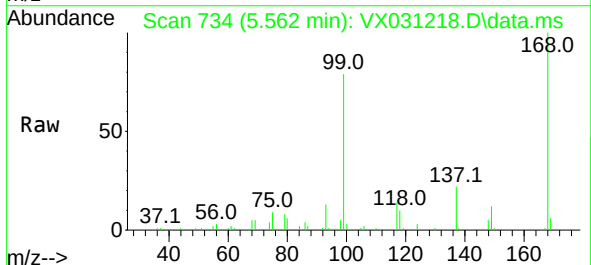



#40

Benzene

Concen: 0.759 ug/l

RT: 6.050 min Scan# 81

Delta R.T. 0.012 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50

Instrument :

MSVOA_X

ClientSampleId :





WC-14-A-SP

Tgt Ion: 78 Resp: 4067

Ion Ratio Lower Upper

78 100

77 26.2 18.0 27.0

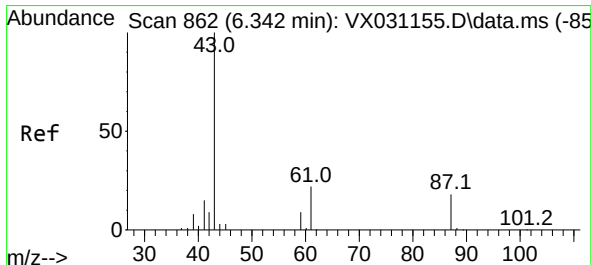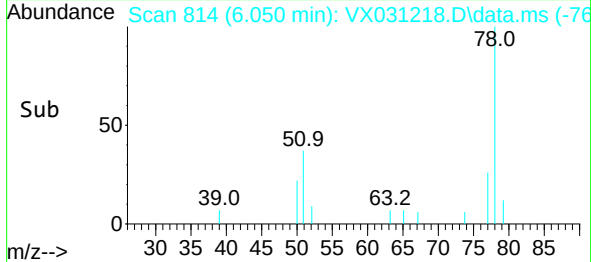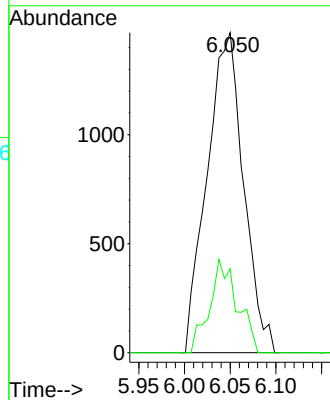

#43

Isopropyl Acetate

Concen: 14.122 ug/l

RT: 6.349 min Scan# 863

Delta R.T. 0.006 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50




Tgt Ion: 43 Resp: 38969


Ion Ratio Lower Upper

43 100

61 21.7 16.5 24.7

87 17.8 11.1 16.7#

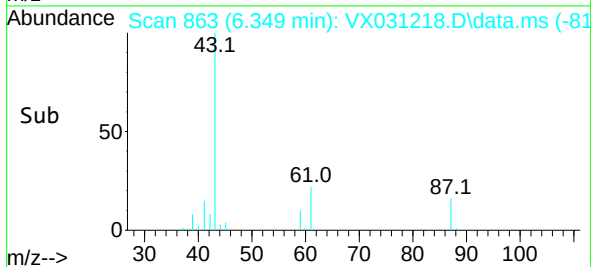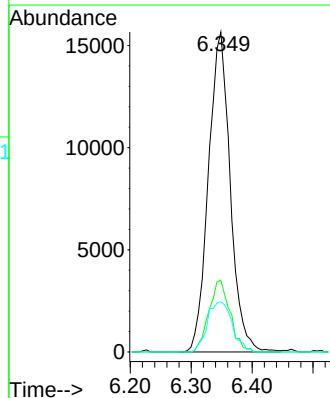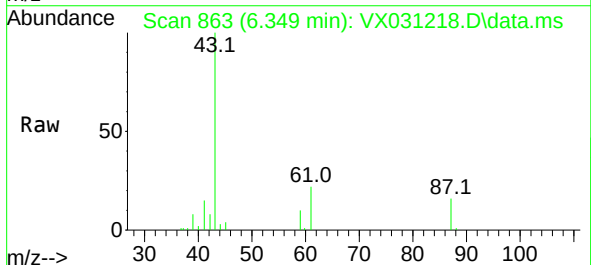

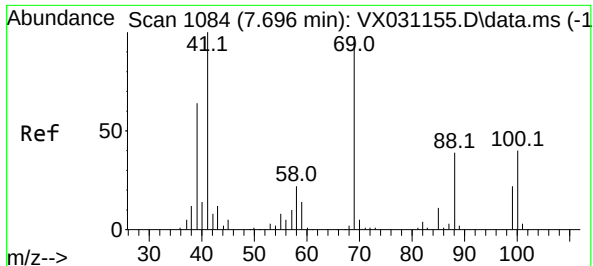

#48

Methyl methacrylate

Concen: 23.422 ug/l

RT: 7.799 min Scan# 1101

Delta R.T. 0.104 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50

Instrument :

MSVOA_X

ClientSampleId :

WC-14-A-SP





Tgt Ion: 41 Resp: 31472

Ion Ratio Lower Upper

41 100

69 0.0 68.8 103.2#

39 56.6 44.6 66.8

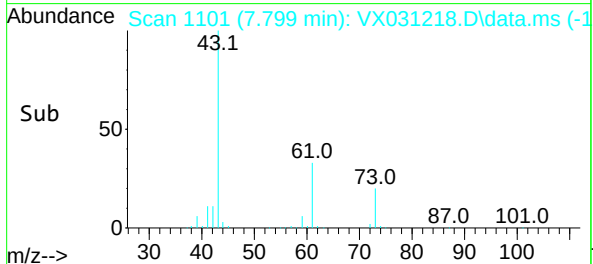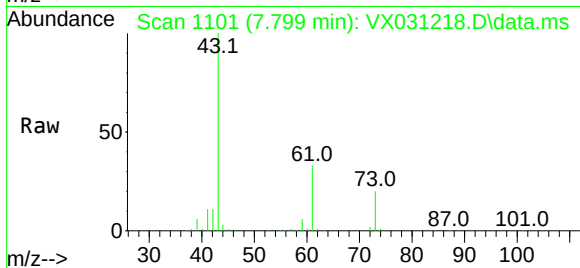

#50

Toluene-d8

Concen: 45.015 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.000 min

Lab File: VX031218.D




Acq: 08 Sep 2022 17:50


Tgt Ion: 98 Resp: 215453

Ion Ratio Lower Upper

98 100

100 66.5 52.3 78.5

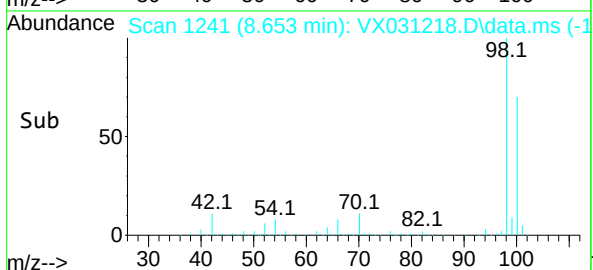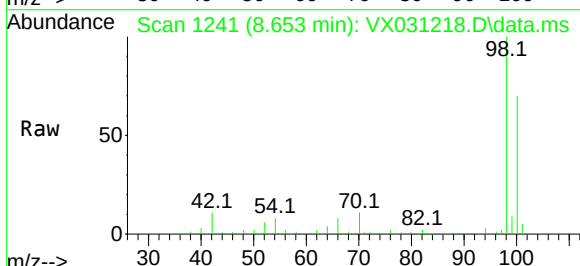



#51

4-Methyl-2-Pentanone

Concen: 17.907 ug/l

RT: 8.549 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50

Instrument :

MSVOA_X

ClientSampleId :





WC-14-A-SP

Tgt Ion: 43 Resp: 30258

Ion Ratio Lower Upper

43 100

58 9.8 31.4 47.2#

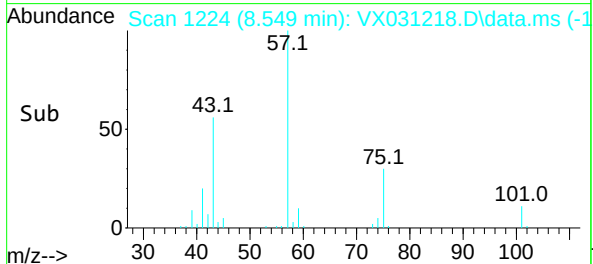

#52

Toluene

Concen: 0.458 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. 0.006 min

Lab File: VX031218.D




Acq: 08 Sep 2022 17:50


Tgt Ion: 92 Resp: 1618

Ion Ratio Lower Upper

92 100

91 177.8 139.2 208.8



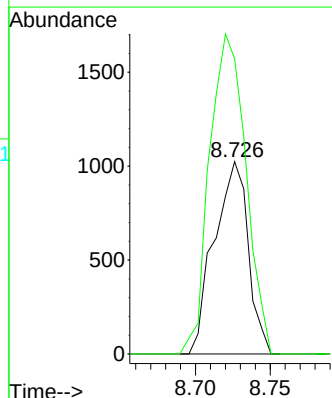
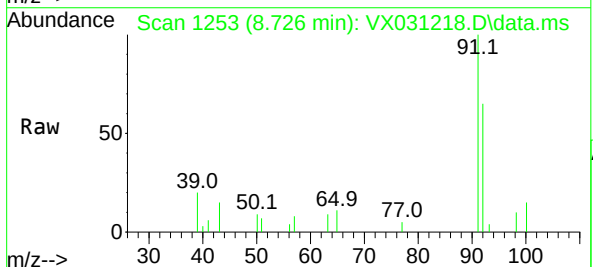




#54
 cis-1,3-Dichloropropene
 Concen: 6.588 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX031218.D
 Acq: 08 Sep 2022 17:50




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-14-A-SP


Tgt Ion: 75 Resp: 14969
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.0 37.4#
 39 30.8 37.5 56.3#

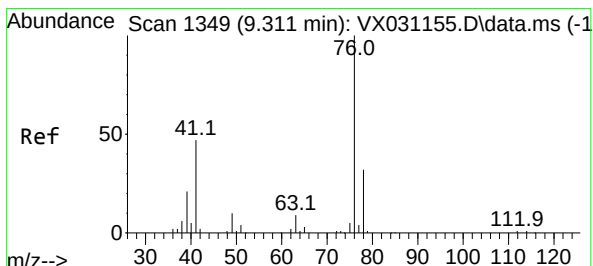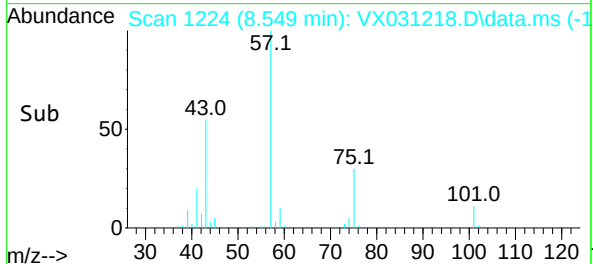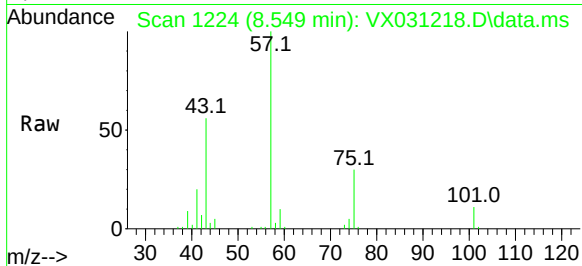

#57
 1,3-Dichloropropane
 Concen: 0.563 ug/l
 RT: 9.488 min Scan# 1378
 Delta R.T. 0.177 min
 Lab File: VX031218.D
 Acq: 08 Sep 2022 17:50

Tgt Ion: 76 Resp: 1414
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.9 38.9#

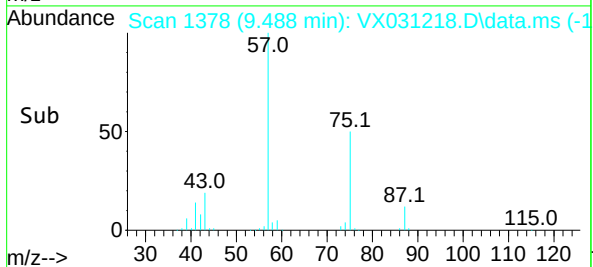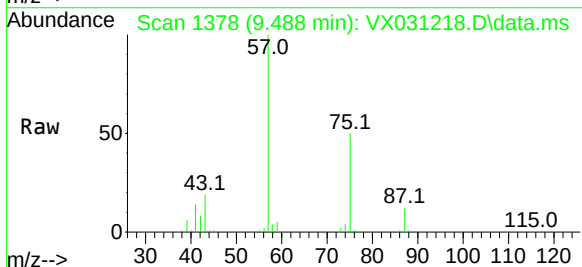



#59

2-Hexanone

Concen: 23.162 ug/l

RT: 9.378 min Scan# 11

Delta R.T. -0.055 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50

Instrument :

MSVOA_X

ClientSampleId :





WC-14-A-SP

Tgt Ion: 43 Resp: 29596

Ion Ratio Lower Upper

43 100

58 0.0 27.6 82.8#

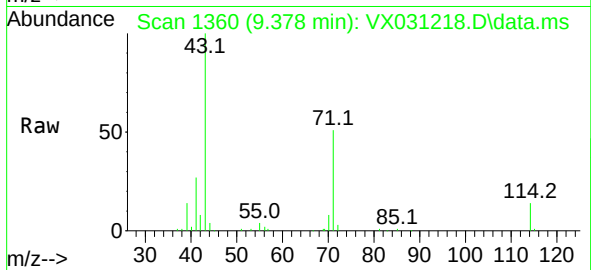

#62

4-Bromofluorobenzene

Concen: 46.631 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50




Tgt Ion: 95 Resp: 81792


Ion Ratio Lower Upper

95 100

174 65.1 0.0 149.0

176 62.0 0.0 146.0



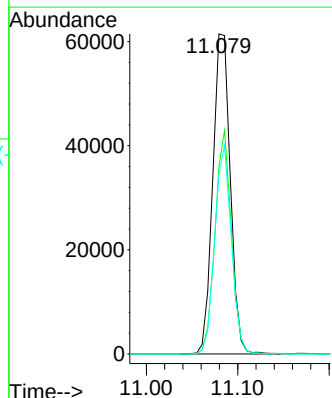
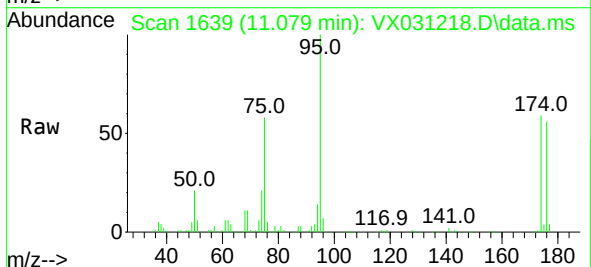




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50




Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Tgt Ion:117 Resp: 104784
Ion Ratio Lower Upper
117 100
82 59.3 42.7 64.1
119 33.7 25.4 38.2

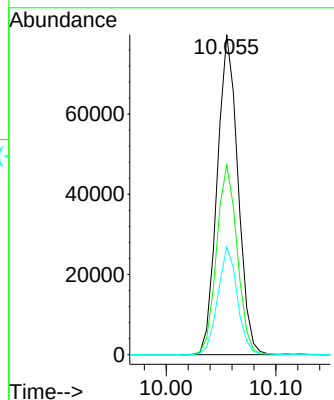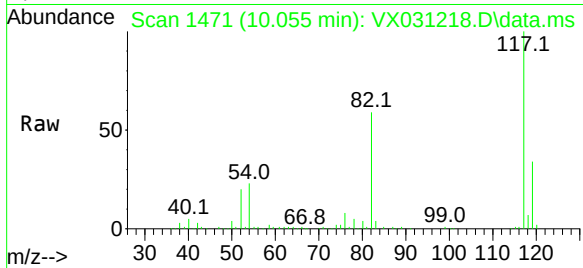

#68
m/p-Xylenes
Concen: 0.292 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Tgt Ion:106 Resp: 606
Ion Ratio Lower Upper
106 100
91 269.0 158.2 237.4#



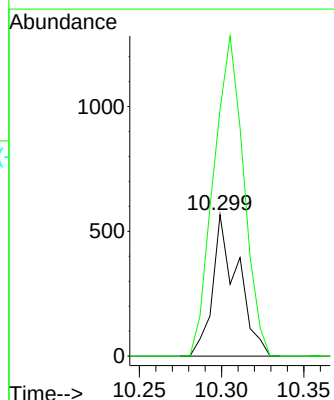
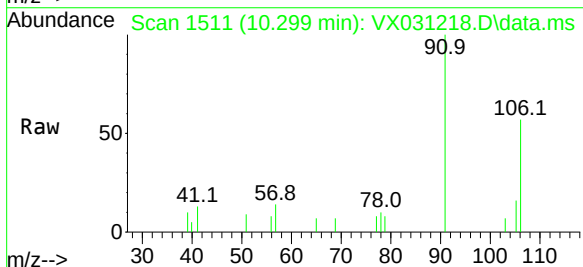




#69
o-Xylene
Concen: 0.398 ug/l
RT: 10.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50




Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Tgt Ion:106 Resp: 824
Ion Ratio Lower Upper
106 100
91 237.6 103.8 311.6

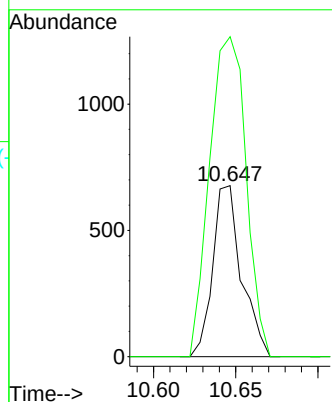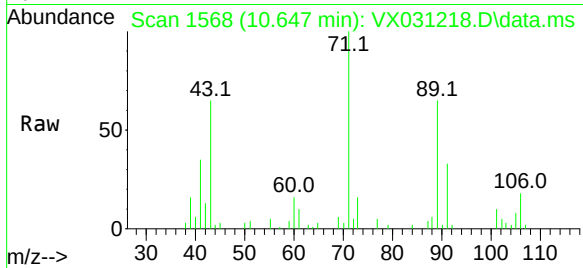

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Tgt Ion:152 Resp: 47897
Ion Ratio Lower Upper
152 100
115 67.2 40.5 121.5
150 155.3 0.0 347.0

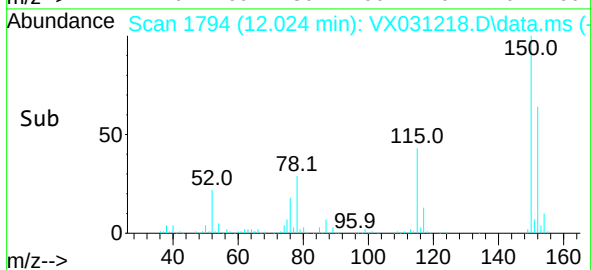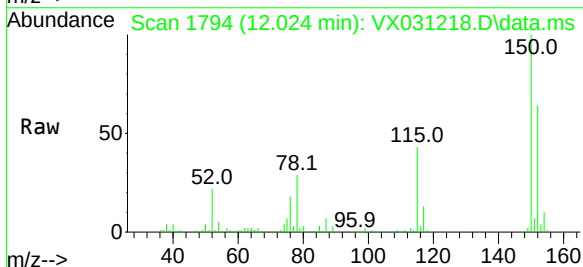



#76

1,2,3-Trichloropropane

Concen: 35.328 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX031218.D

Acq: 08 Sep 2022 17:50

Instrument :

MSVOA_X

ClientSampleId :





WC-14-A-SP

Tgt Ion: 75 Resp: 46180

Ion Ratio Lower Upper

75 100

77 0.8 19.8 59.3#

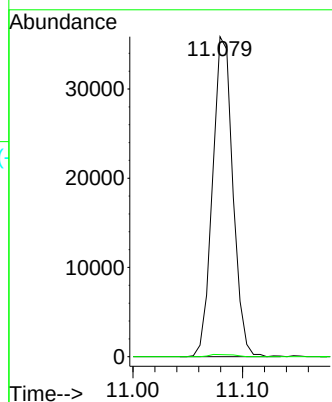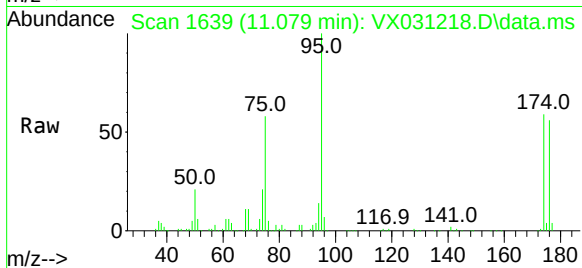

#80

1,3,5-Trimethylbenzene

Concen: 3.160 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX031218.D




Acq: 08 Sep 2022 17:50


Tgt Ion: 105 Resp: 11048

Ion Ratio Lower Upper

105 100

120 45.2 24.4 73.2


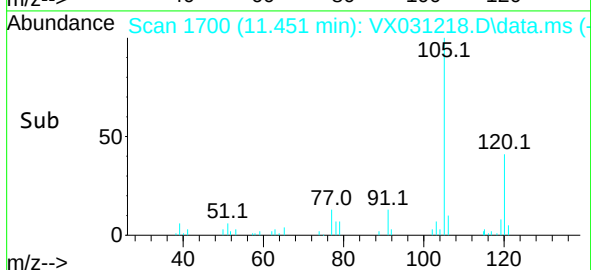

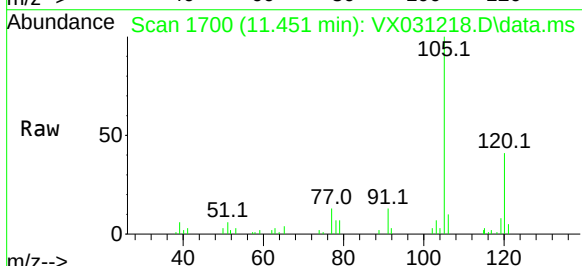




#81
trans-1,4-Dichloro-2-butene
Concen: 113.928 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50




Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Tgt Ion: 75 Resp: 46180
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.0 34.8 52.2#

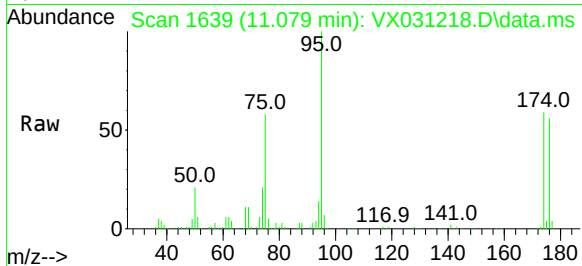

#82
4-Chlorotoluene
Concen: 0.492 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Tgt Ion: 91 Resp: 1673
Ion Ratio Lower Upper
91 100
126 0.0 15.3 45.9#


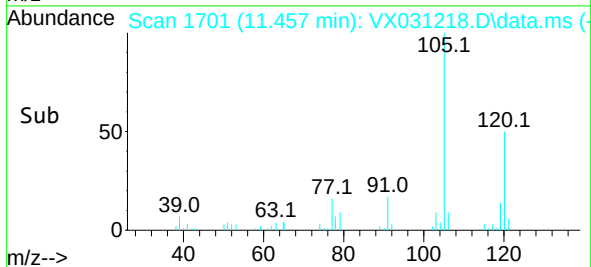

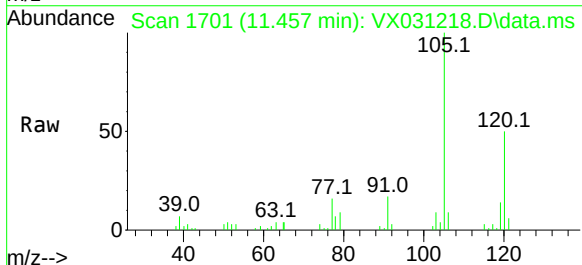




#84
1,2,4-Trimethylbenzene
Concen: 0.979 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50




Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Tgt Ion:105 Resp: 3329
Ion Ratio Lower Upper
105 100
120 41.2 22.9 68.8

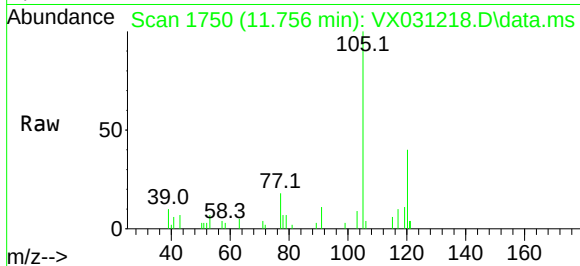

#85
sec-Butylbenzene
Concen: 0.780 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Tgt Ion:105 Resp: 3329
Ion Ratio Lower Upper
105 100
134 0.0 10.0 30.0#


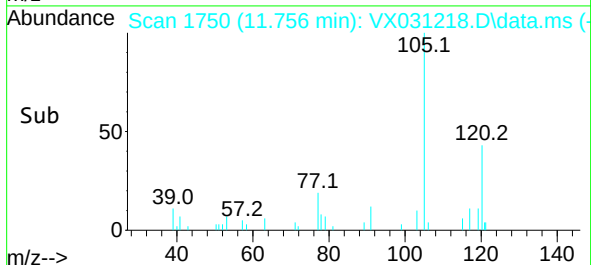

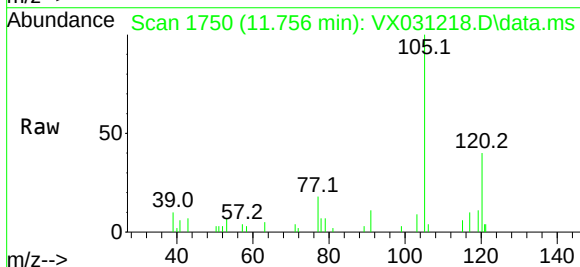




#86
p-Isopropyltoluene
Concen: 0.784 ug/l
RT: 11.976 min Scan# 11
Delta R.T. -0.037 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50




Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Tgt Ion:119 Resp: 2704
Ion Ratio Lower Upper
119 100
134 27.6 13.9 41.6
91 26.8 11.8 35.3

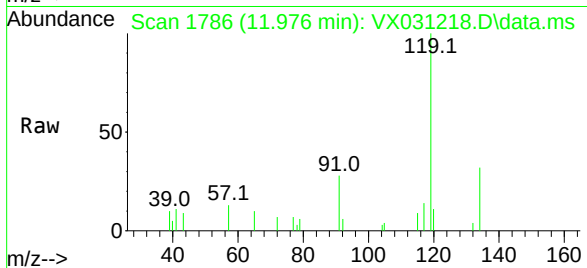

#89
n-Butylbenzene
Concen: 0.580 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Tgt Ion: 91 Resp: 1724
Ion Ratio Lower Upper
91 100
92 8.8 26.2 78.5#
134 117.0 12.6 37.8#


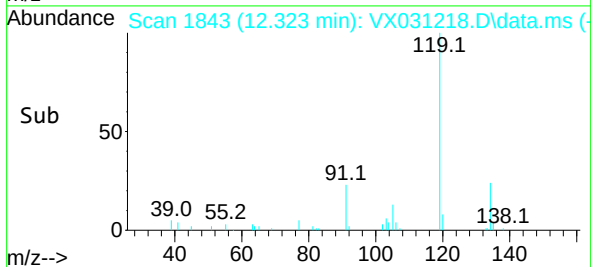

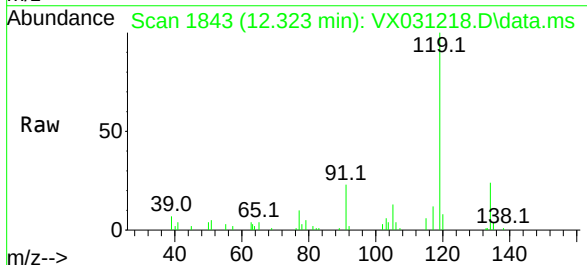




#90
Hexachloroethane
Concen: 1.357 ug/l
RT: 12.567 min Scan# 117
Delta R.T. 0.024 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50




Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP


Tgt Ion:117 Resp: 804
Ion Ratio Lower Upper
117 100
201 0.0 34.2 102.5#

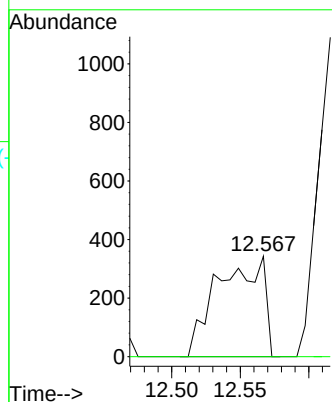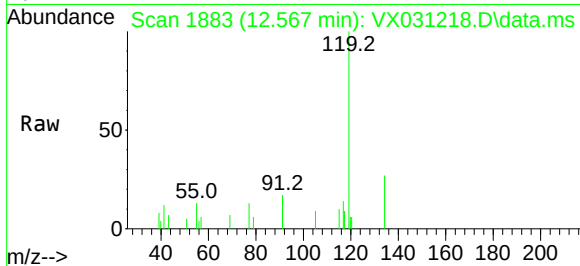

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.376 ug/l
RT: 12.969 min Scan# 1949
Delta R.T. 0.024 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50


Tgt Ion: 75 Resp: 134
Ion Ratio Lower Upper
75 100
155 0.0 45.0 134.8#
157 0.0 56.9 170.7#

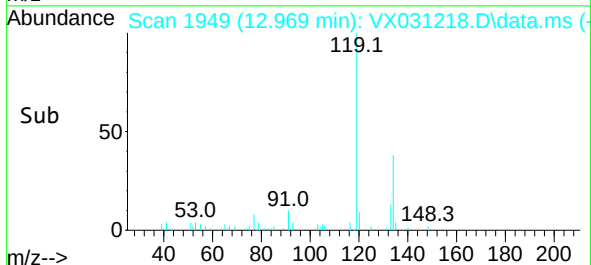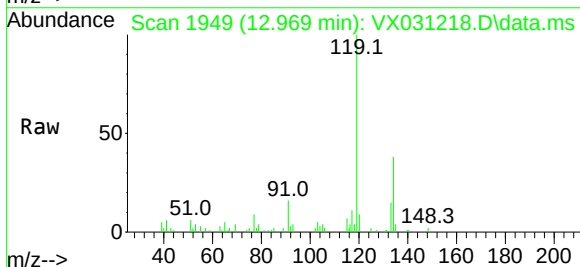

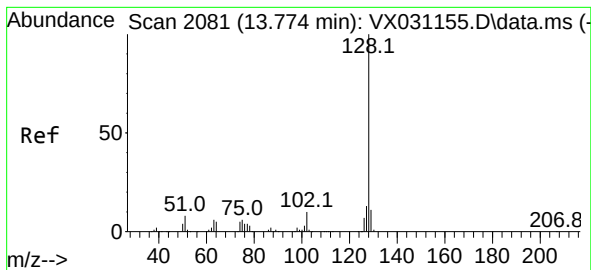

#95
Naphthalene
Concen: 0.735 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX031218.D
Acq: 08 Sep 2022 17:50

Instrument :
MSVOA_X
ClientSampleId :
WC-14-A-SP

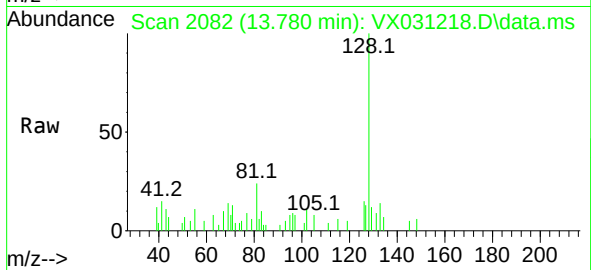

Tgt Ion:128 Resp: 2774
Ion Ratio Lower Upper
128 100
127 10.6 10.2 15.2
129 30.8 8.6 13.0#

