
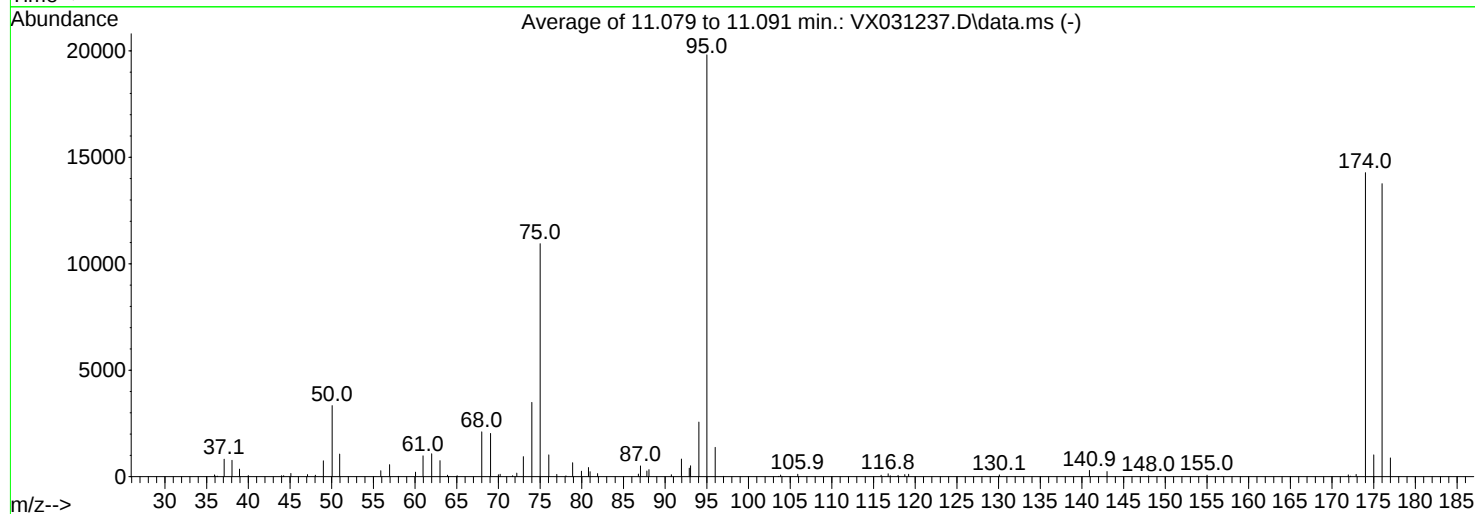


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090822\
Data File : VX031237.D
Acq On : 09 Sep 2022 01:39
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Title : SW846 8260
Last Update : Wed Sep 07 23:22:41 2022

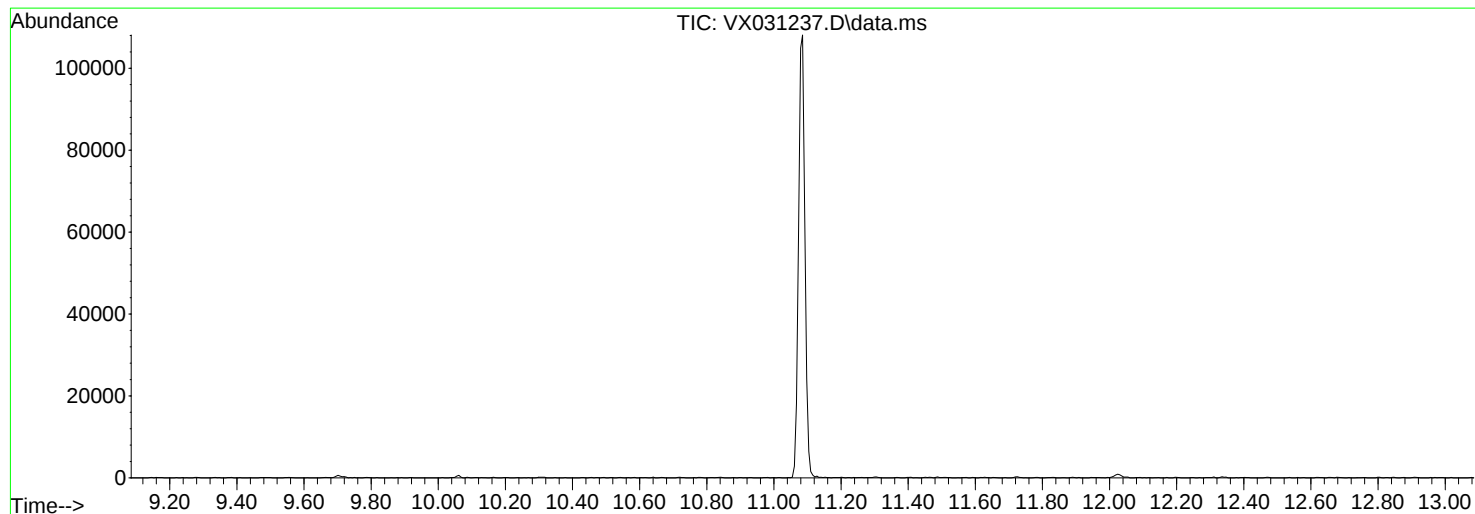

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	3338	PASS
75	95	30	60	55.2	10944	PASS
95	95	100	100	100.0	19815	PASS
96	95	5	9	6.9	1373	PASS
173	174	0.00	2	0.8	108	PASS
174	95	50	100	72.1	14283	PASS
175	174	5	9	7.1	1020	PASS
176	174	95	101	96.4	13763	PASS
177	176	5	9	6.4	881	PASS