
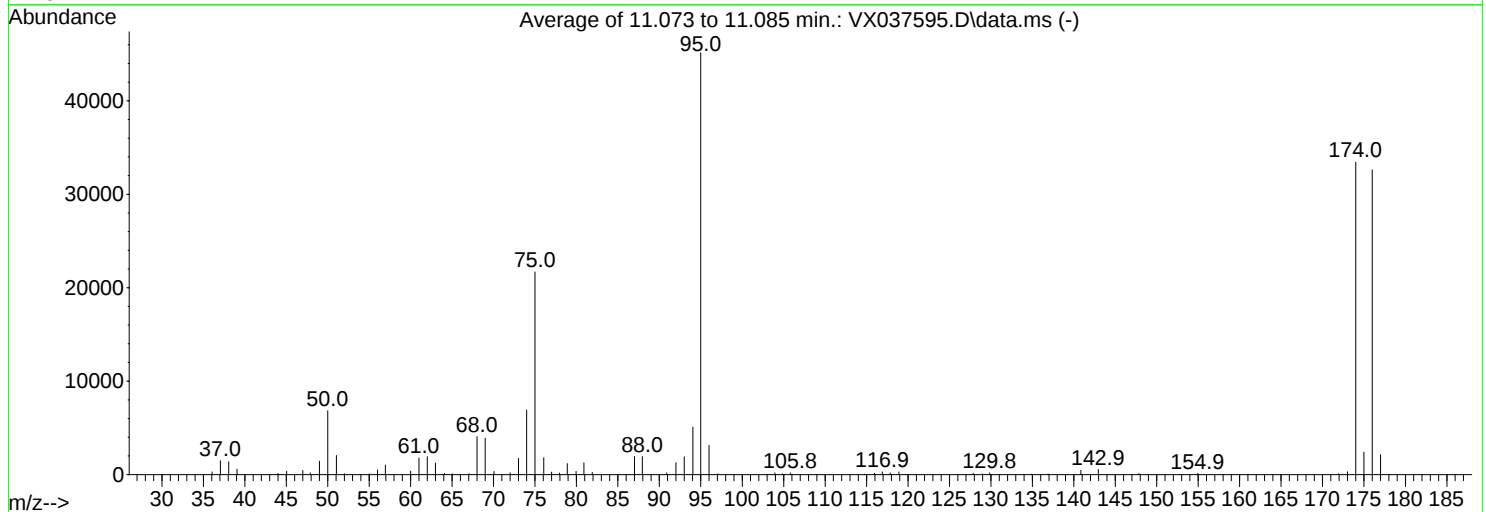


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090823\
Data File : VX037595.D
Acq On : 08 Sep 2023 09:50
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M
Title : SW846 8260
Last Update : Sat Sep 09 06:38:11 2023

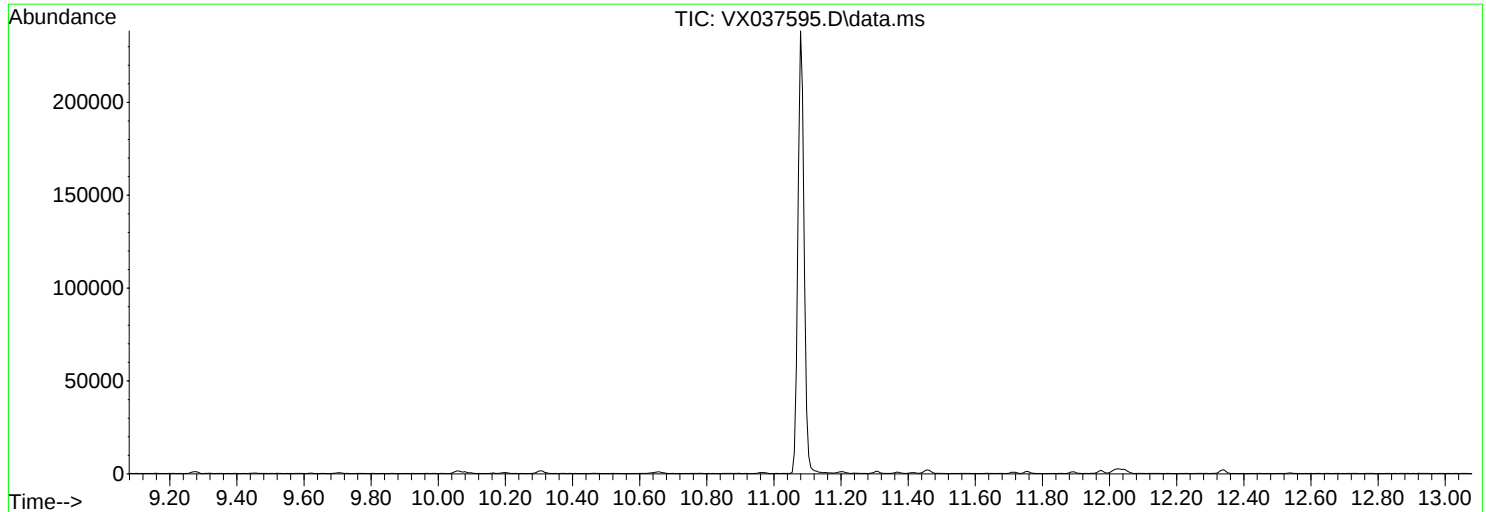

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	6837	PASS
75	95	30	60	48.1	21701	PASS
95	95	100	100	100.0	45133	PASS
96	95	5	9	6.9	3132	PASS
173	174	0.00	2	0.9	306	PASS
174	95	50	100	74.1	33445	PASS
175	174	5	9	7.2	2421	PASS
176	174	95	101	97.5	32611	PASS
177	176	5	9	6.5	2134	PASS