

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090922\
 Data File : VX031267.D
 Acq On : 09 Sep 2022 19:16
 Operator : JC/MD
 Sample : N4360-14RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB02-20220823RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M

Title : SW846 8260

Signal : TIC: VX031267.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	695	706	719	rBV3	52668	150700	39.50%	8.640%
2	5.556	722	733	744	rBV2	57238	160536	42.08%	9.204%
3	5.958	790	799	815	rBB	61683	161529	42.34%	9.261%
4	6.763	922	931	942	rBV	80637	190440	49.92%	10.919%
5	8.653	1234	1241	1250	rBV	240055	381496	100.00%	21.873%
6	10.055	1465	1471	1481	rBB	171874	223795	58.66%	12.831%
7	11.085	1634	1640	1647	rBV	208095	273296	71.64%	15.669%
8	12.024	1789	1794	1800	rBV	168965	202389	53.05%	11.604%




Sum of corrected areas: 1744181

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090922\
Data File : VX031267.D
Acq On : 09 Sep 2022 19:16
Operator : JC/MD
Sample : N4360-14RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB02-20220823RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

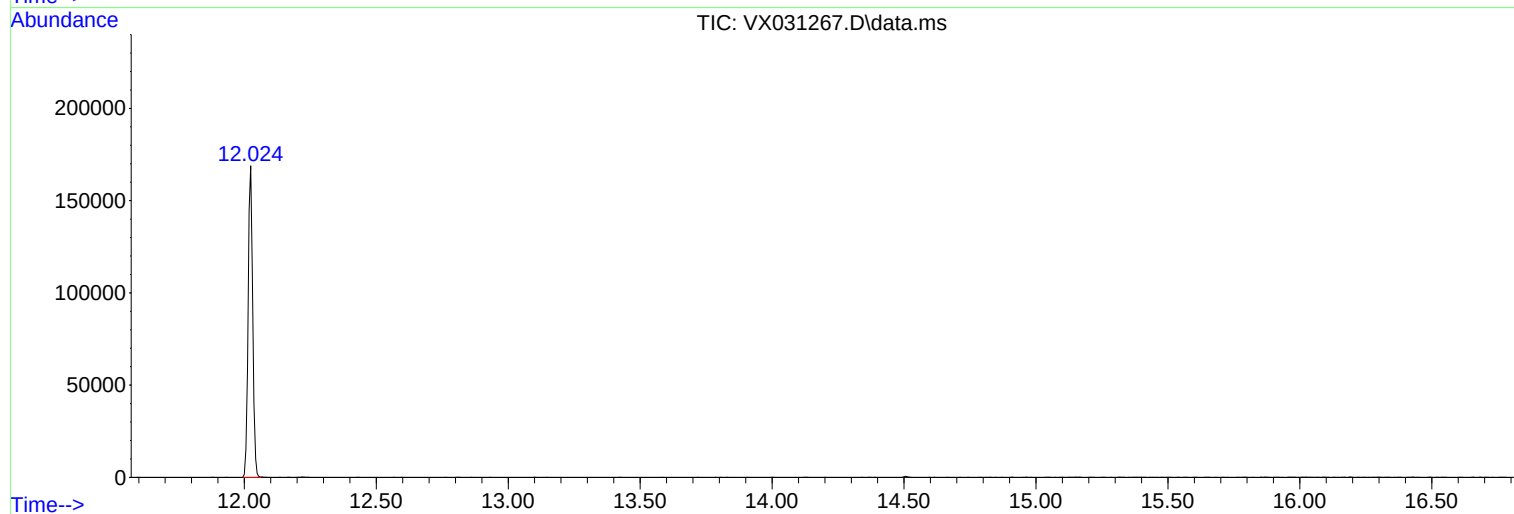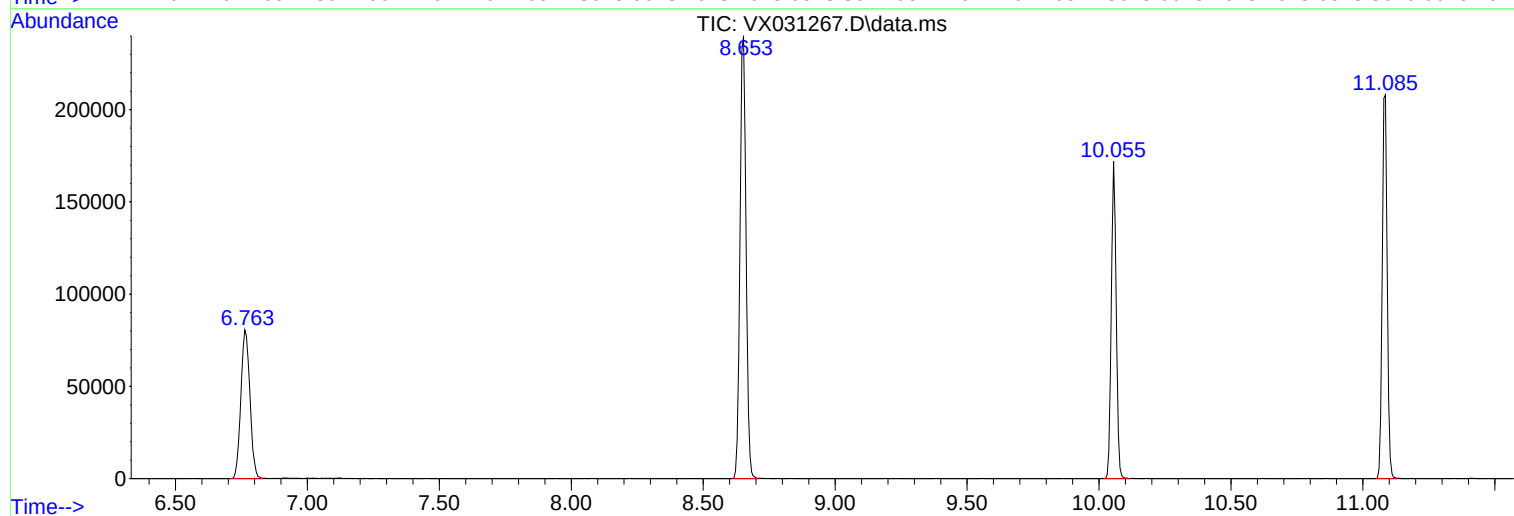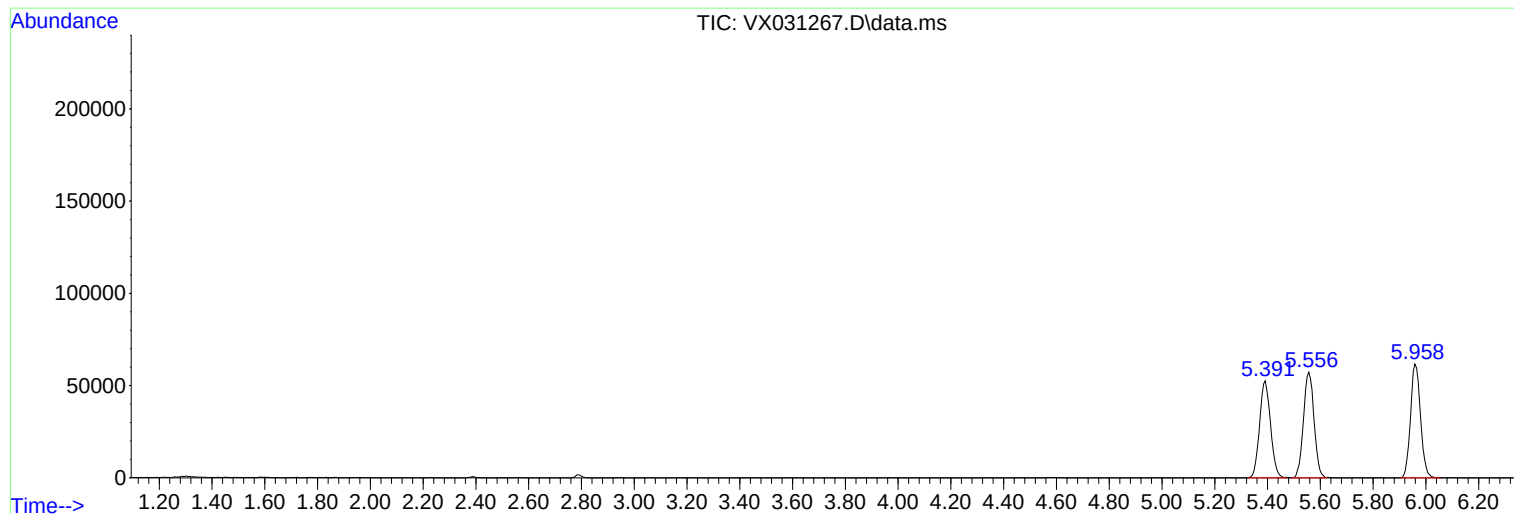

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090922\
Data File : VX031267.D
Acq On : 09 Sep 2022 19:16
Operator : JC/MD
Sample : N4360-14RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB02-20220823RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090922\
Data File : VX031267.D
Acq On : 09 Sep 2022 19:16
Operator : JC/MD
Sample : N4360-14RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB02-20220823RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc