

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090923\
 Data File : VX037633.D
 Acq On : 09 Sep 2023 17:26
 Operator : JC/MD
 Sample : 04297-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 713-G-DIP

Quant Time: Sep 11 01:25:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 09 06:38:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	148909	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	243322	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	216952	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	99031	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	81769	40.679	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	81.360%
35) Dibromofluoromethane	5.385	113	73069	42.934	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	85.860%
50) Toluene-d8	8.647	98	284549	45.586	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	91.180%#
62) 4-Bromofluorobenzene	11.079	95	104768	44.534	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.060%


Target Compounds						Qvalue
11) Tert butyl alcohol	2.965	59	6124	13.615	ug/l #	95
14) Allyl chloride	2.544	41	1203	0.536	ug/l #	78
16) Acetone	2.380	43	60074	72.675	ug/l #	82
18) Methyl Acetate	2.703	43	3722	1.110	ug/l	95
20) Methylene Chloride	2.788	84	435	Below Cal	#	68
25) 2-Butanone	4.556	43	472859	377.183	ug/l #	83
29) Tetrahydrofuran	5.019	42	3557	4.429	ug/l #	47
31) Cyclohexane	5.562	56	2501	1.023	ug/l #	1
36) 1,1-Dichloropropene	5.550	75	10743	4.778	ug/l #	50
37) Ethyl Acetate	4.556	43	472859	205.120	ug/l #	69
38) Carbon Tetrachloride	5.550	117	15388	6.622	ug/l #	15
41) Methacrylonitrile	5.013	41	11236	9.568	ug/l #	45
49) 1,4-Dioxane	7.671	88	889	17.146	ug/l #	100
51) 4-Methyl-2-Pentanone	8.580	43	1663	0.757	ug/l	95
52) Toluene	8.720	92	1402	0.312	ug/l	99
59) 2-Hexanone	9.439	43	2453	1.465	ug/l	98
67) Ethyl Benzene	10.195	91	5310	0.655	ug/l	99
68) m/p-Xylenes	10.299	106	16448	5.161	ug/l	97
69) o-Xylene	10.640	106	4843	1.528	ug/l	99
74) N-amyl acetate	10.750	43	48451	18.896	ug/l #	1
76) 1,2,3-Trichloropropane	11.079	75	48893	21.090	ug/l #	39
78) n-propylbenzene	11.305	91	5126	0.620	ug/l	99
79) 2-Chlorotoluene	11.378	91	3873	0.737	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	11909	1.887	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	48893	63.119	ug/l #	5
82) 4-Chlorotoluene	11.451	91	1547	0.261	ug/l #	46
84) 1,2,4-Trimethylbenzene	11.750	105	45862	7.270	ug/l	94
85) sec-Butylbenzene	11.750	105	45862	5.981	ug/l #	57
89) n-Butylbenzene	12.329	91	2358	0.442	ug/l #	28
90) Hexachloroethane	12.549	117	318	0.288	ug/l #	17
95) Naphthalene	13.774	128	12936	1.754	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090923\
Data File : VX037633.D
Acq On : 09 Sep 2023 17:26
Operator : JC/MD
Sample : 04297-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP

Quant Time: Sep 11 01:25:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 09 06:38:11 2023
Response via : Initial Calibration




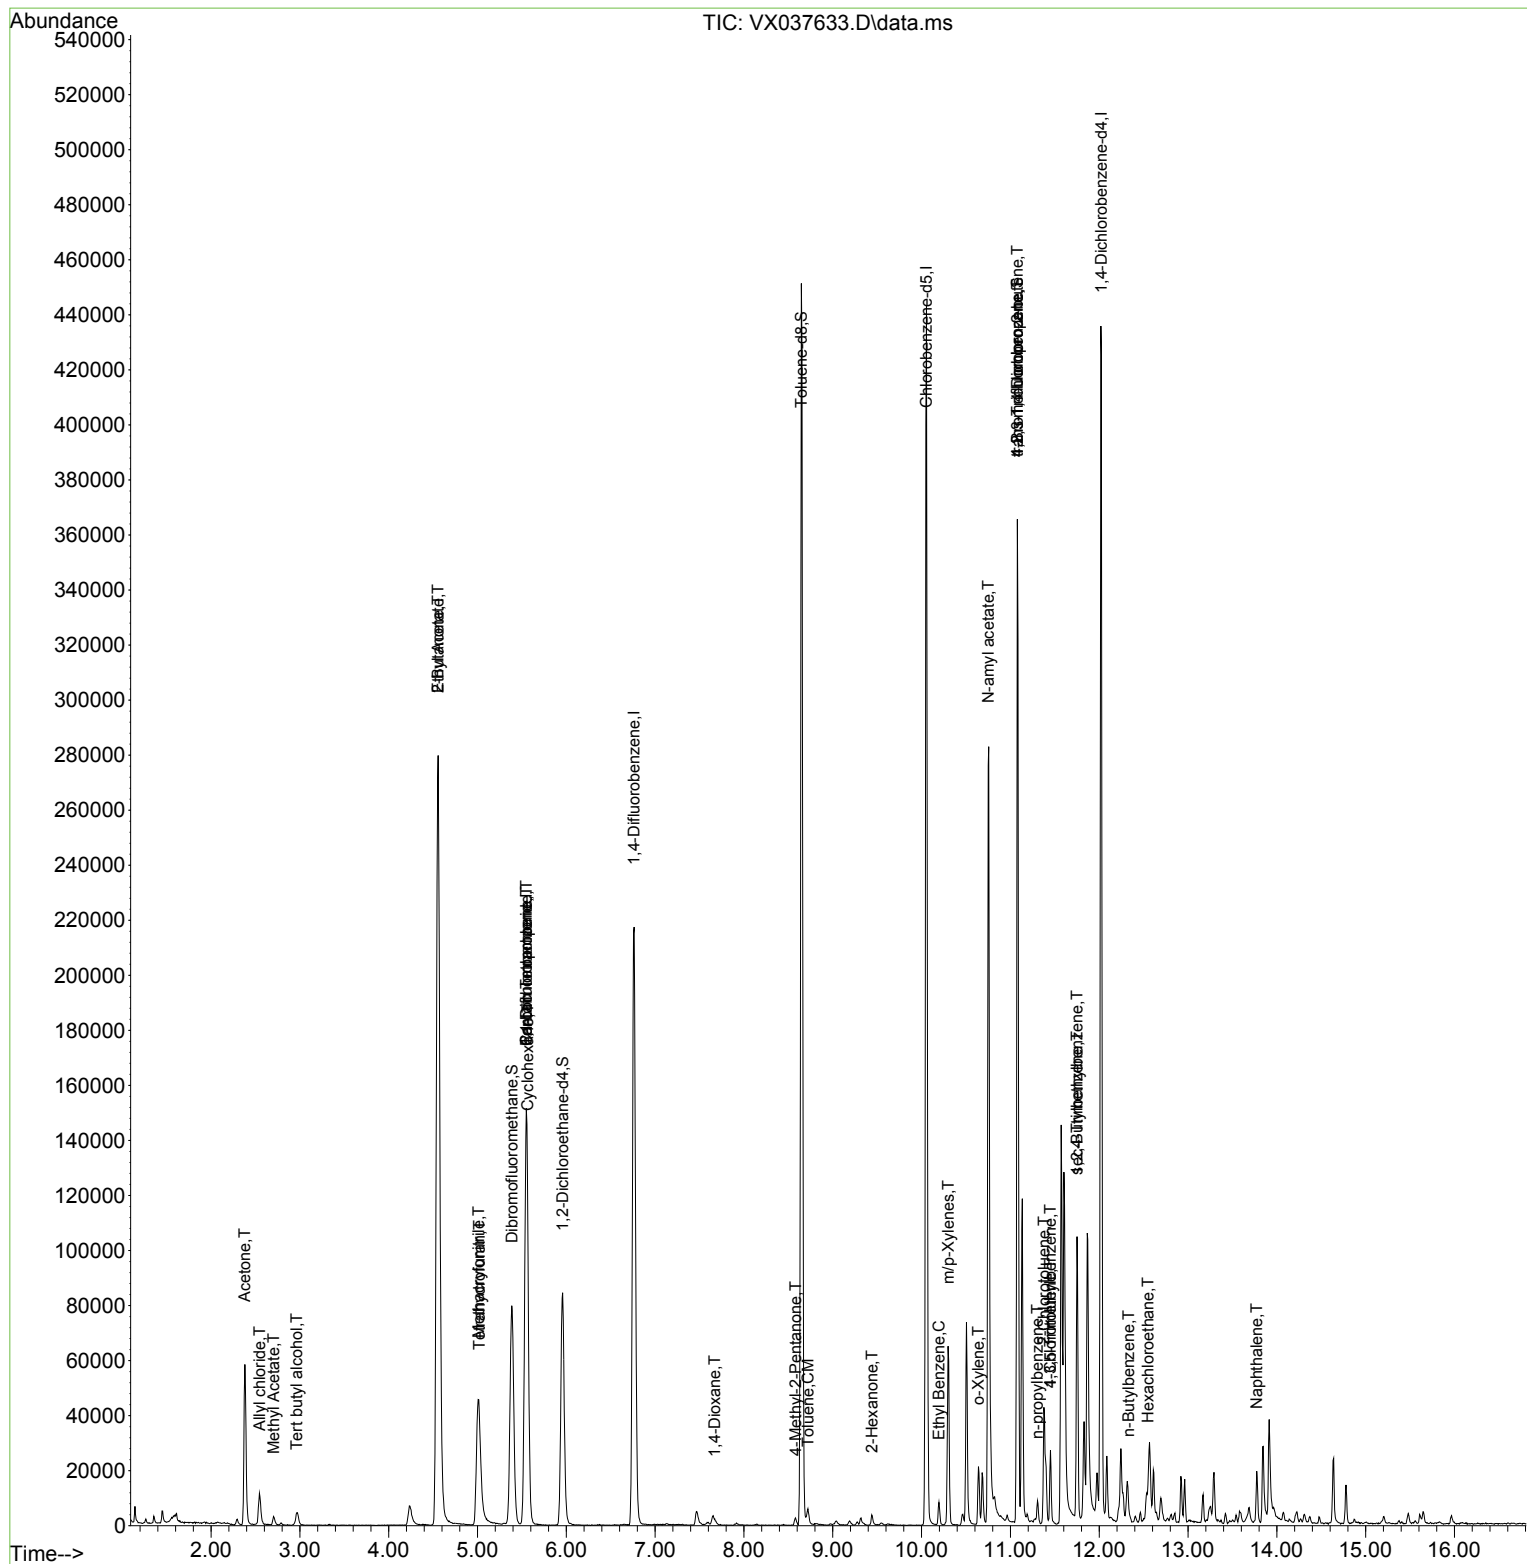


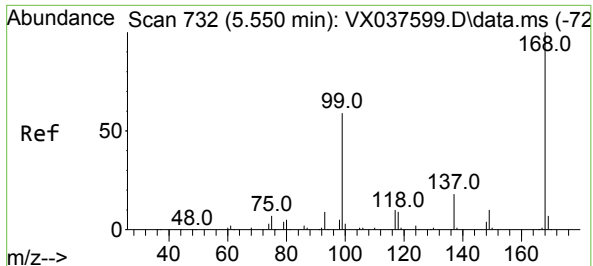

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26




Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP


Tgt Ion:168 Resp: 148909
Ion Ratio Lower Upper
168 100
99 59.7 56.6 85.0

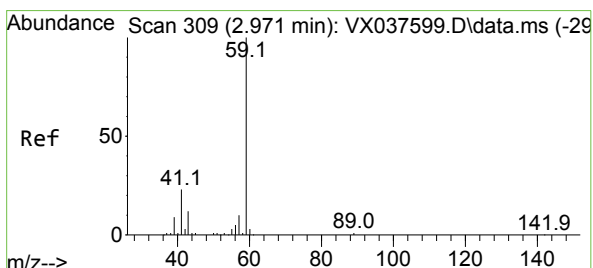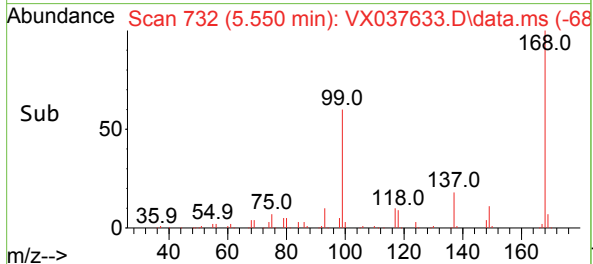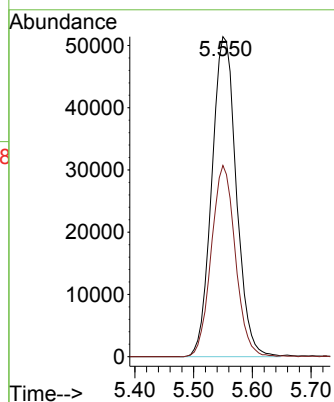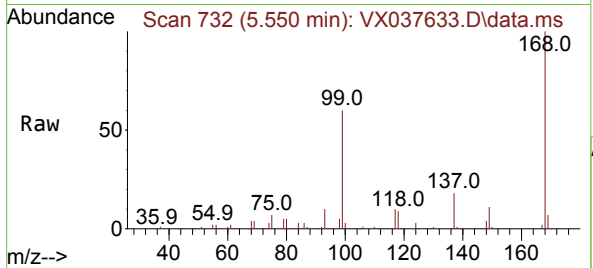

#11
Tert butyl alcohol
Concen: 13.615 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.006 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Tgt Ion: 59 Resp: 6124
Ion Ratio Lower Upper
59 100
57 9.2 6.0 9.0#

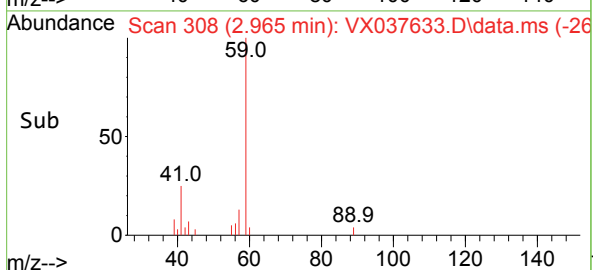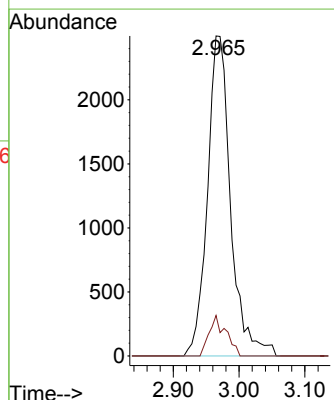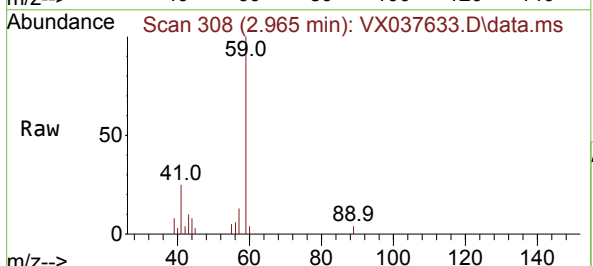



#14

Allyl chloride

Concen: 0.536 ug/l

RT: 2.544 min Scan# 21

Delta R.T. -0.116 min

Lab File: VX037633.D

Acq: 09 Sep 2023 17:26

Instrument :

MSVOA_X

ClientSampleId :

713-G-DIP





Tgt Ion: 41 Resp: 1203

Ion Ratio Lower Upper

41 100

39 75.2 55.8 83.6

76 0.0 24.3 36.5#



#16

Acetone

Concen: 72.675 ug/l

RT: 2.380 min Scan# 212

Delta R.T. -0.006 min

Lab File: VX037633.D




Acq: 09 Sep 2023 17:26


Tgt Ion: 43 Resp: 60074

Ion Ratio Lower Upper

43 100

58 36.9 21.9 32.9#

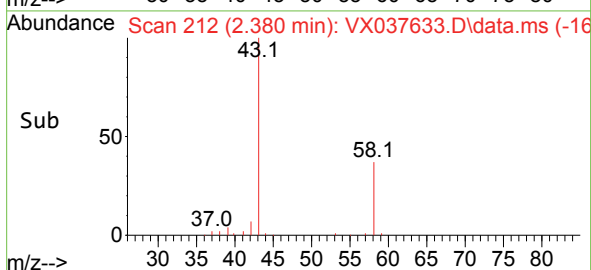



#18

Methyl Acetate

Concen: 1.110 ug/l

RT: 2.703 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX037633.D

Acq: 09 Sep 2023 17:26

Instrument :

MSVOA_X

ClientSampleId :





713-G-DIP

Tgt Ion: 43 Resp: 3722

Ion Ratio Lower Upper

43 100

74 24.7 17.8 26.8

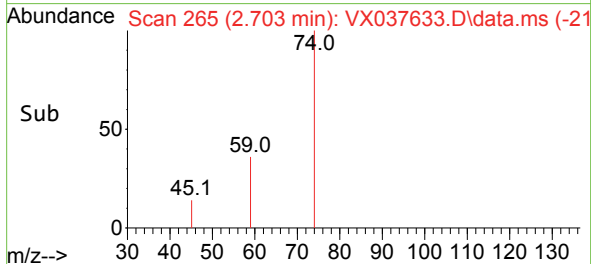

#20

Methylene Chloride

Concen: Below Cal

RT: 2.788 min Scan# 279

Delta R.T. 0.000 min

Lab File: VX037633.D

Acq: 09 Sep 2023 17:26

Tgt Ion: 84 Resp: 435




Ion Ratio Lower Upper


84 100

49 90.2 103.6 155.4#

51 19.3 33.8 50.6#

86 43.2 49.4 74.0#



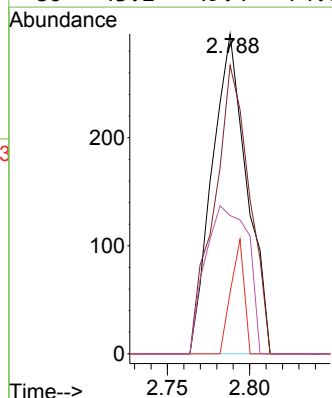





#25
2-Butanone
Concen: 377.183 ug/l
RT: 4.556 min Scan# 50
Delta R.T. -0.006 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26




Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP


Tgt Ion: 43 Resp: 472859
Ion Ratio Lower Upper
43 100
72 32.8 19.4 29.2#

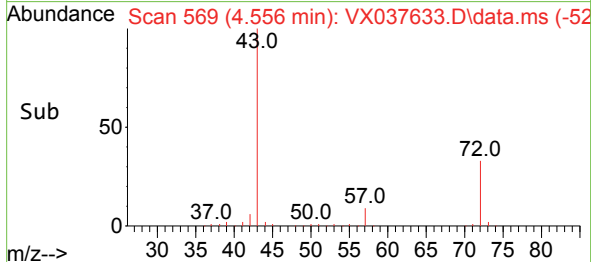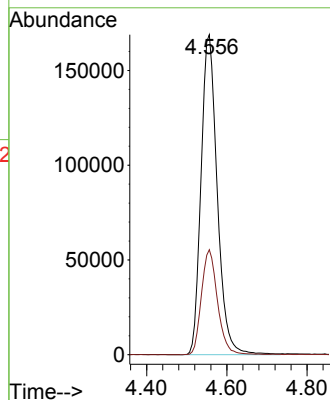

#29
Tetrahydrofuran
Concen: 4.429 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.012 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Tgt Ion: 42 Resp: 3557
Ion Ratio Lower Upper
42 100
72 93.4 34.2 51.4#
71 24.3 32.2 48.2#


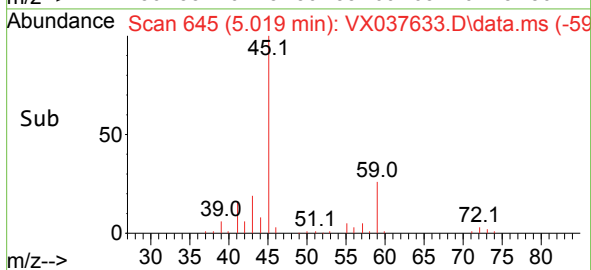
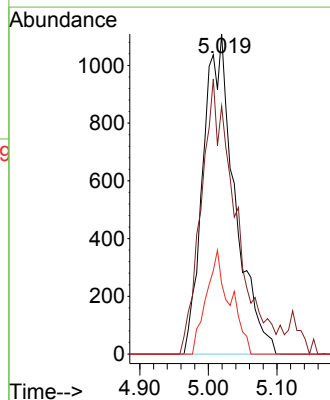
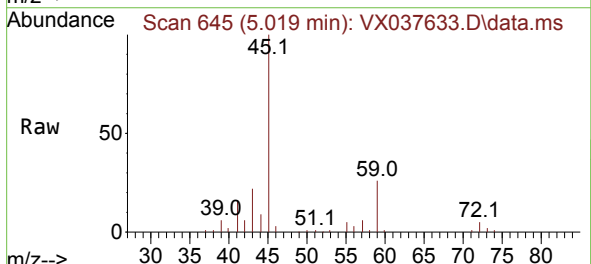


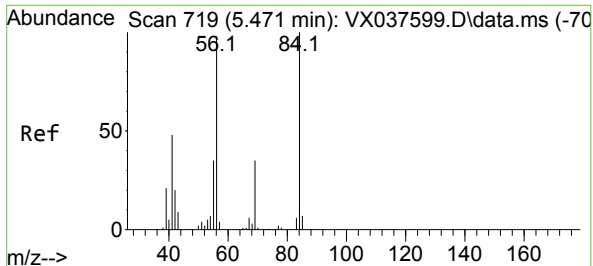

#31
Cyclohexane
Concen: 1.023 ug/l
RT: 5.562 min Scan# 719
Delta R.T. 0.091 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26




Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP


Tgt Ion: 56 Resp: 2501
Ion Ratio Lower Upper
56 100
69 151.4 23.4 35.2#
84 156.2 65.9 98.9#

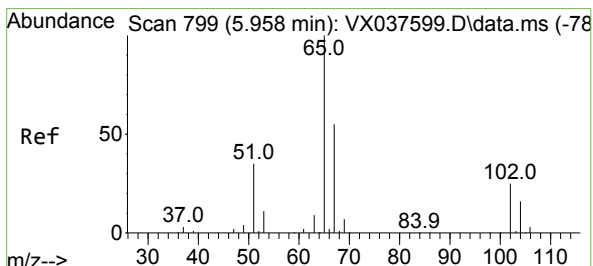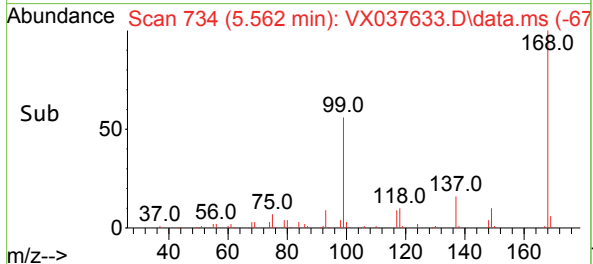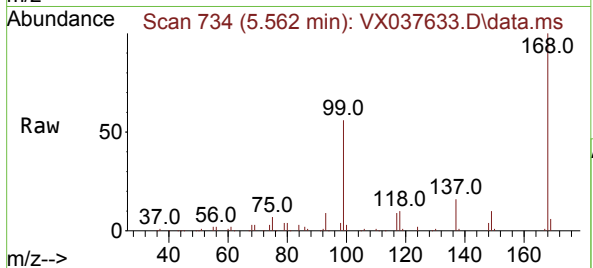

#33
1,2-Dichloroethane-d4
Concen: 40.679 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Tgt Ion: 65 Resp: 81769
Ion Ratio Lower Upper
65 100
67 53.6 0.0 100.2


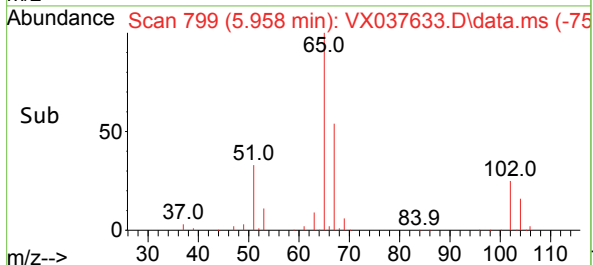

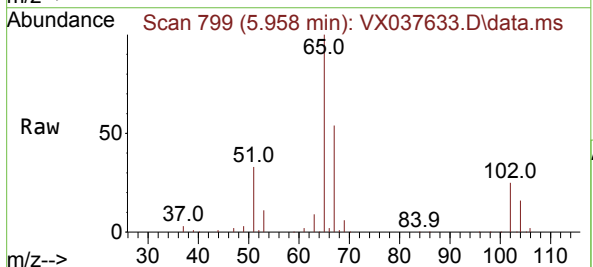




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26




Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP


Tgt Ion:114 Resp: 243322
Ion Ratio Lower Upper
114 100
63 18.2 0.0 45.0
88 16.3 0.0 36.6

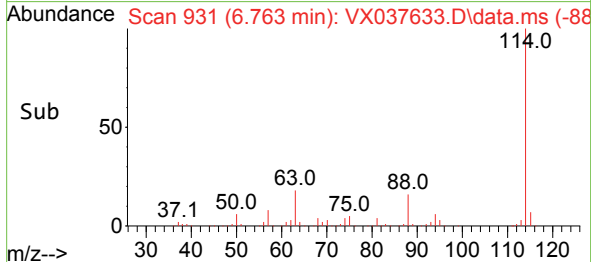

#35
Dibromofluoromethane
Concen: 42.934 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Tgt Ion:113 Resp: 73069
Ion Ratio Lower Upper
113 100
111 103.4 82.9 124.3
192 19.6 13.3 19.9


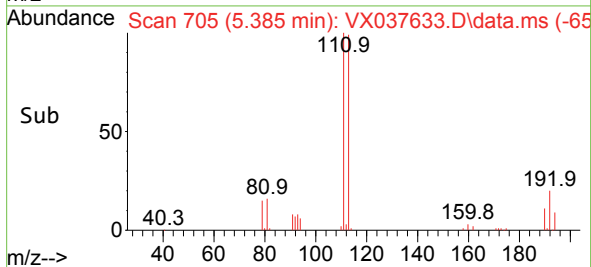

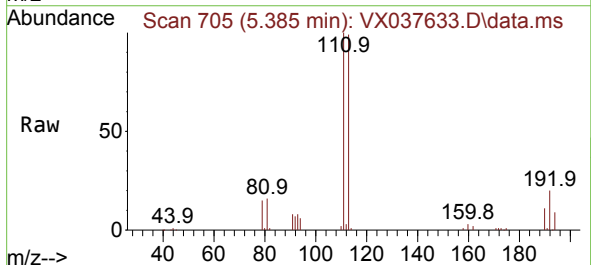




#36
1,1-Dichloropropene
Concen: 4.778 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26




Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP


Tgt Ion: 75 Resp: 10743
Ion Ratio Lower Upper
75 100
110 9.0 17.0 50.9#
77 0.0 24.7 37.1#

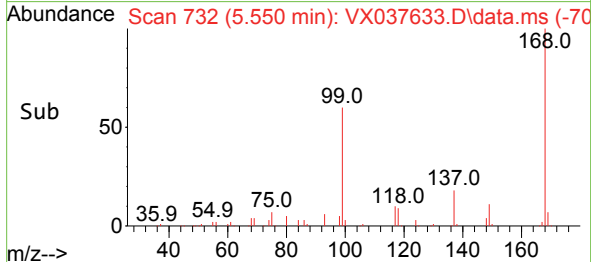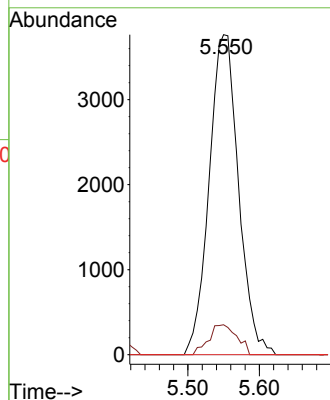

#37
Ethyl Acetate
Concen: 205.120 ug/l
RT: 4.556 min Scan# 569
Delta R.T. -0.165 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26


Tgt Ion: 43 Resp: 472859
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.1 8.3 12.5#

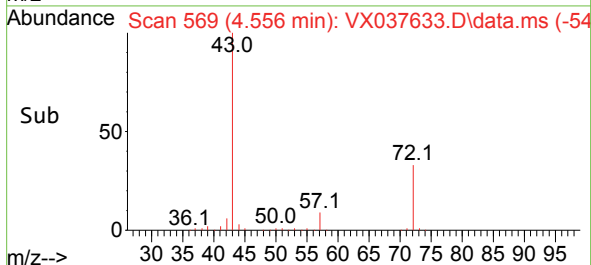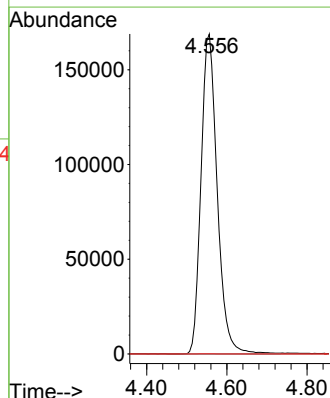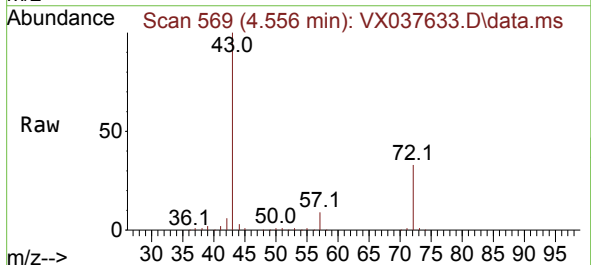






#38
Carbon Tetrachloride
Concen: 6.622 ug/l
RT: 5.550 min Scan# 713
Delta R.T. -0.128 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP



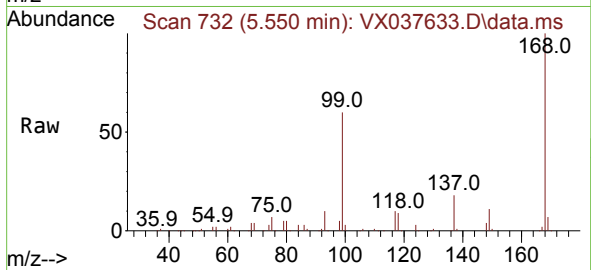



Tgt Ion:117 Resp: 15388
Ion Ratio Lower Upper
117 100
119 4.4 78.2 117.2#
121 0.0 24.4 36.6#



#41
Methacrylonitrile
Concen: 9.568 ug/l
RT: 5.013 min Scan# 644
Delta R.T. 0.091 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Tgt Ion: 41 Resp: 11236
Ion Ratio Lower Upper
41 100
39 37.8 45.2 67.8#
67 0.0 52.6 78.8#
52 1.1 22.7 34.1#

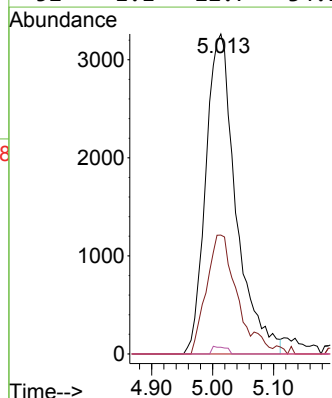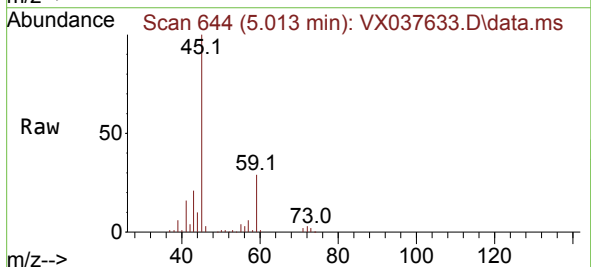



#49

1,4-Dioxane

Concen: 17.146 ug/l

RT: 7.671 min Scan# 1079

Delta R.T. 0.006 min

Lab File: VX037633.D

Acq: 09 Sep 2023 17:26

Instrument :

MSVOA_X

ClientSampleId :

713-G-DIP





Tgt Ion: 88 Resp: 889

Ion Ratio Lower Upper

88 100

43 64.2 0.0 0.0#

58 75.4 60.1 90.1

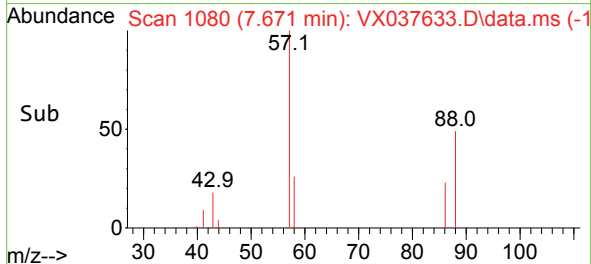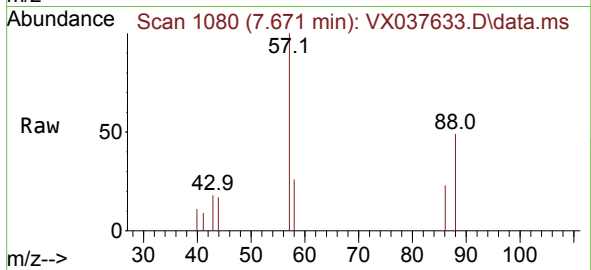

#50

Toluene-d8

Concen: 45.586 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX037633.D




Acq: 09 Sep 2023 17:26


Tgt Ion: 98 Resp: 284549

Ion Ratio Lower Upper

98 100

100 67.0 53.1 79.7


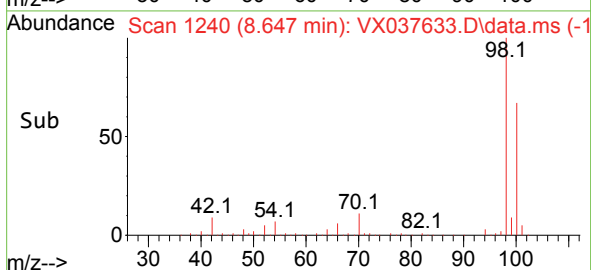






#51
4-Methyl-2-Pentanone
Concen: 0.757 ug/l
RT: 8.580 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26




Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP


Tgt Ion: 43 Resp: 1663
Ion Ratio Lower Upper
43 100
58 41.3 30.4 45.6

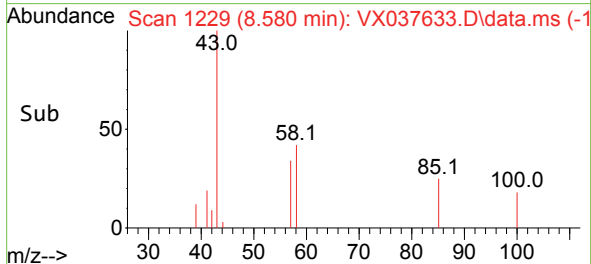

#52
Toluene
Concen: 0.312 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Tgt Ion: 92 Resp: 1402
Ion Ratio Lower Upper
92 100
91 166.8 134.2 201.2


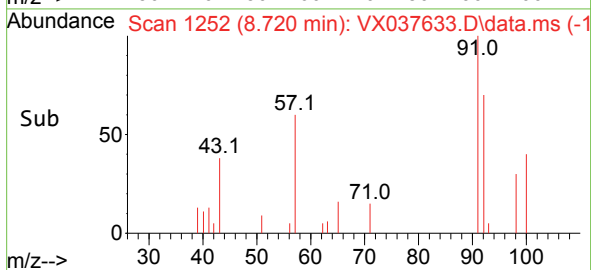

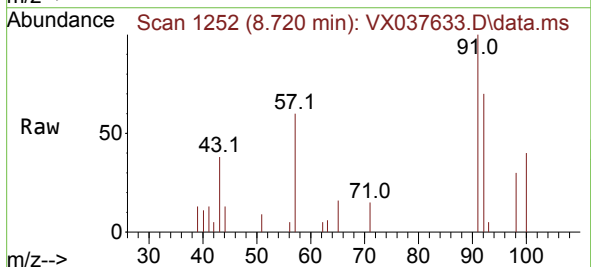




#59
2-Hexanone
Concen: 1.465 ug/l
RT: 9.439 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26




Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP


Tgt Ion: 43 Resp: 2453
Ion Ratio Lower Upper
43 100
58 53.8 26.2 78.5

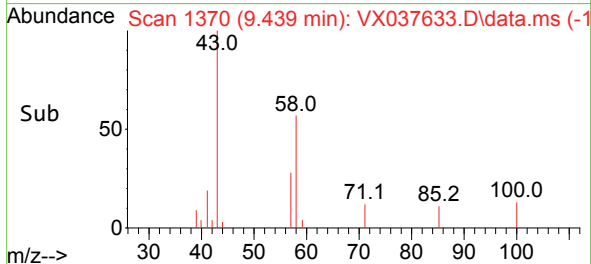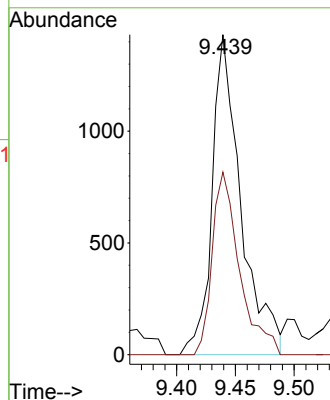

#62
4-Bromofluorobenzene
Concen: 44.534 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Tgt Ion: 95 Resp: 104768
Ion Ratio Lower Upper
95 100
174 76.1 0.0 135.6
176 73.6 0.0 131.0



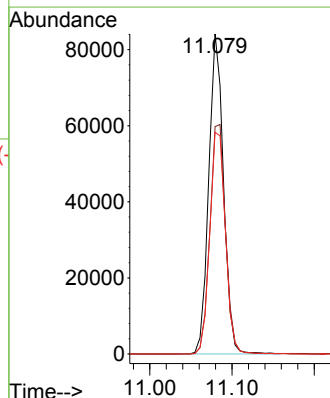
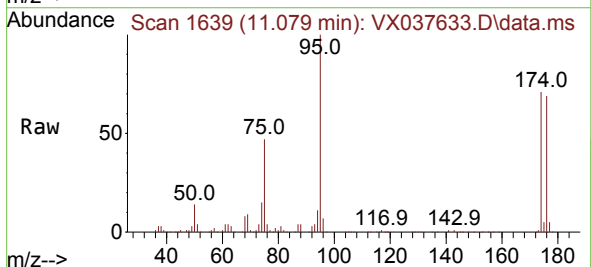




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26




Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP


Tgt Ion:117 Resp: 216952
Ion Ratio Lower Upper
117 100
82 52.9 46.2 69.4
119 31.9 25.5 38.3

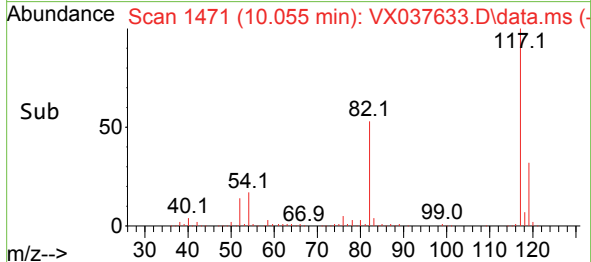

#67
Ethyl Benzene
Concen: 0.655 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Tgt Ion: 91 Resp: 5310
Ion Ratio Lower Upper
91 100
106 31.8 24.9 37.3


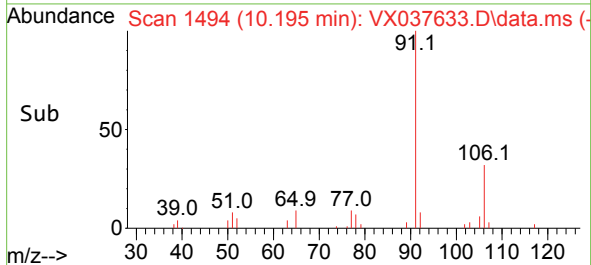

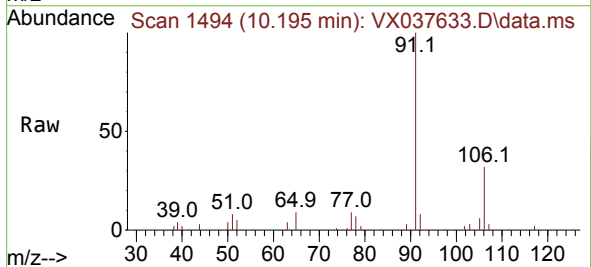


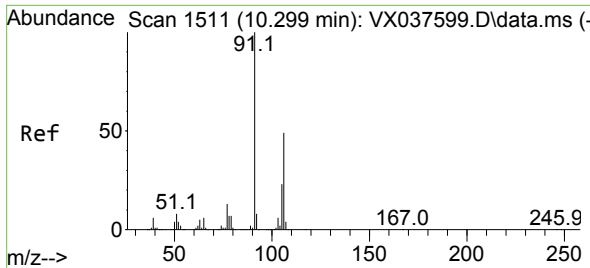

#68
m/p-Xylenes
Concen: 5.161 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26




Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP


Tgt Ion:106 Resp: 16448
Ion Ratio Lower Upper
106 100
91 202.1 165.5 248.3

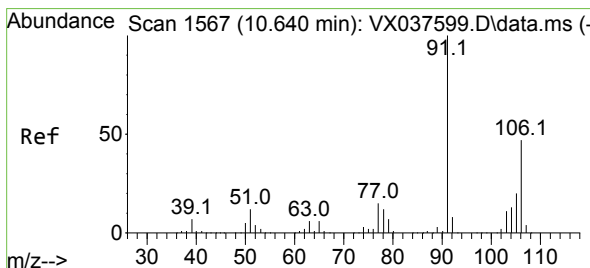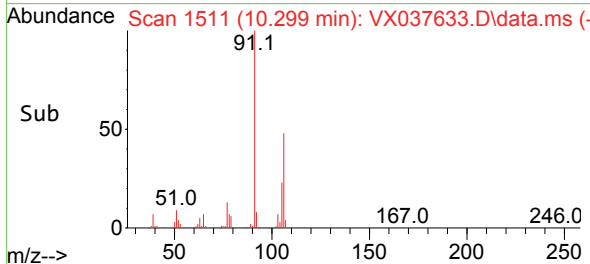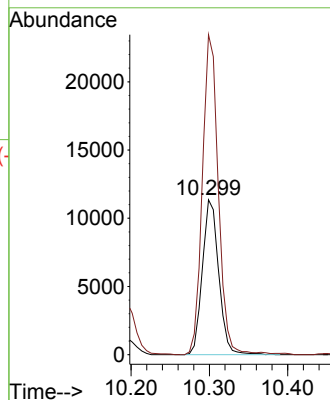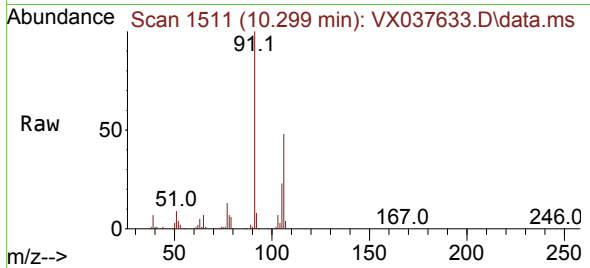

#69
o-Xylene
Concen: 1.528 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Tgt Ion:106 Resp: 4843
Ion Ratio Lower Upper
106 100
91 216.8 108.9 326.8

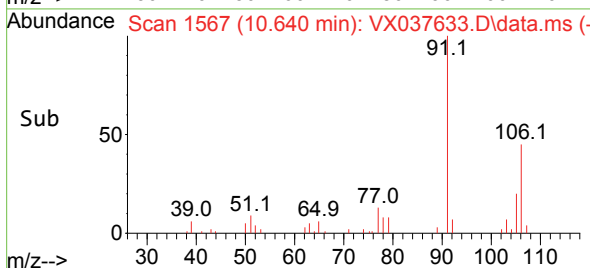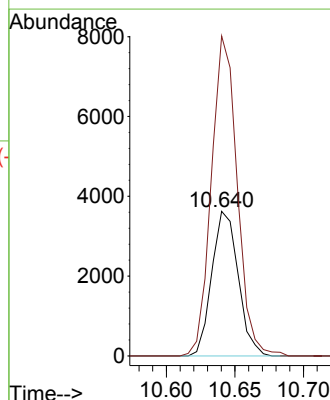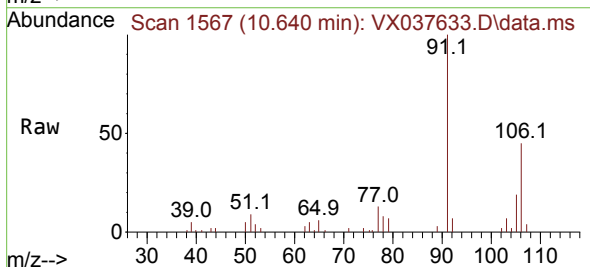



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX037633.D

Acq: 09 Sep 2023 17:26

Instrument :

MSVOA_X

ClientSampleId :

713-G-DIP





Tgt Ion:152 Resp: 99031

Ion Ratio Lower Upper

152 100

115 61.7 43.3 129.9

150 155.7 0.0 345.0

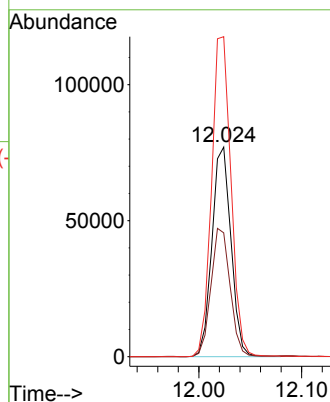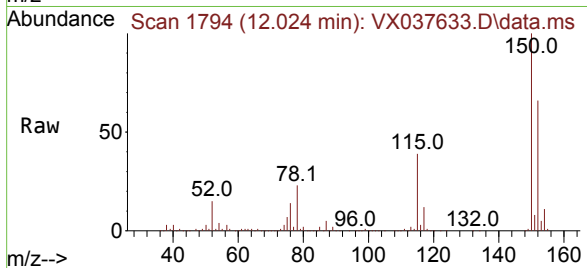

#74

N-ethyl acetate

Concen: 18.896 ug/l

RT: 10.750 min Scan# 1585

Delta R.T. -0.092 min

Lab File: VX037633.D

Acq: 09 Sep 2023 17:26

Tgt Ion: 43 Resp: 48451




Ion Ratio Lower Upper


43 100

70 6.3 32.9 49.3#

55 244.4 19.3 28.9#

61 0.0 18.8 28.2#

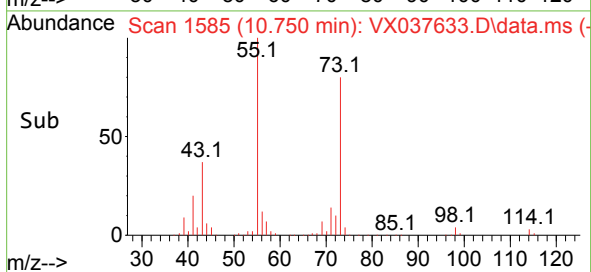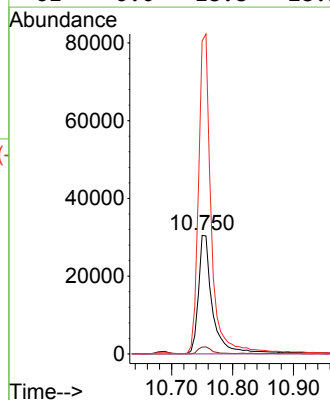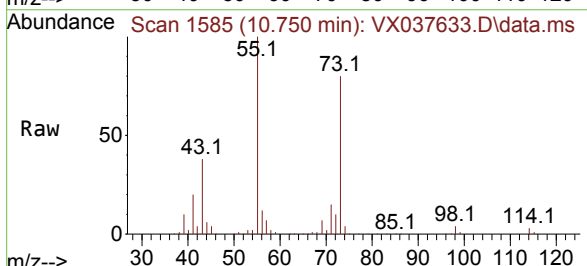



#76

1,2,3-Trichloropropane

Concen: 21.090 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.159 min

Lab File: VX037633.D

Acq: 09 Sep 2023 17:26

Instrument :

MSVOA_X

ClientSampleId :





713-G-DIP

Tgt Ion: 75 Resp: 48893

Ion Ratio Lower Upper

75 100

77 1.3 19.1 57.5#

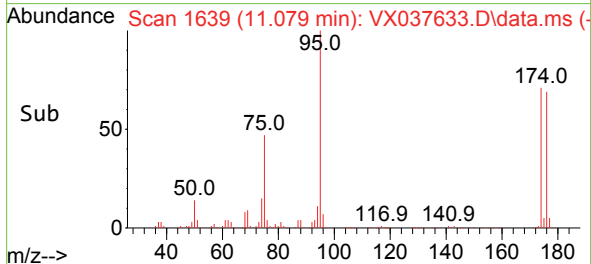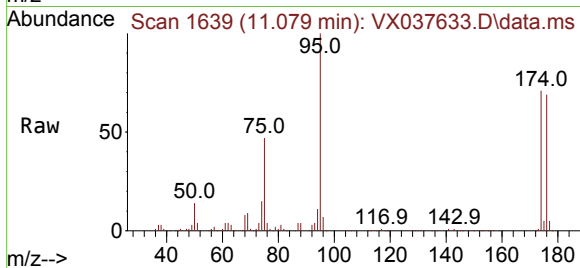

#78

n-propylbenzene

Concen: 0.620 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX037633.D




Acq: 09 Sep 2023 17:26


Tgt Ion: 91 Resp: 5126

Ion Ratio Lower Upper

91 100

120 22.2 11.5 34.4

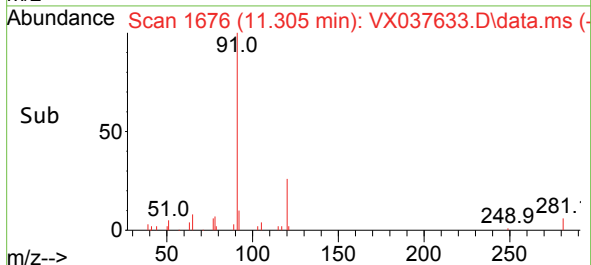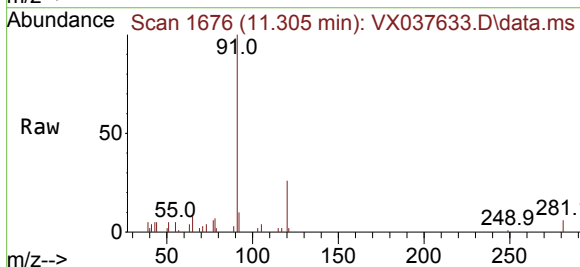



#79

2-Chlorotoluene

Concen: 0.737 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX037633.D

Acq: 09 Sep 2023 17:26

Instrument :

MSVOA_X

ClientSampleId :





713-G-DIP

Tgt Ion: 91 Resp: 3873

Ion Ratio Lower Upper

91 100

126 0.0 16.3 48.8#

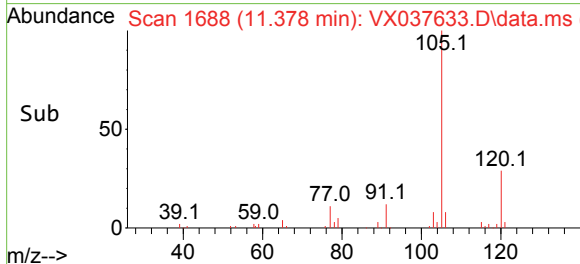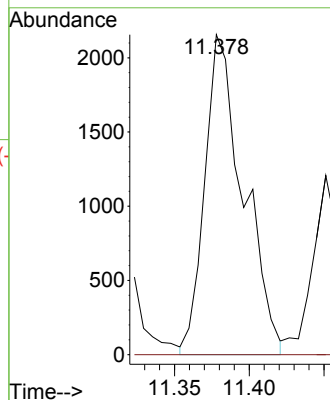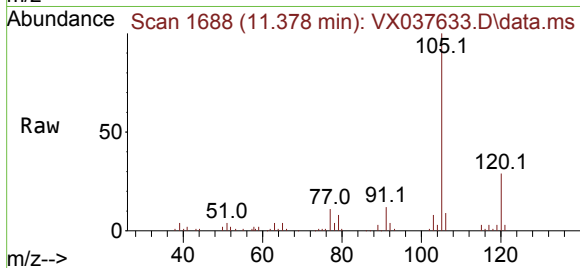

#80

1,3,5-Trimethylbenzene

Concen: 1.887 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX037633.D




Acq: 09 Sep 2023 17:26


Tgt Ion: 105 Resp: 11909

Ion Ratio Lower Upper

105 100

120 49.8 24.1 72.3


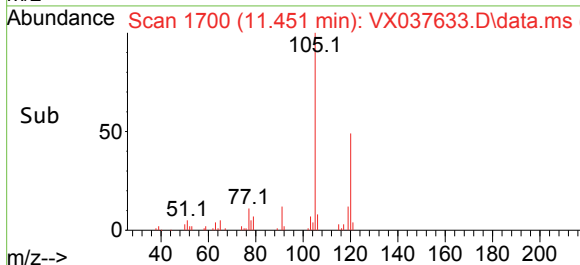
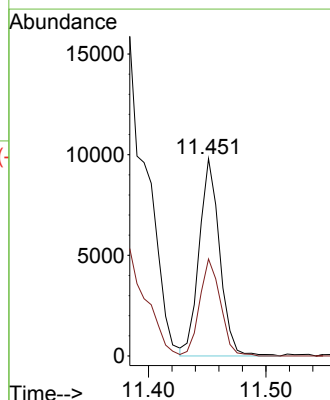
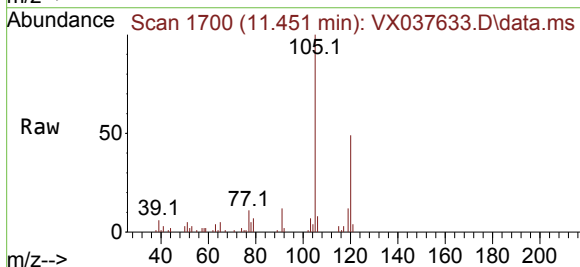




#81
trans-1,4-Dichloro-2-butene
Concen: 63.119 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26




Instrument :
MSVOA_X
ClientSampleId :
713-G-DIP


Tgt Ion: 75 Resp: 48893
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

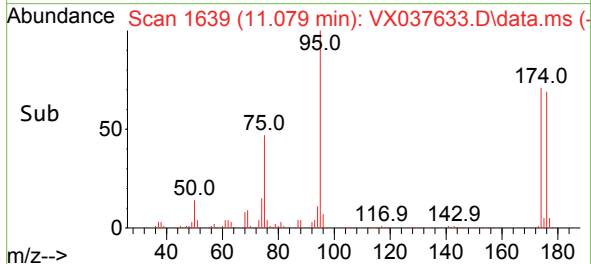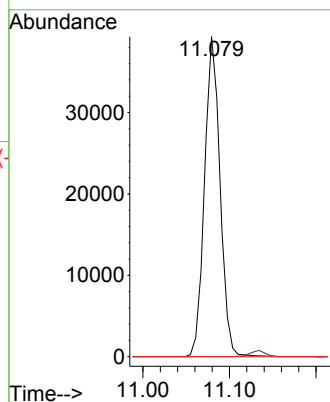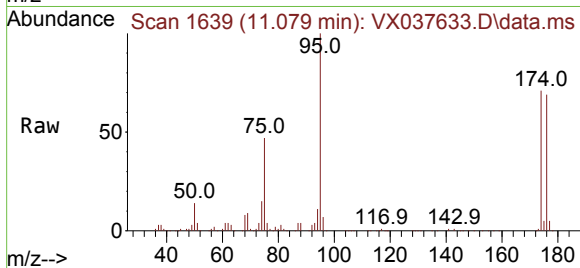

#82
4-Chlorotoluene
Concen: 0.261 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX037633.D
Acq: 09 Sep 2023 17:26

Tgt Ion: 91 Resp: 1547
Ion Ratio Lower Upper
91 100
126 0.0 14.2 42.6#

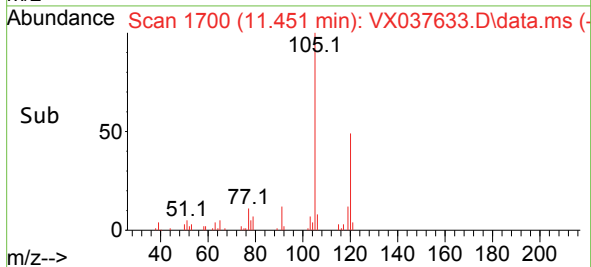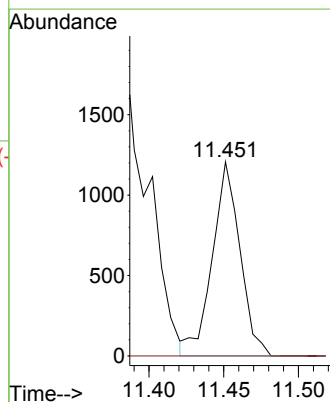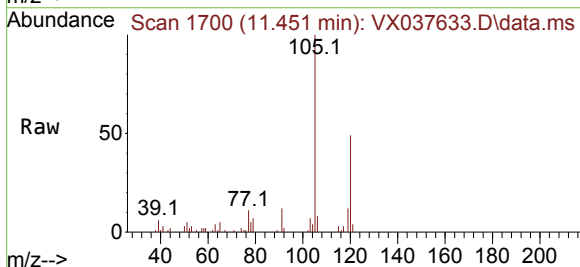



#84

1,2,4-Trimethylbenzene

Concen: 7.270 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.006 min

Lab File: VX037633.D

Acq: 09 Sep 2023 17:26

Instrument :

MSVOA_X

ClientSampleId :





713-G-DIP

Tgt Ion:105 Resp: 45862

Ion Ratio Lower Upper

105 100

120 46.2 21.2 63.6

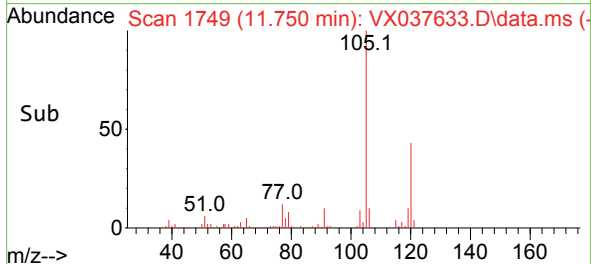

#85

sec-Butylbenzene

Concen: 5.981 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.140 min

Lab File: VX037633.D




Acq: 09 Sep 2023 17:26


Tgt Ion:105 Resp: 45862

Ion Ratio Lower Upper

105 100

134 0.0 9.8 29.4#

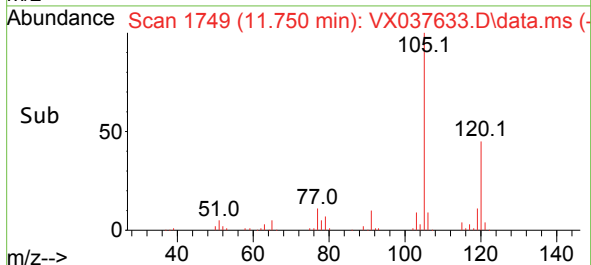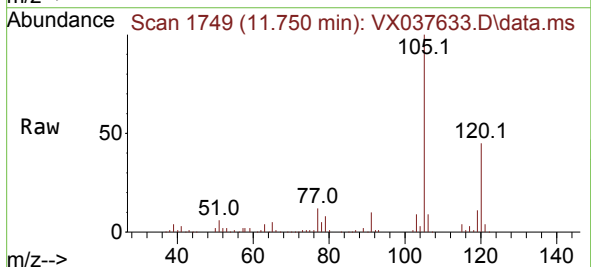



#89

n-Butylbenzene

Concen: 0.442 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.006 min

Lab File: VX037633.D

Acq: 09 Sep 2023 17:26

Instrument :

MSVOA_X

ClientSampleId :

713-G-DIP





Tgt Ion: 91 Resp: 2358

Ion Ratio Lower Upper

91 100

92 27.4 27.4 82.0

134 98.3 12.6 37.8#

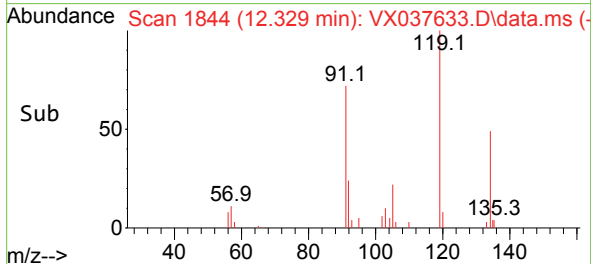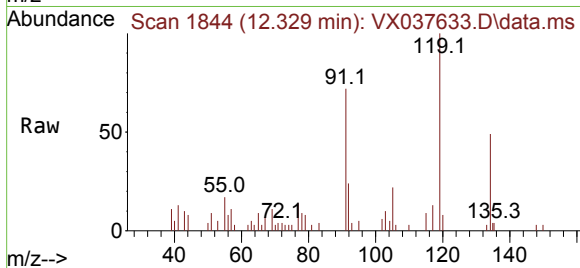

#90

Hexachloroethane

Concen: 0.288 ug/l

RT: 12.549 min Scan# 1880

Delta R.T. 0.006 min

Lab File: VX037633.D




Acq: 09 Sep 2023 17:26


Tgt Ion: 117 Resp: 318

Ion Ratio Lower Upper

117 100


201 0.0 32.9 98.6#

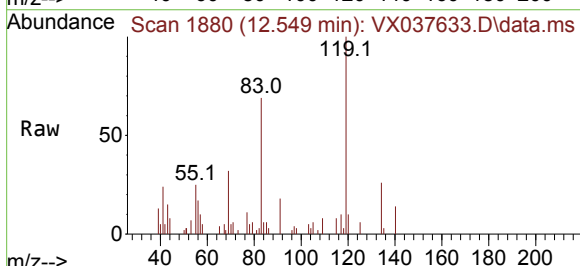



#95
 Naphthalene
 Concen: 1.754 ug/l
 RT: 13.774 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VX037633.D
 Acq: 09 Sep 2023 17:26

Instrument :
 MSVOA_X
 ClientSampleId :
 713-G-DIP

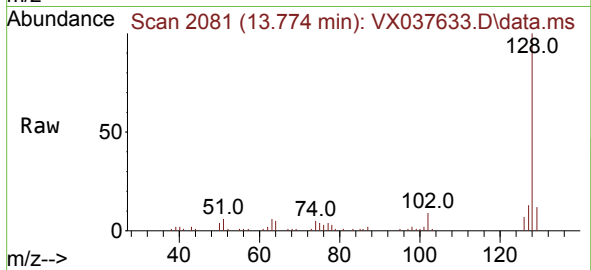

Tgt Ion:128 Resp: 12936
 Ion Ratio Lower Upper
 128 100
 127 12.4 10.3 15.5
 129 11.8 8.8 13.2

