

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090923\  
Data File : VX037626.D  
Acq On : 09 Sep 2023 14:35  
Operator : JC/MD  
Sample : 04254-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RW11-MW01S-20230830

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X090823W.M

Title : SW846 8260

Signal : TIC: VX037626.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.538       | 230           | 238         | 245          | rBV      | 4719           | 8809          | 1.20%           | 0.220%        |
| 2         | 4.574       | 563           | 572         | 584          | rBV2     | 3745           | 12536         | 1.71%           | 0.314%        |
| 3         | 5.385       | 694           | 705         | 721          | rBV      | 89872          | 264378        | 36.08%          | 6.614%        |
| 4         | 5.556       | 721           | 733         | 747          | rVV      | 157212         | 446944        | 61.00%          | 11.181%       |
| 5         | 5.958       | 789           | 799         | 813          | rBV      | 90510          | 242134        | 33.04%          | 6.058%        |
| 6         | 6.763       | 921           | 931         | 950          | rBV      | 236833         | 558690        | 76.25%          | 13.977%       |
| 7         | 8.647       | 1234          | 1240        | 1250         | rBV      | 466112         | 732741        | 100.00%         | 18.331%       |
| 8         | 10.055      | 1465          | 1471        | 1484         | rBV      | 481739         | 645956        | 88.16%          | 16.160%       |
| 9         | 11.079      | 1634          | 1639        | 1653         | rBV      | 383246         | 491871        | 67.13%          | 12.305%       |
| 10        | 12.024      | 1788          | 1794        | 1805         | rBV      | 466028         | 593131        | 80.95%          | 14.839%       |




Sum of corrected areas: 3997190

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090923\  
Data File : VX037626.D  
Acq On : 09 Sep 2023 14:35  
Operator : JC/MD  
Sample : 04254-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RW11-MW01S-20230830

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X090823W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

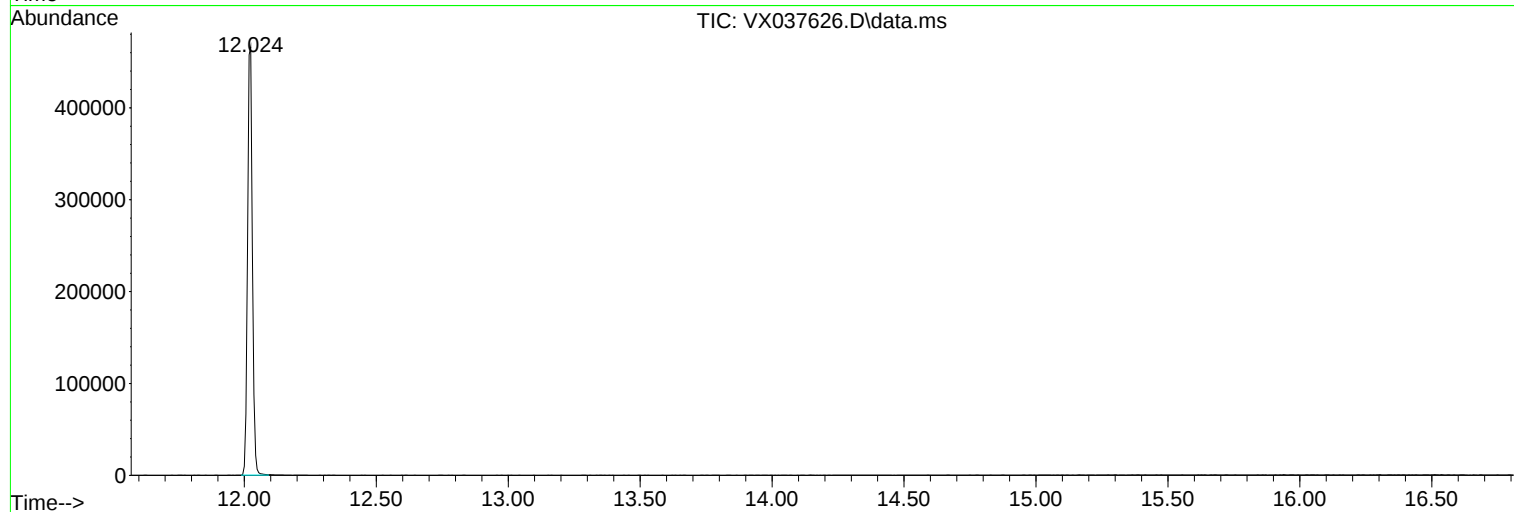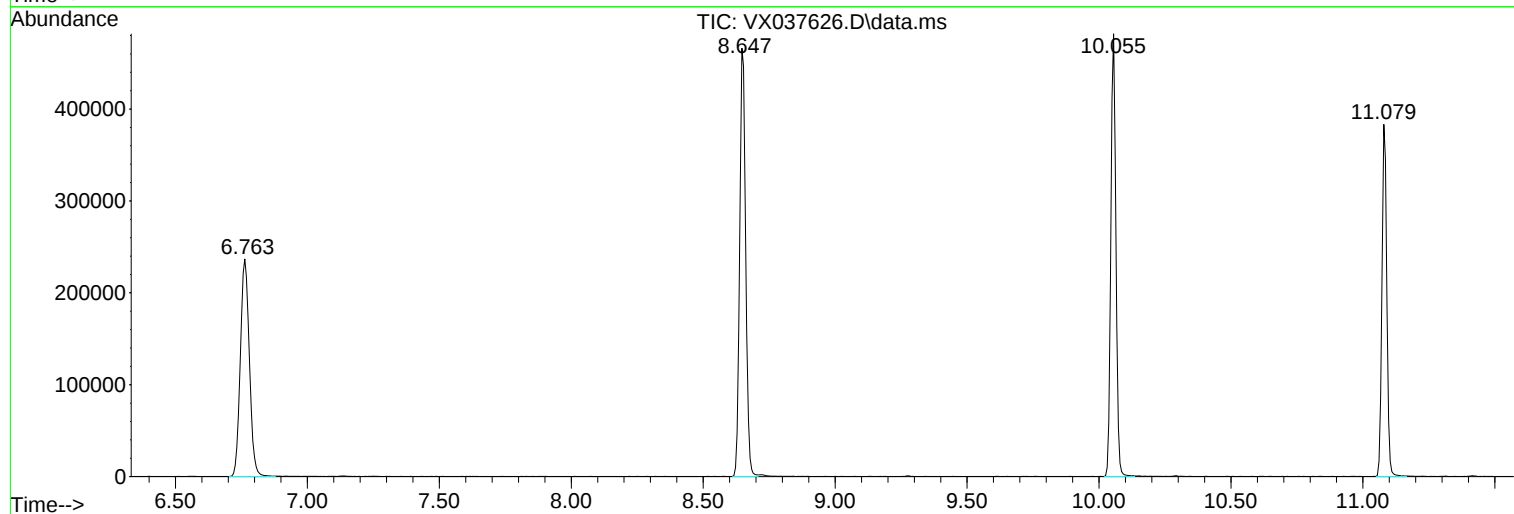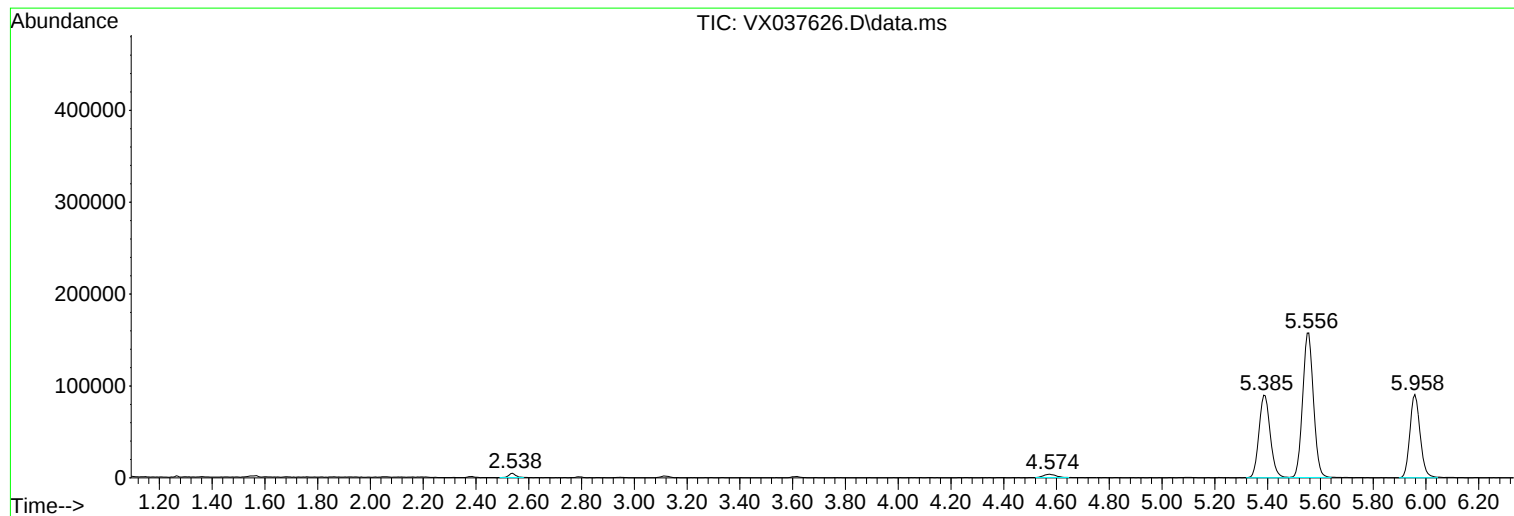

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090923\  
Data File : VX037626.D  
Acq On : 09 Sep 2023 14:35  
Operator : JC/MD  
Sample : 04254-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RW11-MW01S-20230830

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X090823W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090923\  
Data File : VX037626.D  
Acq On : 09 Sep 2023 14:35  
Operator : JC/MD  
Sample : 04254-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RW11-MW01S-20230830

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X090823W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|