

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090923\
Data File : VX037627.D
Acq On : 09 Sep 2023 14:59
Operator : JC/MD
Sample : 04315-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOWER-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M

Title : SW846 8260

Signal : TIC: VX037627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.380	207	212	222	rBV	10558	18184	2.79%	0.537%
2	5.385	691	705	722	rBV2	73491	217321	33.40%	6.412%
3	5.550	722	732	755	rVB	135317	387357	59.53%	11.429%
4	5.952	789	798	820	rBV	77200	207358	31.87%	6.118%
5	6.763	921	931	947	rBV	203533	483063	74.24%	14.253%
6	8.647	1234	1240	1257	rBV	412650	650717	100.00%	19.200%
7	9.525	1379	1384	1390	rVB	5082	7192	1.11%	0.212%
8	10.055	1465	1471	1487	rBV	402567	544819	83.73%	16.075%
9	11.079	1634	1639	1654	rBV	296595	397112	61.03%	11.717%
10	12.024	1788	1794	1804	rBV	368541	476101	73.17%	14.047%




Sum of corrected areas: 3389224

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090923\
Data File : VX037627.D
Acq On : 09 Sep 2023 14:59
Operator : JC/MD
Sample : 04315-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOWER-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

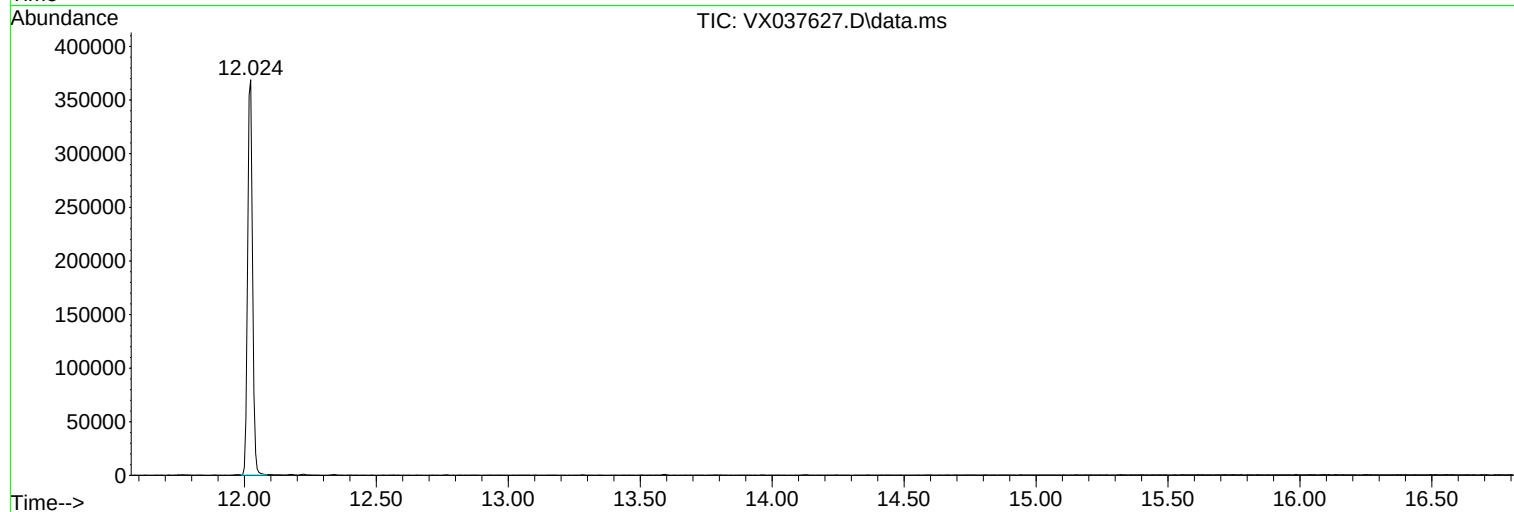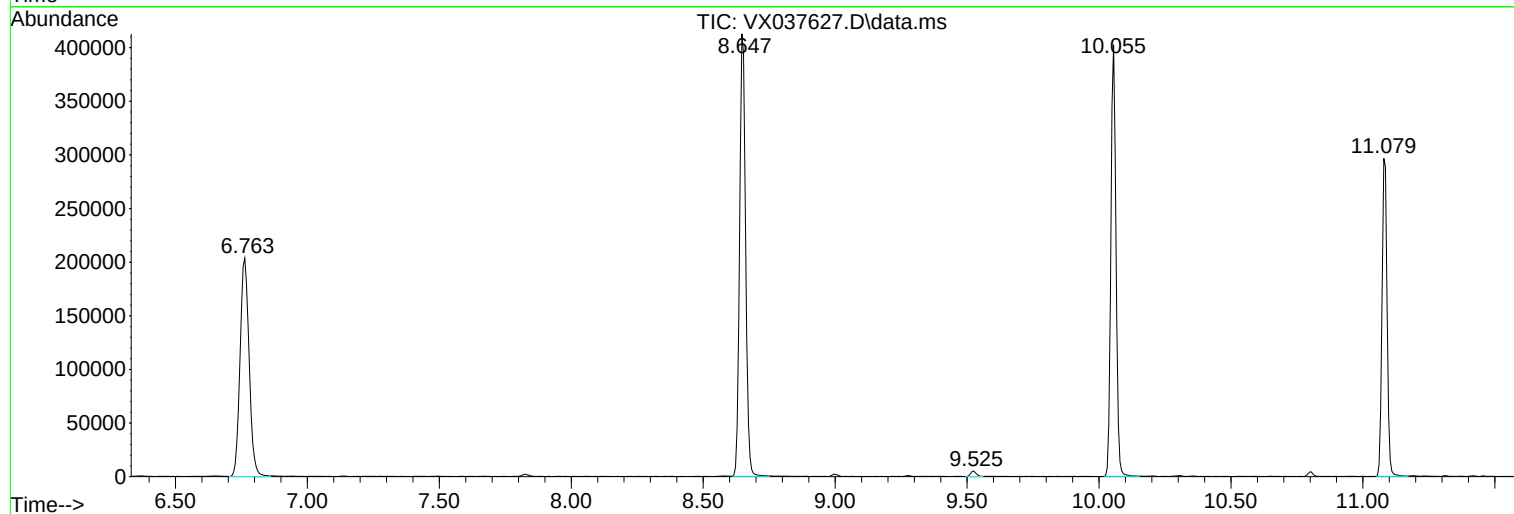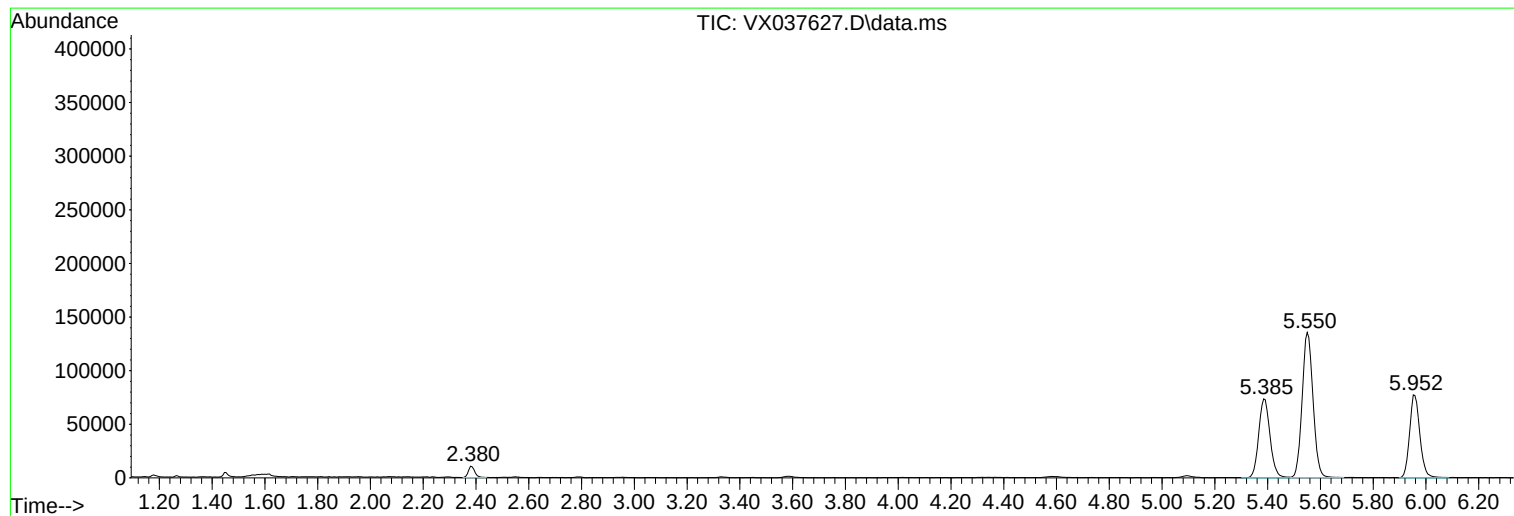

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090923\
Data File : VX037627.D
Acq On : 09 Sep 2023 14:59
Operator : JC/MD
Sample : 04315-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOWER-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090923\
Data File : VX037627.D
Acq On : 09 Sep 2023 14:59
Operator : JC/MD
Sample : 04315-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOWER-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------