

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090923\
 Data File : VX037628.D
 Acq On : 09 Sep 2023 15:24
 Operator : JC/MD
 Sample : 04315-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TOWER-2

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M
 Title : SW846 8260

Signal : TIC: VX037628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	69	rBV	5412	7107	1.11%	0.207%
2	1.599	69	84	87	rBV4	2790	9267	1.44%	0.270%
3	2.380	206	212	220	rBV	10752	17378	2.70%	0.506%
4	5.385	692	705	720	rBV2	72798	215425	33.50%	6.268%
5	5.550	721	732	751	rVB	137195	384907	59.86%	11.199%
6	5.958	789	799	813	rBV	76091	205295	31.92%	5.973%
7	6.763	921	931	954	rBV	202136	480800	74.77%	13.989%
8	8.647	1234	1240	1255	rBV	409466	643061	100.00%	18.711%
9	9.275	1334	1343	1352	rBV	7730	12667	1.97%	0.369%
10	9.525	1379	1384	1389	rVB	5502	7646	1.19%	0.222%
11	10.055	1465	1471	1484	rBV	414040	549989	85.53%	16.003%
12	11.079	1634	1639	1653	rBV	315831	403344	62.72%	11.736%
13	11.311	1673	1677	1683	rVB2	9138	12345	1.92%	0.359%
14	12.024	1788	1794	1806	rBV	379867	487635	75.83%	14.188%




Sum of corrected areas: 3436866

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090923\
Data File : VX037628.D
Acq On : 09 Sep 2023 15:24
Operator : JC/MD
Sample : 04315-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOWER-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

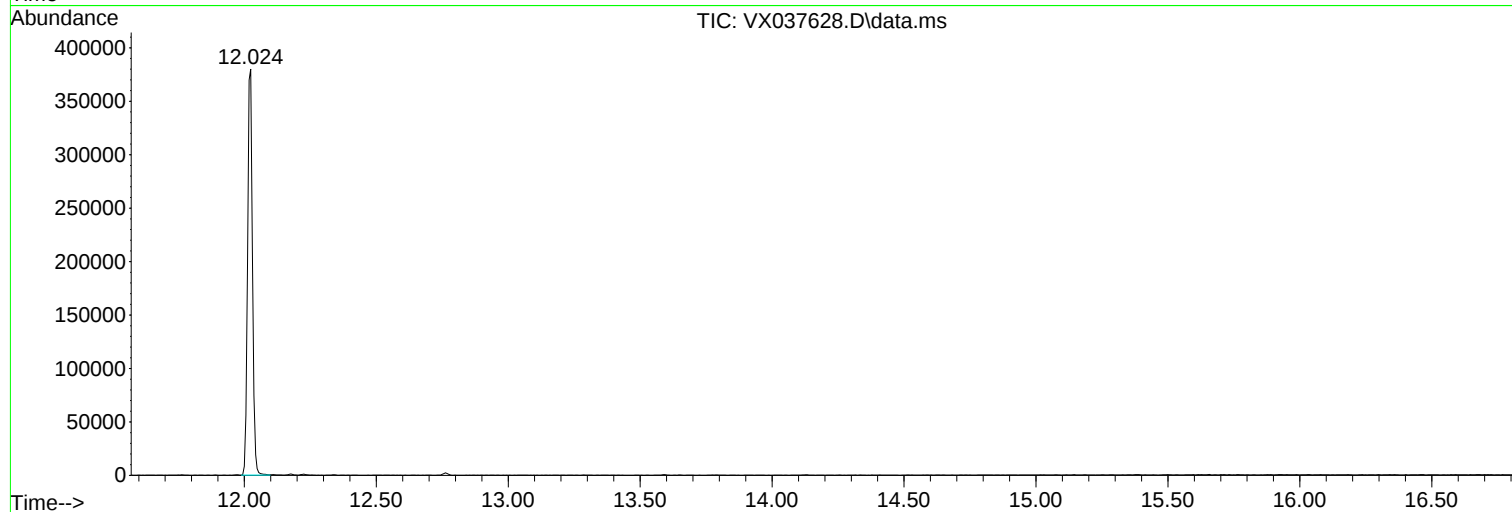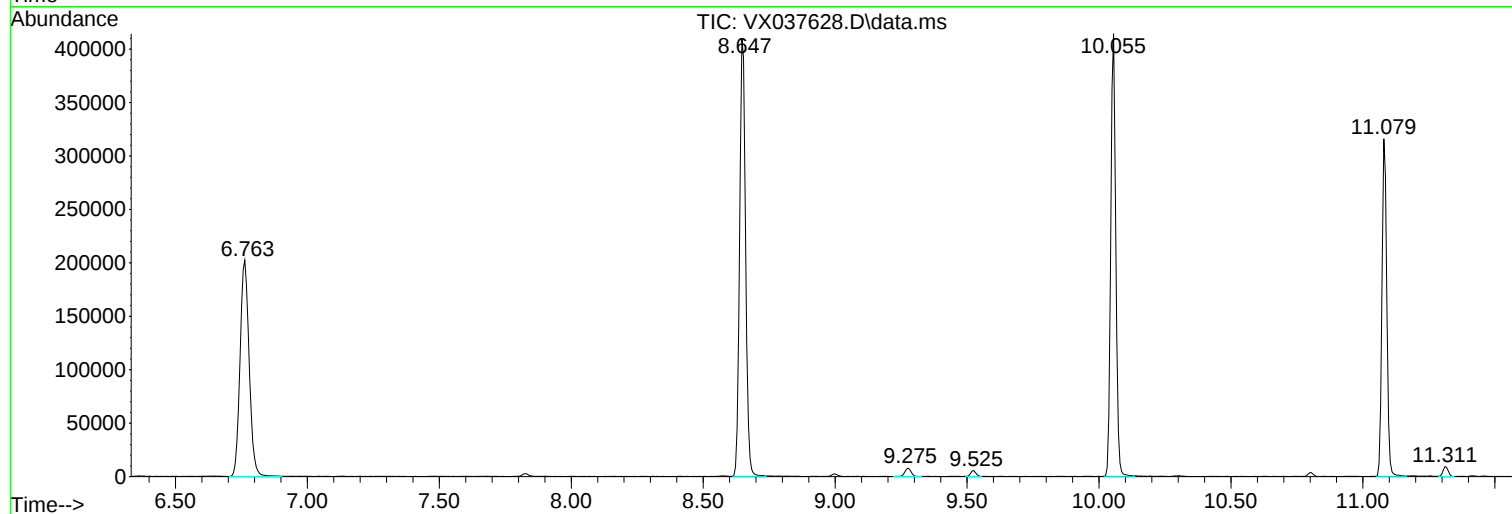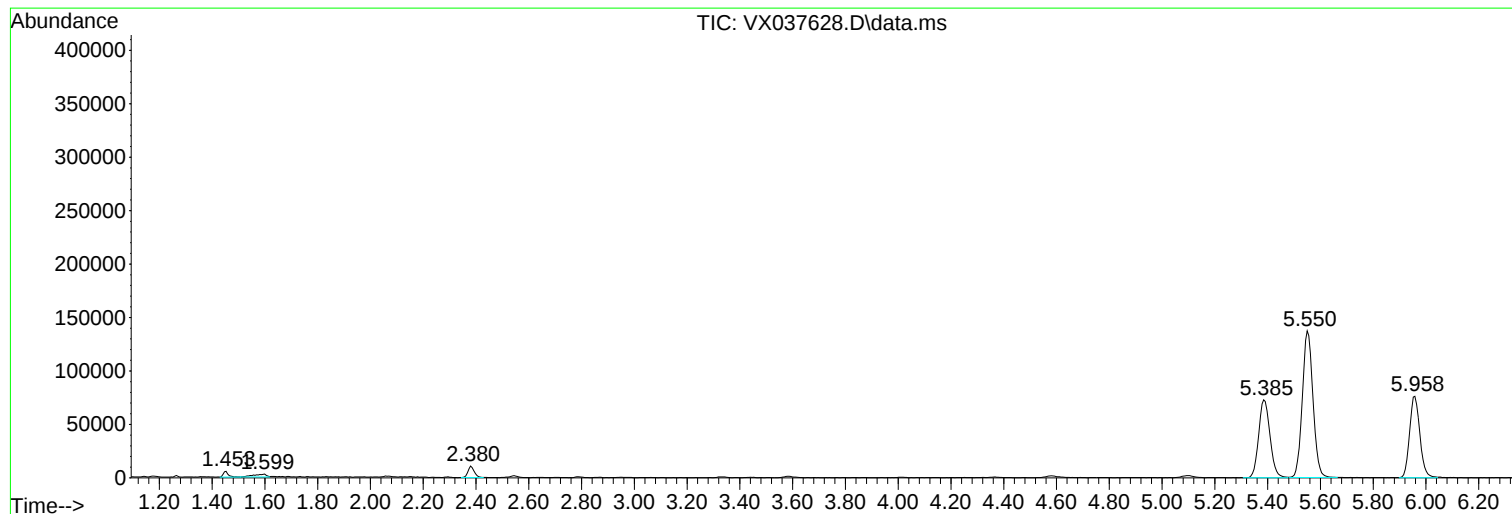

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090923\
Data File : VX037628.D
Acq On : 09 Sep 2023 15:24
Operator : JC/MD
Sample : 04315-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOWER-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX090923\
Data File : VX037628.D
Acq On : 09 Sep 2023 15:24
Operator : JC/MD
Sample : 04315-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOWER-2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X090823W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------