

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090923\  
 Data File : VX037634.D  
 Acq On : 09 Sep 2023 17:50  
 Operator : JC/MD  
 Sample : 04297-04  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 1731-DRIP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X090823W.M  
 Title : SW846 8260

Signal : TIC: VX037634.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.453       | 48            | 60          | 63           | rBV4     | 5388           | 17247         | 2.66%           | 0.482%        |
| 2         | 2.380       | 205           | 212         | 223          | rBV      | 20089          | 33349         | 5.14%           | 0.932%        |
| 3         | 2.514       | 227           | 234         | 236          | rBV      | 4845           | 8486          | 1.31%           | 0.237%        |
| 4         | 4.239       | 508           | 517         | 532          | rBV2     | 3501           | 10359         | 1.60%           | 0.290%        |
| 5         | 5.385       | 693           | 705         | 720          | rBV      | 73375          | 214827        | 33.10%          | 6.004%        |
| 6         | 5.550       | 720           | 732         | 752          | rVB      | 137370         | 387599        | 59.71%          | 10.833%       |
| 7         | 5.958       | 789           | 799         | 811          | rBV      | 76661          | 203923        | 31.42%          | 5.699%        |
| 8         | 6.763       | 921           | 931         | 948          | rBV      | 202666         | 484300        | 74.61%          | 13.536%       |
| 9         | 8.647       | 1234          | 1240        | 1250         | rBV      | 408942         | 649103        | 100.00%         | 18.142%       |
| 10        | 9.031       | 1297          | 1303        | 1315         | rBV      | 5922           | 11336         | 1.75%           | 0.317%        |
| 11        | 10.055      | 1465          | 1471        | 1486         | rBV      | 418540         | 553007        | 85.20%          | 15.456%       |
| 12        | 10.299      | 1507          | 1511        | 1520         | rBV      | 16988          | 24685         | 3.80%           | 0.690%        |
| 13        | 10.646      | 1563          | 1568        | 1574         | rVB      | 5290           | 7026          | 1.08%           | 0.196%        |
| 14        | 11.079      | 1634          | 1639        | 1651         | rBV      | 317597         | 407401        | 62.76%          | 11.387%       |
| 15        | 11.378      | 1683          | 1688        | 1691         | rBV      | 10729          | 15703         | 2.42%           | 0.439%        |
| 16        | 11.451      | 1697          | 1700        | 1707         | rVB      | 6926           | 8234          | 1.27%           | 0.230%        |
| 17        | 11.750      | 1745          | 1749        | 1755         | rVB      | 23760          | 30162         | 4.65%           | 0.843%        |
| 18        | 12.024      | 1788          | 1794        | 1801         | rBV      | 386852         | 494085        | 76.12%          | 13.809%       |
| 19        | 12.085      | 1801          | 1804        | 1818         | rVV      | 6047           | 10023         | 1.54%           | 0.280%        |
| 20        | 12.244      | 1828          | 1830        | 1838         | rVV4     | 4692           | 7061          | 1.09%           | 0.197%        |




Sum of corrected areas: 3577916

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090923\  
Data File : VX037634.D  
Acq On : 09 Sep 2023 17:50  
Operator : JC/MD  
Sample : 04297-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1731-DRIP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X090823W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

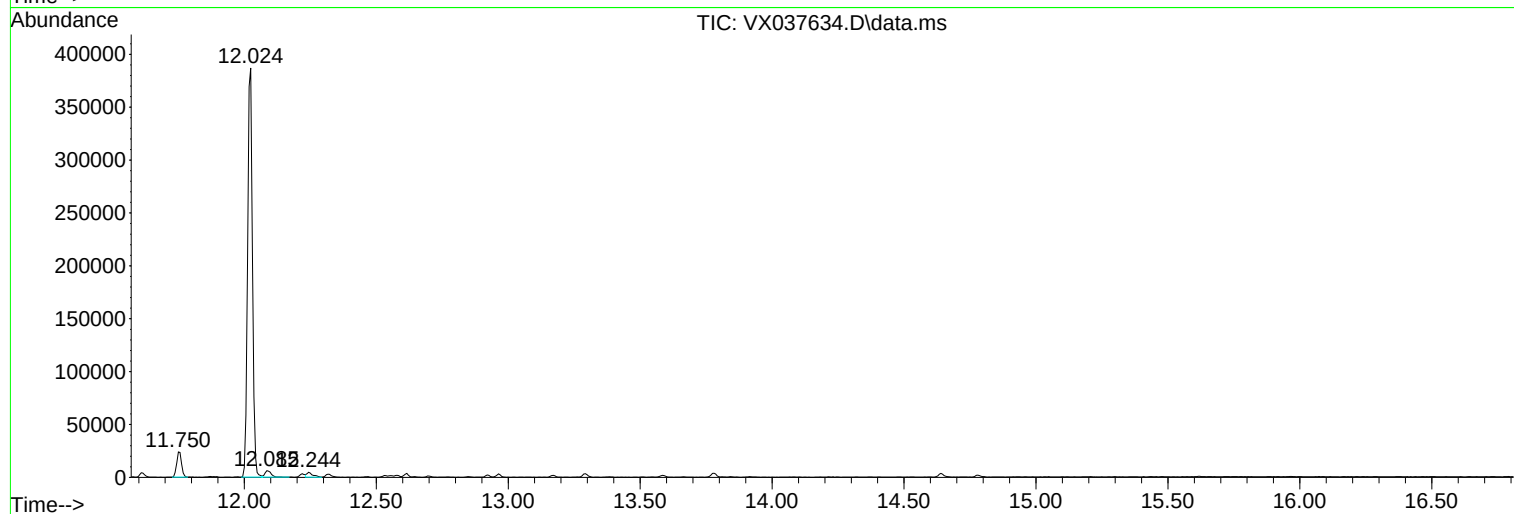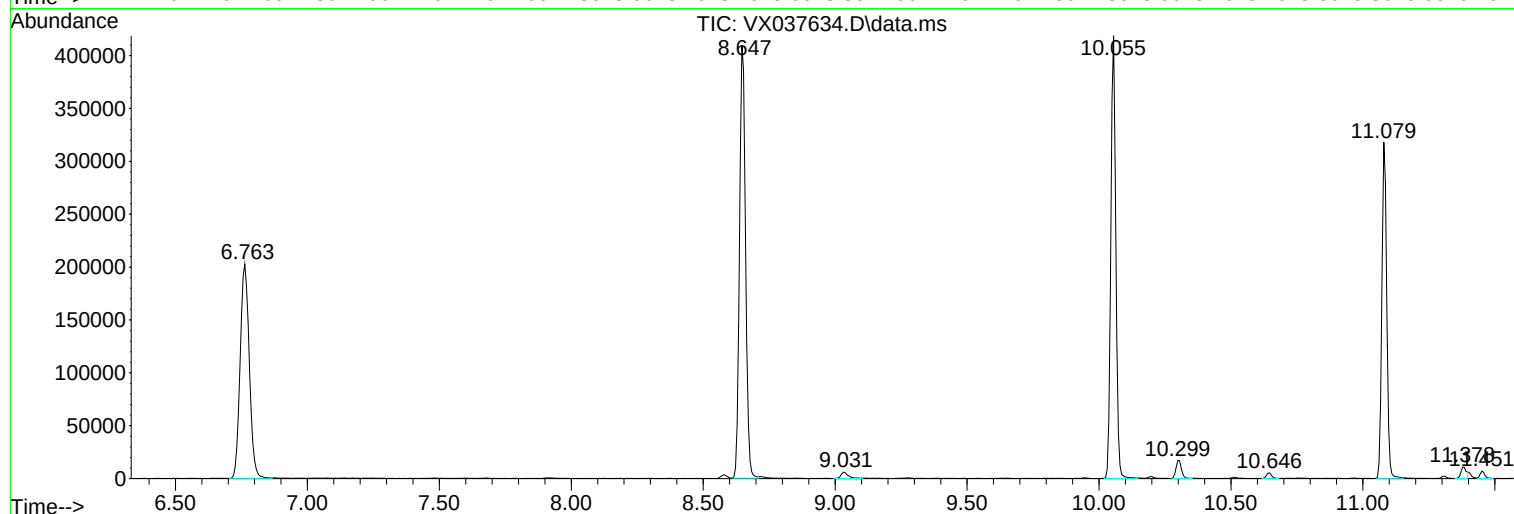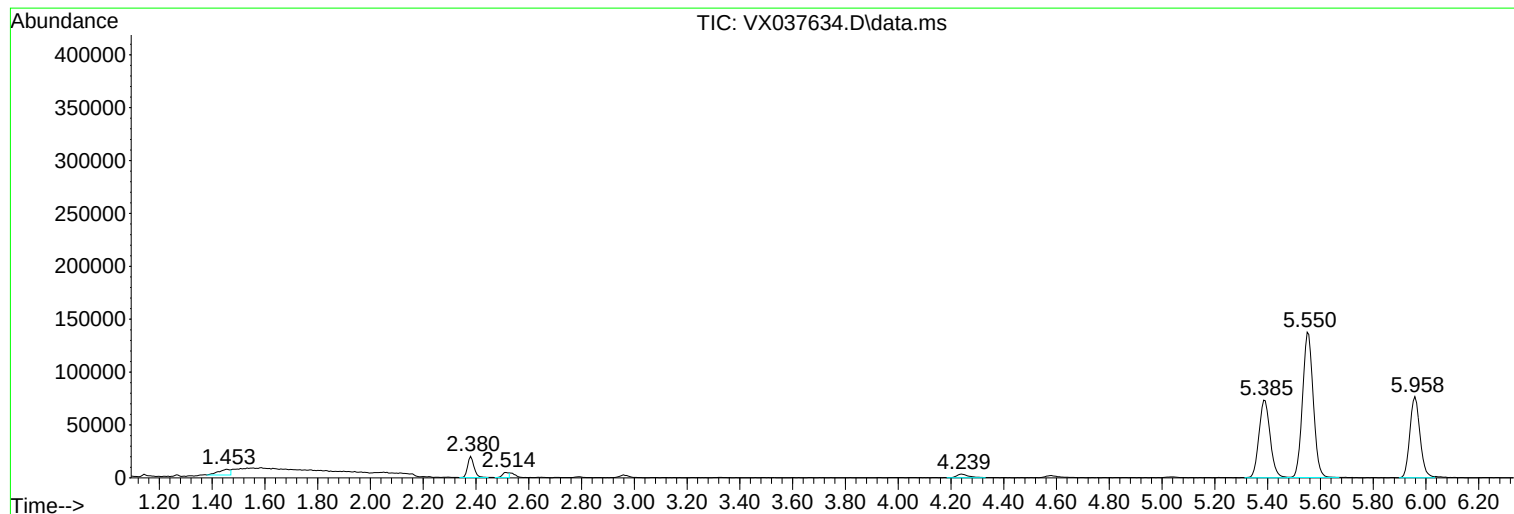

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090923\  
Data File : VX037634.D  
Acq On : 09 Sep 2023 17:50  
Operator : JC/MD  
Sample : 04297-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1731-DRIP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X090823W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX090923\  
Data File : VX037634.D  
Acq On : 09 Sep 2023 17:50  
Operator : JC/MD  
Sample : 04297-04  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
1731-DRIP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X090823W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|