


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091018\
Data File : VX004439.D
Acq On : 10 Sep 2018 10:04
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Title : SW846 8260
Last Update : Thu Aug 23 05:39:44 2018

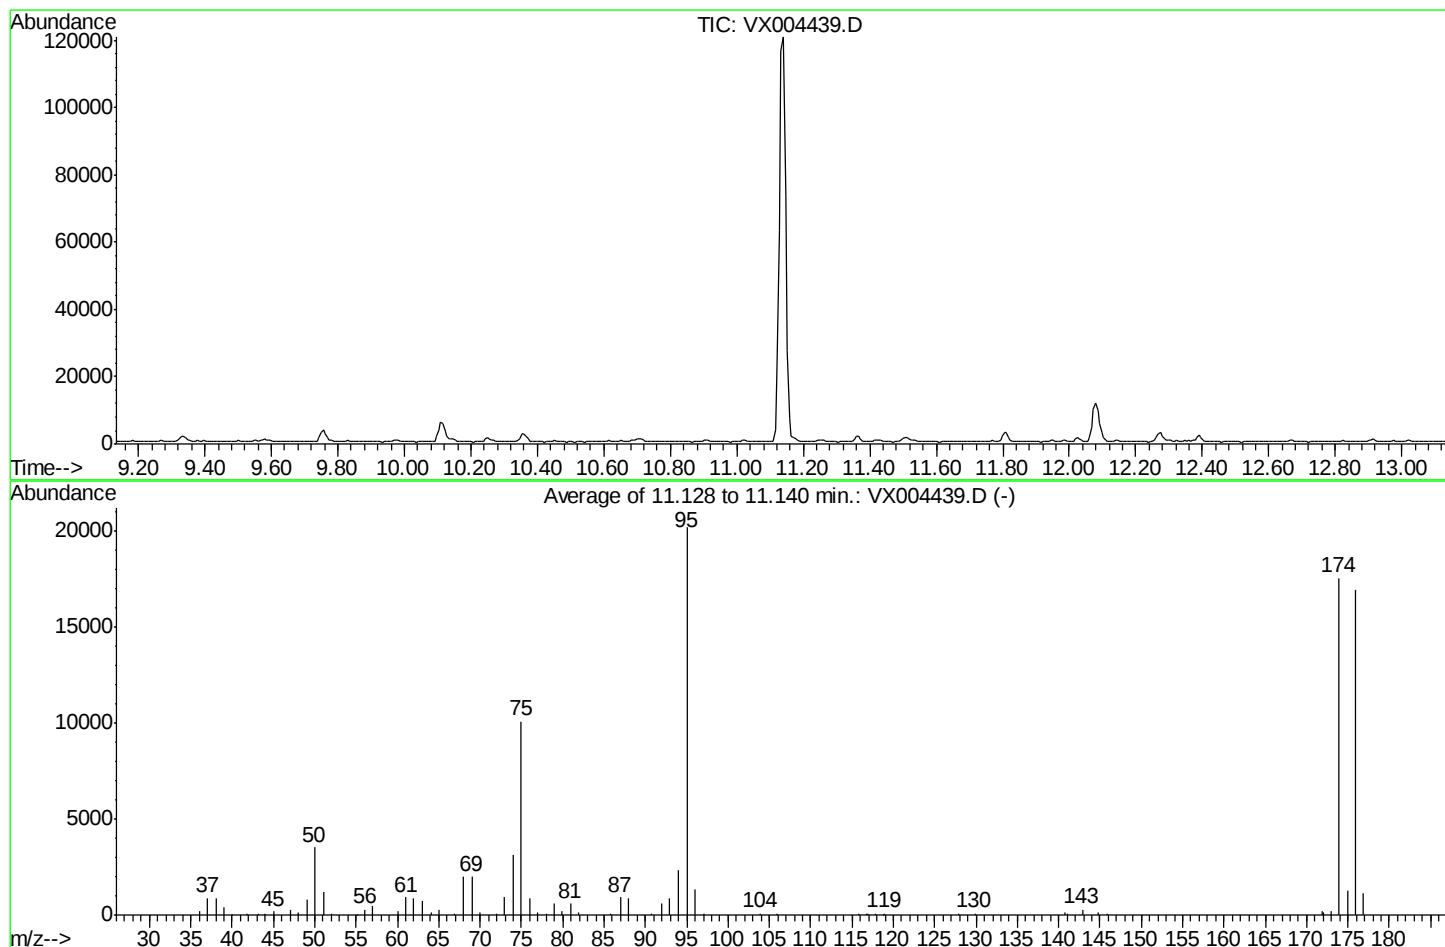

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	3505	PASS
75	95	30	60	49.9	10069	PASS
95	95	100	100	100.0	20193	PASS
96	95	5	9	6.6	1342	PASS
173	174	0.00	2	1.3	234	PASS
174	95	50	100	87.0	17567	PASS
175	174	5	9	7.1	1255	PASS
176	174	95	101	96.4	16941	PASS
177	176	5	9	6.6	1114	PASS