


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091019\
Data File : VX012244.D
Acq On : 10 Sep 2019 08:36
Operator : SY/SP
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_X/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091019S.M
Title : SW846 8260
Last Update : Tue Sep 10 11:00:13 2019

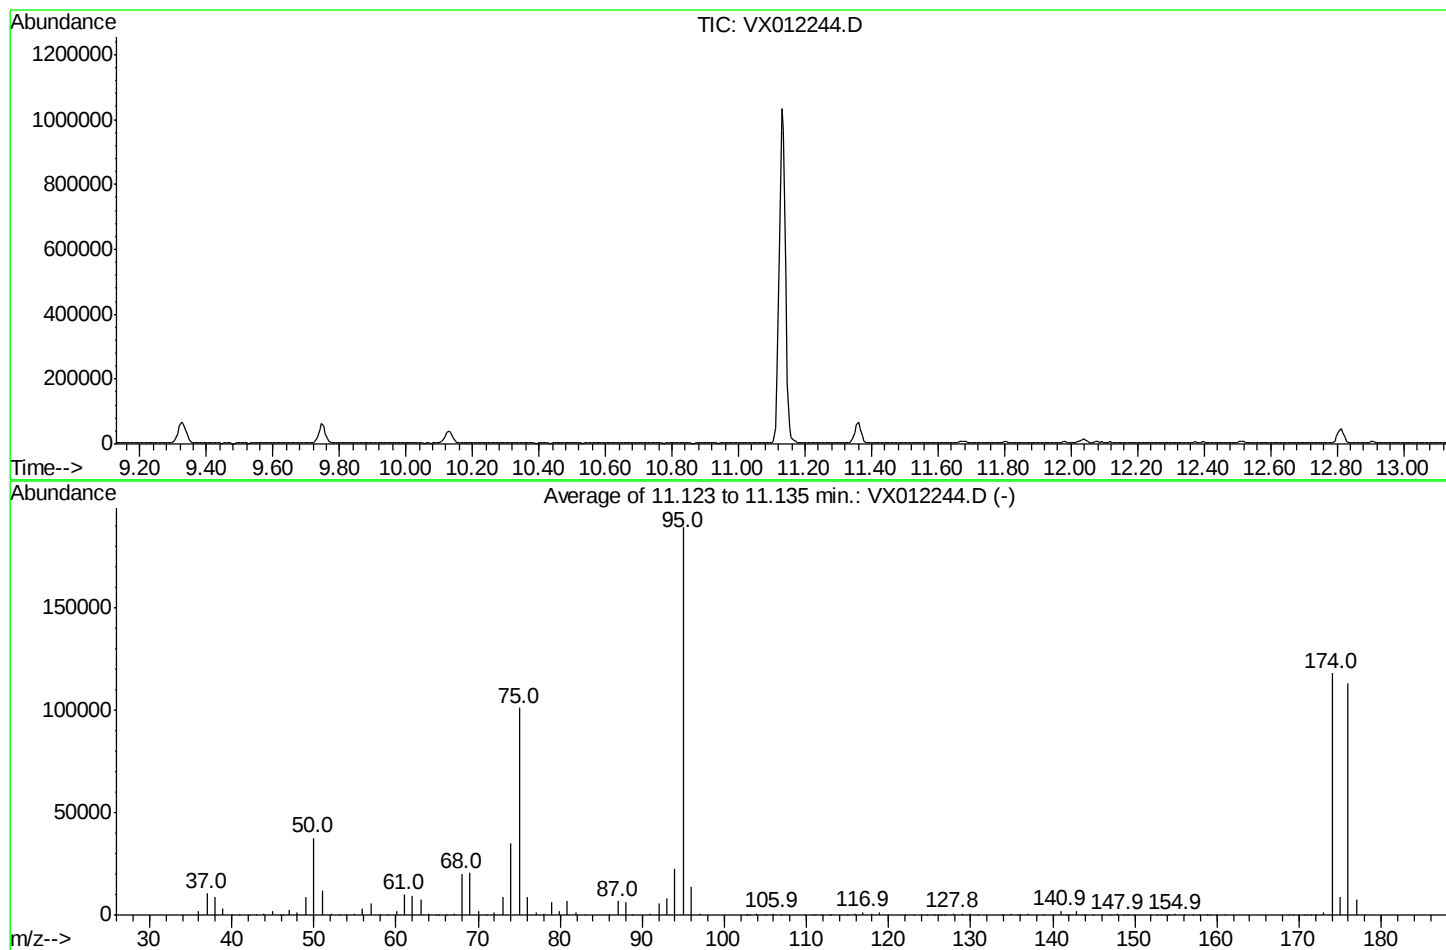

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	37549	PASS
75	95	30	60	53.4	100906	PASS
95	95	100	100	100.0	188970	PASS
96	95	5	9	7.2	13574	PASS
173	174	0.00	2	0.9	1040	PASS
174	95	50	100	62.4	117829	PASS
175	174	5	9	7.7	9037	PASS
176	174	95	101	95.7	112722	PASS
177	176	5	9	6.8	7720	PASS