


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091019\
Data File : VX012267.D
Acq On : 10 Sep 2019 21:05
Operator : SY/SP
Sample : BFB
Misc : 5.00µ/5.0mL/MSVOA X/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091019S.M
Title : SW846 8260
Last Update : Tue Sep 10 12:55:26 2019

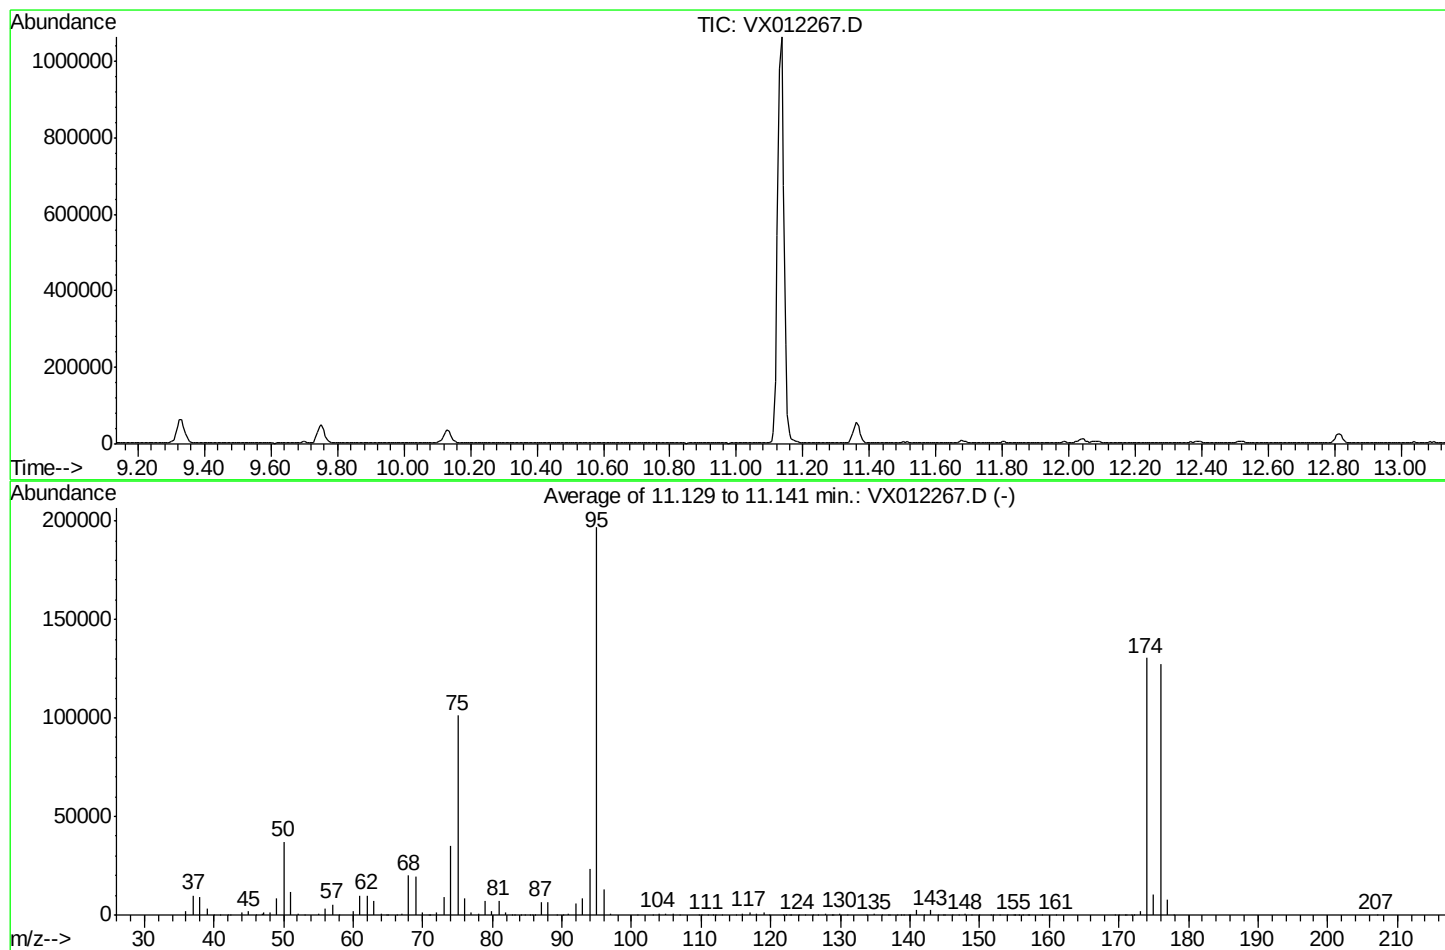

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	37066	PASS
75	95	30	60	51.4	101114	PASS
95	95	100	100	100.0	196757	PASS
96	95	5	9	6.5	12887	PASS
173	174	0.00	2	1.4	1805	PASS
174	95	50	100	66.3	130546	PASS
175	174	5	9	7.8	10164	PASS
176	174	95	101	97.7	127514	PASS
177	176	5	9	6.2	7960	PASS