
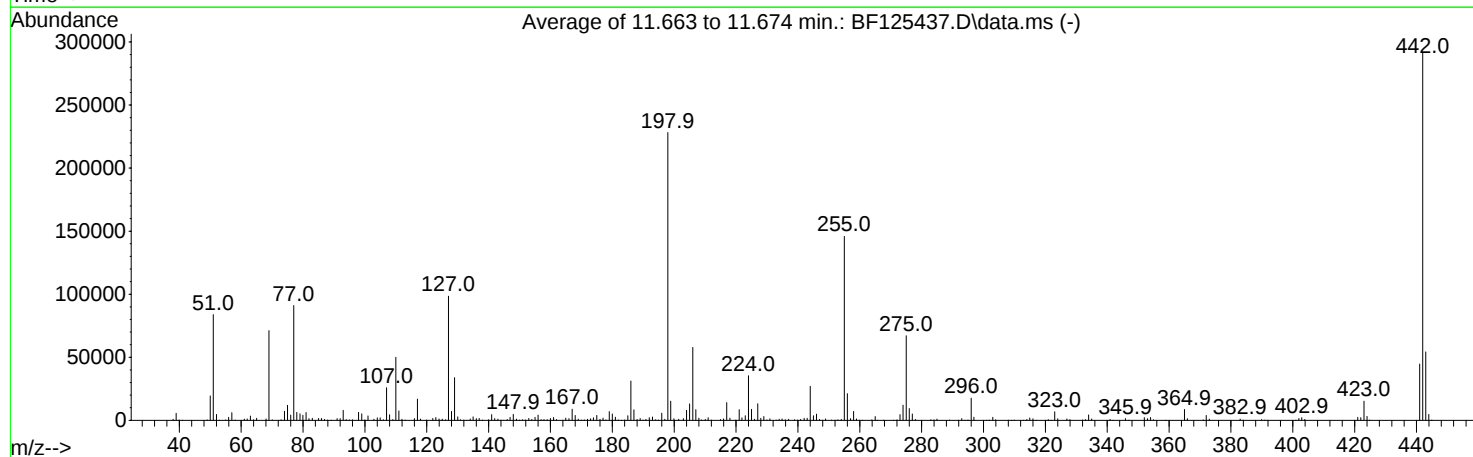


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091321\
 Data File : BF125437.D
 Acq On : 13 Sep 2021 10:25
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\625.1-Tune.M
 Title : D
 Last Update : Wed Oct 07 11:38:17 2020

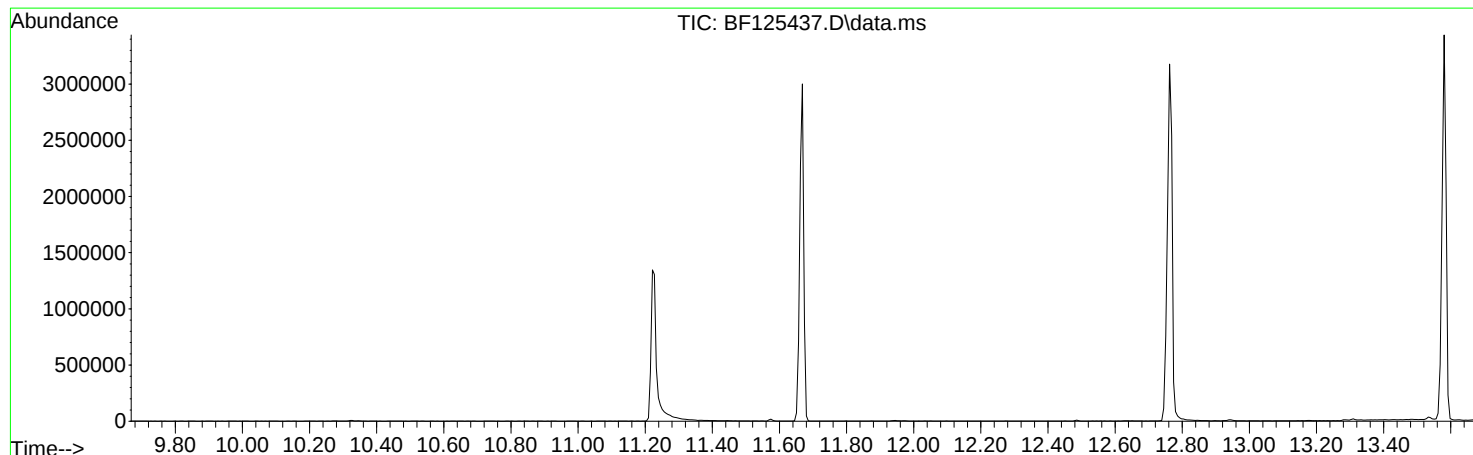

Spectrum Information: Average of 11.663 to 11.674 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.8	83880	PASS
68	69	0.00	2	1.6	1144	PASS
69	69	100	100	100.0	71126	PASS
70	69	0.00	2	0.6	420	PASS
127	198	40	60	43.1	98437	PASS
197	198	0.00	1	0.4	939	PASS
198	198	100	100	100.0	228203	PASS
199	198	5	9	6.7	15197	PASS
275	198	10	30	29.4	67075	PASS
365	198	1	100	3.8	8583	PASS
441	443	0.01	100	82.2	44669	PASS
442	198	40	100	127.8	291669	FAIL*
443	442	17	23	18.6	54363	PASS