

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091021\
 Data File : VX024170.D
 Acq On : 10 Sep 2021 16:56
 Operator : JC/MD
 Sample : M3689-02 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 253

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M

Title : SW846 8260

Signal : TIC: VX024170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	40	rVB	23244	28396	3.46%	0.639%
2	1.575	68	80	84	rBV6	4225	9562	1.17%	0.215%
3	3.123	326	334	345	rVB3	5315	13014	1.59%	0.293%
4	5.397	695	707	720	rBV	96672	278265	33.93%	6.262%
5	5.562	723	734	751	rVB2	158722	449096	54.76%	10.106%
6	5.964	789	800	813	rBV2	104279	279293	34.06%	6.285%
7	6.769	921	932	945	rBV	252283	597173	72.82%	13.439%
8	8.653	1234	1241	1253	rBV	527531	820065	100.00%	18.455%
9	10.055	1465	1471	1487	rBV	549858	741693	90.44%	16.691%
10	11.085	1634	1640	1654	rVB	457886	574913	70.11%	12.938%
11	12.024	1789	1794	1801	rBV	537504	652226	79.53%	14.678%




Sum of corrected areas: 4443696

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091021\
Data File : VX024170.D
Acq On : 10 Sep 2021 16:56
Operator : JC/MD
Sample : M3689-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

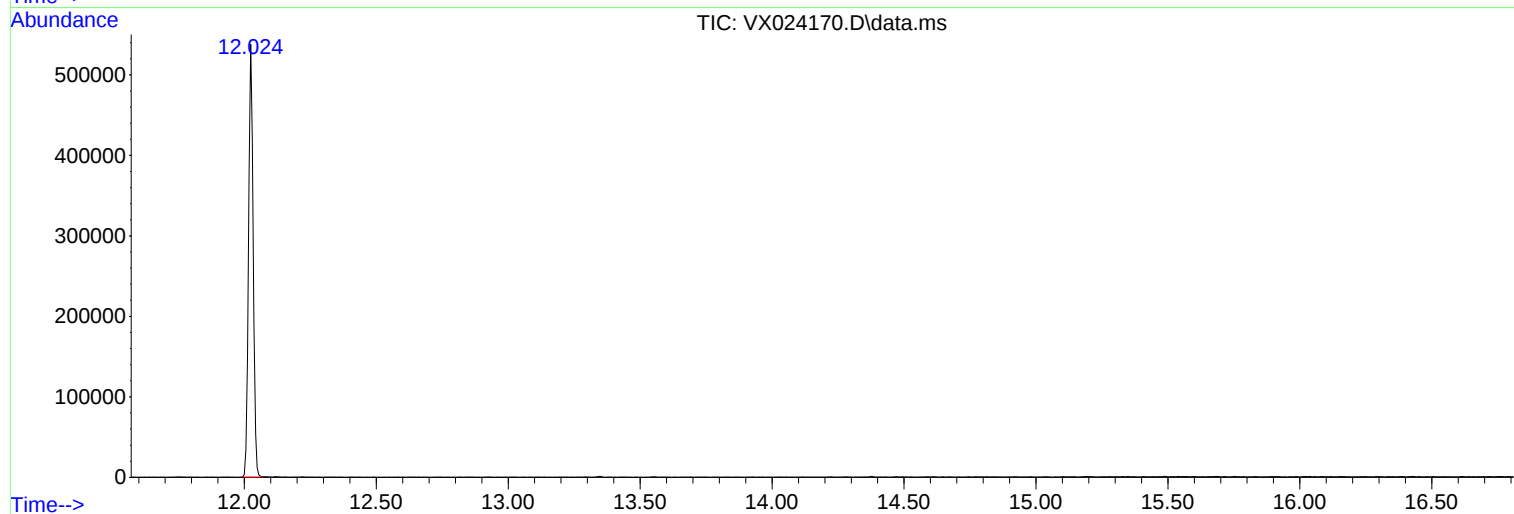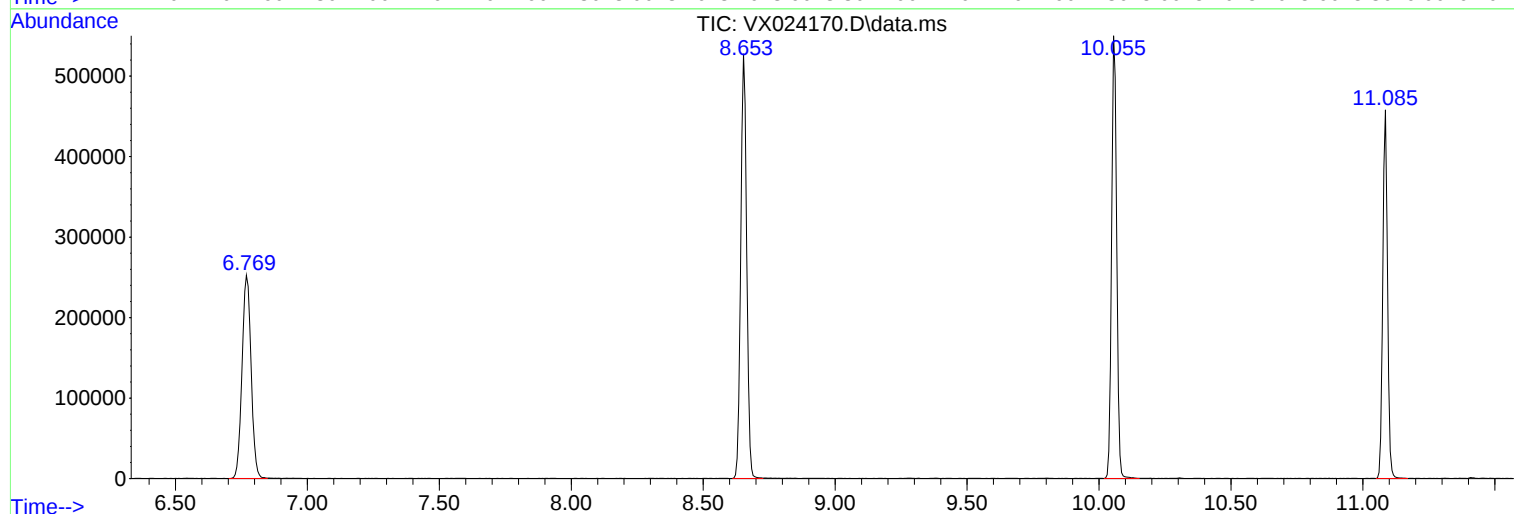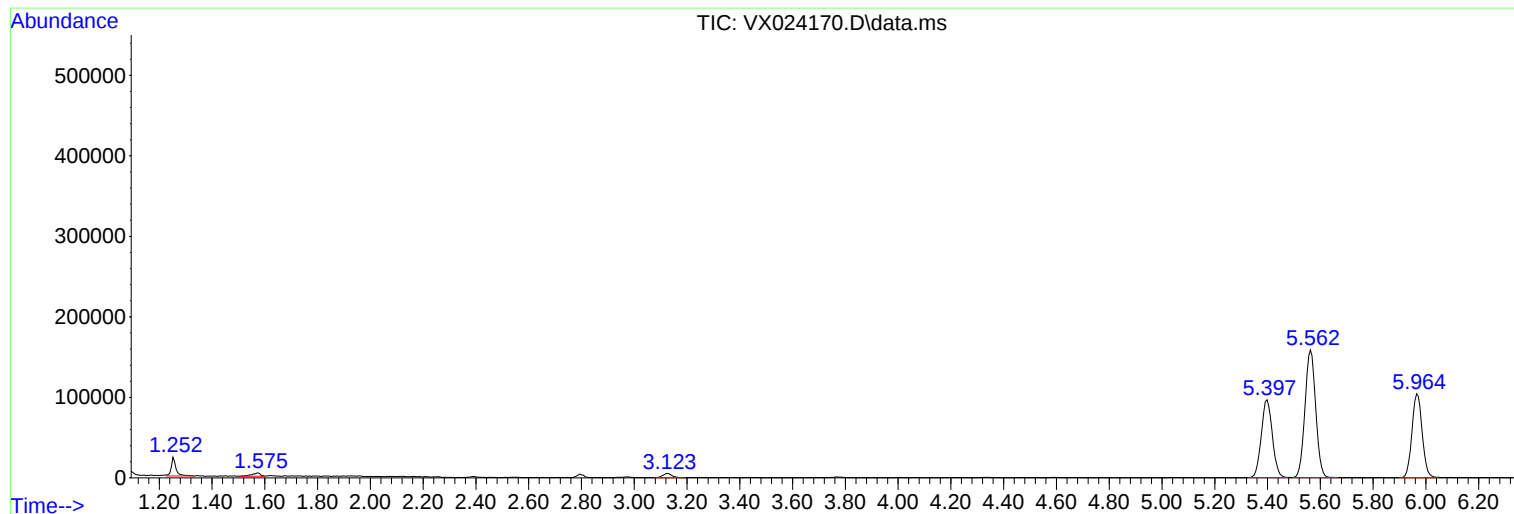

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091021\
Data File : VX024170.D
Acq On : 10 Sep 2021 16:56
Operator : JC/MD
Sample : M3689-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091021\
Data File : VX024170.D
Acq On : 10 Sep 2021 16:56
Operator : JC/MD
Sample : M3689-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
