
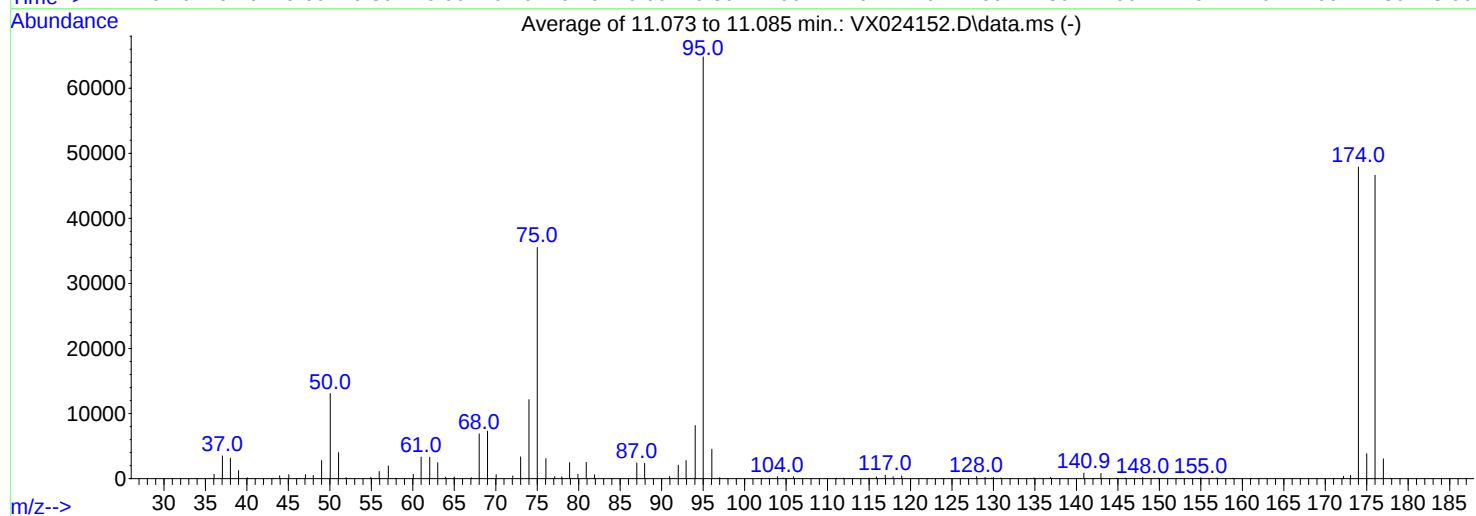


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091021\
 Data File : VX024152.D
 Acq On : 10 Sep 2021 08:48
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Title : SW846 8260
 Last Update : Tue Aug 17 11:57:51 2021

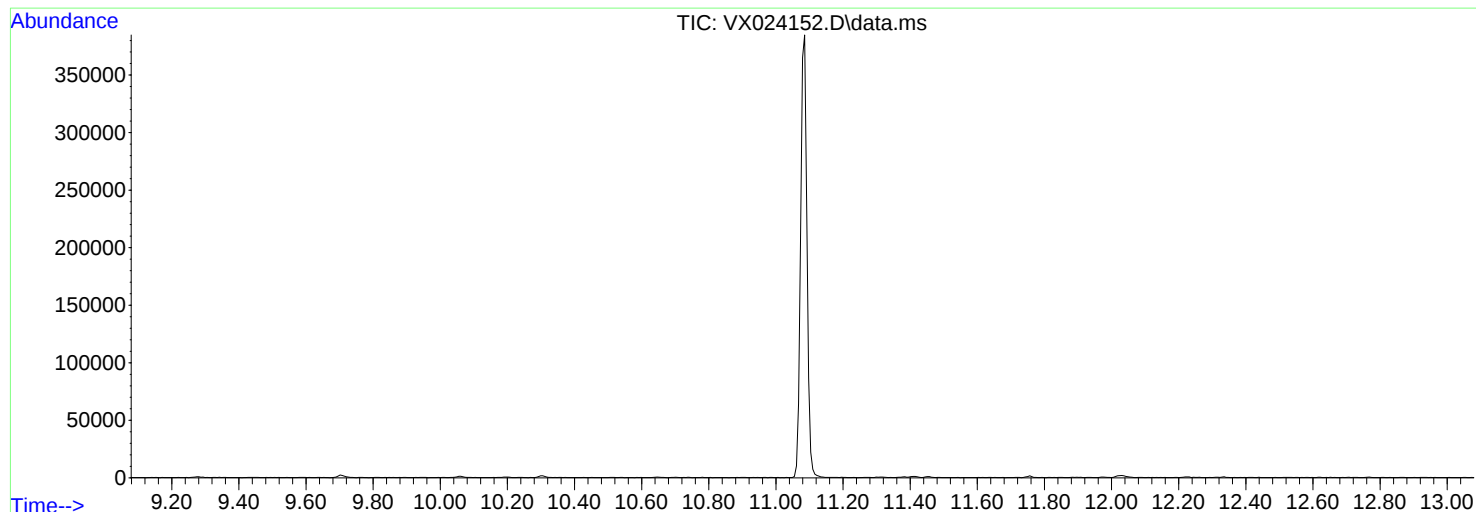

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	13075	PASS
75	95	30	60	54.8	35533	PASS
95	95	100	100	100.0	64824	PASS
96	95	5	9	7.0	4527	PASS
173	174	0.00	2	1.1	505	PASS
174	95	50	100	73.9	47883	PASS
175	174	5	9	8.0	3833	PASS
176	174	95	101	97.4	46621	PASS
177	176	5	9	6.5	3041	PASS