


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091118\
Data File : VX004463.D
Acq On : 11 Sep 2018 12:00
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091118W.M
Title : SW846 8260
Last Update : Wed Sep 12 02:17:23 2018

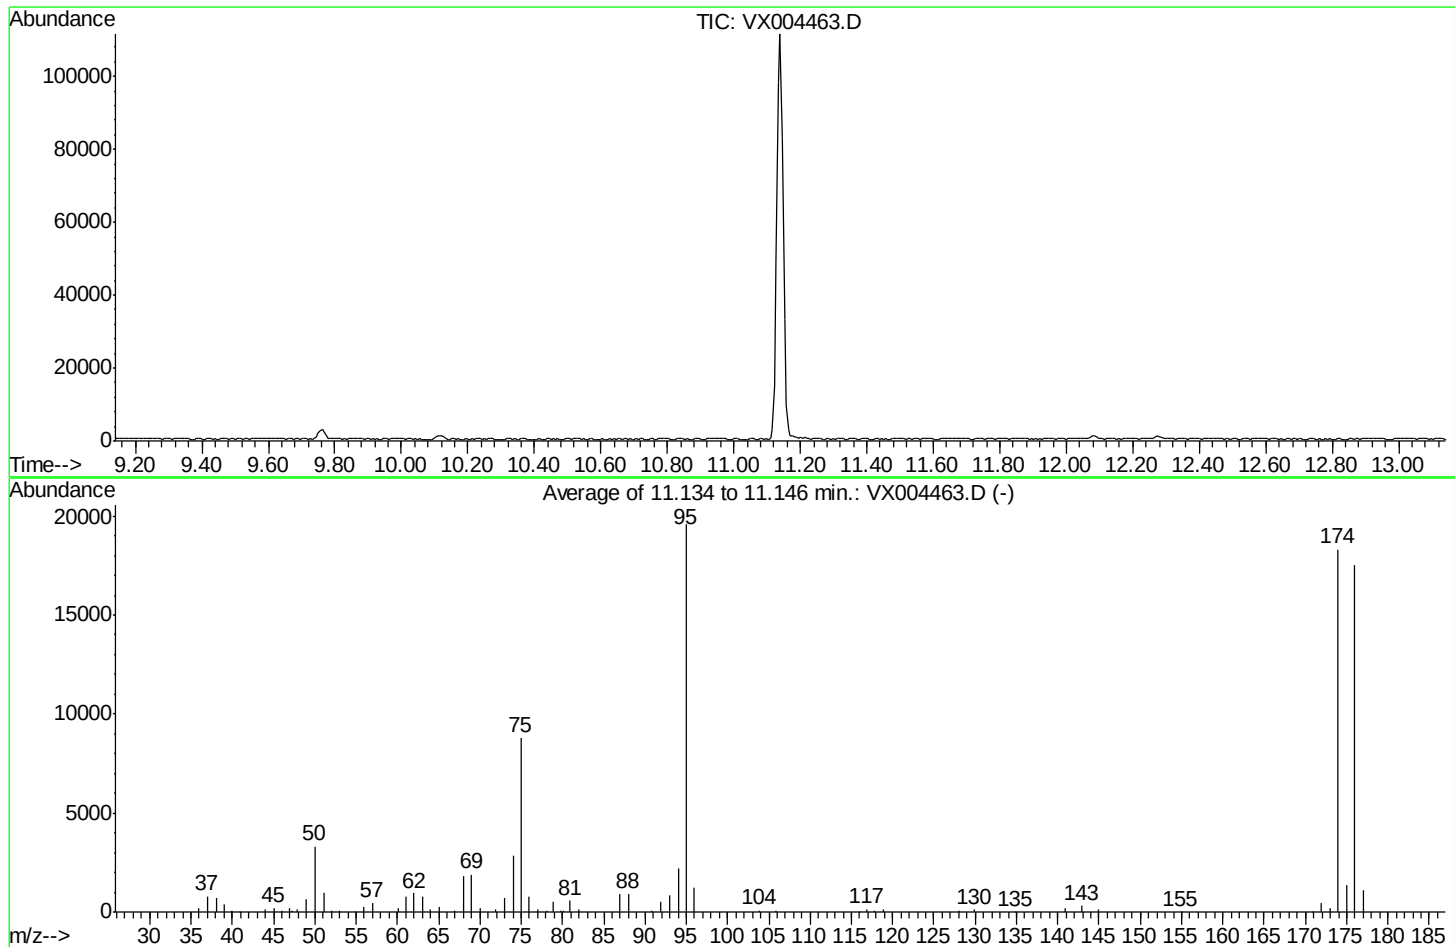

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	3314	PASS
75	95	30	60	45.0	8802	PASS
95	95	100	100	100.0	19576	PASS
96	95	5	9	6.3	1240	PASS
173	174	0.00	2	1.2	224	PASS
174	95	50	100	93.5	18310	PASS
175	174	5	9	7.5	1382	PASS
176	174	95	101	95.5	17490	PASS
177	176	5	9	6.4	1114	PASS