


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091119\
 Data File : VX012290.D
 Acq On : 11 Sep 2019 08:43
 Operator : SY/SP
 Sample : BFB
 Misc : 5.00µ/5.0mL/MSVOA X/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091019S.M
 Title : SW846 8260
 Last Update : Tue Sep 10 12:55:26 2019

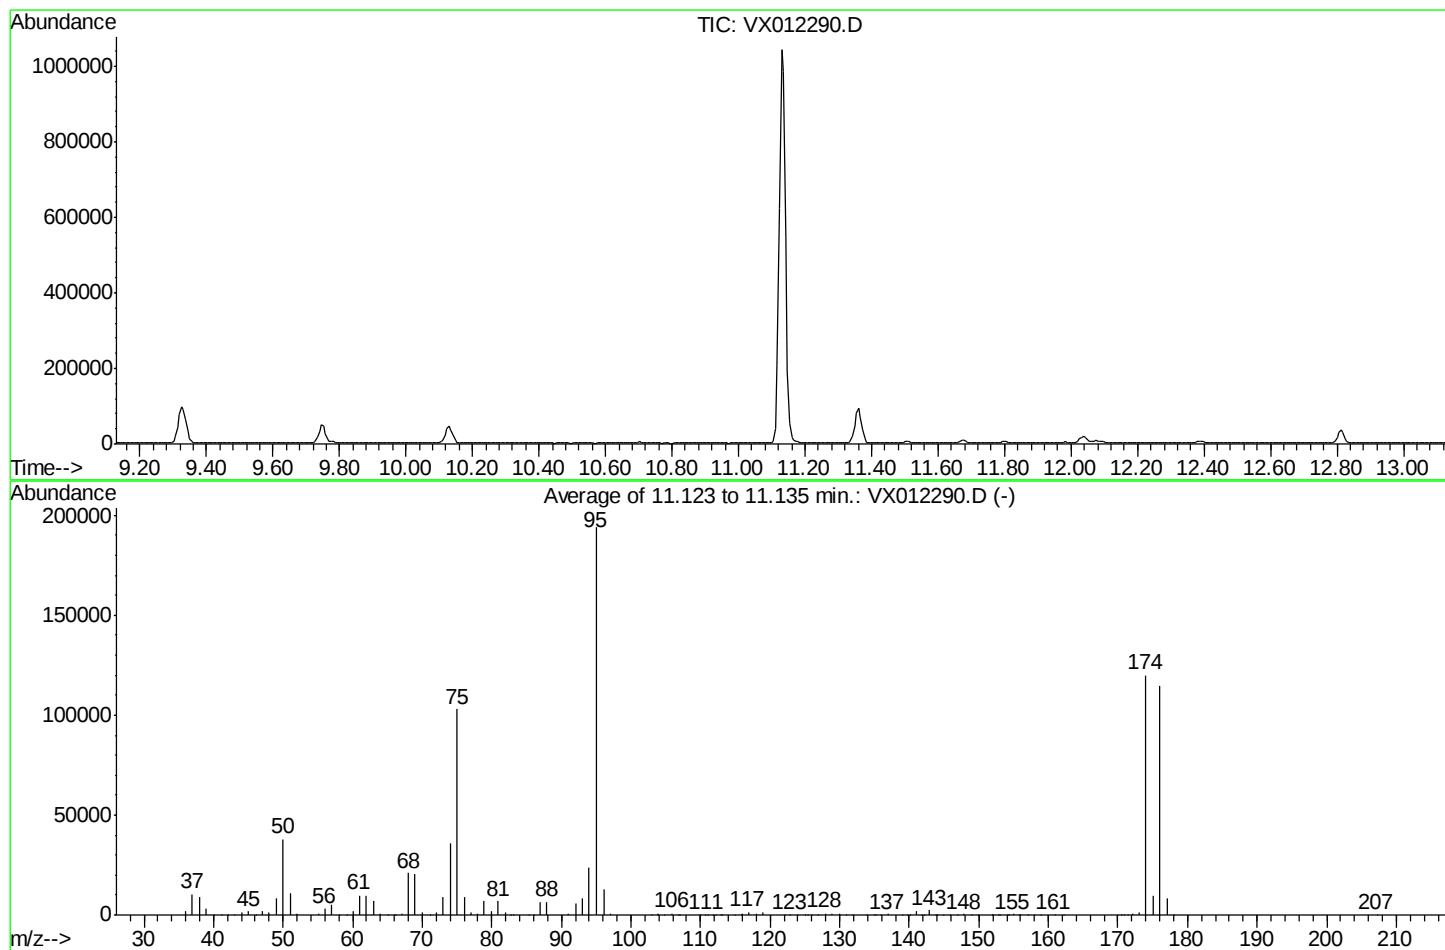

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	38097	PASS
75	95	30	60	53.1	103058	PASS
95	95	100	100	100.0	193962	PASS
96	95	5	9	6.6	12807	PASS
173	174	0.00	2	1.1	1376	PASS
174	95	50	100	61.8	119797	PASS
175	174	5	9	7.9	9408	PASS
176	174	95	101	95.8	114752	PASS
177	176	5	9	7.0	8065	PASS