

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX091120\
 Data File : VX018352.D
 Acq On : 11 Sep 2020 11:16
 Operator : JC/SP
 Sample : VX0911WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0911WBL01

Quant Time: Sep 12 06:21:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X090420W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Sep 04 12:13:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	4.98	128	79344	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.83	114	397923	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.10	117	365080	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	6.03	65	185017	29.56	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	98.53%
60) 4-Bromofluorobenzene	11.12	95	168720	26.66	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	88.87%
63) Toluene-d8	8.70	98	463873	28.83	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	96.10%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX091120\
Data File : VX018352.D
Acq On : 11 Sep 2020 11:16
Operator : JC/SP
Sample : VX0911WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0911WBL01

Quant Time: Sep 12 06:21:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X090420W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Sep 04 12:13:41 2020
Response via : Initial Calibration

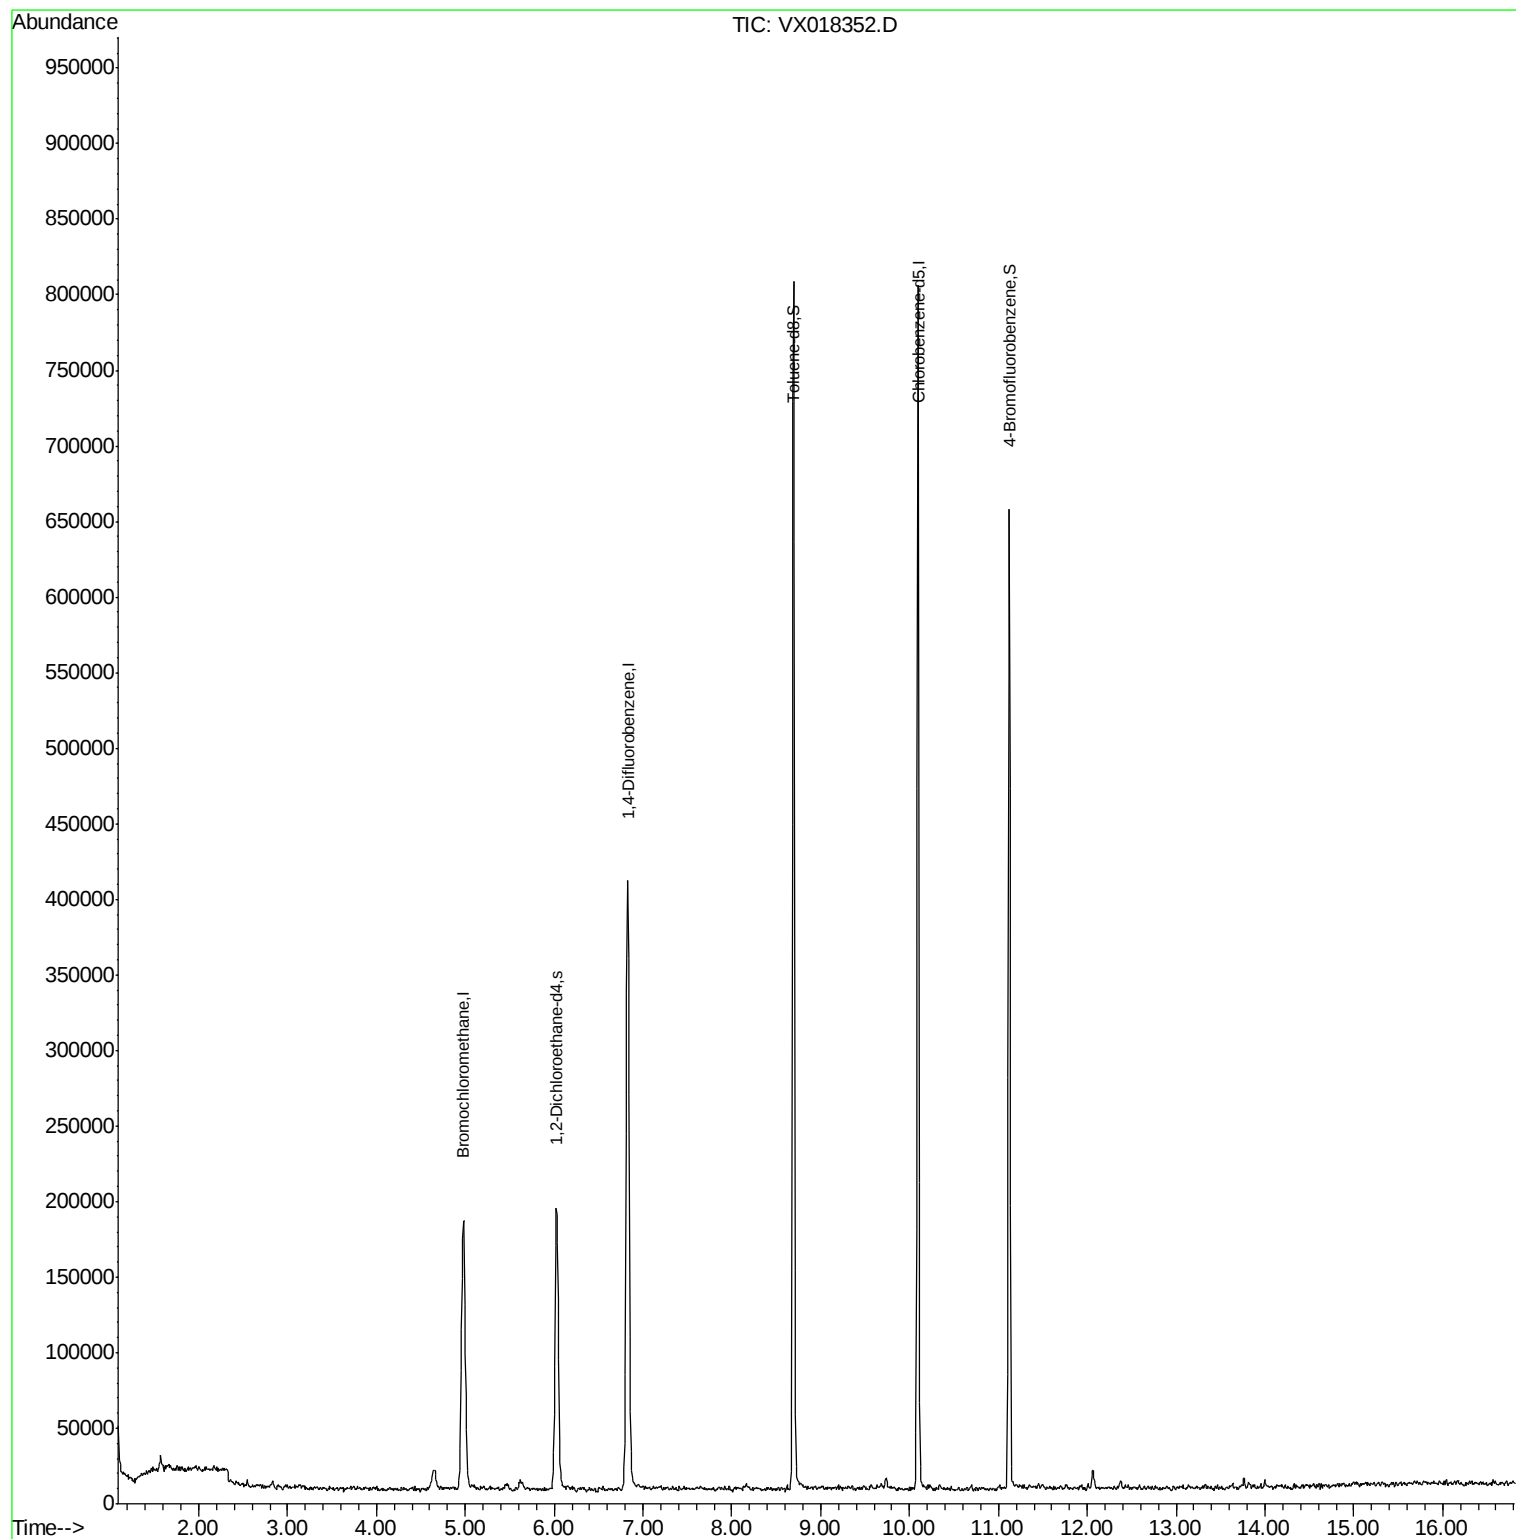

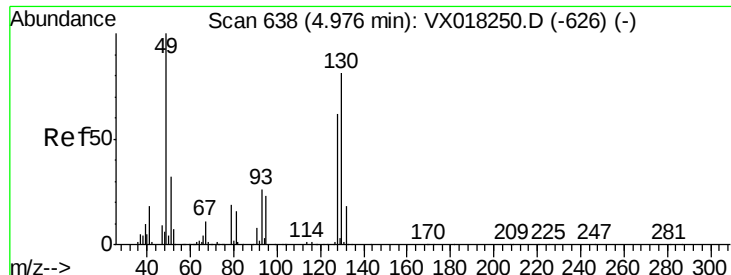

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 4.98 min Scan# 639

Delta R.T. 0.01 min

Lab File: VX018352.D

Acq: 11 Sep 2020 11:16

Instrument :

MSVOA_X

ClientSampleId :

VX0911WBL01


Tot Ion:128 Resp: 79344

Ion Ratio Lower Upper

128 100

49 149.3 0.0 392.0




130 130.3 0.0 320.2

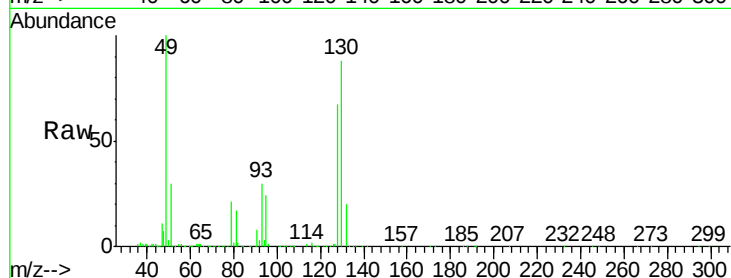

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

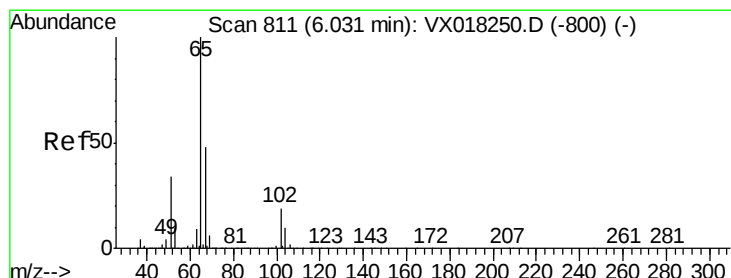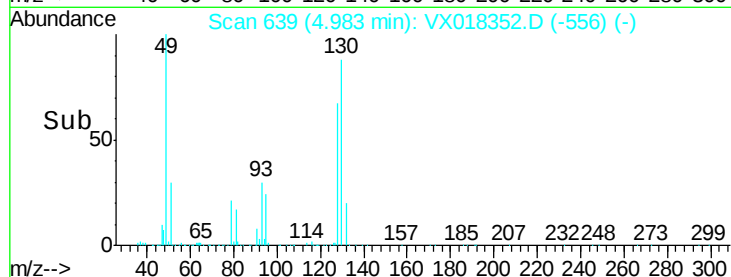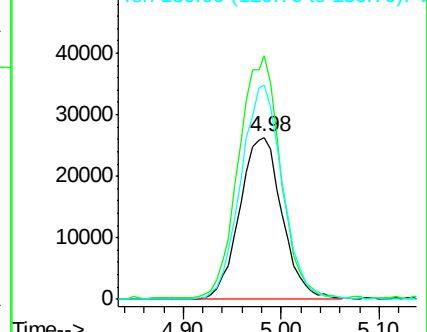

#27

1,2-Dichloroethane-d4

Concen: 29.557 ug/l

RT: 6.03 min Scan# 810

Delta R.T. -0.01 min

Lab File: VX018352.D


Acq: 11 Sep 2020 11:16

Tgt Ion: 65 Resp: 185017

Ion Ratio Lower Upper



65 100


67 52.1 39.9 59.9

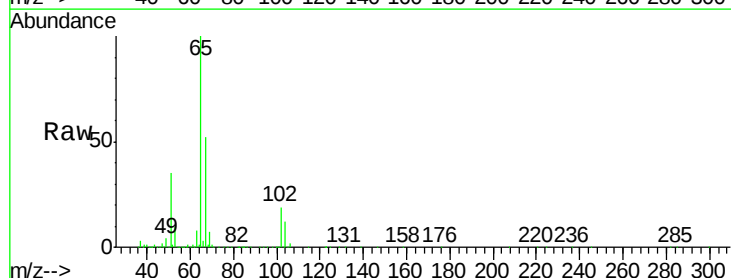

Abundance Ion 65.00 (64.70 to 65.70): VX0

Ion 67.00 (66.70 to 67.70): VX0



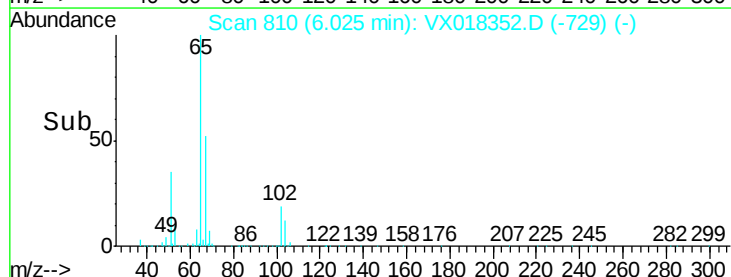
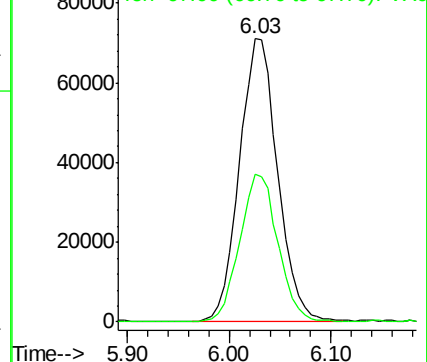


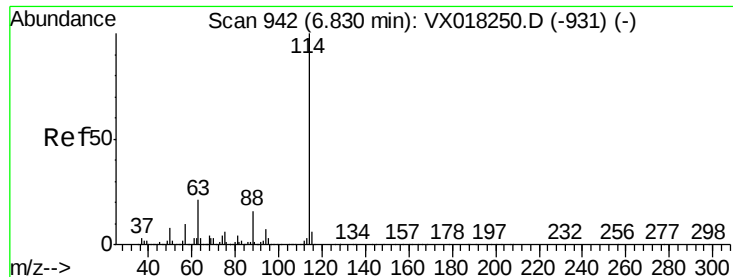

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. 0.00 min
 Lab File: VX018352.D
 Acq: 11 Sep 2020 11:16




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0911WBL01


Tot Ion	Ratio	Lower	Upper
114	100		
63	21.2	16.7	25.1
88	15.6	12.6	18.8

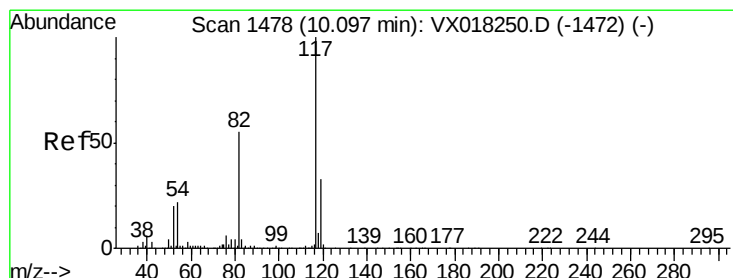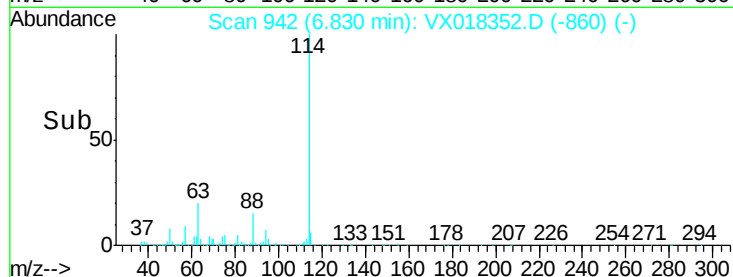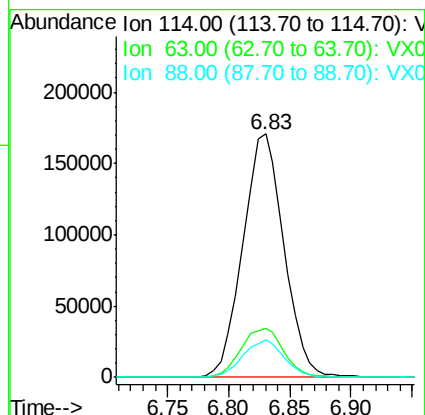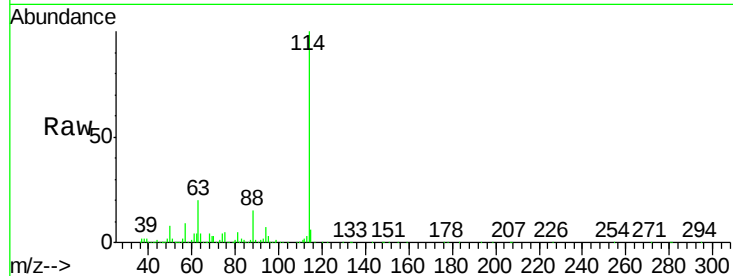

#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 10.10 min Scan# 1478
 Delta R.T. 0.00 min
 Lab File: VX018352.D
 Acq: 11 Sep 2020 11:16

Tgt Ion	Ratio	Lower	Upper
117	100		
82	54.8	44.2	66.4
119	31.7	26.1	39.1

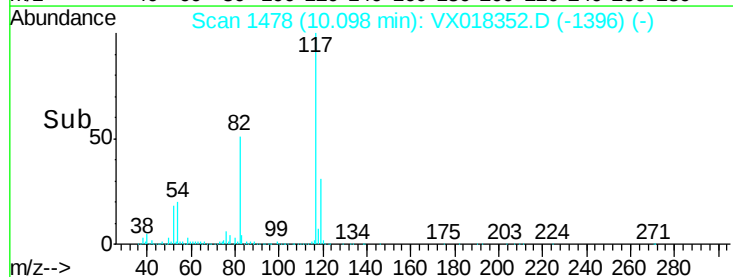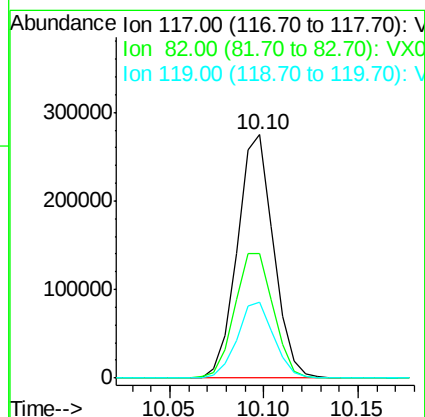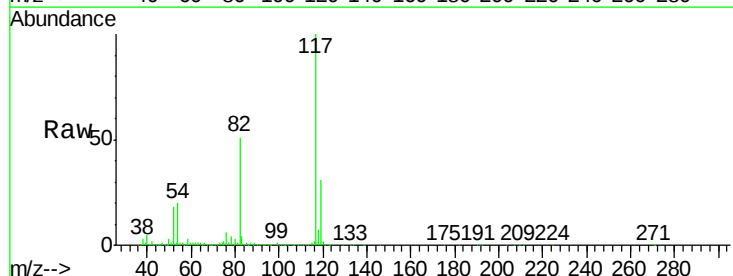

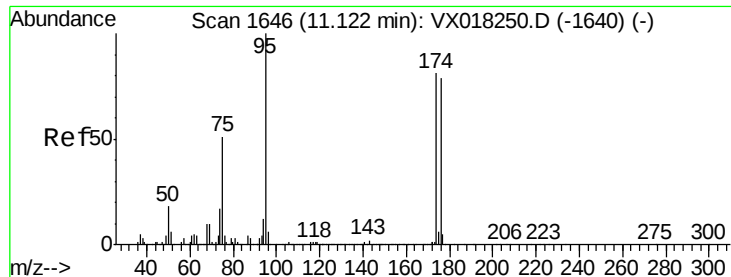

#60

4-Bromofluorobenzene

Concen: 26.663 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.00 min

Lab File: VX018352.D

Acq: 11 Sep 2020 11:16

Instrument :

MSVOA_X

ClientSampleId :

VX0911WBL01


Tot Ion: 95 Resp: 168720

Ion Ratio Lower Upper

95 100

174 78.9 64.2 96.4




176 74.7 62.2 93.4

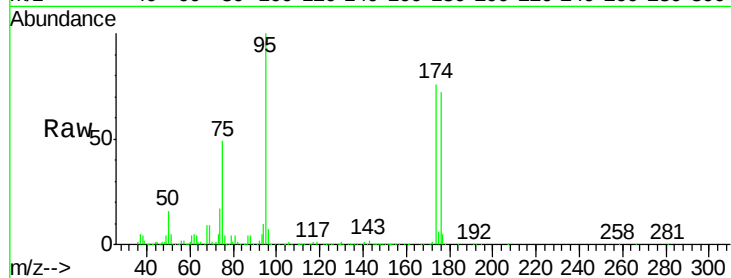

Abundance Ion 95.00 (94.70 to 95.70): VX0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

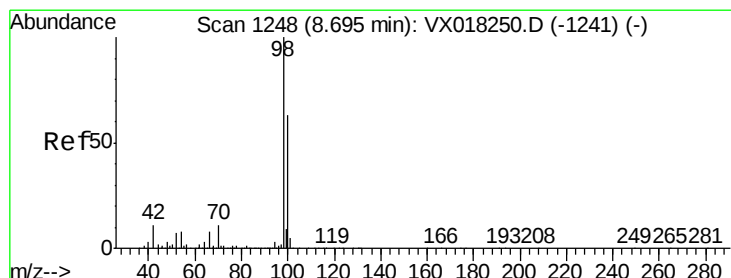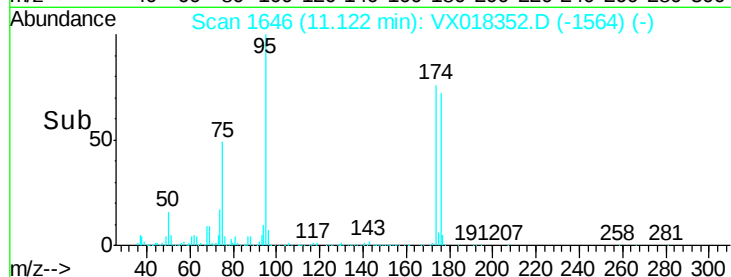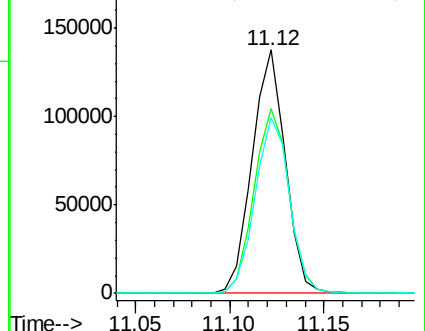

#63

Toluene-d8

Concen: 28.828 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. 0.00 min

Lab File: VX018352.D


Acq: 11 Sep 2020 11:16

Tgt Ion: 98 Resp: 463873

Ion Ratio Lower Upper

98 100

100 65.6 51.4 77.0

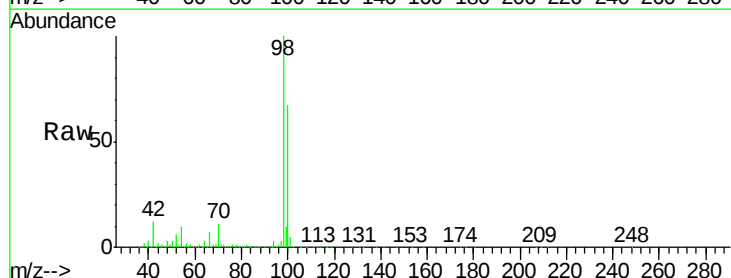

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

