

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX091120\
Data File : VX018359.D
Acq On : 11 Sep 2020 14:02
Operator : JC/SP
Sample : L3977-01 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EFF-WW

Integration Parameters: RTEINT3.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X090420W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.422	212	219	232	rBV	1852612	3339994	1.82%	1.784%
2	2.672	236	260	264	rBV2	39137868	183884810	100.00%	98.216%




Sum of corrected areas: 187224804

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX091120\
Data File : VX018359.D
Acq On : 11 Sep 2020 14:02
Operator : JC/SP
Sample : L3977-01 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EFF-WW

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X090420W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

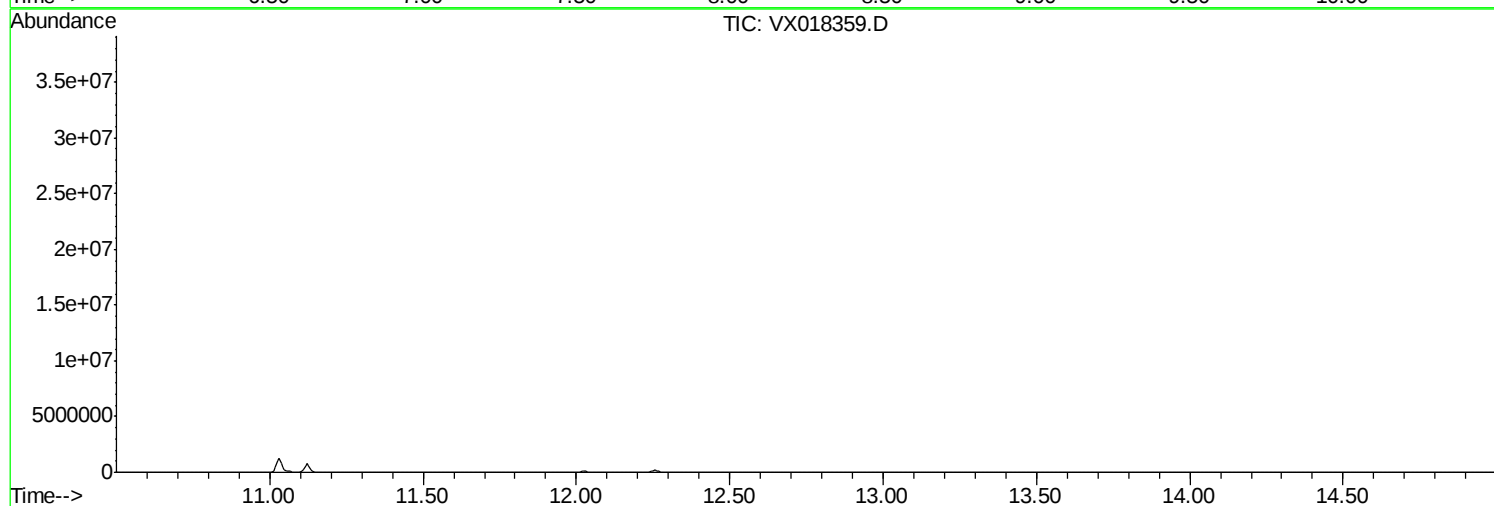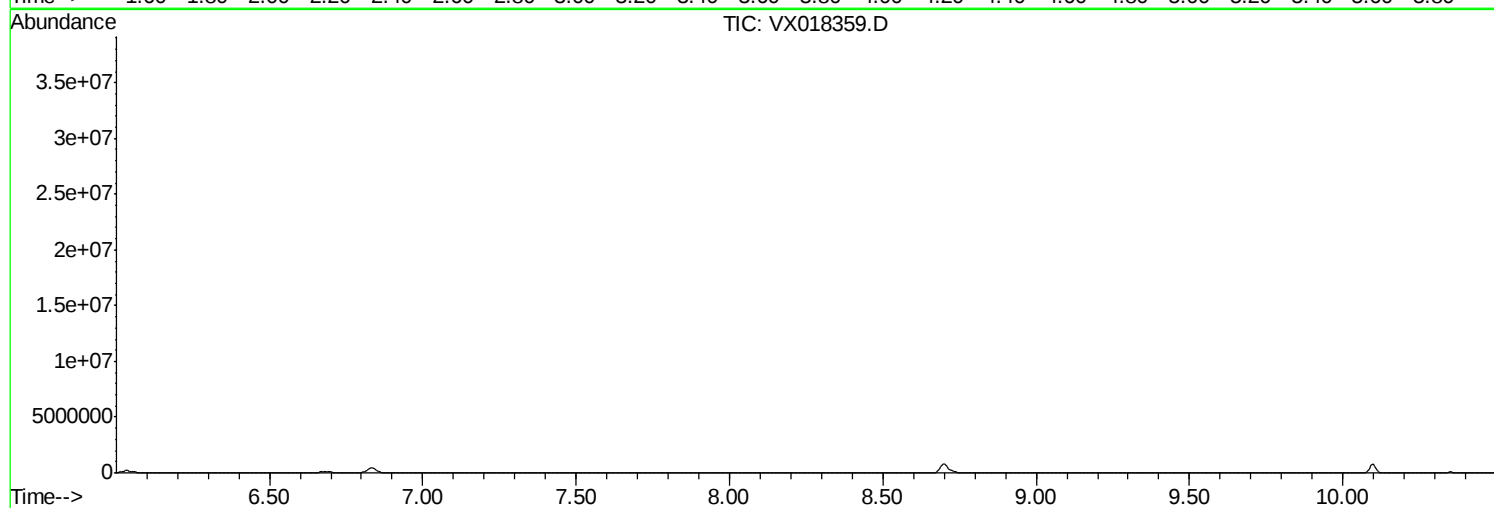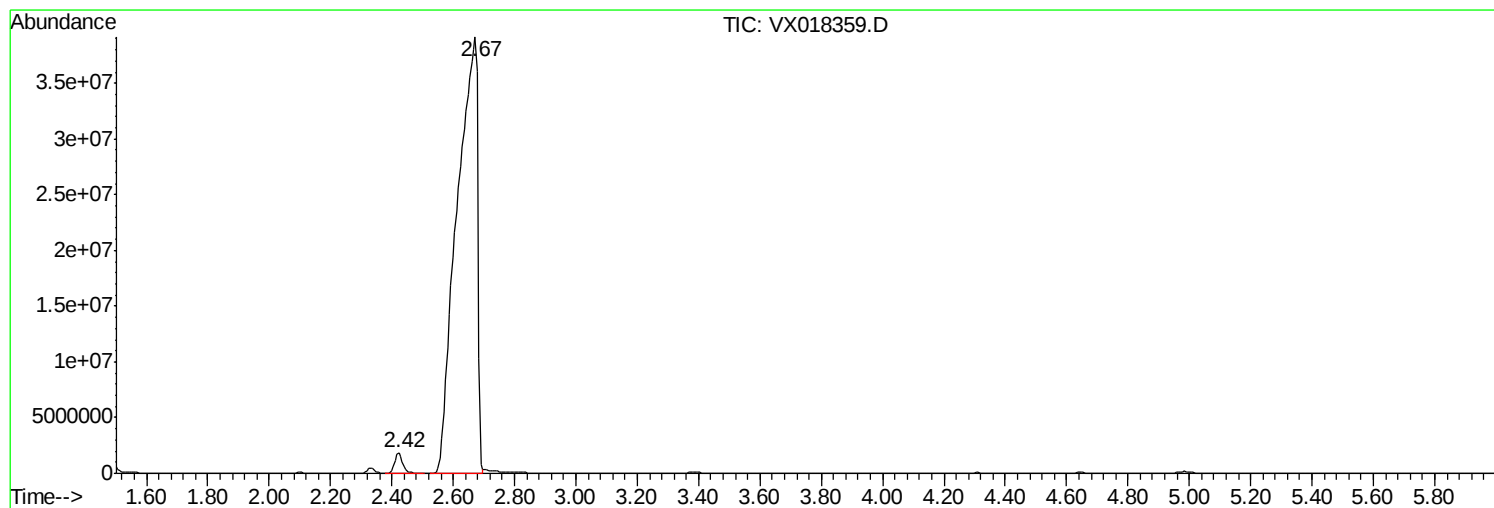

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX091120\
Data File : VX018359.D
Acq On : 11 Sep 2020 14:02
Operator : JC/SP
Sample : L3977-01 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EFF-WW










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X090420W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.67 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.67	30.00 ug/l	183885000	Bromochloromethane	4.98

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	16
2		Methane, nitroso-	45	CH3NO	000865-40-7	9
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	8
4		Isopropyl Alcohol	60	C3H8O	000067-63-0	7
5		Acetic acid, hydroxy-, ethyl ester	104	C4H8O3	000623-50-7	4

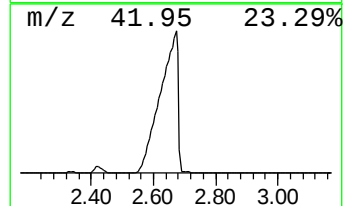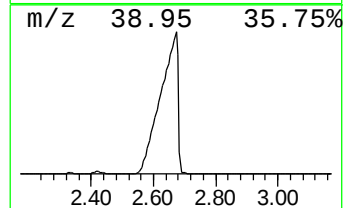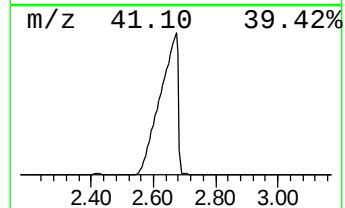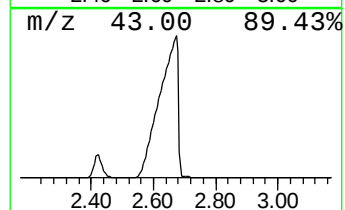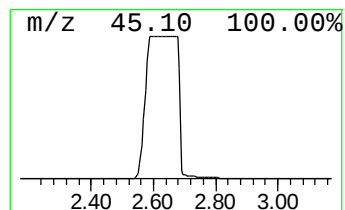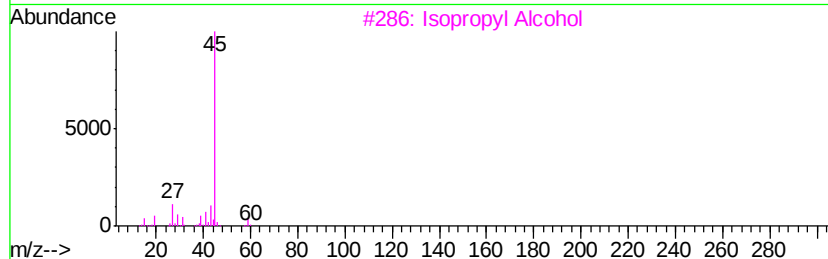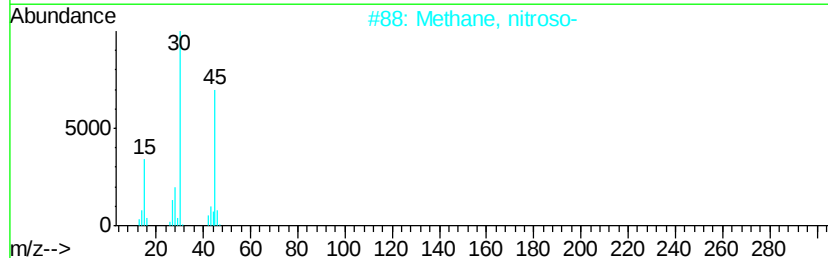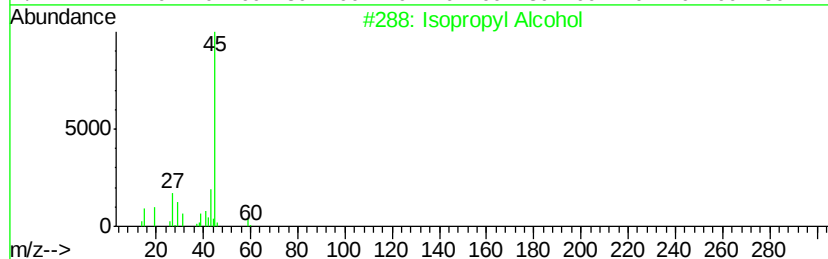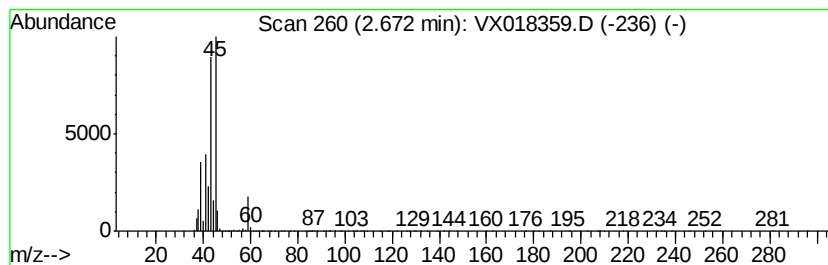

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX091120\
Data File : VX018359.D
Acq On : 11 Sep 2020 14:02
Operator : JC/SP
Sample : L3977-01 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EFF-WW

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X090420W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.67	2.67	30.0	ug/l	183885000	1	4.98	183885000	30.0