


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX091120\
 Data File : VX018349.D
 Acq On : 11 Sep 2020 09:26
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X090420W.M
 Title : SW846 624
 Last Update : Fri Aug 21 03:03:56 2020

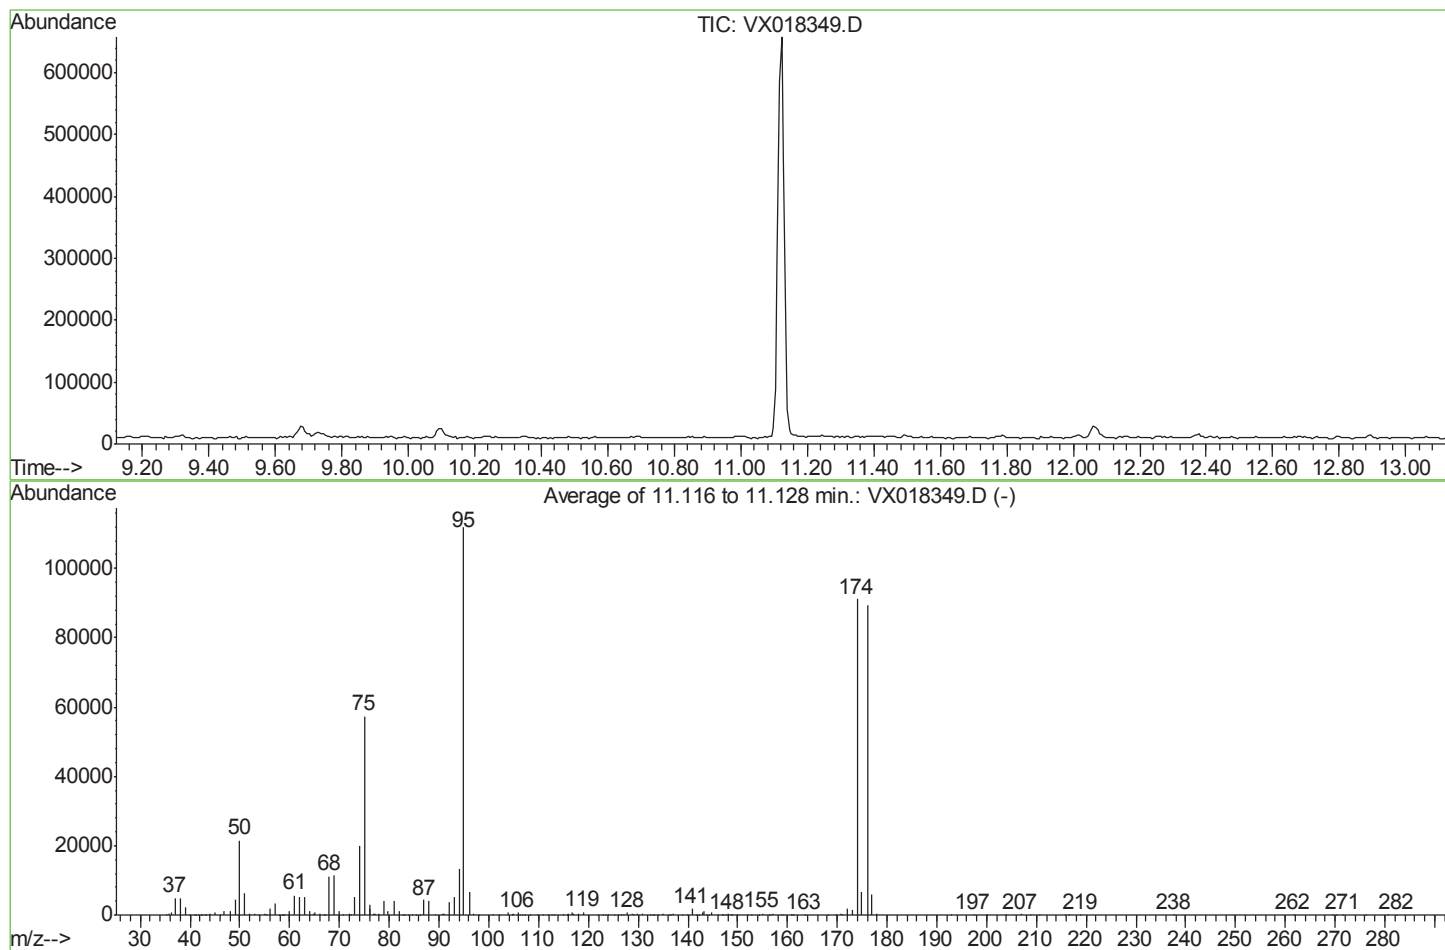

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1636

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	21510	PASS
75	95	30	60	51.3	57421	PASS
95	95	100	100	100.0	111826	PASS
96	95	5	9	6.1	6794	PASS
173	174	0.00	2	1.6	1476	PASS
174	95	50	100	81.5	91128	PASS
175	174	5	9	7.5	6828	PASS
176	174	95	101	98.0	89298	PASS
177	176	5	9	6.7	5959	PASS