

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091123\
 Data File : VX037644.D
 Acq On : 11 Sep 2023 16:11
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Sep 12 09:29:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 12 09:13:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	130141	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	224700	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	203525	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	82906	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	93128	44.229	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	88.460%
35) Dibromofluoromethane	5.385	113	72690	45.640	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.280%
50) Toluene-d8	8.647	98	282170	46.975	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	93.960%
62) 4-Bromofluorobenzene	11.079	95	89413	41.260	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	82.520%#
Target Compounds						
					Qvalue	
5) Bromomethane	1.599	94	480	0.314	ug/l #	41
11) Tert butyl alcohol	2.940	59	3505	Below Cal	#	78
13) Acrolein	2.239	56	442	1.285	ug/l #	76
15) Acrylonitrile	3.081	53	630	0.636	ug/l #	85
16) Acetone	2.380	43	1502	1.726	ug/l #	71
17) Carbon Disulfide	2.501	76	1258	0.369	ug/l #	77
18) Methyl Acetate	2.697	43	820	0.225	ug/l #	82
20) Methylene Chloride	2.776	84	467	Below Cal	#	58
23) Vinyl Acetate	3.739	43	1153	0.306	ug/l #	73
25) 2-Butanone	4.574	43	680	0.487	ug/l #	51
26) 2,2-Dichloropropane	4.586	77	904	0.434	ug/l #	54
29) Tetrahydrofuran	5.038	42	601	0.667	ug/l #	55
31) Cyclohexane	5.550	56	3467	1.430	ug/l #	3
36) 1,1-Dichloropropene	5.544	75	11815	5.379	ug/l #	52
38) Carbon Tetrachloride	5.550	117	13963	6.365	ug/l #	14
49) 1,4-Dioxane	7.671	88	135	2.772	ug/l #	30
51) 4-Methyl-2-Pentanone	8.580	43	1191	0.451	ug/l #	86
58) 2-Chloroethyl Vinyl ether	8.263	63	325	0.247	ug/l #	72
59) 2-Hexanone	9.445	43	741	0.366	ug/l	96
68) m/p-Xylenes	10.305	106	668	0.225	ug/l	92
76) 1,2,3-Trichloropropane	11.079	75	49686	26.512	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.079	75	49686	82.863	ug/l #	5
82) 4-Chlorotoluene	11.457	91	1053	0.209	ug/l	92
84) 1,2,4-Trimethylbenzene	11.756	105	1130	0.213	ug/l	96
87) 1,3-Dichlorobenzene	11.975	146	752	0.264	ug/l	94
88) 1,4-Dichlorobenzene	11.975	146	752	0.260	ug/l	93
89) n-Butylbenzene	12.341	91	1132	0.236	ug/l	94
91) 1,2-Dichlorobenzene	12.341	146	672	0.232	ug/l	84
93) 1,2,4-Trichlorobenzene	13.597	180	899	0.535	ug/l	88
94) Hexachlorobutadiene	13.725	225	178	0.244	ug/l	68
95) Naphthalene	13.780	128	3367	0.554	ug/l #	95
96) 1,2,3-Trichlorobenzene	13.963	180	1061	0.612	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX091123\
Data File : VX037644.D
Acq On : 11 Sep 2023 16:11
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Sep 12 09:29:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091123W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 12 09:13:03 2023
Response via : Initial Calibration




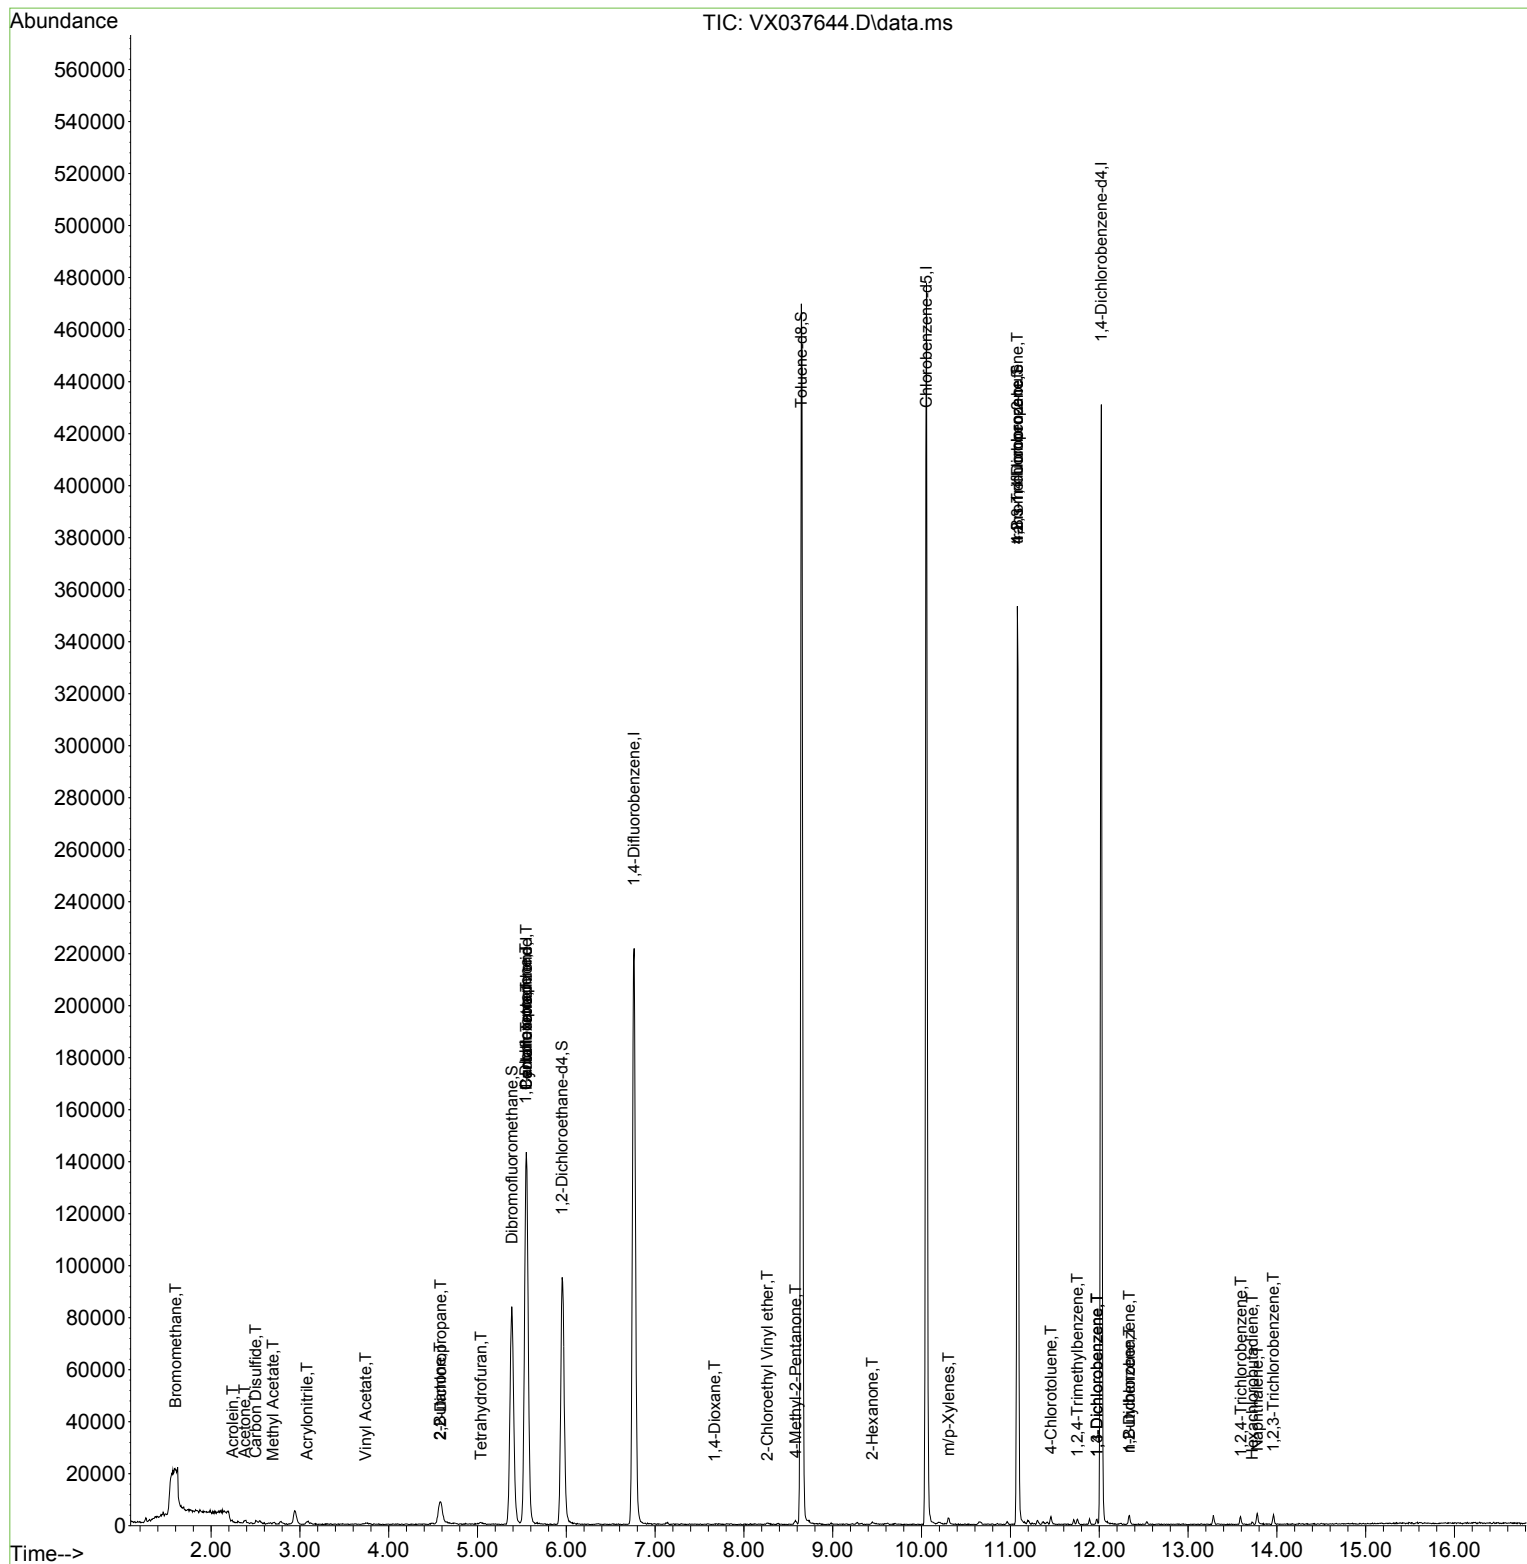




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 130141
Ion Ratio Lower Upper
168 100
99 62.6 56.6 85.0

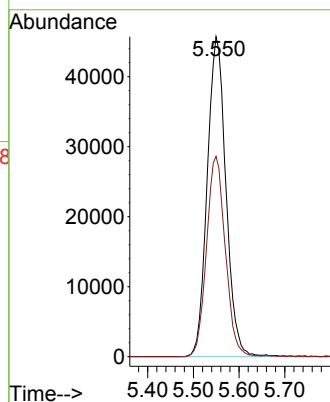

#5
Bromomethane
Concen: 0.314 ug/l
RT: 1.599 min Scan# 84
Delta R.T. -0.000 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Tgt Ion: 94 Resp: 480
Ion Ratio Lower Upper
94 100
96 36.8 74.6 111.8#

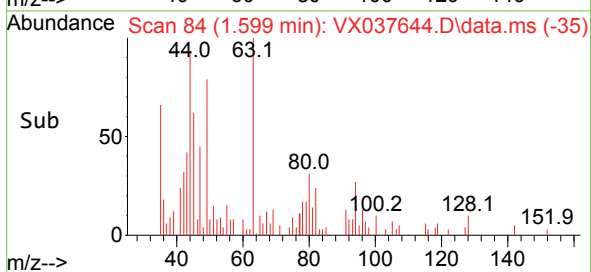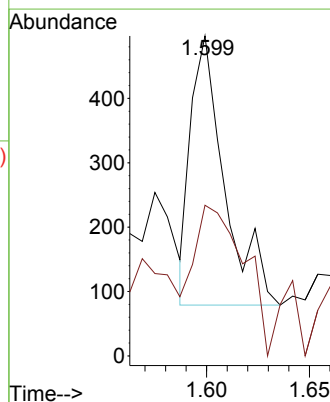

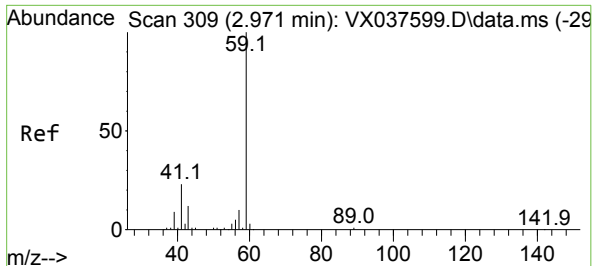

#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.940 min Scan# 309

Delta R.T. -0.031 min


Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :



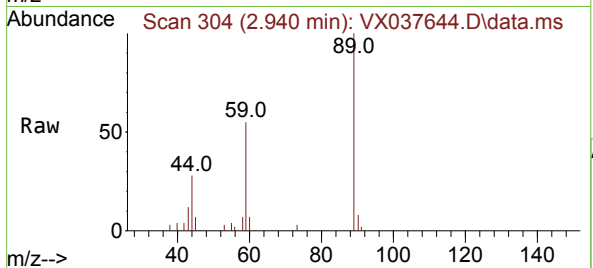


Tgt Ion: 59 Resp: 3505

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

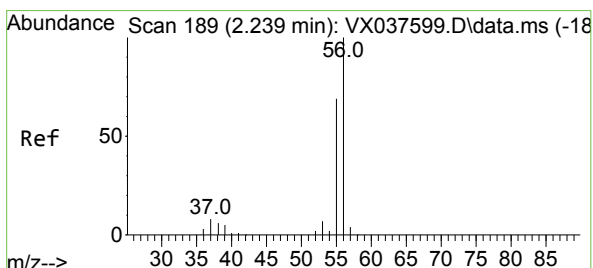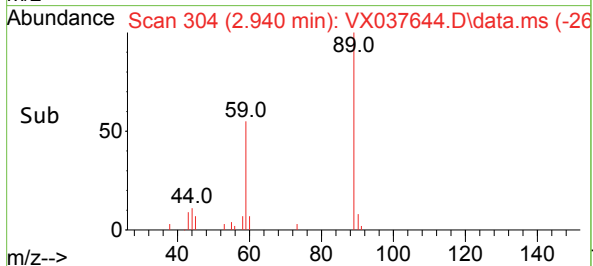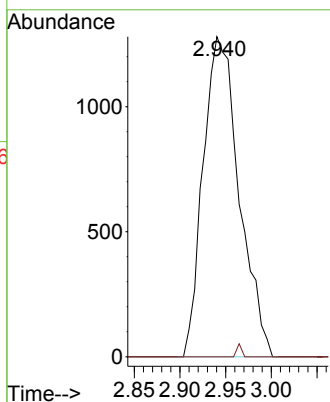

#13

Acrolein

Concen: 1.285 ug/l

RT: 2.239 min Scan# 189

Delta R.T. -0.000 min

Lab File: VX037644.D




Acq: 11 Sep 2023 16:11


Tgt Ion: 56 Resp: 442

Ion Ratio Lower Upper

56 100


55 51.1 57.1 85.7#

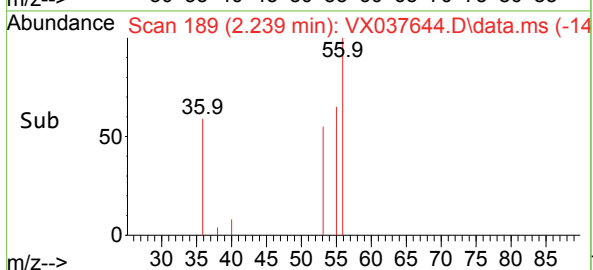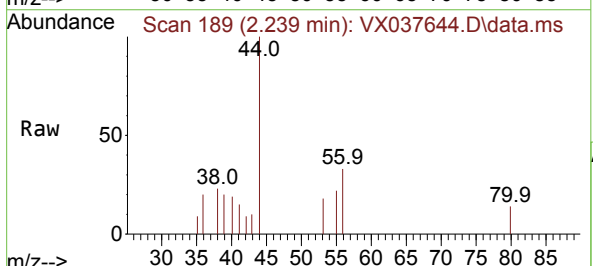






#15
Acrylonitrile
Concen: 0.636 ug/l
RT: 3.081 min Scan# 31
Delta R.T. 0.018 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 53 Resp: 630
Ion Ratio Lower Upper
53 100
52 74.0 66.0 99.0
51 21.3 29.8 44.6#



#16
Acetone
Concen: 1.726 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Tgt Ion: 43 Resp: 1502
Ion Ratio Lower Upper
43 100
58 42.5 21.9 32.9#

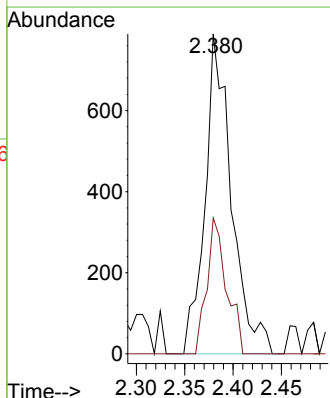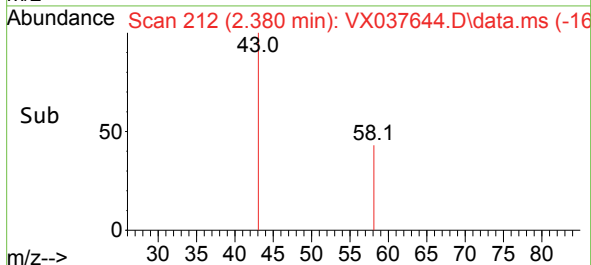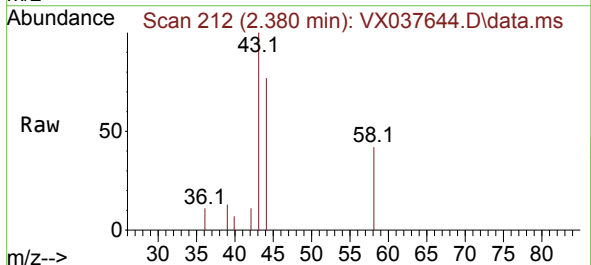



#17

Carbon Disulfide

Concen: 0.369 ug/l

RT: 2.501 min Scan# 21

Delta R.T. -0.006 min


Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 76 Resp: 1258

Ion Ratio Lower Upper

76 100

78 17.1 7.0 10.6#

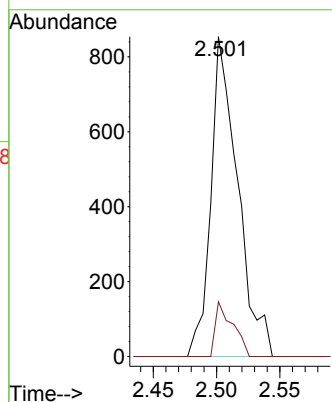

#18

Methyl Acetate

Concen: 0.225 ug/l

RT: 2.697 min Scan# 264

Delta R.T. -0.006 min

Lab File: VX037644.D




Acq: 11 Sep 2023 16:11


Tgt Ion: 43 Resp: 820

Ion Ratio Lower Upper

43 100


74 13.7 17.8 26.8#

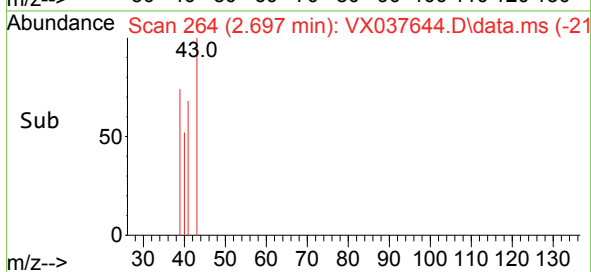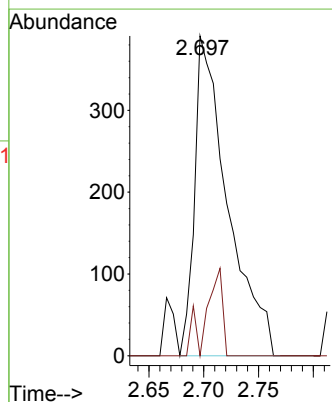






#20
Methylene Chloride
Concen: Below Cal
RT: 2.776 min Scan# 21
Delta R.T. -0.012 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 84 Resp: 467
Ion Ratio Lower Upper
84 100
49 77.2 103.6 155.4#
51 29.7 33.8 50.6#
86 23.2 49.4 74.0#



#23
Vinyl Acetate
Concen: 0.306 ug/l
RT: 3.739 min Scan# 435
Delta R.T. 0.018 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Tgt Ion: 43 Resp: 1153
Ion Ratio Lower Upper
43 100
86 0.0 7.8 11.8#





#25

2-Butanone

Concen: 0.487 ug/l

RT: 4.574 min Scan# 5

Delta R.T. 0.012 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 680

Ion Ratio Lower Upper

43 100

72 0.0 19.4 29.2#

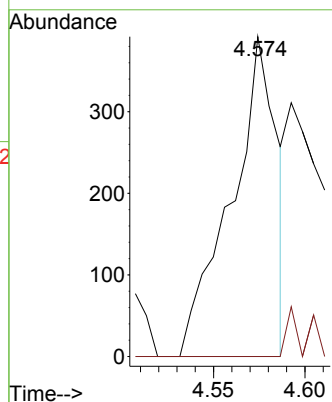

#26

2,2-Dichloropropane

Concen: 0.434 ug/l

RT: 4.586 min Scan# 574

Delta R.T. 0.110 min

Lab File: VX037644.D




Acq: 11 Sep 2023 16:11


Tgt Ion: 77 Resp: 904

Ion Ratio Lower Upper

77 100

97 0.0 10.8 32.3#

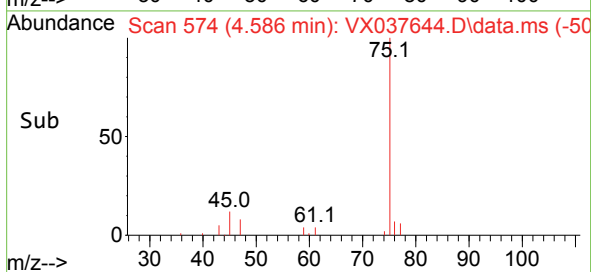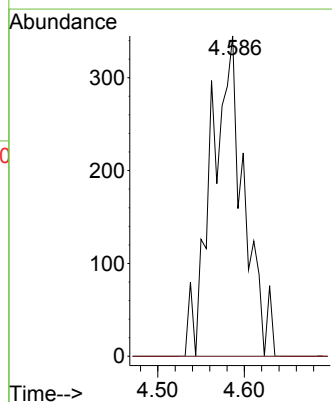

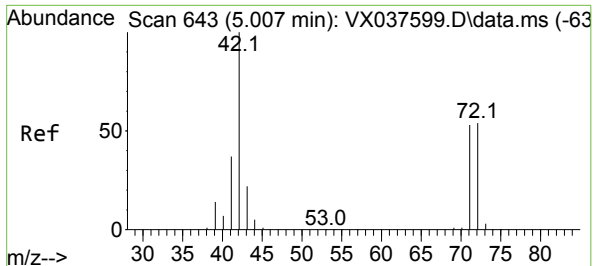

#29

Tetrahydrofuran

Concen: 0.667 ug/l

RT: 5.038 min Scan# 64

Delta R.T. 0.030 min


Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :

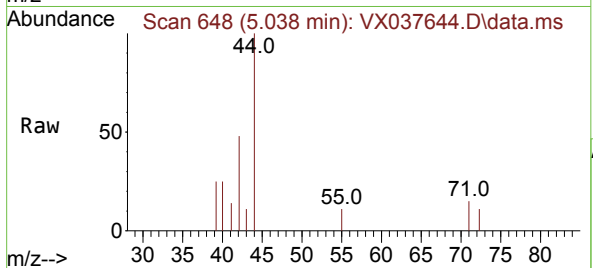




Tgt Ion: 42 Resp: 601

Ion Ratio Lower Upper

42 100

72 11.8 34.2 51.4#

71 14.6 32.2 48.2#

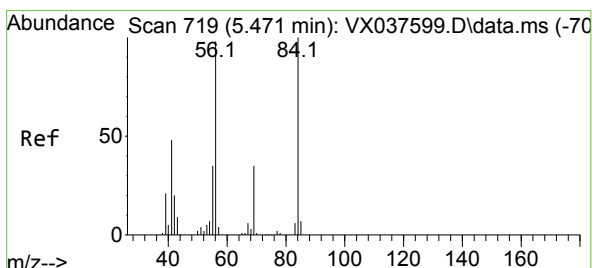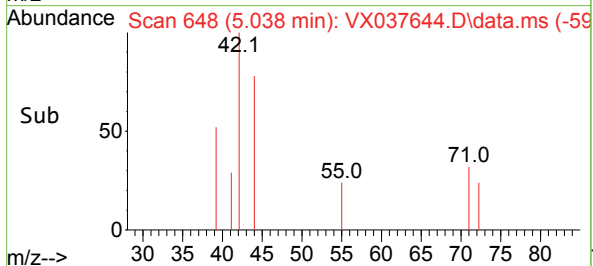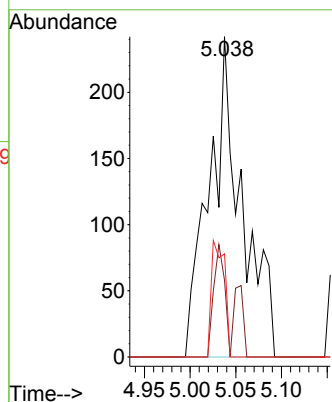

#31

Cyclohexane

Concen: 1.430 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.079 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11




Tgt Ion: 56 Resp: 3467


Ion Ratio Lower Upper

56 100

69 161.8 23.4 35.2#

84 121.4 65.9 98.9#

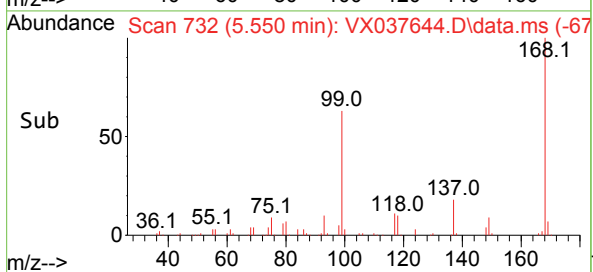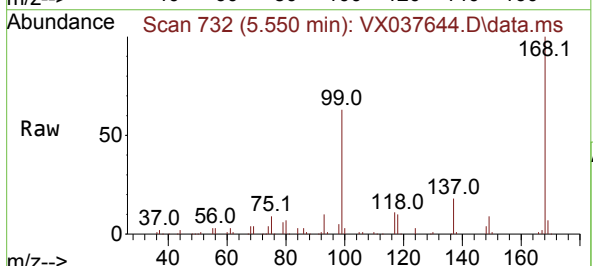



#33

1,2-Dichloroethane-d4

Concen: 44.229 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 93128

Ion Ratio Lower Upper

65 100

67 52.1 0.0 100.2

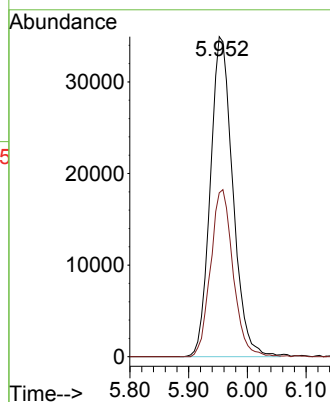

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11




Tgt Ion:114 Resp: 224700


Ion Ratio Lower Upper

114 100

63 20.8 0.0 45.0


88 15.6 0.0 36.6








#35
Dibromofluoromethane
Concen: 45.640 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:113 Resp: 72690
Ion Ratio Lower Upper
113 100
111 103.2 82.9 124.3
192 17.5 13.3 19.9



#36
1,1-Dichloropropene
Concen: 5.379 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.146 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Tgt Ion: 75 Resp: 11815
Ion Ratio Lower Upper
75 100
110 10.4 17.0 50.9#
77 0.0 24.7 37.1#





#38

Carbon Tetrachloride

Concen: 6.365 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.128 min


Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion:117 Resp: 13963

Ion Ratio Lower Upper

117 100

119 3.1 78.2 117.2#

121 0.0 24.4 36.6#

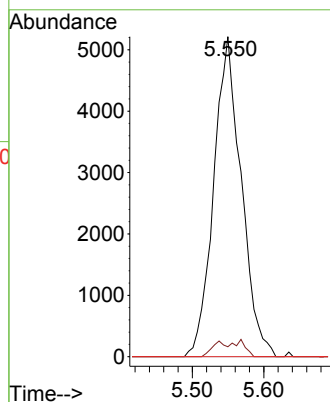

#49

1,4-Dioxane

Concen: 2.772 ug/l

RT: 7.671 min Scan# 1080

Delta R.T. 0.006 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11




Tgt Ion: 88 Resp: 135


Ion Ratio Lower Upper

88 100

43 155.6 0.0 0.0#

58 15.6 60.1 90.1#


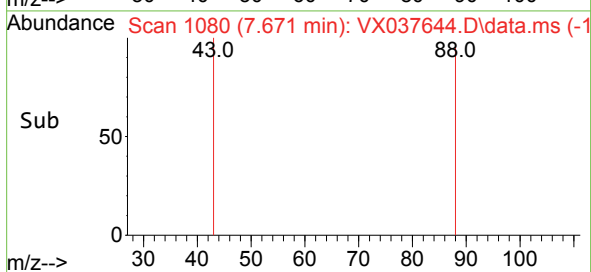
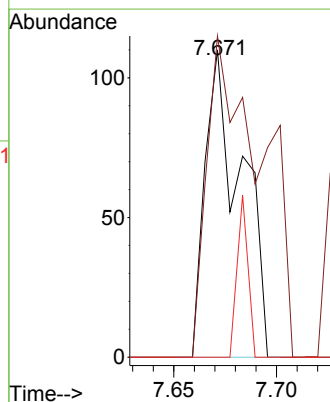
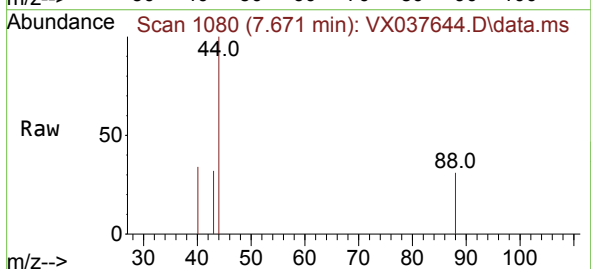




#50
Toluene-d8
Concen: 46.975 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 282170
Ion Ratio Lower Upper
98 100
100 62.9 53.1 79.7



#51
4-Methyl-2-Pentanone
Concen: 0.451 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Tgt Ion: 43 Resp: 1191
Ion Ratio Lower Upper
43 100
58 29.4 30.4 45.6#




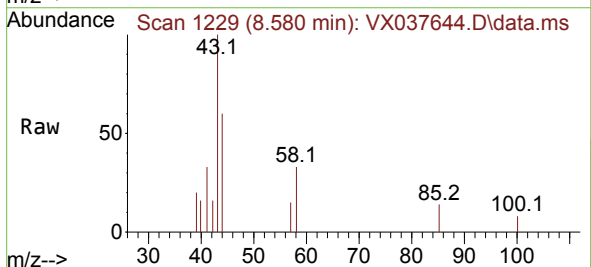




#58
2-Chloroethyl Vinyl ether
Concen: 0.247 ug/l
RT: 8.263 min Scan# 1177
Delta R.T. 0.018 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 63 Resp: 325
Ion Ratio Lower Upper
63 100
106 13.5 22.5 33.7#

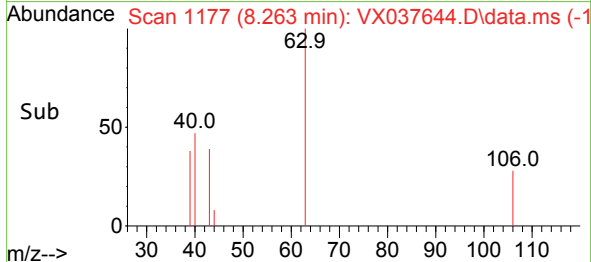

#59
2-Hexanone
Concen: 0.366 ug/l
RT: 9.445 min Scan# 1371
Delta R.T. 0.012 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Tgt Ion: 43 Resp: 741
Ion Ratio Lower Upper
43 100
58 54.8 26.2 78.5


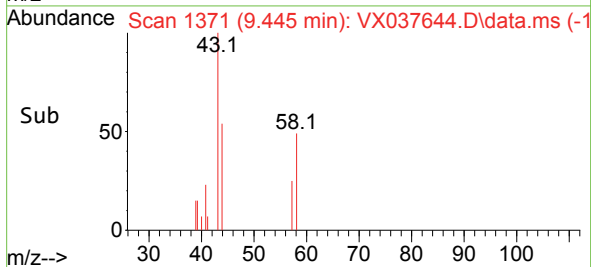

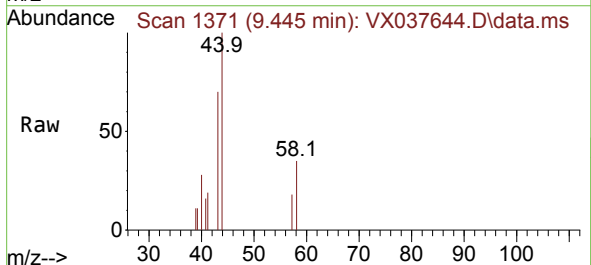




#62
4-Bromofluorobenzene
Concen: 41.260 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 89413
Ion Ratio Lower Upper
95 100
174 77.7 0.0 135.6
176 74.3 0.0 131.0

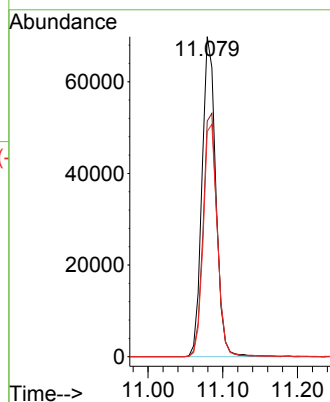

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Tgt Ion: 117 Resp: 203525
Ion Ratio Lower Upper
117 100
82 58.1 46.2 69.4
119 31.5 25.5 38.3


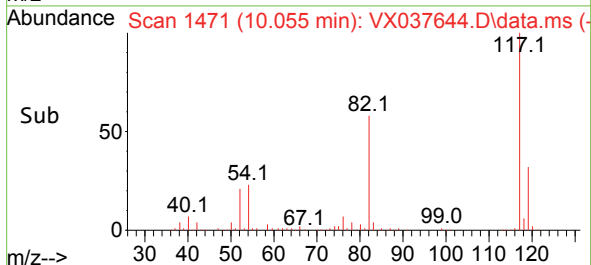

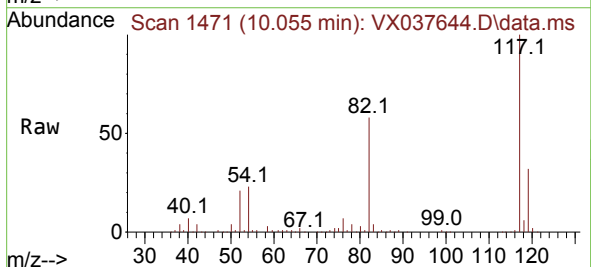




#68
m/p-Xylenes
Concen: 0.225 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 668
Ion Ratio Lower Upper
106 100
91 218.7 165.5 248.3

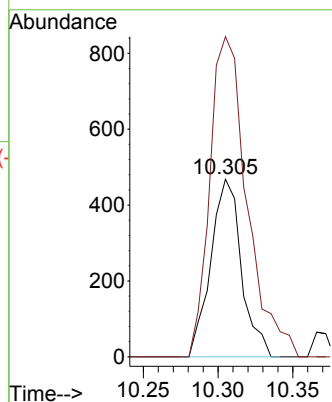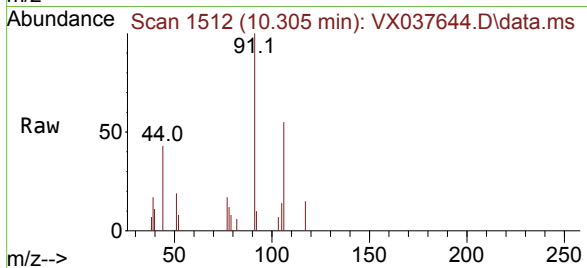

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Tgt Ion:152 Resp: 82906
Ion Ratio Lower Upper
152 100
115 62.1 43.3 129.9
150 157.3 0.0 345.0

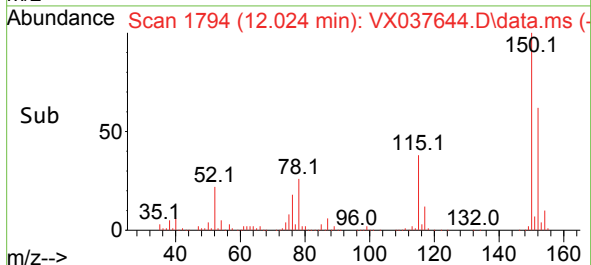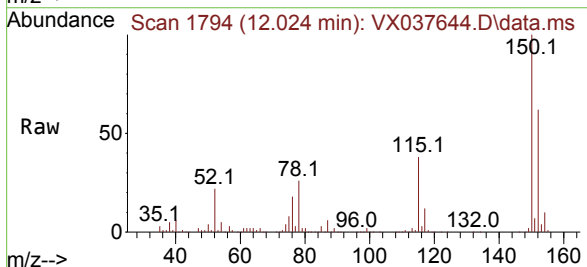



#76

1,2,3-Trichloropropane

Concen: 26.512 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.159 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 49686

Ion Ratio Lower Upper

75 100

77 1.1 19.1 57.5#

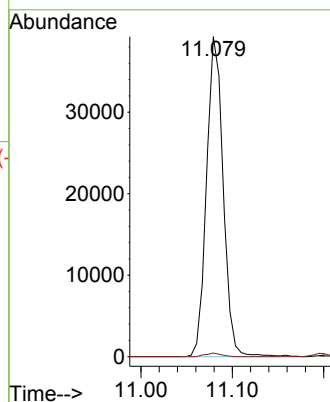

#81

trans-1,4-Dichloro-2-butene

Concen: 82.863 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11




Tgt Ion: 75 Resp: 49686


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.2 36.9 55.3#









#82
4-Chlorotoluene
Concen: 0.209 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. -0.000 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 1053
Ion Ratio Lower Upper
91 100
126 32.4 14.2 42.6

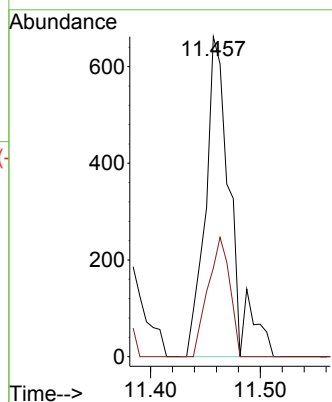

#84
1,2,4-Trimethylbenzene
Concen: 0.213 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX037644.D
Acq: 11 Sep 2023 16:11

Tgt Ion: 105 Resp: 1130
Ion Ratio Lower Upper
105 100
120 45.0 21.2 63.6

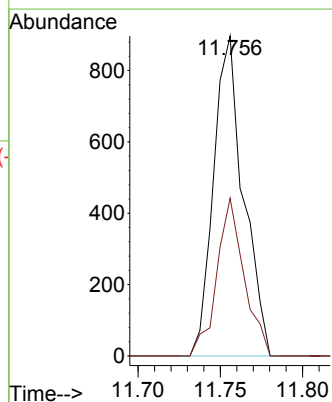



#87

1,3-Dichlorobenzene

Concen: 0.264 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. 0.006 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:146 Resp: 752

Ion Ratio Lower Upper

146 100

111 51.5 22.1 66.1

148 62.0 31.8 95.3



#88

1,4-Dichlorobenzene

Concen: 0.260 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. -0.067 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11




Tgt Ion:146 Resp: 752


Ion Ratio Lower Upper

146 100

111 51.5 21.3 63.7

148 62.0 31.8 95.4

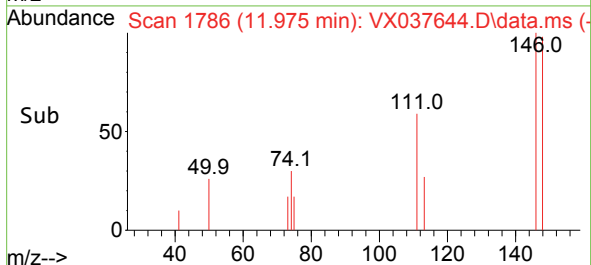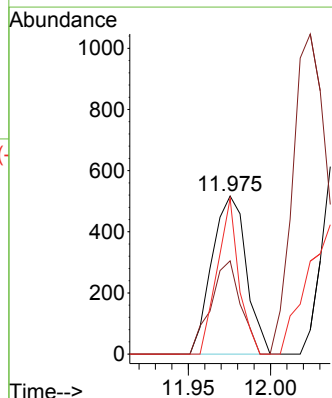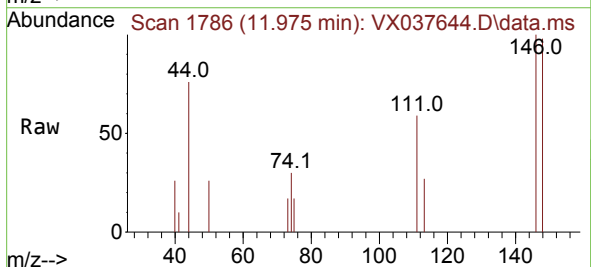

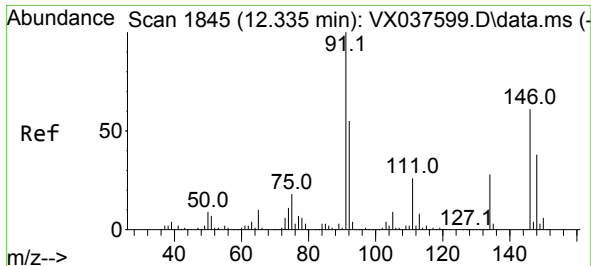

#89

n-Butylbenzene

Concen: 0.236 ug/l

RT: 12.341 min Scan# 1846

Delta R.T. 0.006 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 91 Resp: 1132

Ion Ratio Lower Upper

91 100

92 50.1 27.4 82.0

134 22.2 12.6 37.8

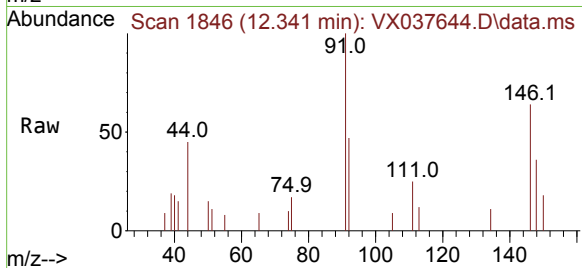

#91

1,2-Dichlorobenzene

Concen: 0.232 ug/l

RT: 12.341 min Scan# 1846

Delta R.T. 0.006 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11




Tgt Ion:146 Resp: 672


Ion Ratio Lower Upper

146 100

111 41.8 22.4 67.0

148 45.1 31.6 95.0

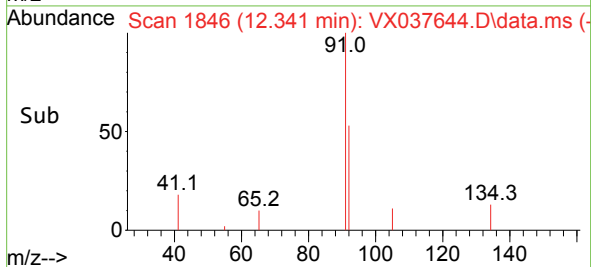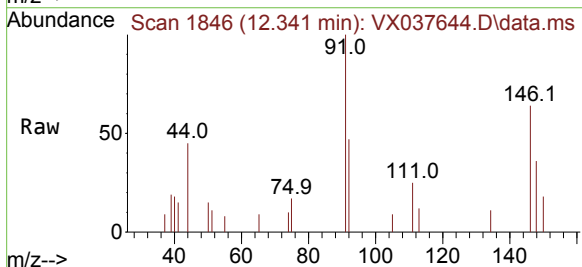



#93

1,2,4-Trichlorobenzene

Concen: 0.535 ug/l

RT: 13.597 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:180 Resp: 899

Ion Ratio Lower Upper

180 100

182 88.7 48.3 144.8

145 23.5 18.0 54.0



#94

Hexachlorobutadiene

Concen: 0.244 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. -0.000 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11




Tgt Ion:225 Resp: 178


Ion Ratio Lower Upper

225 100

223 79.8 31.1 93.2

227 33.1 32.5 97.5





#95

Naphthalene

Concen: 0.554 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min


Lab File: VX037644.D

Acq: 11 Sep 2023 16:11




Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion:	128	Resp:	3367
Ion	Ratio	Lower	Upper
128	100		
127	10.1	10.3	15.5#
129	9.7	8.8	13.2



#96

1,2,3-Trichlorobenzene

Concen: 0.612 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX037644.D

Acq: 11 Sep 2023 16:11

Tgt Ion:	180	Resp:	1061
Ion	Ratio	Lower	Upper
180	100		
182	99.0	46.9	140.6
145	33.7	17.8	53.5

