

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091123\  
 Data File : VX037651.D  
 Acq On : 11 Sep 2023 19:26  
 Operator : JC/MD  
 Sample : IBLK  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :

Quant Time: Sep 12 09:15:49 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091123W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Sep 12 09:13:03 2023  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon  | Response | Conc      | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|-----------|--------|----------|
| -----                         |        |       |          |           |        |          |
| Internal Standards            |        |       |          |           |        |          |
| 1) Pentafluorobenzene         | 5.550  | 168   | 155989   | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.763  | 114   | 268809   | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 10.055 | 117   | 236629   | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024 | 152   | 92024    | 50.000    | ug/l   | 0.00     |
| System Monitoring Compounds   |        |       |          |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 5.958  | 65    | 106647   | 42.257    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 78 - 117 | Recovery  | =      | 84.520%  |
| 35) Dibromofluoromethane      | 5.391  | 113   | 84805    | 44.509    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 75 - 124 | Recovery  | =      | 89.020%  |
| 50) Toluene-d8                | 8.647  | 98    | 330698   | 46.021    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 92 - 112 | Recovery  | =      | 92.040%  |
| 62) 4-Bromofluorobenzene      | 11.079 | 95    | 105744   | 40.789    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 83 - 123 | Recovery  | =      | 81.580%# |
| Target Compounds              |        |       |          |           |        |          |
|                               |        |       |          |           | Qvalue |          |
| 2) Dichlorodifluoromethane    | 1.166  | 85    | 635      | 0.381     | ug/l   | 82       |
| 3) Chloromethane              | 1.294  | 50    | 755      | 0.386     | ug/l   | 100      |
| 4) Vinyl Chloride             | 1.373  | 62    | 793      | 0.368     | ug/l # | 45       |
| 5) Bromomethane               | 1.611  | 94    | 736      | 0.401     | ug/l # | 59       |
| 6) Chloroethane               | 1.690  | 64    | 345      | 0.236     | ug/l # | 62       |
| 7) Trichlorofluoromethane     | 1.886  | 101   | 1461     | 0.400     | ug/l   | 98       |
| 9) 1,1,2-Trichlorotrifluo...  | 2.331  | 101   | 518      | 0.321     | ug/l   | 96       |
| 10) Methyl Iodide             | 2.453  | 142   | 1280     | 0.667     | ug/l # | 81       |
| 11) Tert butyl alcohol        | 2.959  | 59    | 2475     | Below Cal | #      | 78       |
| 12) 1,1-Dichloroethene        | 2.324  | 96    | 829      | 0.523     | ug/l # | 70       |
| 13) Acrolein                  | 2.239  | 56    | 1186     | 2.876     | ug/l   | 89       |
| 14) Allyl chloride            | 2.660  | 41    | 1056     | 0.374     | ug/l # | 76       |
| 15) Acrylonitrile             | 3.068  | 53    | 1537     | 1.295     | ug/l   | 94       |
| 16) Acetone                   | 2.379  | 43    | 1629     | 1.561     | ug/l # | 86       |
| 17) Carbon Disulfide          | 2.507  | 76    | 6886     | 1.684     | ug/l   | 97       |
| 18) Methyl Acetate            | 2.709  | 43    | 1075     | 0.246     | ug/l # | 77       |
| 20) Methylene Chloride        | 2.794  | 84    | 1127     | Below Cal |        | 84       |
| 21) trans-1,2-Dichloroethene  | 3.087  | 96    | 1420     | 0.755     | ug/l # | 80       |
| 23) Vinyl Acetate             | 3.745  | 43    | 2437     | 0.539     | ug/l # | 89       |
| 25) 2-Butanone                | 4.574  | 43    | 1836     | 1.096     | ug/l # | 85       |
| 27) cis-1,2-Dichloroethene    | 4.495  | 96    | 814      | 0.362     | ug/l   | 76       |
| 29) Tetrahydrofuran           | 5.025  | 42    | 358      | 0.331     | ug/l # | 34       |
| 31) Cyclohexane               | 5.482  | 56    | 1009     | 0.347     | ug/l # | 82       |
| 36) 1,1-Dichloropropene       | 5.702  | 75    | 2099     | 0.799     | ug/l # | 87       |
| 38) Carbon Tetrachloride      | 5.678  | 117   | 806      | 0.307     | ug/l # | 76       |
| 39) Methylcyclohexane         | 7.378  | 83    | 1085     | 0.351     | ug/l   | 96       |
| 40) Benzene                   | 6.049  | 78    | 1948     | 0.244     | ug/l   | 100      |
| 42) 1,2-Dichloroethane        | 6.098  | 62    | 965      | 0.312     | ug/l # | 77       |
| 44) Trichloroethene           | 7.128  | 130   | 1247     | 0.640     | ug/l   | 81       |
| 46) Dibromomethane            | 7.580  | 93    | 521      | 0.341     | ug/l # | 84       |
| 51) 4-Methyl-2-Pentanone      | 8.586  | 43    | 1586     | 0.502     | ug/l   | 89       |
| 52) Toluene                   | 8.720  | 92    | 1685     | 0.333     | ug/l   | 86       |
| 53) t-1,3-Dichloropropene     | 8.982  | 75    | 776      | 0.280     | ug/l # | 83       |
| 54) cis-1,3-Dichloropropene   | 8.384  | 75    | 777      | 0.257     | ug/l # | 77       |
| 58) 2-Chloroethyl Vinyl ether | 8.250  | 63    | 810      | 0.514     | ug/l # | 89       |
| 59) 2-Hexanone                | 9.445  | 43    | 1272     | 0.525     | ug/l   | 95       |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091123\  
 Data File : VX037651.D  
 Acq On : 11 Sep 2023 19:26  
 Operator : JC/MD  
 Sample : IBLK  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :

Quant Time: Sep 12 09:15:49 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091123W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Sep 12 09:13:03 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| 64) Tetrachloroethene         | 9.281  | 164  | 1222     | 0.806  | ug/l # | 84       |
| 65) Chlorobenzene             | 10.085 | 112  | 2284     | 0.448  | ug/l # | 82       |
| 67) Ethyl Benzene             | 10.201 | 91   | 4232     | 0.467  | ug/l   | 100      |
| 68) m/p-Xylenes               | 10.305 | 106  | 3482     | 1.007  | ug/l   | 96       |
| 69) o-Xylene                  | 10.646 | 106  | 1245     | 0.363  | ug/l   | 91       |
| 70) Styrene                   | 10.658 | 104  | 2104     | 0.372  | ug/l # | 90       |
| 73) Isopropylbenzene          | 10.963 | 105  | 3777     | 0.545  | ug/l   | 99       |
| 74) N-amyl acetate            | 10.847 | 43   | 747      | 0.244  | ug/l # | 78       |
| 76) 1,2,3-Trichloropropane    | 11.079 | 75   | 57415    | 27.601 | ug/l # | 39       |
| 77) Bromobenzene              | 11.195 | 156  | 935      | 0.563  | ug/l   | 99       |
| 78) n-propylbenzene           | 11.305 | 91   | 5900     | 0.738  | ug/l   | 100      |
| 79) 2-Chlorotoluene           | 11.366 | 91   | 3627     | 0.738  | ug/l   | 89       |
| 80) 1,3,5-Trimethylbenzene    | 11.451 | 105  | 3729     | 0.637  | ug/l   | 87       |
| 81) trans-1,4-Dichloro-2-b... | 11.079 | 75   | 57415    | 86.266 | ug/l # | 5        |
| 82) 4-Chlorotoluene           | 11.457 | 91   | 4832     | 0.864  | ug/l   | 94       |
| 83) tert-Butylbenzene         | 11.713 | 119  | 2963     | 0.508  | ug/l   | 95       |
| 84) 1,2,4-Trimethylbenzene    | 11.756 | 105  | 4154     | 0.707  | ug/l   | 98       |
| 85) sec-Butylbenzene          | 11.890 | 105  | 4422     | 0.612  | ug/l   | 99       |
| 86) p-Isopropyltoluene        | 12.012 | 119  | 3929     | 0.660  | ug/l   | 89       |
| 87) 1,3-Dichlorobenzene       | 11.969 | 146  | 3078     | 0.975  | ug/l   | 97       |
| 88) 1,4-Dichlorobenzene       | 11.969 | 146  | 3078     | 0.957  | ug/l   | 96       |
| 89) n-Butylbenzene            | 12.335 | 91   | 4440     | 0.833  | ug/l   | 92       |
| 90) Hexachloroethane          | 12.542 | 117  | 456      | 0.453  | ug/l   | 75       |
| 91) 1,2-Dichlorobenzene       | 12.335 | 146  | 2194     | 0.683  | ug/l   | 96       |
| 93) 1,2,4-Trichlorobenzene    | 13.591 | 180  | 2986     | 1.601  | ug/l   | 93       |
| 94) Hexachlorobutadiene       | 13.725 | 225  | 693      | 0.857  | ug/l   | 87       |
| 95) Naphthalene               | 13.780 | 128  | 9945     | 1.473  | ug/l   | 97       |
| 96) 1,2,3-Trichlorobenzene    | 13.963 | 180  | 3112     | 1.618  | ug/l   | 98       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX091123\  
 Data File : VX037651.D  
 Acq On : 11 Sep 2023 19:26  
 Operator : JC/MD  
 Sample : IBLK  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :


Quant Time: Sep 12 09:15:49 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091123W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Sep 12 09:13:03 2023  
 Response via : Initial Calibration

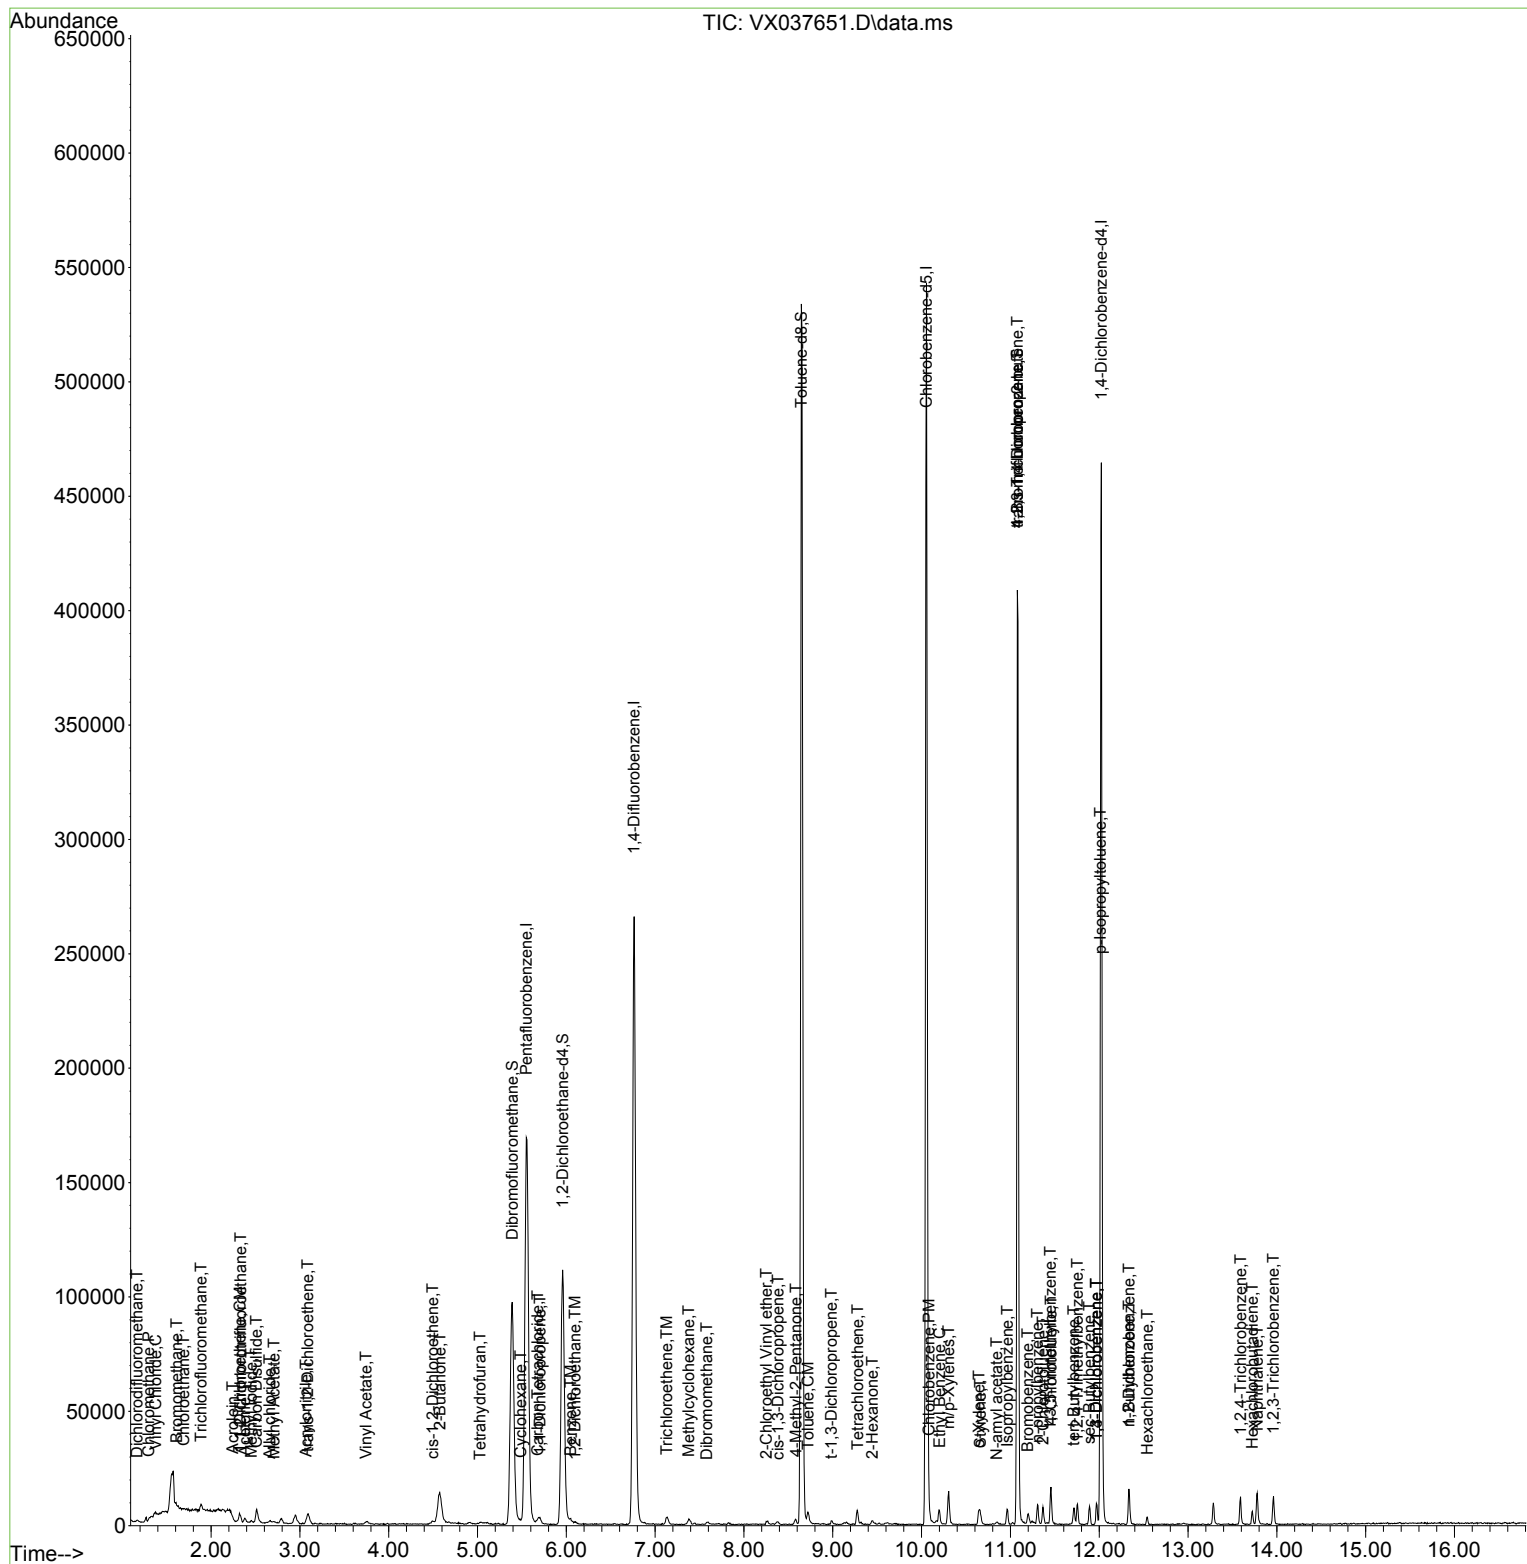






#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 71  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion:168 Resp: 155989  
Ion Ratio Lower Upper  
168 100  
99 64.1 56.6 85.0

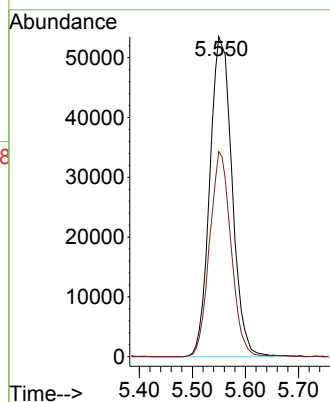

#2  
Dichlorodifluoromethane  
Concen: 0.381 ug/l  
RT: 1.166 min Scan# 13  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 85 Resp: 635  
Ion Ratio Lower Upper  
85 100  
87 23.3 16.7 50.1



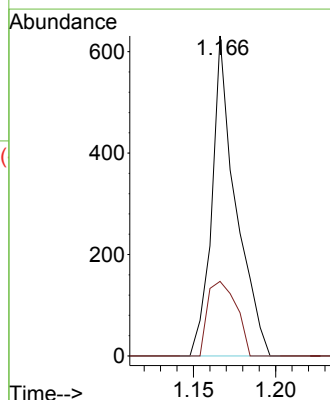



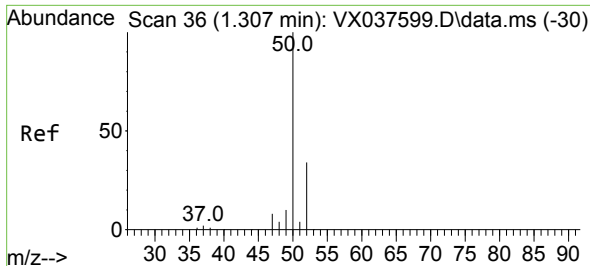

#3  
Chloromethane  
Concen: 0.386 ug/l  
RT: 1.294 min Scan# 34  
Delta R.T. -0.013 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 50 Resp: 755  
Ion Ratio Lower Upper  
50 100  
52 31.7 25.5 38.3

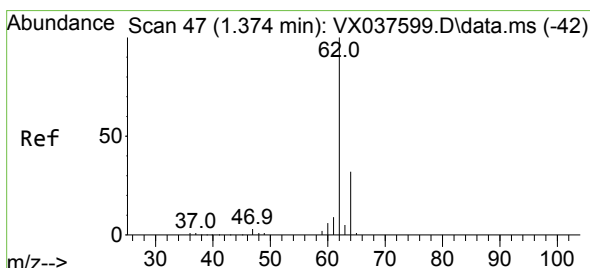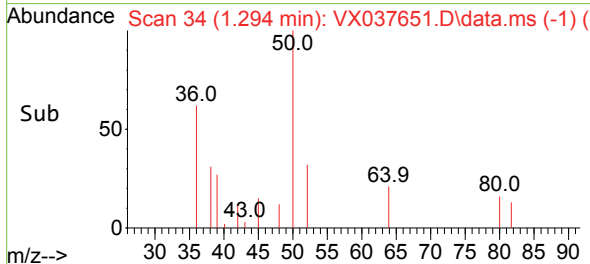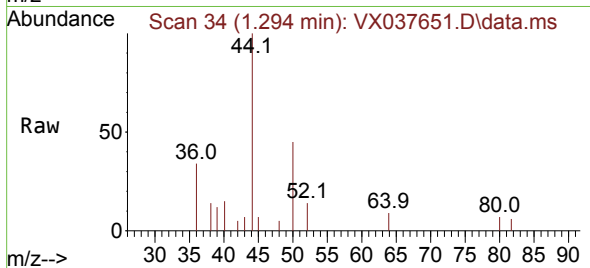

#4  
Vinyl Chloride  
Concen: 0.368 ug/l  
RT: 1.373 min Scan# 47  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 62 Resp: 793  
Ion Ratio Lower Upper  
62 100  
64 62.0 25.4 38.0#


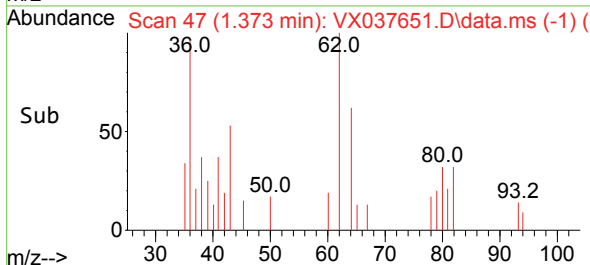

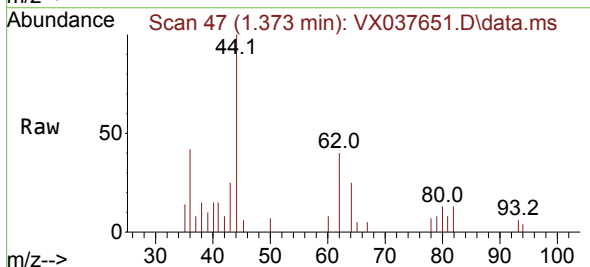


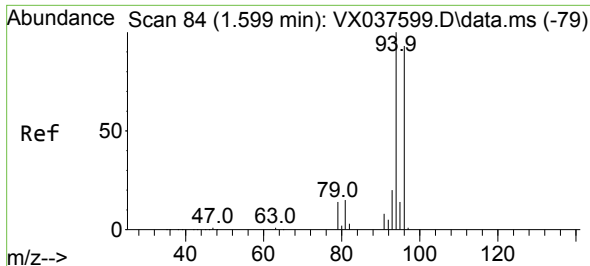

#5  
Bromomethane  
Concen: 0.401 ug/l  
RT: 1.611 min Scan# 80  
Delta R.T. 0.012 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 94 Resp: 736  
Ion Ratio Lower Upper  
94 100  
96 132.4 74.6 111.8#

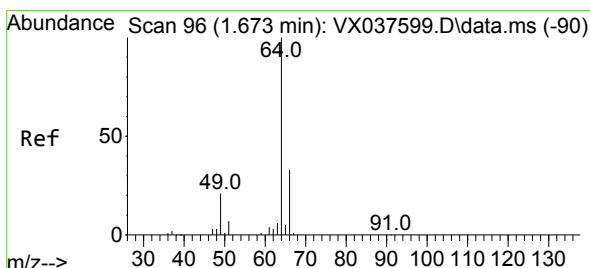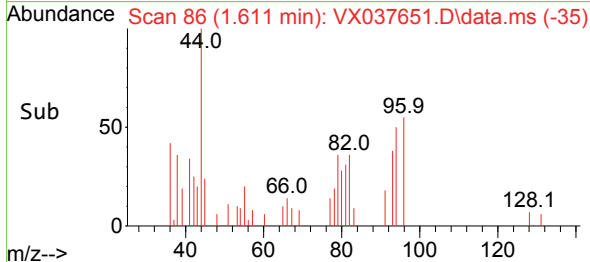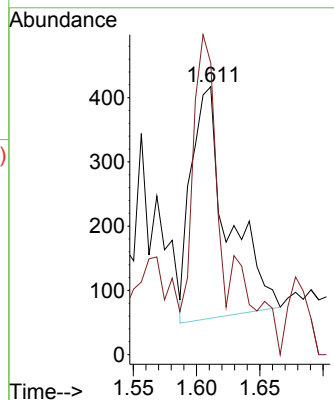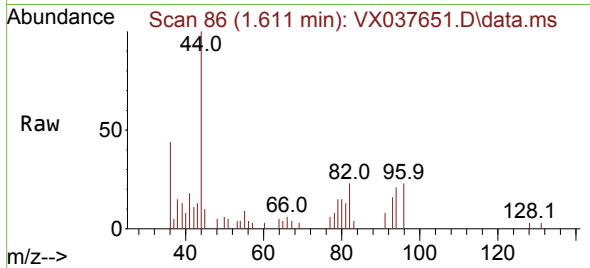

#6  
Chloroethane  
Concen: 0.236 ug/l  
RT: 1.690 min Scan# 99  
Delta R.T. 0.017 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26


Tgt Ion: 64 Resp: 345  
Ion Ratio Lower Upper  
64 100  
66 52.4 25.1 37.7#

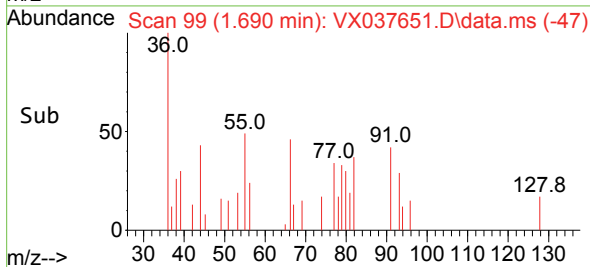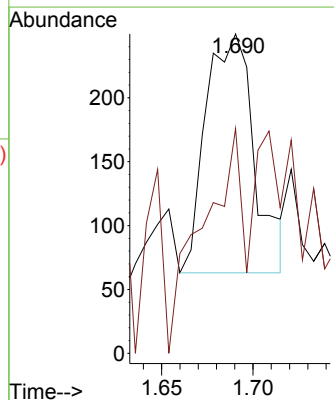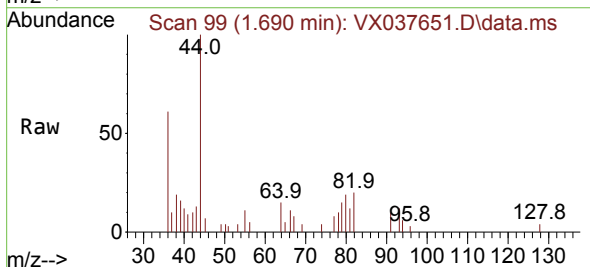






#7  
 Trichlorofluoromethane  
 Concen: 0.400 ug/l  
 RT: 1.886 min Scan# 11  
 Delta R.T. 0.006 min  
 Lab File: VX037651.D  
 Acq: 11 Sep 2023 19:26

Instrument :  
 MSVOA\_X  
 ClientSampleId :







Tgt Ion:101 Resp: 1461  
 Ion Ratio Lower Upper  
 101 100  
 103 62.4 51.4 77.2



#9  
 1,1,2-Trichlorotrifluoroethane  
 Concen: 0.321 ug/l  
 RT: 2.331 min Scan# 204  
 Delta R.T. 0.006 min  
 Lab File: VX037651.D  
 Acq: 11 Sep 2023 19:26


Tgt Ion:101 Resp: 518  
 Ion Ratio Lower Upper  
 101 100  
 85 41.9 37.0 55.6  
 151 71.2 58.6 87.8

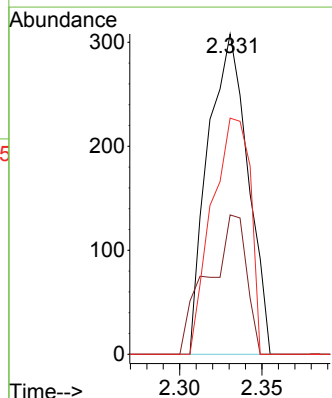






#10  
Methyl Iodide  
Concen: 0.667 ug/l  
RT: 2.453 min Scan# 21  
Delta R.T. 0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion:142 Resp: 1280  
Ion Ratio Lower Upper  
142 100  
127 38.4 41.6 62.4#  
141 6.6 11.6 17.4#

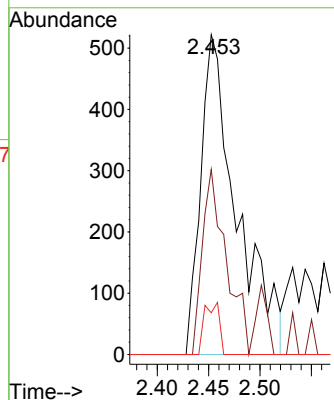

#11  
Tert butyl alcohol  
Concen: Below Cal  
RT: 2.959 min Scan# 307  
Delta R.T. -0.012 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26


Tgt Ion: 59 Resp: 2475  
Ion Ratio Lower Upper  
59 100  
57 0.0 6.0 9.0#

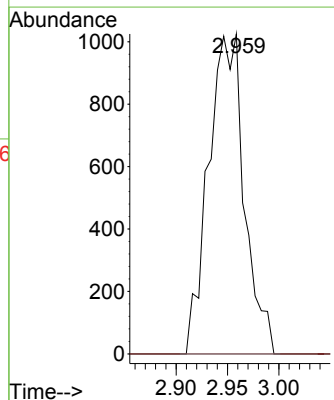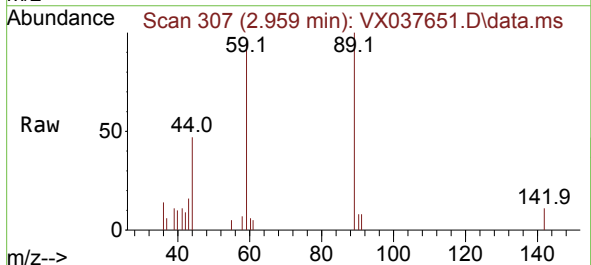






#12  
1,1-Dichloroethene  
Concen: 0.523 ug/l  
RT: 2.324 min Scan# 201  
Delta R.T. 0.012 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion: 96 Resp: 829  
Ion Ratio Lower Upper  
96 100  
61 131.9 144.6 216.8#  
98 48.3 50.4 75.6#

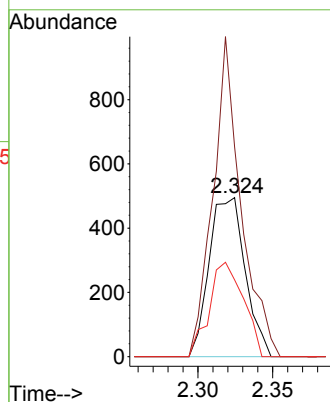

#13  
Acrolein  
Concen: 2.876 ug/l  
RT: 2.239 min Scan# 189  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 56 Resp: 1186  
Ion Ratio Lower Upper  
56 100  
55 80.5 57.1 85.7


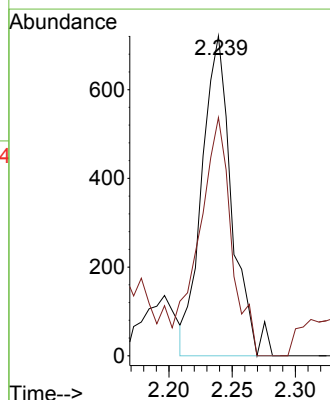






#14  
 Allyl chloride  
 Concen: 0.374 ug/l  
 RT: 2.660 min Scan# 21  
 Delta R.T. -0.000 min  
 Lab File: VX037651.D  
 Acq: 11 Sep 2023 19:26




Instrument :  
 MSVOA\_X  
 ClientSampleId :


Tgt Ion: 41 Resp: 1056  
 Ion Ratio Lower Upper  
 41 100  
 39 61.4 55.8 83.6  
 76 0.0 24.3 36.5#



#15  
 Acrylonitrile  
 Concen: 1.295 ug/l  
 RT: 3.068 min Scan# 325  
 Delta R.T. 0.006 min  
 Lab File: VX037651.D  
 Acq: 11 Sep 2023 19:26


Tgt Ion: 53 Resp: 1537  
 Ion Ratio Lower Upper  
 53 100  
 52 89.7 66.0 99.0  
 51 36.2 29.8 44.6








#16  
Acetone  
Concen: 1.561 ug/l  
RT: 2.379 min Scan# 213  
Delta R.T. -0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion: 43 Resp: 1629  
Ion Ratio Lower Upper  
43 100  
58 34.8 21.9 32.9#



#17  
Carbon Disulfide  
Concen: 1.684 ug/l  
RT: 2.507 min Scan# 233  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 76 Resp: 6886  
Ion Ratio Lower Upper  
76 100  
78 7.6 7.0 10.6









#18  
Methyl Acetate  
Concen: 0.246 ug/l  
RT: 2.709 min Scan# 20  
Delta R.T. 0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 43 Resp: 1075  
Ion Ratio Lower Upper  
43 100  
74 11.1 17.8 26.8#



#20  
Methylene Chloride  
Concen: Below Cal  
RT: 2.794 min Scan# 280  
Delta R.T. 0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 84 Resp: 1127  
Ion Ratio Lower Upper  
84 100  
49 104.5 103.6 155.4  
51 42.5 33.8 50.6  
86 73.3 49.4 74.0









#21  
trans-1,2-Dichloroethene  
Concen: 0.755 ug/l  
RT: 3.087 min Scan# 31  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 96 Resp: 1420  
Ion Ratio Lower Upper  
96 100  
61 115.3 119.2 178.8#  
98 59.1 48.7 73.1



#23  
Vinyl Acetate  
Concen: 0.539 ug/l  
RT: 3.745 min Scan# 436  
Delta R.T. 0.024 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 43 Resp: 2437  
Ion Ratio Lower Upper  
43 100  
86 13.9 7.8 11.8#









#25  
2-Butanone  
Concen: 1.096 ug/l  
RT: 4.574 min Scan# 51  
Delta R.T. 0.012 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 43 Resp: 1836  
Ion Ratio Lower Upper  
43 100  
72 16.9 19.4 29.2#

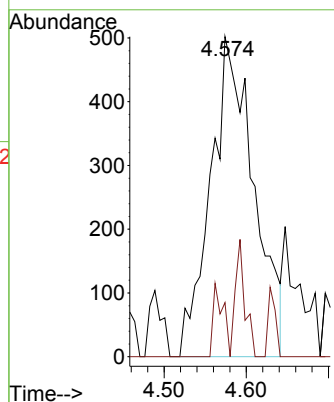

#27  
cis-1,2-Dichloroethene  
Concen: 0.362 ug/l  
RT: 4.495 min Scan# 559  
Delta R.T. 0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 96 Resp: 814  
Ion Ratio Lower Upper  
96 100  
61 115.7 0.0 312.2  
98 59.5 0.0 129.0

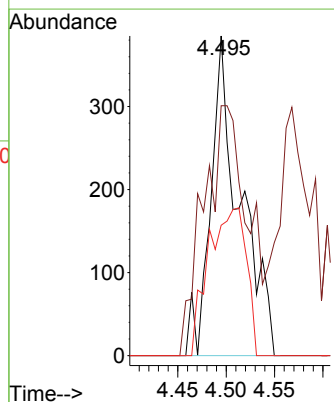



#29

Tetrahydrofuran

Concen: 0.331 ug/l

RT: 5.025 min Scan# 643

Delta R.T. 0.018 min


Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Instrument :

MSVOA\_X

ClientSampleId :

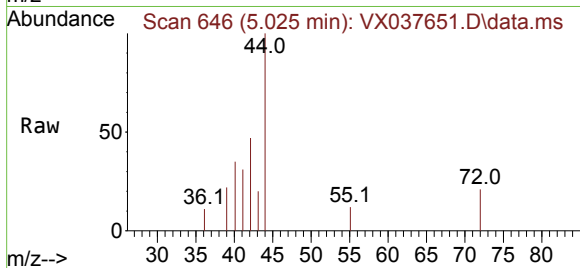




Tgt Ion: 42 Resp: 358

Ion Ratio Lower Upper

42 100

72 0.0 34.2 51.4#

71 0.0 32.2 48.2#



#31

Cyclohexane

Concen: 0.347 ug/l

RT: 5.482 min Scan# 721

Delta R.T. 0.012 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26




Tgt Ion: 56 Resp: 1009


Ion Ratio Lower Upper

56 100

69 47.9 23.4 35.2#

84 71.2 65.9 98.9

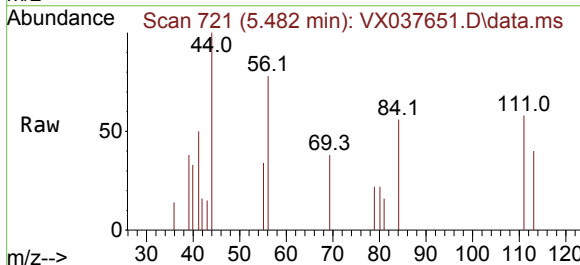



#33

1,2-Dichloroethane-d4

Concen: 42.257 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Instrument :

MSVOA\_X





ClientSampleId :

Tgt Ion: 65 Resp: 106647

Ion Ratio Lower Upper

65 100

67 51.8 0.0 100.2

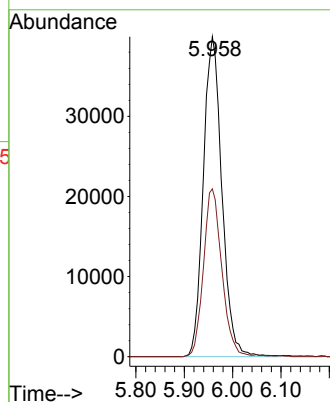

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26




Tgt Ion:114 Resp: 268809


Ion Ratio Lower Upper

114 100

63 19.6 0.0 45.0

88 15.9 0.0 36.6



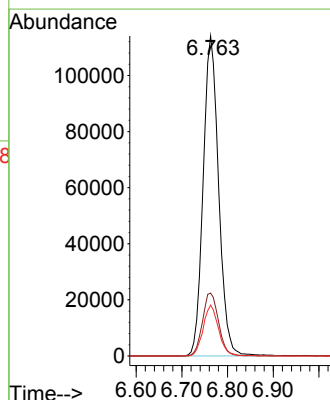





#35  
Dibromofluoromethane  
Concen: 44.509 ug/l  
RT: 5.391 min Scan# 705  
Delta R.T. 0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion:113 Resp: 84805  
Ion Ratio Lower Upper  
113 100  
111 102.3 82.9 124.3  
192 17.5 13.3 19.9



#36  
1,1-Dichloropropene  
Concen: 0.799 ug/l  
RT: 5.702 min Scan# 757  
Delta R.T. 0.012 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26


Tgt Ion: 75 Resp: 2099  
Ion Ratio Lower Upper  
75 100  
110 26.0 17.0 50.9  
77 24.5 24.7 37.1#








#38  
Carbon Tetrachloride  
Concen: 0.307 ug/l  
RT: 5.678 min Scan# 753  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion:117 Resp: 806  
Ion Ratio Lower Upper  
117 100  
119 72.9 78.2 117.2#  
121 19.9 24.4 36.6#

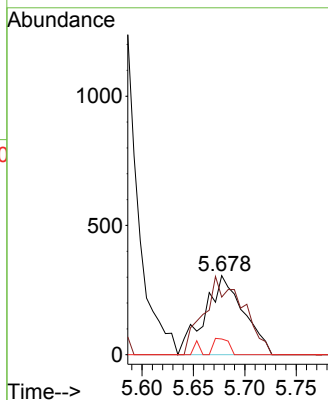

#39  
Methylcyclohexane  
Concen: 0.351 ug/l  
RT: 7.378 min Scan# 1032  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 83 Resp: 1085  
Ion Ratio Lower Upper  
83 100  
55 82.5 64.6 97.0  
98 40.8 36.7 55.1


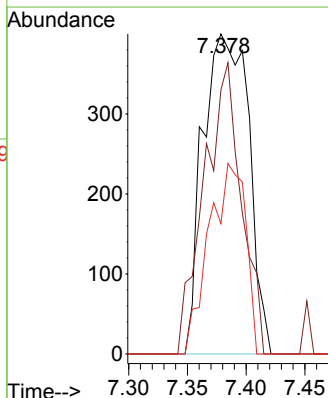




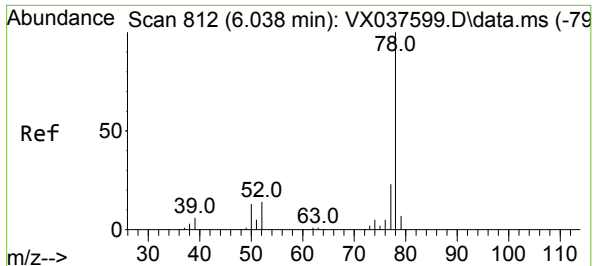

#40  
Benzene  
Concen: 0.244 ug/l  
RT: 6.049 min Scan# 812  
Delta R.T. 0.012 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 78 Resp: 1948  
Ion Ratio Lower Upper  
78 100  
77 23.9 19.3 28.9

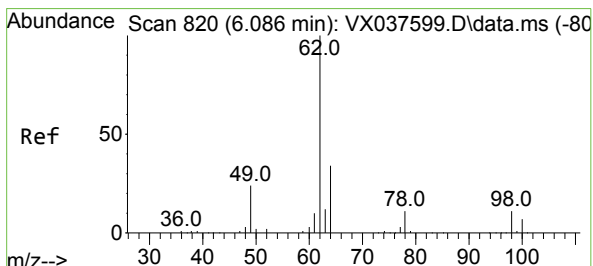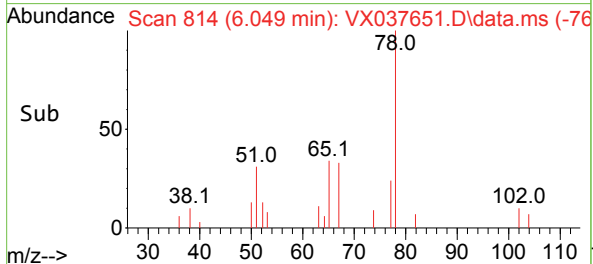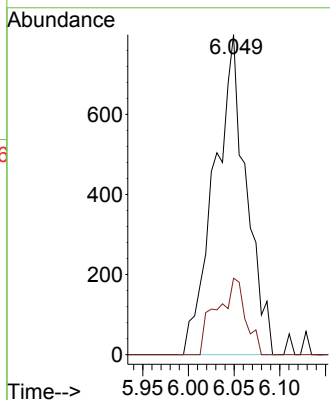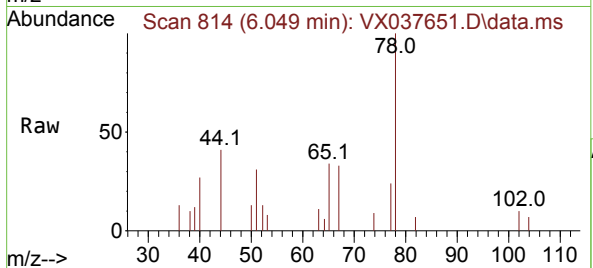

#42  
1,2-Dichloroethane  
Concen: 0.312 ug/l  
RT: 6.098 min Scan# 822  
Delta R.T. 0.012 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26


Tgt Ion: 62 Resp: 965  
Ion Ratio Lower Upper  
62 100  
98 0.0 0.0 16.0

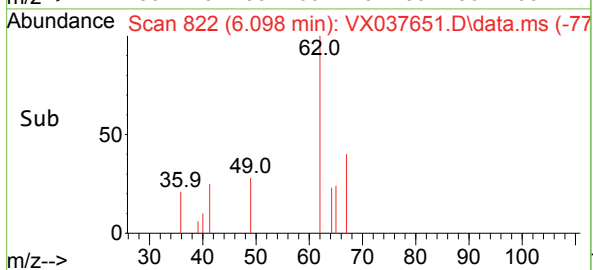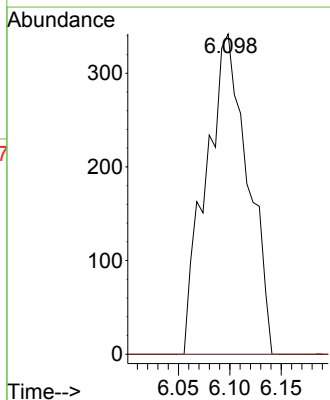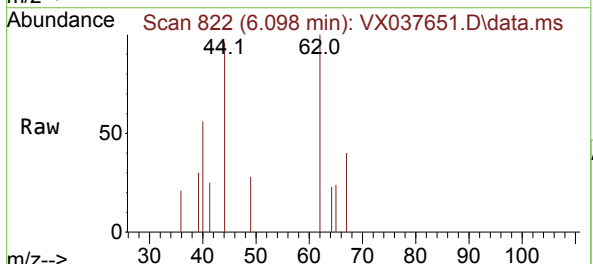



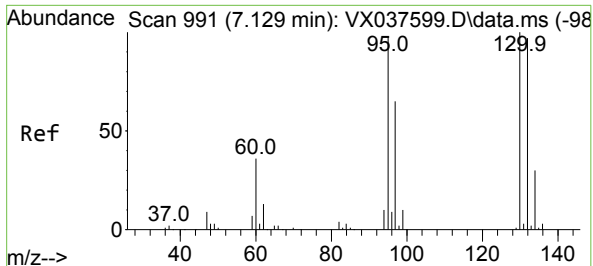


#44  
Trichloroethene  
Concen: 0.640 ug/l  
RT: 7.128 min Scan# 991  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Instrument :  
MSVOA\_X  
ClientSampleId :



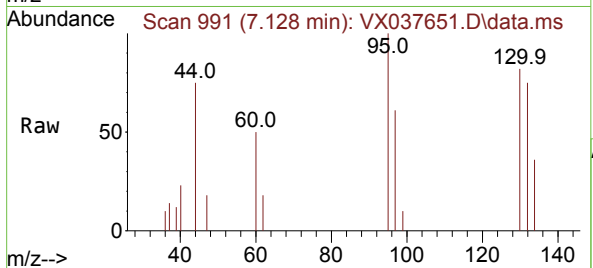



Tgt Ion:130 Resp: 1247  
Ion Ratio Lower Upper  
130 100  
95 121.5 0.0 204.4

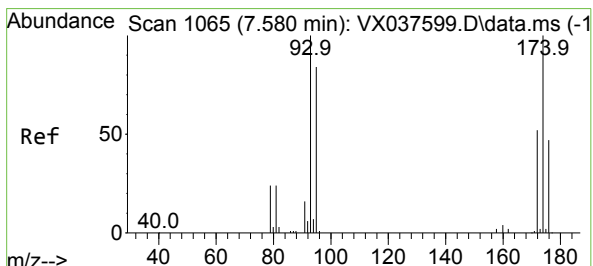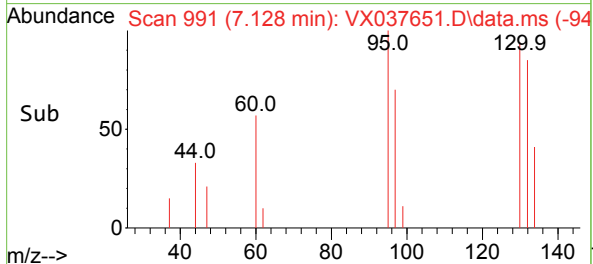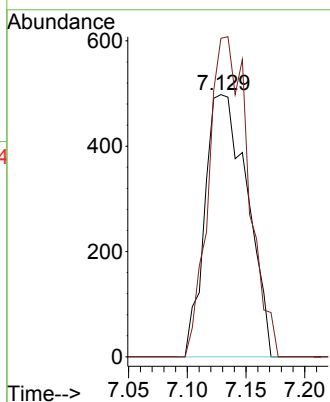

#46  
Dibromomethane  
Concen: 0.341 ug/l  
RT: 7.580 min Scan# 1065  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 93 Resp: 521  
Ion Ratio Lower Upper  
93 100  
95 61.4 66.6 100.0#  
174 78.9 69.4 104.0


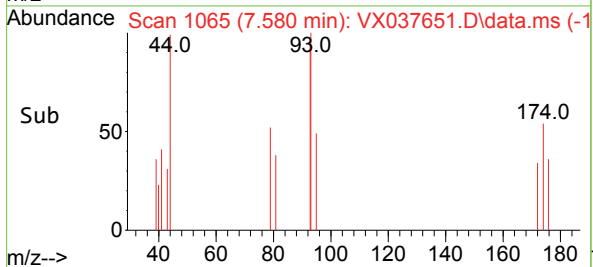
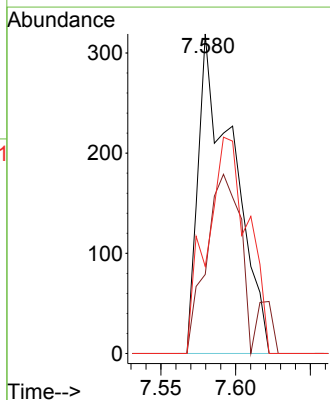
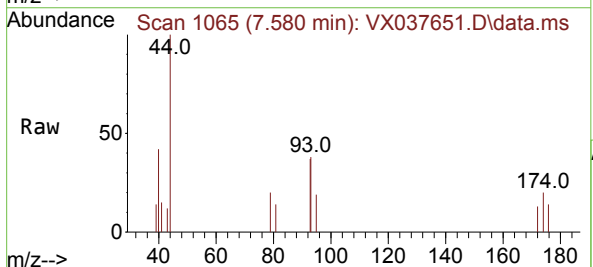




#50  
Toluene-d8  
Concen: 46.021 ug/l  
RT: 8.647 min Scan# 11  
Delta R.T. -0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 98 Resp: 330698  
Ion Ratio Lower Upper  
98 100  
100 62.9 53.1 79.7

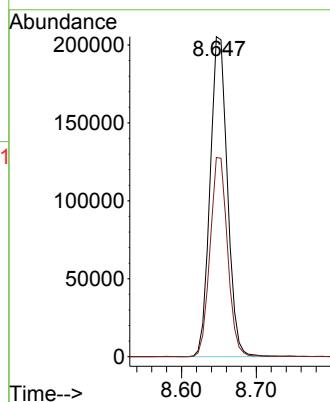

#51  
4-Methyl-2-Pentanone  
Concen: 0.502 ug/l  
RT: 8.586 min Scan# 1230  
Delta R.T. 0.012 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 43 Resp: 1586  
Ion Ratio Lower Upper  
43 100  
58 31.5 30.4 45.6



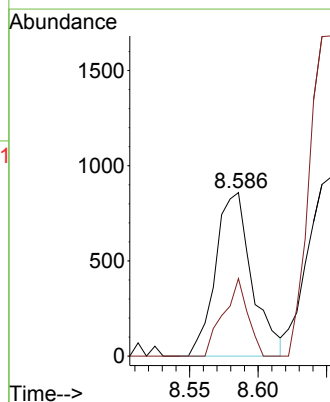





#52  
Toluene  
Concen: 0.333 ug/l  
RT: 8.720 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 92 Resp: 1685  
Ion Ratio Lower Upper  
92 100  
91 186.9 134.2 201.2

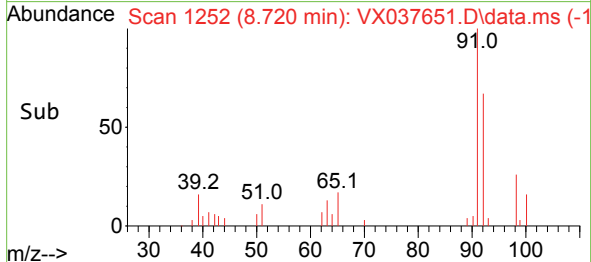

#53  
t-1,3-Dichloropropene  
Concen: 0.280 ug/l  
RT: 8.982 min Scan# 1295  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26


Tgt Ion: 75 Resp: 776  
Ion Ratio Lower Upper  
75 100  
77 22.7 25.7 38.5#








#54  
 cis-1,3-Dichloropropene  
 Concen: 0.257 ug/l  
 RT: 8.384 min Scan# 1197  
 Delta R.T. 0.018 min  
 Lab File: VX037651.D  
 Acq: 11 Sep 2023 19:26

Instrument :  
 MSVOA\_X  
 ClientSampleId :







Tgt Ion: 75 Resp: 777  
 Ion Ratio Lower Upper  
 75 100  
 77 24.3 25.3 37.9#  
 39 36.9 46.7 70.1#

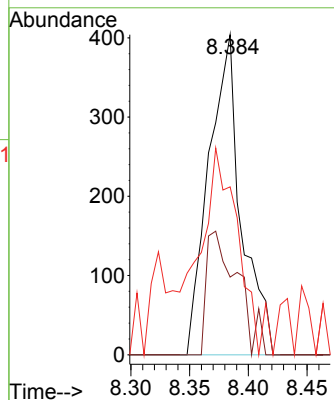

#58  
 2-Chloroethyl Vinyl ether  
 Concen: 0.514 ug/l  
 RT: 8.250 min Scan# 1175  
 Delta R.T. 0.006 min  
 Lab File: VX037651.D  
 Acq: 11 Sep 2023 19:26

Tgt Ion: 63 Resp: 810  
 Ion Ratio Lower Upper  
 63 100  
 106 22.1 22.5 33.7#



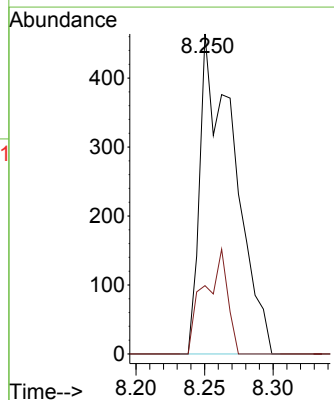





#59  
2-Hexanone  
Concen: 0.525 ug/l  
RT: 9.445 min Scan# 11  
Delta R.T. 0.012 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 43 Resp: 1272  
Ion Ratio Lower Upper  
43 100  
58 48.9 26.2 78.5



#62  
4-Bromofluorobenzene  
Concen: 40.789 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 95 Resp: 105744  
Ion Ratio Lower Upper  
95 100  
174 76.9 0.0 135.6  
176 74.3 0.0 131.0

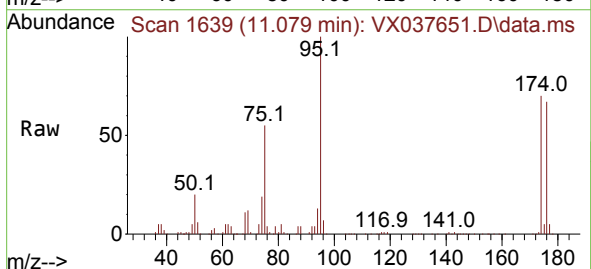



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min


Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Instrument :

MSVOA\_X

ClientSampleId :






Tgt Ion:117 Resp: 236629

Ion Ratio Lower Upper

117 100

82 56.4 46.2 69.4

119 31.4 25.5 38.3



#64

Tetrachloroethene

Concen: 0.806 ug/l

RT: 9.281 min Scan# 1344

Delta R.T. 0.006 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Tgt Ion:164 Resp: 1222




Ion Ratio Lower Upper


164 100

166 111.3 102.7 154.1

129 88.0 80.4 120.6

131 74.5 76.5 114.7#


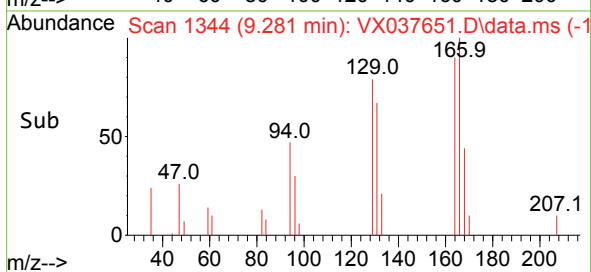






#65  
Chlorobenzene  
Concen: 0.448 ug/l  
RT: 10.085 min Scan# 1475  
Delta R.T. 0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion:112 Resp: 2284  
Ion Ratio Lower Upper  
112 100  
114 22.2 25.7 38.5#



#67  
Ethyl Benzene  
Concen: 0.467 ug/l  
RT: 10.201 min Scan# 1495  
Delta R.T. 0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 91 Resp: 4232  
Ion Ratio Lower Upper  
91 100  
106 30.9 24.9 37.3









#68  
m/p-Xylenes  
Concen: 1.007 ug/l  
RT: 10.305 min Scan# 1512  
Delta R.T. 0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion:106 Resp: 3482  
Ion Ratio Lower Upper  
106 100  
91 200.7 165.5 248.3

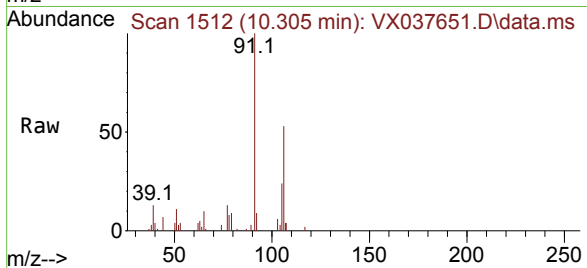

#69  
o-Xylene  
Concen: 0.363 ug/l  
RT: 10.646 min Scan# 1568  
Delta R.T. 0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion:106 Resp: 1245  
Ion Ratio Lower Upper  
106 100  
91 231.9 108.9 326.8

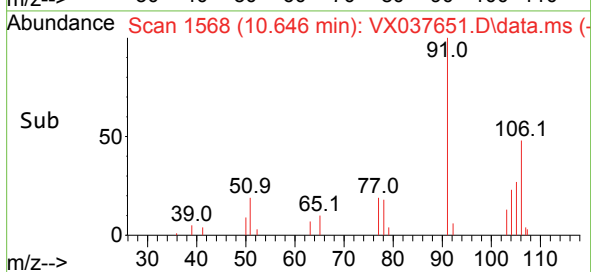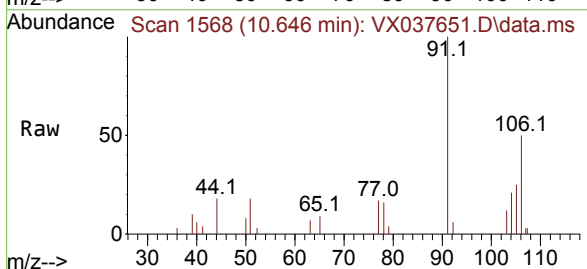



#70

Styrene

Concen: 0.372 ug/l

RT: 10.658 min Scan# 11

Delta R.T. -0.001 min


Lab File: VX037651.D

Acq: 11 Sep 2023 19:26




Instrument :

MSVOA\_X

ClientSampleId :



|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 104   | Resp: | 2104  |
| Ion Ratio | Lower | Upper |       |
| 104       | 100   |       |       |
| 78        | 67.1  | 43.6  | 65.4# |
| 103       | 56.2  | 43.6  | 65.4  |

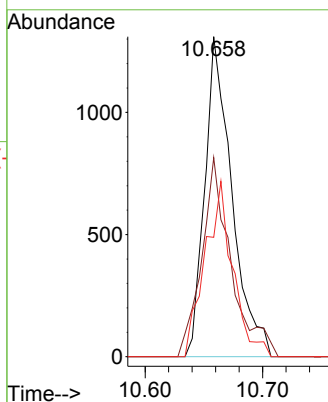

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l




RT: 12.024 min Scan# 1794


Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 152   | Resp: | 92024 |
| Ion Ratio | Lower | Upper |       |
| 152       | 100   |       |       |
| 115       | 62.8  | 43.3  | 129.9 |
| 150       | 161.2 | 0.0   | 345.0 |



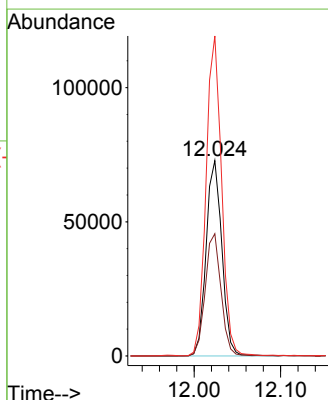





#73  
Isopropylbenzene  
Concen: 0.545 ug/l  
RT: 10.963 min Scan# 1601  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion:105 Resp: 3777  
Ion Ratio Lower Upper  
105 100  
120 26.3 12.9 38.6



#74  
N-ethyl acetate  
Concen: 0.244 ug/l  
RT: 10.847 min Scan# 1601  
Delta R.T. 0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 43 Resp: 747  
Ion Ratio Lower Upper  
43 100  
70 30.4 32.9 49.3#  
55 26.6 19.3 28.9  
61 0.0 18.8 28.2#









#76  
1,2,3-Trichloropropane  
Concen: 27.601 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.159 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 75 Resp: 57415  
Ion Ratio Lower Upper  
75 100  
77 1.3 19.1 57.5#

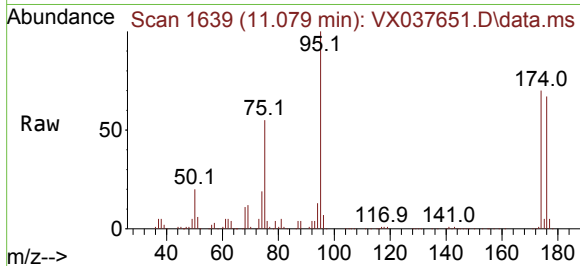

#77  
Bromobenzene  
Concen: 0.563 ug/l  
RT: 11.195 min Scan# 1658  
Delta R.T. -0.006 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 156 Resp: 935  
Ion Ratio Lower Upper  
156 100  
77 177.0 88.4 265.3  
158 99.8 48.0 144.0

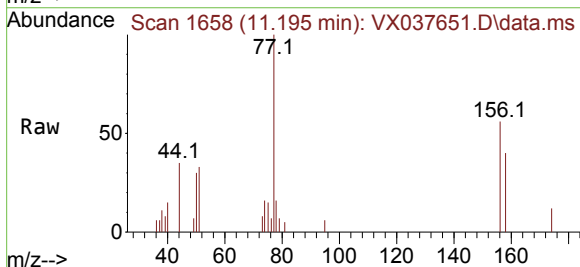



#78

n-propylbenzene

Concen: 0.738 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Instrument :

MSVOA\_X





ClientSampleId :

Tgt Ion: 91 Resp: 5900

Ion Ratio Lower Upper

91 100

120 22.8 11.5 34.4



#79

2-Chlorotoluene

Concen: 0.738 ug/l

RT: 11.366 min Scan# 1686

Delta R.T. -0.000 min

Lab File: VX037651.D




Acq: 11 Sep 2023 19:26


Tgt Ion: 91 Resp: 3627

Ion Ratio Lower Upper

91 100

126 26.5 16.3 48.8





#80

1,3,5-Trimethylbenzene

Concen: 0.637 ug/l

RT: 11.451 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Instrument :

MSVOA\_X





ClientSampleId :

Tgt Ion:105 Resp: 3729

Ion Ratio Lower Upper

105 100

120 39.7 24.1 72.3



#81

trans-1,4-Dichloro-2-butene

Concen: 86.266 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26




Tgt Ion: 75 Resp: 57415


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.0 36.9 55.3#









#82  
4-Chlorotoluene  
Concen: 0.864 ug/l  
RT: 11.457 min Scan# 1701  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 91 Resp: 4832  
Ion Ratio Lower Upper  
91 100  
126 31.7 14.2 42.6



#83  
tert-Butylbenzene  
Concen: 0.508 ug/l  
RT: 11.713 min Scan# 1743  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion: 119 Resp: 2963  
Ion Ratio Lower Upper  
119 100  
91 67.6 31.2 93.6  
134 23.3 11.7 35.0

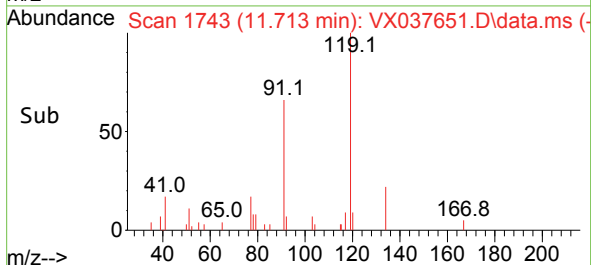



#84

1,2,4-Trimethylbenzene

Concen: 0.707 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Instrument :

MSVOA\_X





ClientSampleId :

Tgt Ion:105 Resp: 4154

Ion Ratio Lower Upper

105 100

120 43.4 21.2 63.6

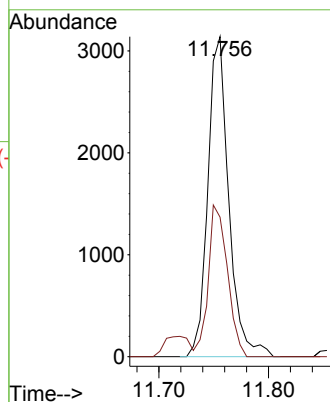

#85

sec-Butylbenzene

Concen: 0.612 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. -0.000 min

Lab File: VX037651.D




Acq: 11 Sep 2023 19:26


Tgt Ion:105 Resp: 4422

Ion Ratio Lower Upper

105 100

134 19.2 9.8 29.4



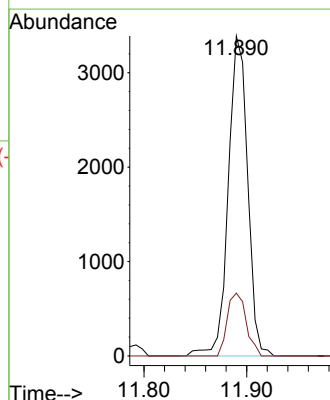





#86  
 p-Isopropyltoluene  
 Concen: 0.660 ug/l  
 RT: 12.012 min Scan# 1792  
 Delta R.T. -0.000 min  
 Lab File: VX037651.D  
 Acq: 11 Sep 2023 19:26




Instrument :  
 MSVOA\_X  
 ClientSampleId :


|             |       |           |
|-------------|-------|-----------|
| Tgt Ion:119 | Resp: | 3929      |
| Ion Ratio   | Lower | Upper     |
| 119         | 100   |           |
| 134         | 28.6  | 12.8 38.3 |
| 91          | 34.2  | 13.1 39.3 |

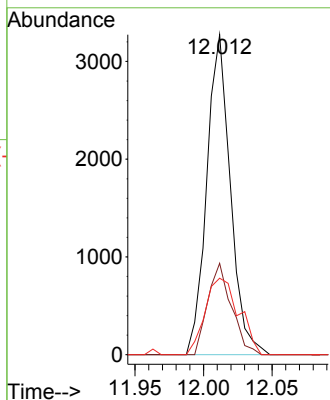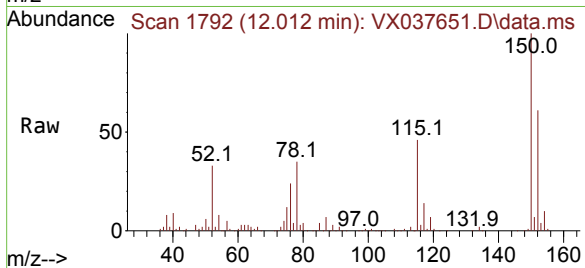

#87  
 1,3-Dichlorobenzene  
 Concen: 0.975 ug/l  
 RT: 11.969 min Scan# 1785  
 Delta R.T. -0.000 min  
 Lab File: VX037651.D  
 Acq: 11 Sep 2023 19:26


|             |       |           |
|-------------|-------|-----------|
| Tgt Ion:146 | Resp: | 3078      |
| Ion Ratio   | Lower | Upper     |
| 146         | 100   |           |
| 111         | 45.9  | 22.1 66.1 |
| 148         | 66.0  | 31.8 95.3 |

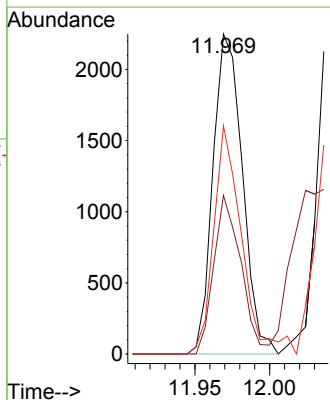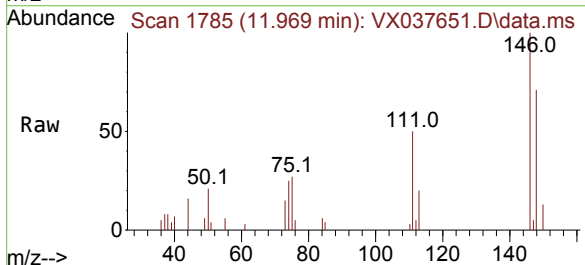






#88  
1,4-Dichlorobenzene  
Concen: 0.957 ug/l  
RT: 11.969 min Scan# 1797  
Delta R.T. -0.074 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion:146 Resp: 3078  
Ion Ratio Lower Upper  
146 100  
111 45.9 21.3 63.7  
148 66.0 31.8 95.4



#89  
n-Butylbenzene  
Concen: 0.833 ug/l  
RT: 12.335 min Scan# 1845  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26


Tgt Ion: 91 Resp: 4440  
Ion Ratio Lower Upper  
91 100  
92 49.1 27.4 82.0  
134 21.4 12.6 37.8








#90  
Hexachloroethane  
Concen: 0.453 ug/l  
RT: 12.542 min Scan# 117  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Instrument :  
MSVOA\_X  
ClientSampleId :



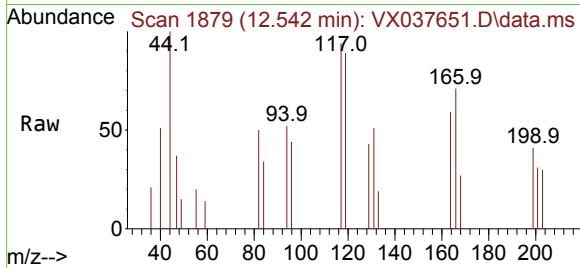



Tgt Ion:117 Resp: 456  
Ion Ratio Lower Upper  
117 100  
201 45.8 32.9 98.6

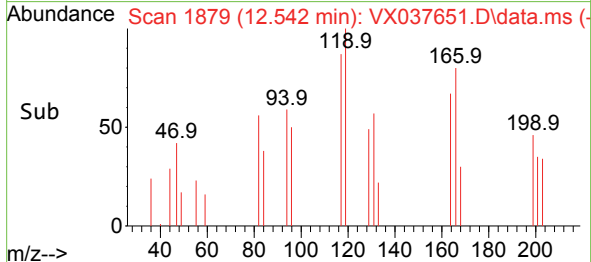

#91  
1,2-Dichlorobenzene  
Concen: 0.683 ug/l  
RT: 12.335 min Scan# 1845  
Delta R.T. -0.000 min  
Lab File: VX037651.D  
Acq: 11 Sep 2023 19:26

Tgt Ion:146 Resp: 2194  
Ion Ratio Lower Upper  
146 100  
111 50.2 22.4 67.0  
148 64.6 31.6 95.0

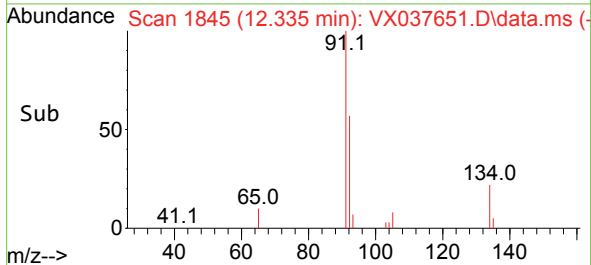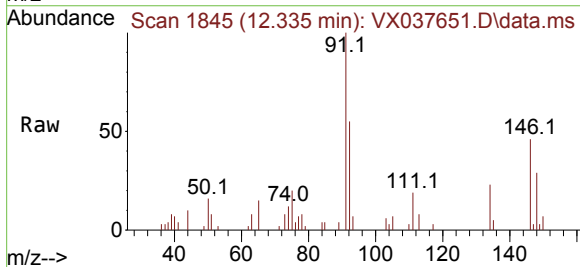



#93

1,2,4-Trichlorobenzene

Concen: 1.601 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. -0.000 min

Lab File: VX037651.D





Acq: 11 Sep 2023 19:26

Instrument :

MSVOA\_X

ClientSampleId :

|             |       |            |
|-------------|-------|------------|
| Tgt Ion:180 | Resp: | 2986       |
| Ion Ratio   | Lower | Upper      |
| 180         | 100   |            |
| 182         | 91.5  | 48.3 144.8 |
| 145         | 28.5  | 18.0 54.0  |



#94

Hexachlorobutadiene

Concen: 0.857 ug/l




RT: 13.725 min Scan# 2073


Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

|             |       |           |
|-------------|-------|-----------|
| Tgt Ion:225 | Resp: | 693       |
| Ion Ratio   | Lower | Upper     |
| 225         | 100   |           |
| 223         | 77.1  | 31.1 93.2 |
| 227         | 59.6  | 32.5 97.5 |





#95

Naphthalene

Concen: 1.473 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min


Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Instrument :

MSVOA\_X

ClientSampleId :

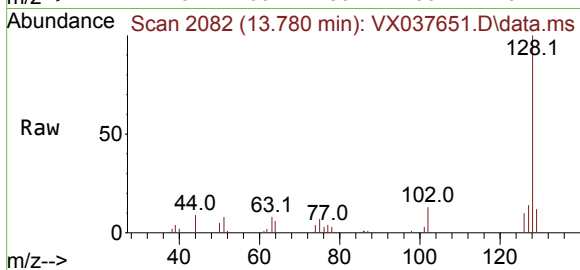




Tgt Ion:128 Resp: 9945

Ion Ratio Lower Upper

128 100

127 12.3 10.3 15.5

129 9.5 8.8 13.2



#96

1,2,3-Trichlorobenzene

Concen: 1.618 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX037651.D

Acq: 11 Sep 2023 19:26

Tgt Ion:180 Resp: 3112

Ion Ratio Lower Upper

180 100

182 95.9 46.9 140.6

145 35.7 17.8 53.5

